

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040323\
 Data File : PS022570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 09:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 11:57:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.304	6.723	1126.9E6	1189.9E6	461.012	577.715 #
Target Compounds							
1) T	Dalapon	2.434	0.000	709740	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.734f	0.000	112227	0	<MDL	N.D. #
3) T	4-Nitroph...	6.121	6.352	1278933	1496212	<MDL	1.066 #
7) T	MCPA	0.000	7.138f	0	10772372	N.D.	1.025
8) T	DICHLORPROP	0.000	7.548f	0	463680	N.D.	<MDL
9) T	2,4-D	7.190	0.000	287012	0	<MDL	N.D. #
10) T	Pentachlo...	7.462	8.215	8574953	6498862	<MDL	<MDL #
11) T	2,4,5-TP ...	7.954	8.595	495583	3252811	<MDL	<MDL #
13) T	2,4-DB	8.740	0.000	153332	0	<MDL	N.D. #
14) T	DINOSEB	9.790	9.783	3489467	1959544	<MDL	<MDL #
15) T	Picloram	9.580	10.700	109102	5395114	<MDL	<MDL #
16) T	DCPA	10.047	10.700	4663313	5395114	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040323\
Data File : PS022570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 09:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 11:57:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

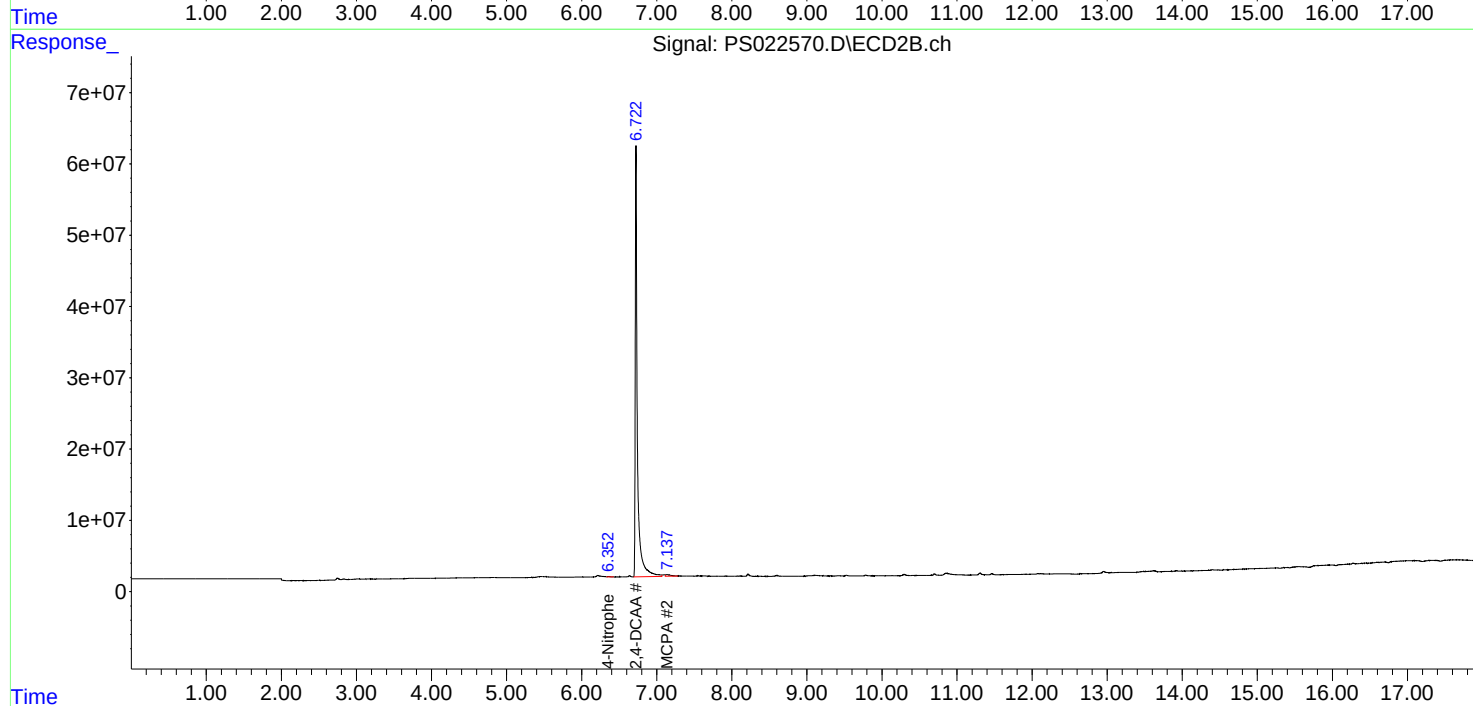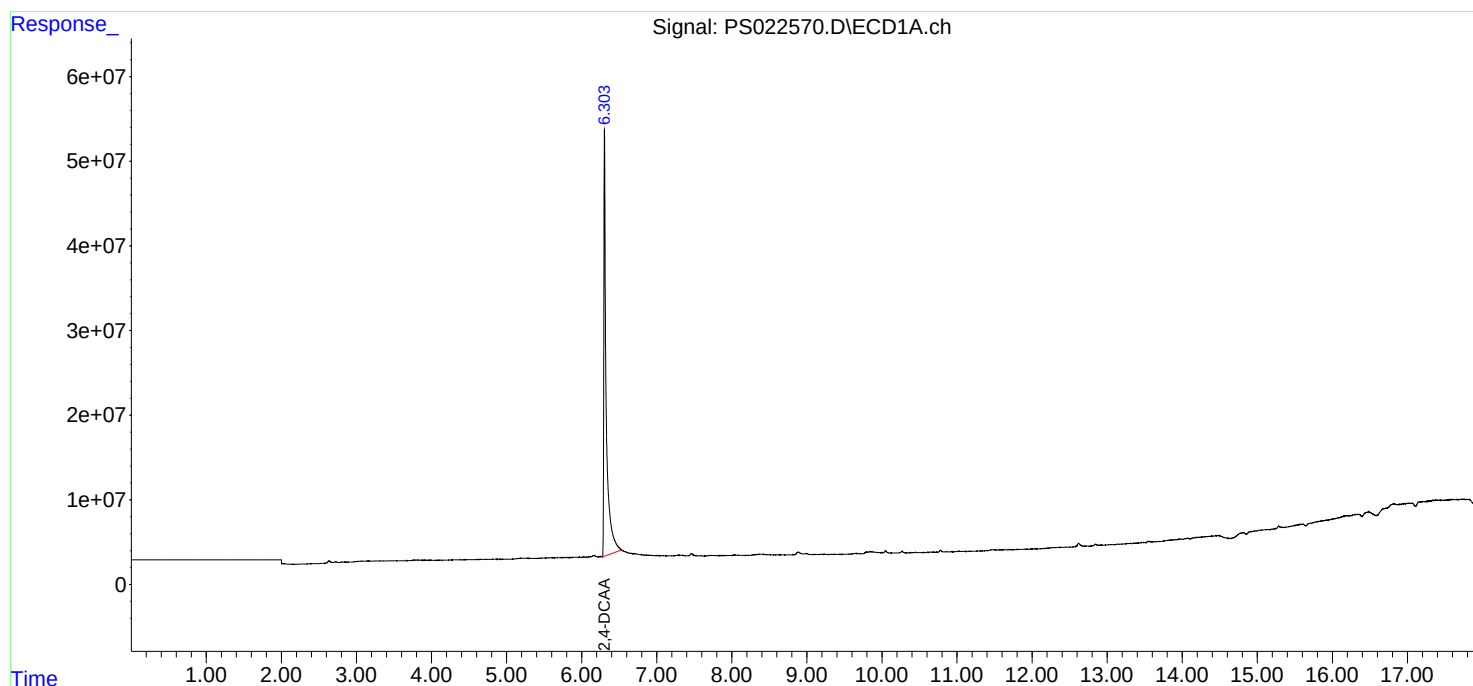


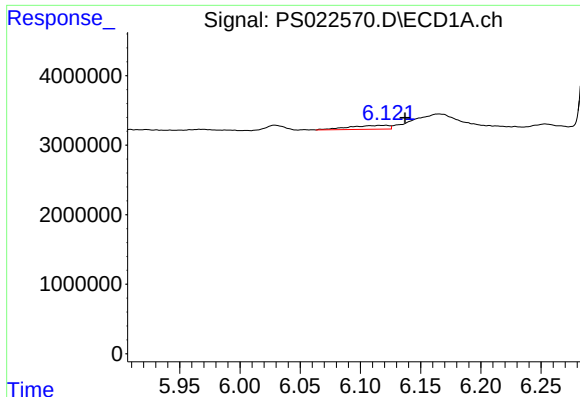

#3 4-Nitrophenol


R.T.: 6.121 min
Delta R.T.: -0.016 min
Response: 1278933
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

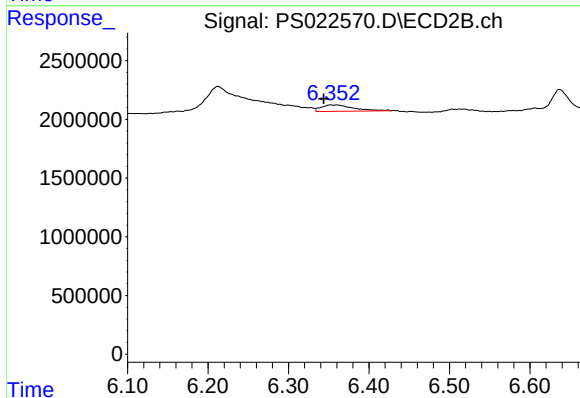


#3 4-Nitrophenol

R.T.: 6.352 min
Delta R.T.: 0.009 min
Response: 1496212
Conc: 1.07 ng/ml

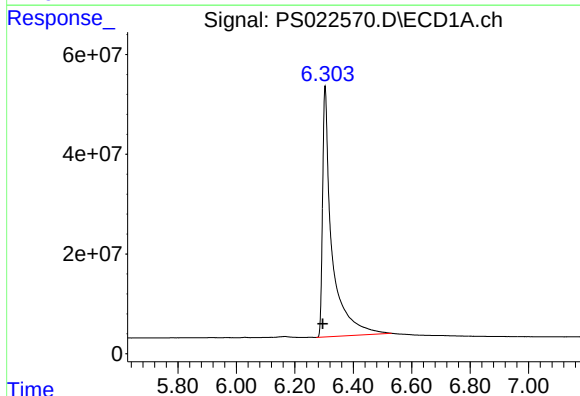


#4 2,4-DCAA

R.T.: 6.304 min
Delta R.T.: 0.007 min
Response: 1126888338
Conc: 461.01 ng/ml

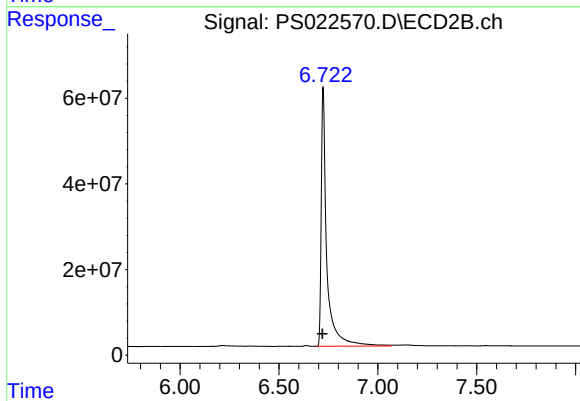

#4 2,4-DCAA


R.T.: 6.723 min
Delta R.T.: 0.003 min
Response: 1189911477
Conc: 577.71 ng/ml

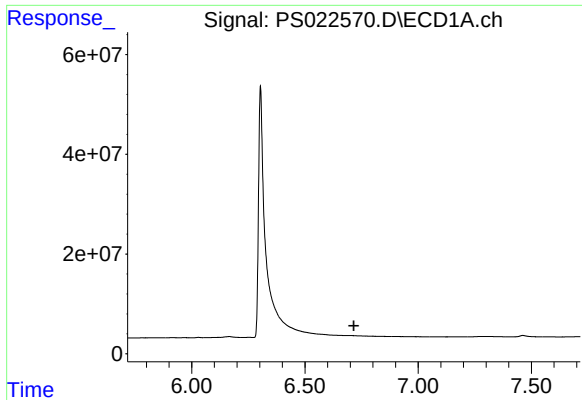

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.716 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

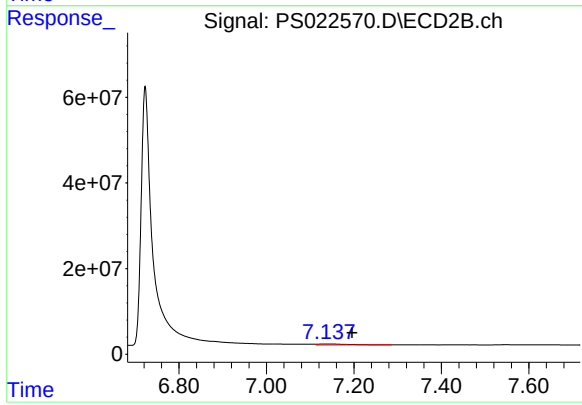

#7 MCPA

R.T.: 7.138 min
Delta R.T.: -0.058 min
Response: 10772372
Conc: 1.03 ug/ml