

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040423\
 Data File : PS022576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2023 08:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 21:59:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.315	0.000	441775	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.432	0.000	63212	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.708	0.000	51740	0	<MDL	N.D. #
3) T	4-Nitroph...	6.132	0.000	2488142	0	1.816	N.D. #
5) T	DICAMBA	6.443	0.000	274428	0	<MDL	N.D. #
8) T	DICHLORPROP	7.009	0.000	89940	0	<MDL	N.D. #
9) T	2,4-D	7.208	0.000	1775057	0	<MDL	N.D. #
10) T	Pentachlo...	7.449	0.000	1332679	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.951	8.541	321545	1795953	<MDL	<MDL #
12) T	2,4,5-T	8.221	0.000	8517235	0	<MDL	N.D. #
13) T	2,4-DB	8.734	0.000	911452	0	<MDL	N.D. #
14) T	DINOSEB	9.731	9.781	38474284	1104210	2.969	<MDL #
15) T	Picloram	9.643	10.696f	18579555	27543530	<MDL	1.373 #
16) T	DCPA	10.050	10.696	488193	27543530	<MDL	1.736 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040423\
Data File : PS022576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2023 08:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 21:59:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

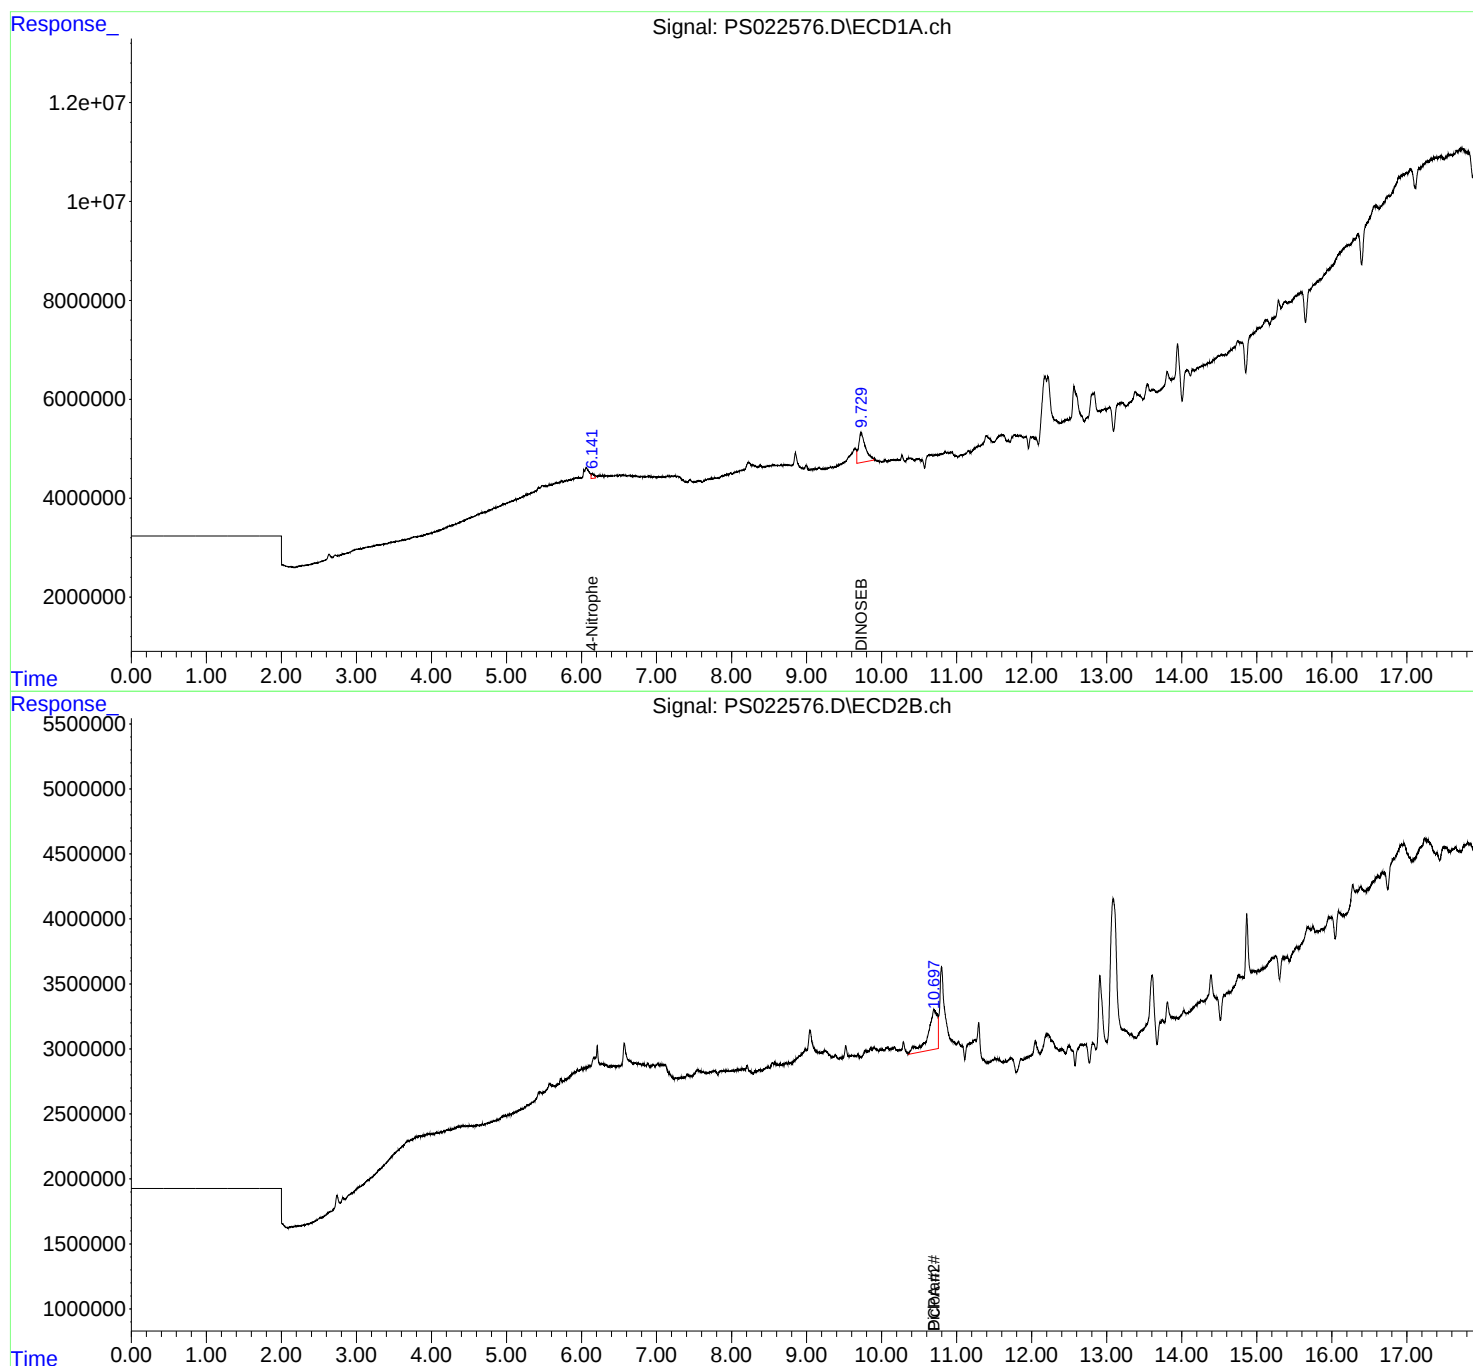


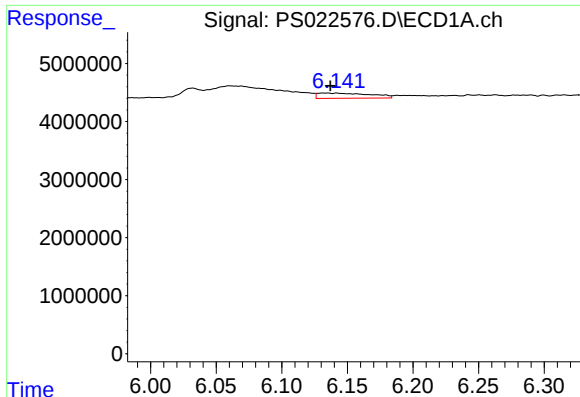

#3 4-Nitrophenol


R.T.: 6.132 min
Delta R.T.: -0.005 min
Response: 2488142
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

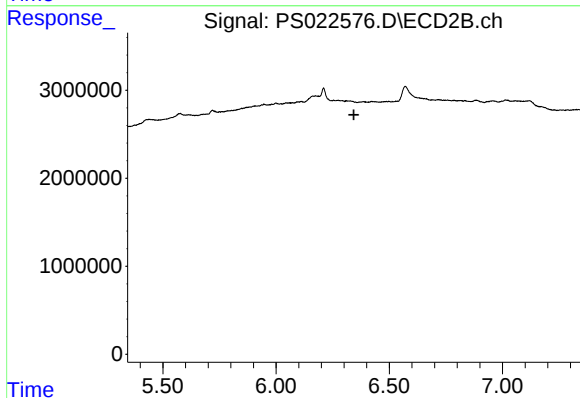


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

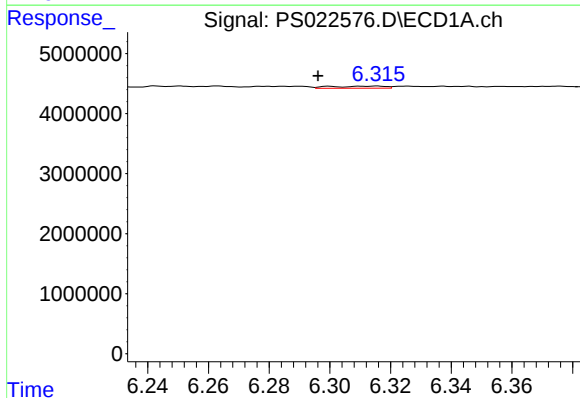


#4 2,4-DCAA

R.T.: 6.315 min
Delta R.T.: 0.019 min
Response: 441775
Conc: N.D.

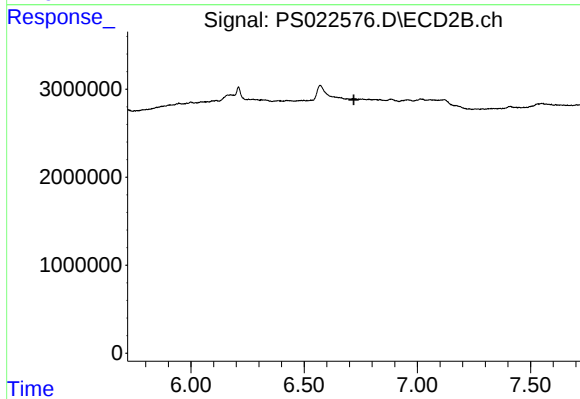

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.719 min
Response: 0
Conc: N.D.

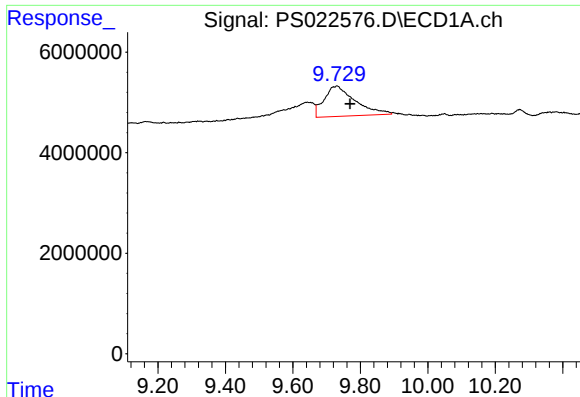

#14 DINOSEB


R.T.: 9.731 min
Delta R.T.: -0.039 min
Response: 38474284
Conc: 2.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

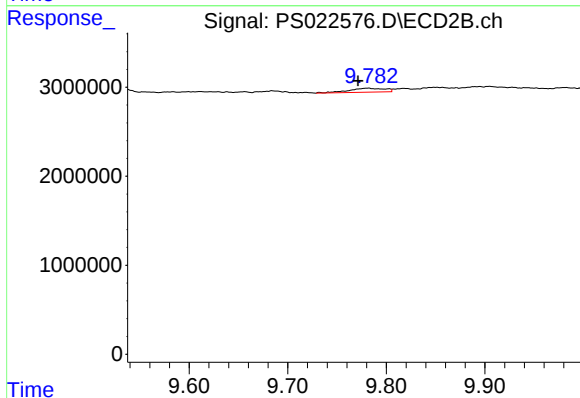


#14 DINOSEB

R.T.: 9.781 min
Delta R.T.: 0.010 min
Response: 1104210
Conc: N.D.

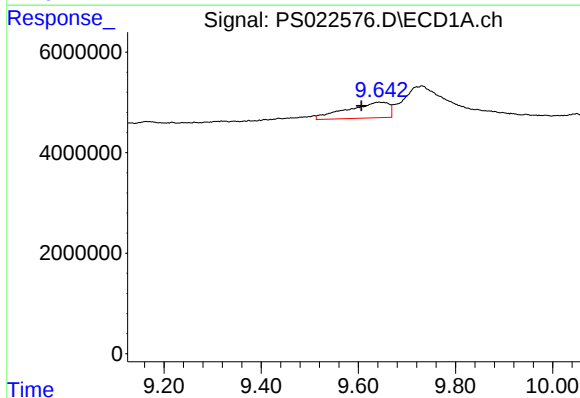


#15 Picloram

R.T.: 9.643 min
Delta R.T.: 0.036 min
Response: 18579555
Conc: N.D.

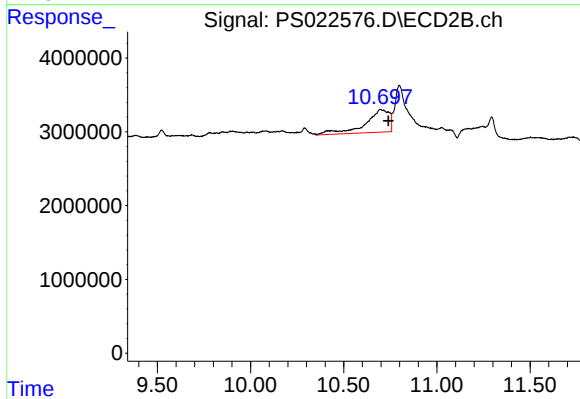

#15 Picloram


R.T.: 10.696 min
Delta R.T.: -0.043 min
Response: 27543530
Conc: 1.37 ng/ml

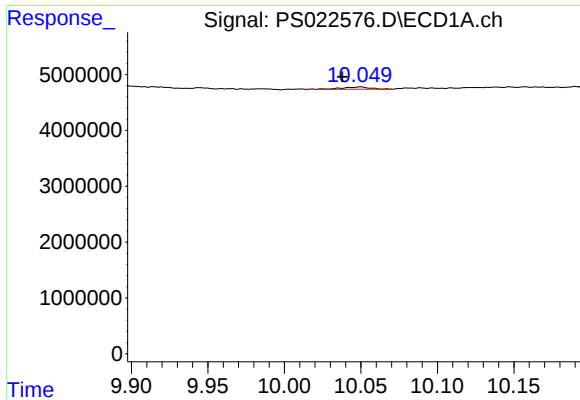

#16 DCPA

R.T.: 10.050 min
Delta R.T.: 0.012 min
Response: 488193
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

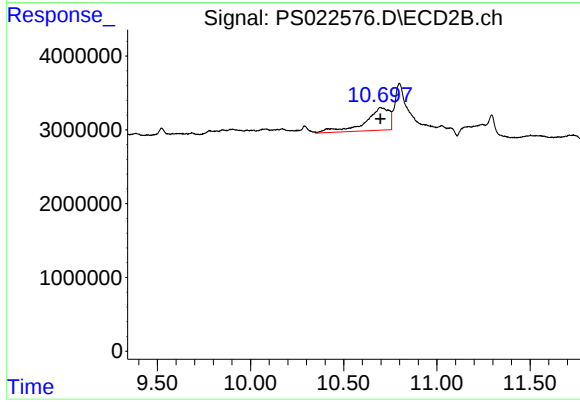

#16 DCPA

R.T.: 10.696 min
Delta R.T.: 0.000 min
Response: 27543530
Conc: 1.74 ng/ml