

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040423\
 Data File : PS022577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2023 08:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 21:59:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.305	6.724	1223.9E6	1259.0E6	500.684	611.247
Target Compounds							
1) T	Dalapon	2.445	0.000	1202731	0	<MDL	N.D. #
3) T	4-Nitroph...	6.172	0.000	4816996	0	3.516	N.D. #
6) T	MCP	0.000	7.023	0	8133707	N.D.	1.045
7) T	MCPA	0.000	7.150f	0	21567623	N.D.	2.053
9) T	2,4-D	7.182	0.000	474595	0	<MDL	N.D. #
10) T	Pentachlo...	7.470	8.218	7365430	8192098	<MDL	<MDL #
11) T	2,4,5-TP ...	7.947	8.611f	1089893	3251507	<MDL	<MDL #
12) T	2,4,5-T	8.188	0.000	488348	0	<MDL	N.D. #
14) T	DINOSEB	9.793	9.790	1028636	2195833	<MDL	<MDL #
15) T	Picloram	9.566f	10.702	202730	6315496	<MDL	<MDL #
16) T	DCPA	10.053	10.702	4838145	6315496	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040423\
Data File : PS022577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2023 08:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 21:59:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

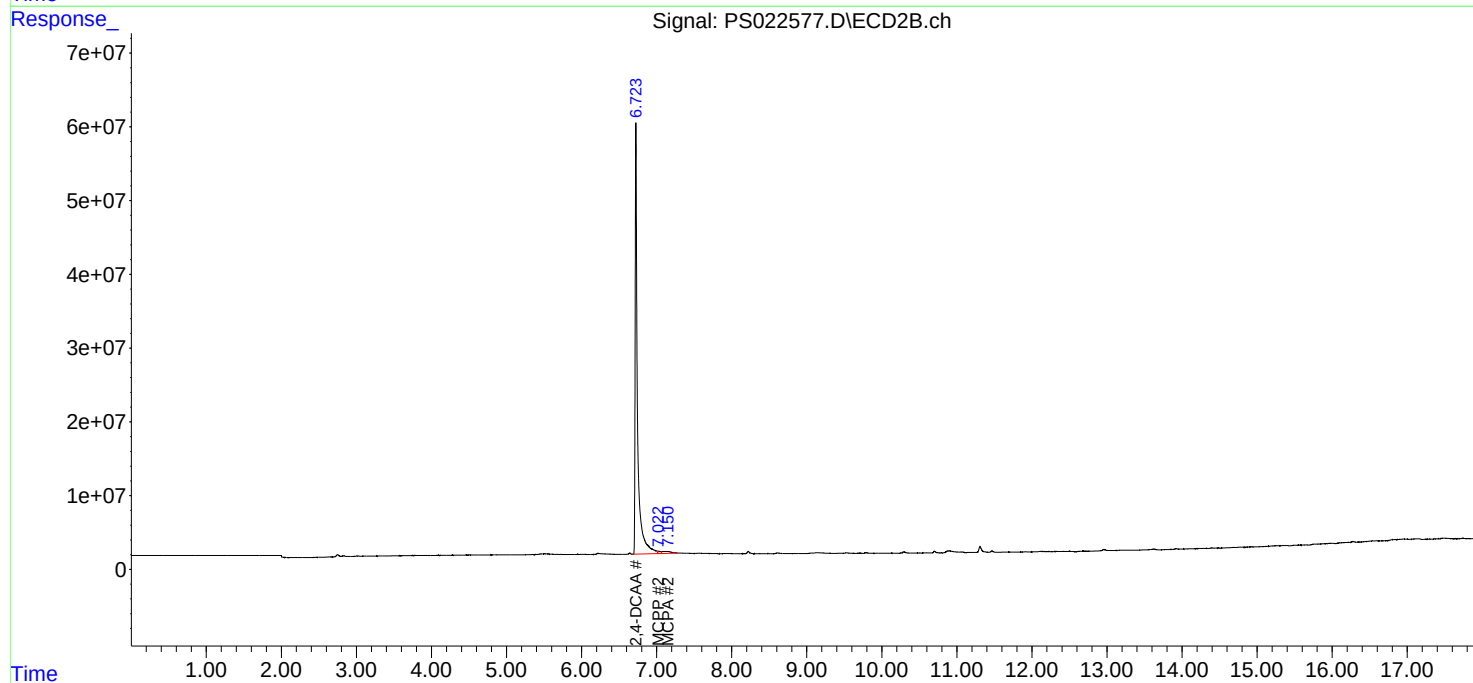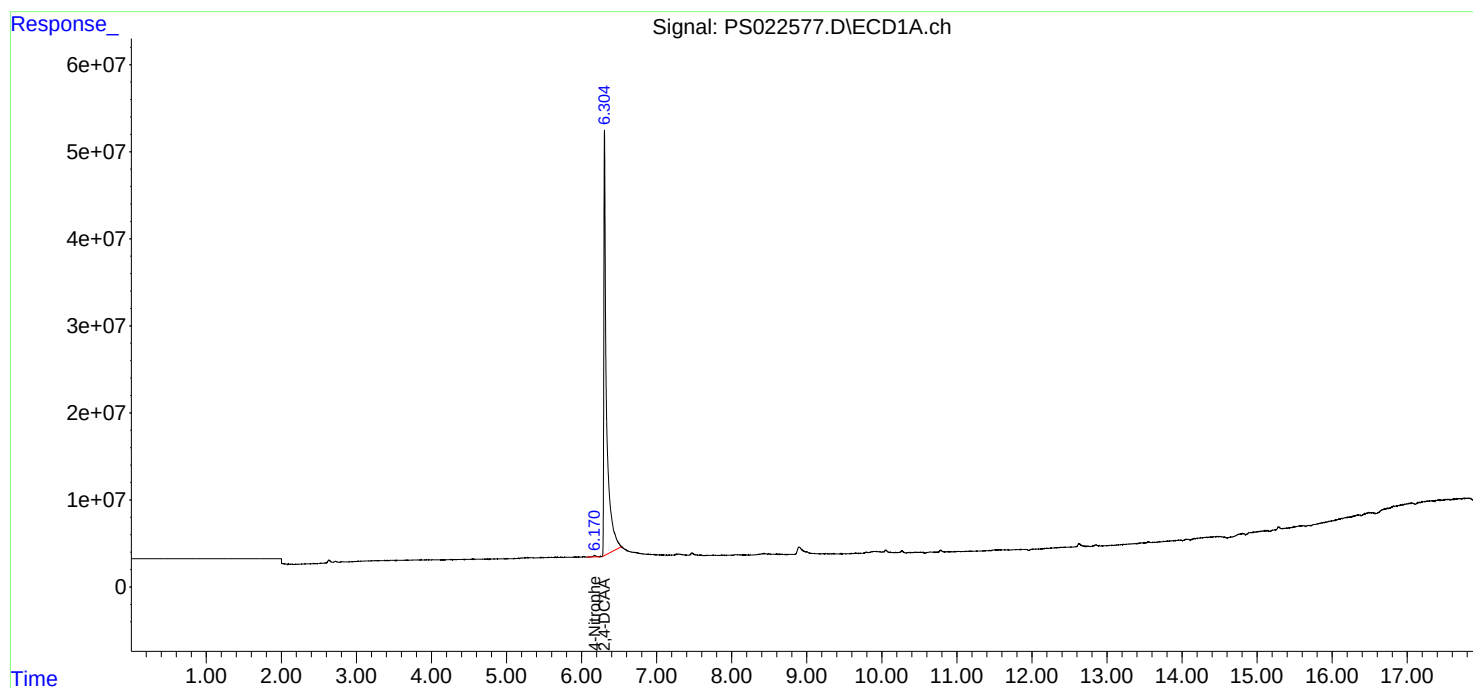


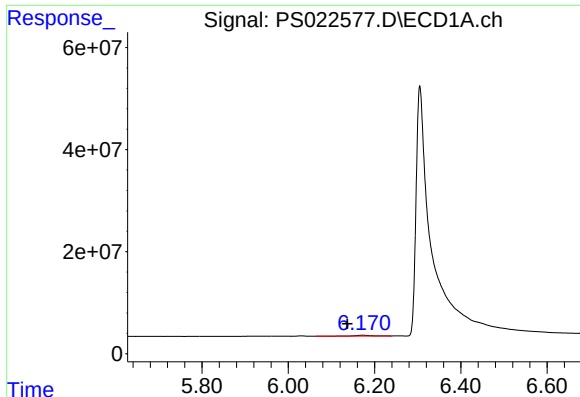

#3 4-Nitrophenol


R.T.: 6.172 min
Delta R.T.: 0.035 min
Response: 4816996
Conc: 3.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

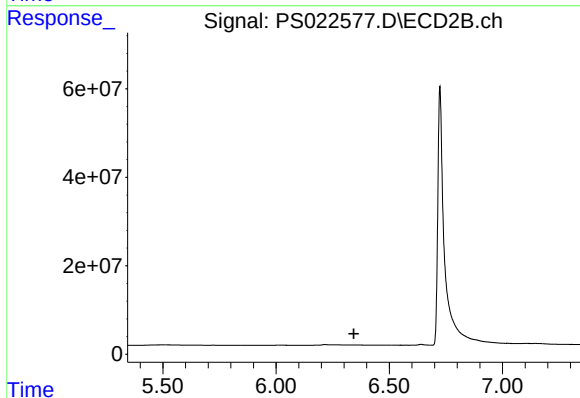


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

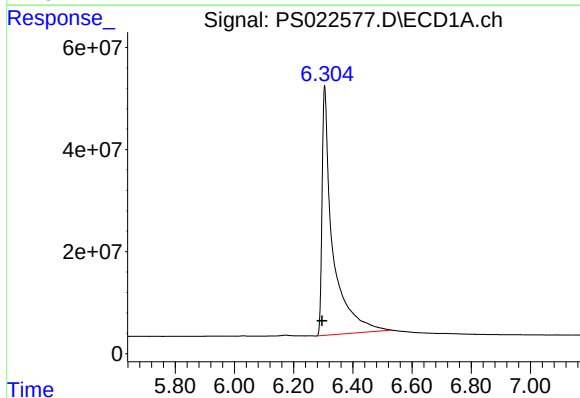


#4 2,4-DCAA

R.T.: 6.305 min
Delta R.T.: 0.009 min
Response: 1223862921
Conc: 500.68 ng/ml

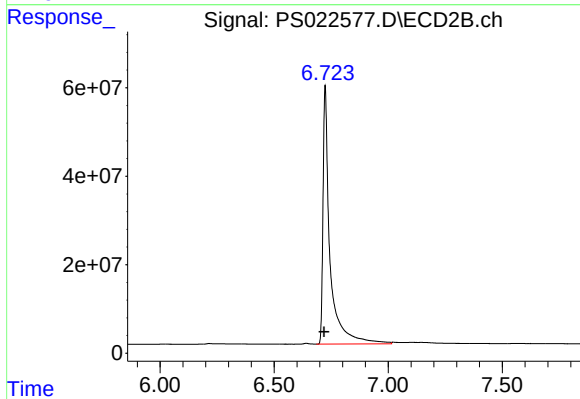

#4 2,4-DCAA


R.T.: 6.724 min
Delta R.T.: 0.004 min
Response: 1258978035
Conc: 611.25 ng/ml

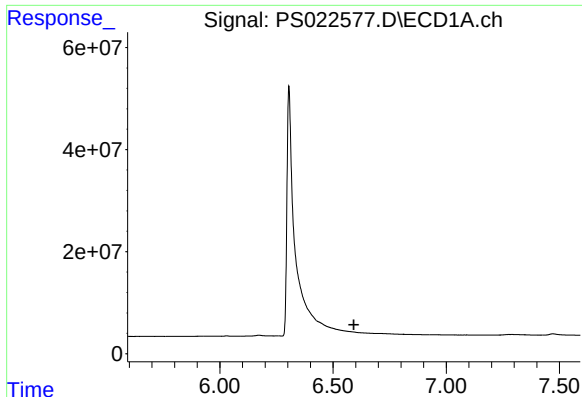

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

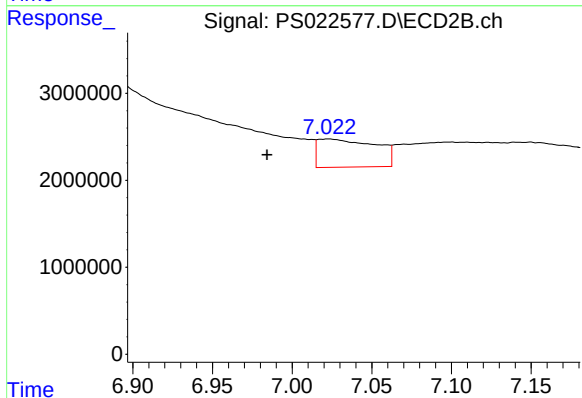


#6 MCPP

R.T.: 7.023 min
Delta R.T.: 0.039 min
Response: 8133707
Conc: 1.04 ug/ml

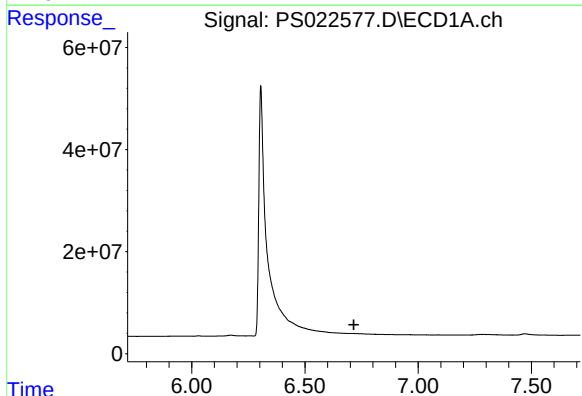

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.716 min
Response: 0
Conc: N.D.

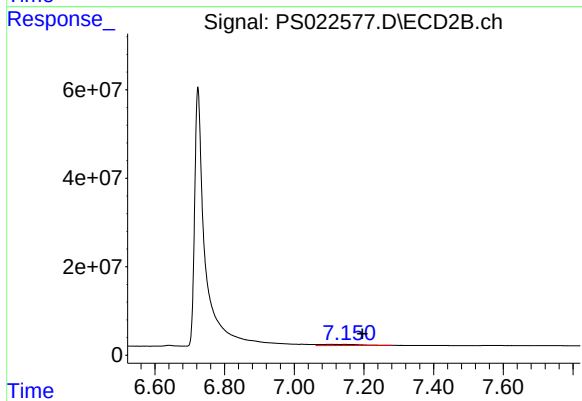

#7 MCPA

R.T.: 7.150 min
Delta R.T.: -0.046 min
Response: 21567623
Conc: 2.05 ug/ml