

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040423\
 Data File : PS022591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2023 19:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 04 22:04:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.306	6.724	1218.2E6	1208.0E6	498.347	586.475
Target Compounds							
1) T	Dalapon	2.435	0.000	1450003	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.734f	0.000	237852	0	<MDL	N.D. #
3) T	4-Nitroph...	6.170	6.360	7443637	1051966	5.433	<MDL #
6) T	MCP	0.000	7.022	0	1377382	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.548f	0	2273275	N.D.	<MDL
10) T	Pentachlo...	7.469	8.219	10163424	8343739	<MDL	<MDL #
11) T	2,4,5-TP ...	7.950	8.602	761911	5727637	<MDL	<MDL #
13) T	2,4-DB	8.661f	9.415	2479336	5985410	<MDL	3.564 #
14) T	DINOSEB	9.790	9.785	2278586	2484989	<MDL	<MDL #
15) T	Picloram	9.655f	10.702	821689	10923161	<MDL	<MDL #
16) T	DCPA	10.050	10.702	5445077	10923161	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040423\
Data File : PS022591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2023 19:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 04 22:04:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

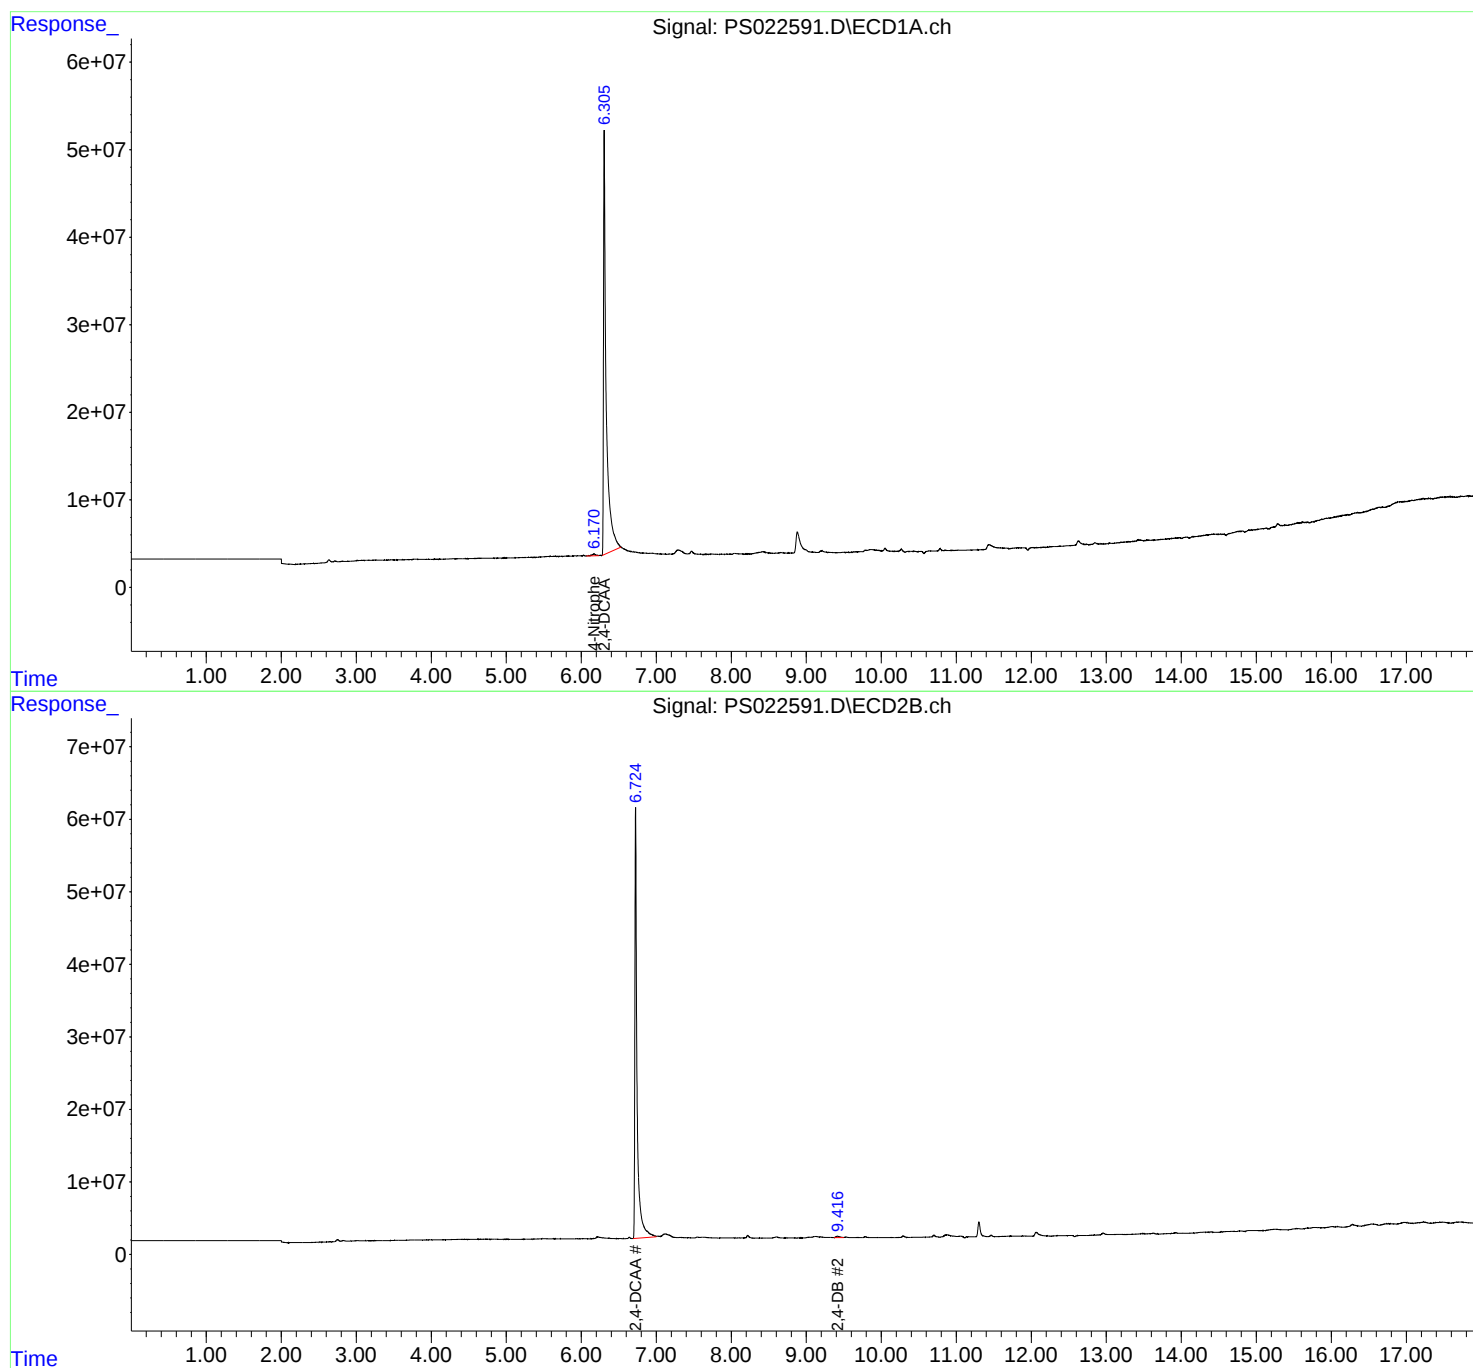


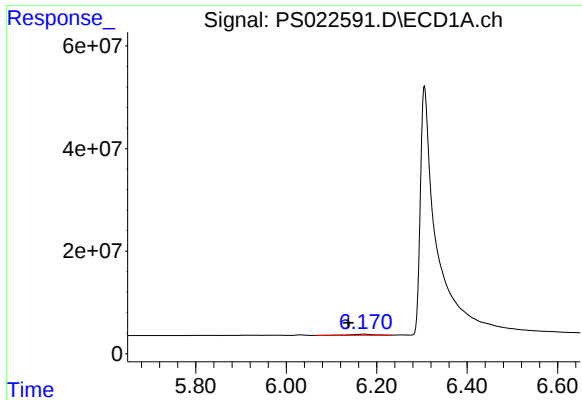

#3 4-Nitrophenol


R.T.: 6.170 min
Delta R.T.: 0.033 min
Response: 7443637
Conc: 5.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

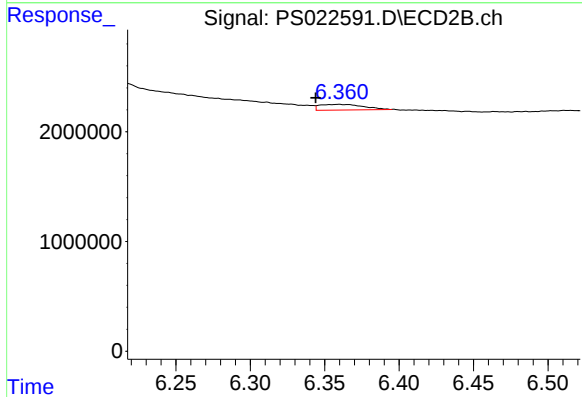


#3 4-Nitrophenol

R.T.: 6.360 min
Delta R.T.: 0.016 min
Response: 1051966
Conc: N.D.

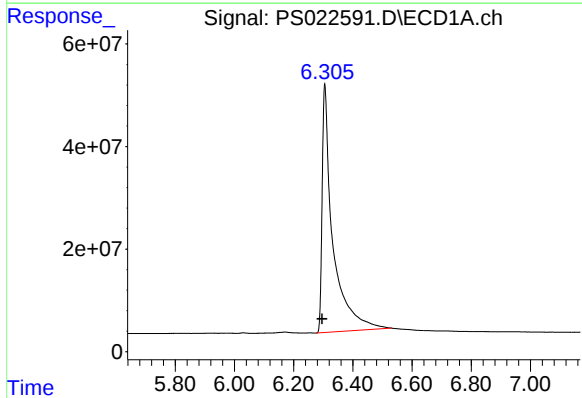


#4 2,4-DCAA

R.T.: 6.306 min
Delta R.T.: 0.010 min
Response: 1218151424
Conc: 498.35 ng/ml

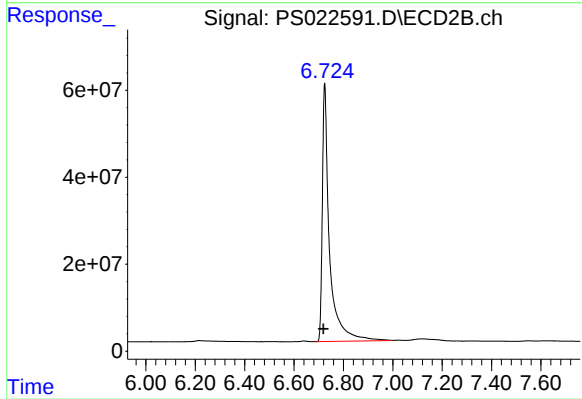

#4 2,4-DCAA


R.T.: 6.724 min
Delta R.T.: 0.005 min
Response: 1207954416
Conc: 586.47 ng/ml

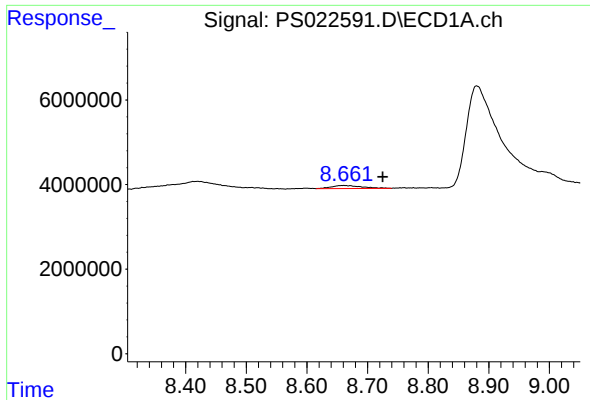

#13 2,4-DB

R.T.: 8.661 min
Delta R.T.: -0.065 min
Response: 2479336
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

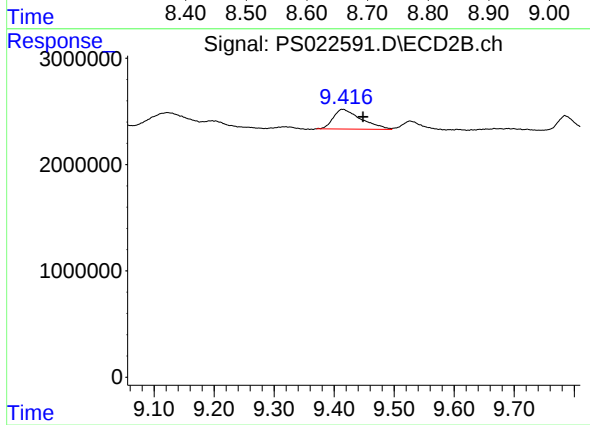

#13 2,4-DB

R.T.: 9.415 min
Delta R.T.: -0.034 min
Response: 5985410
Conc: 3.56 ng/ml