

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040521\
 Data File : PS014465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 09:38
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 13:40:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.430	0.000	9358160	0	4.847	N.D. #
3) T	4-Nitroph...	6.953f	0.000	1285963	0	1.722	N.D. #
5) T	DICAMBA	0.000	7.121f	0	4231841	N.D.	2.112
6) T	MCP	0.000	7.121	0	4231841	N.D.	2.541
7) T	MCPA	7.638	0.000	5329561	0	<MDL	N.D. #
12) T	2,4,5-T	9.419	0.000	6665855	0	<MDL	N.D. #
15) T	Picloram	10.949	10.983	39412913	29991200	3.774	7.906 #
16) T	DCPA	11.365	10.901	4050574	1909718	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040521\
Data File : PS014465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 09:38
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 13:40:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

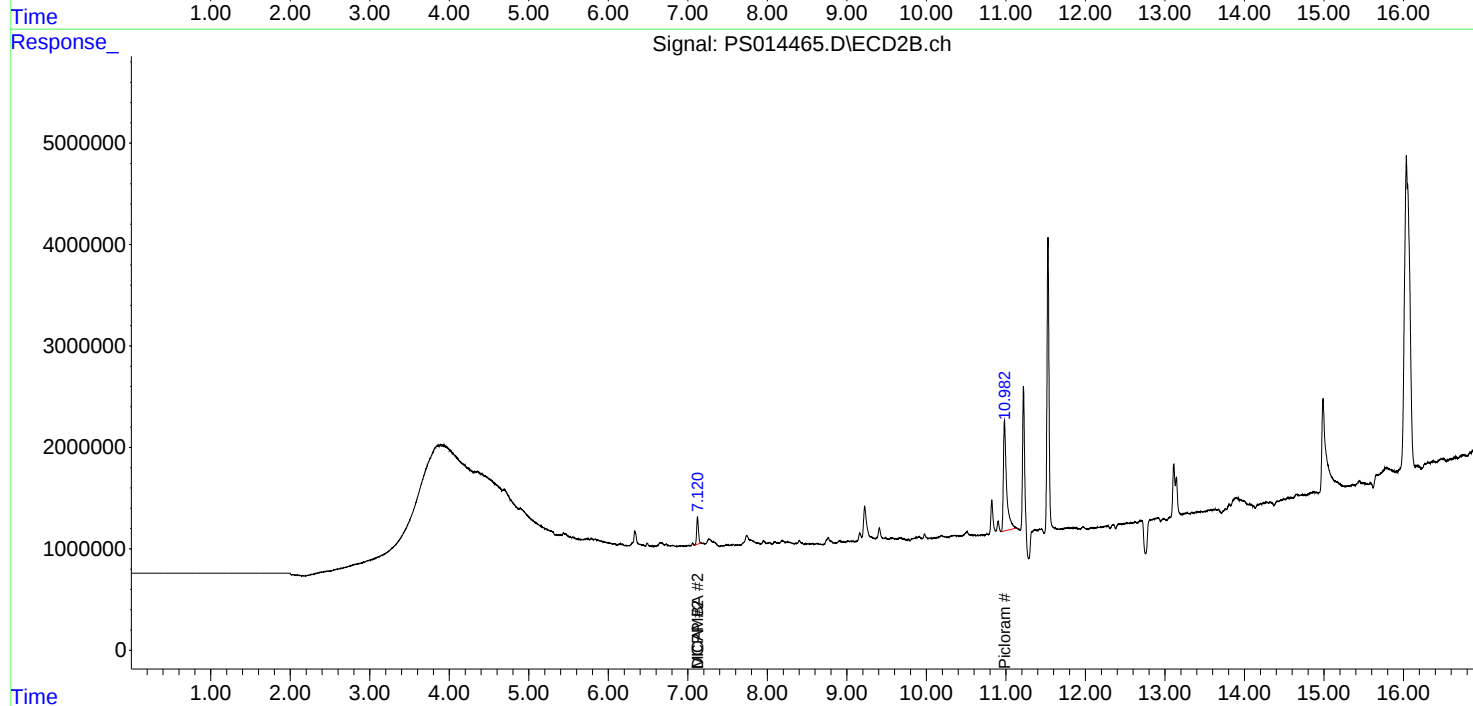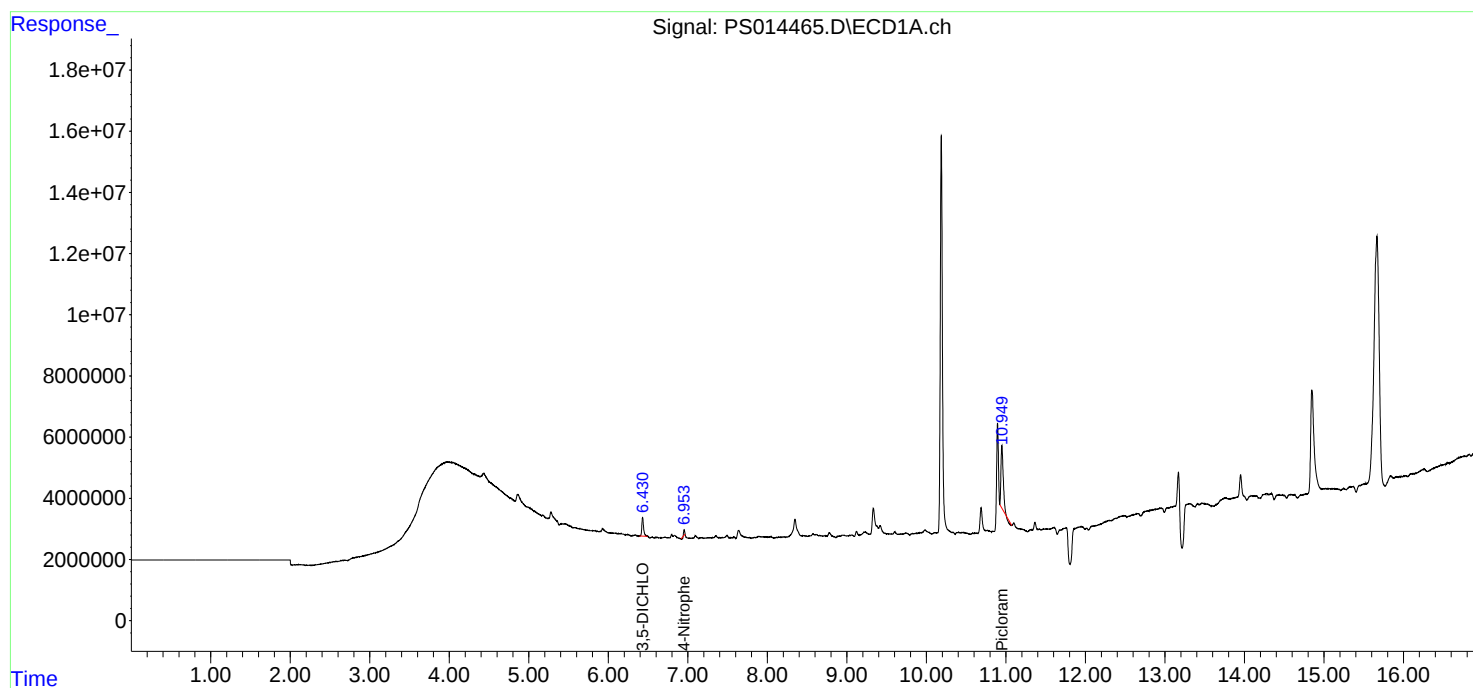


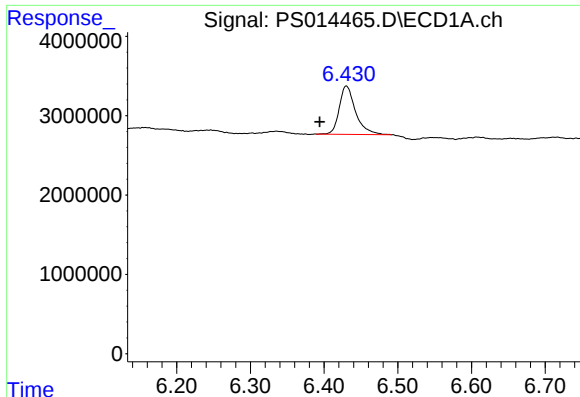

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.430 min
Delta R.T.: 0.036 min
Response: 9358160
Conc: 4.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

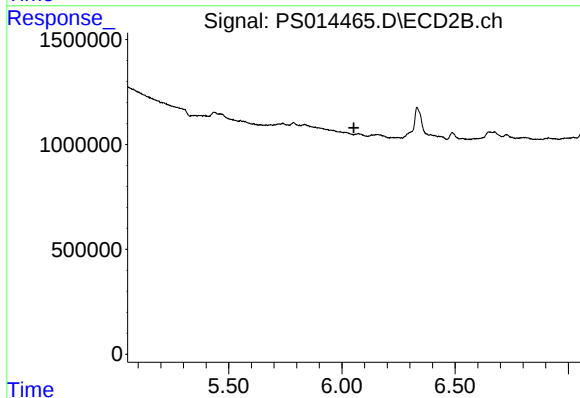


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

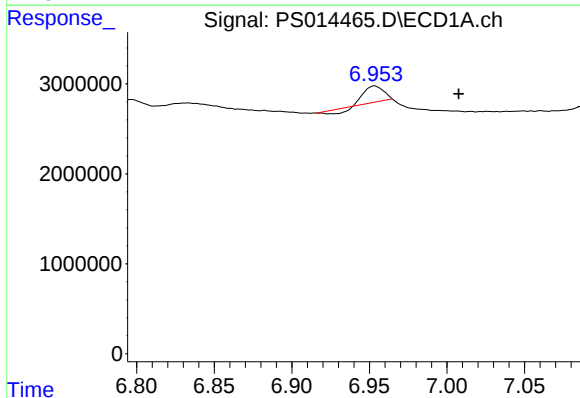


#3 4-Nitrophenol

R.T.: 6.953 min
Delta R.T.: -0.054 min
Response: 1285963
Conc: 1.72 ng/ml

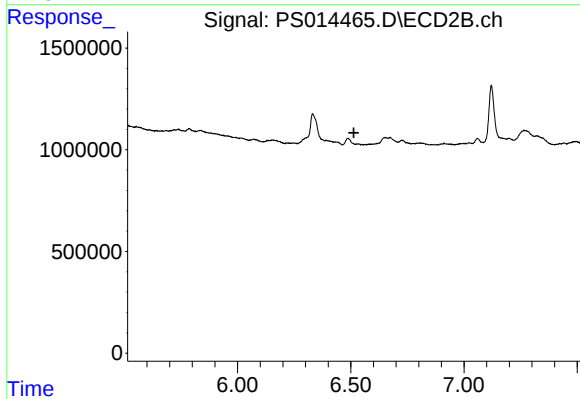

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.513 min
Response: 0
Conc: N.D.

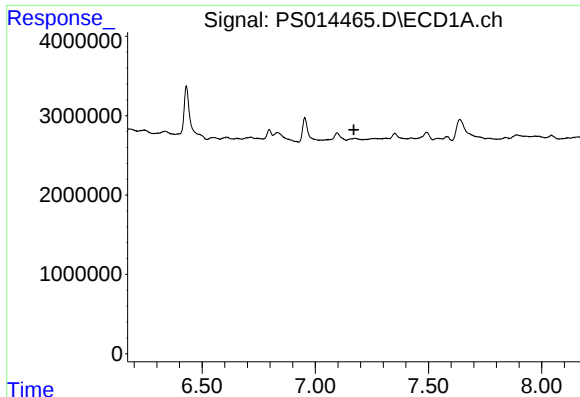

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

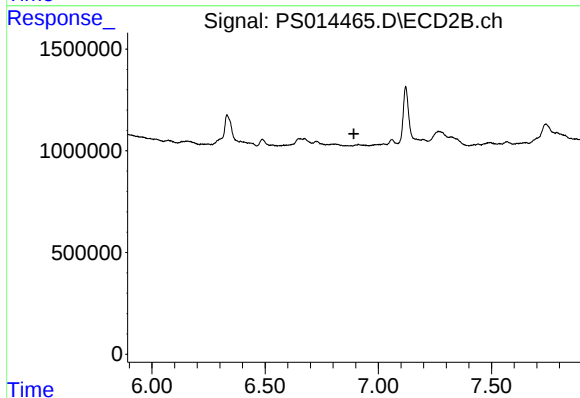


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.892 min
Response: 0
Conc: N.D.

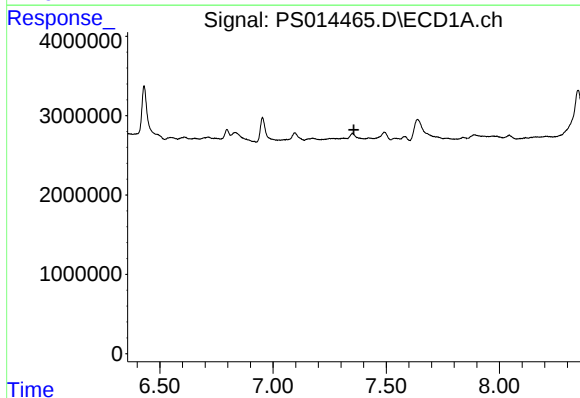


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

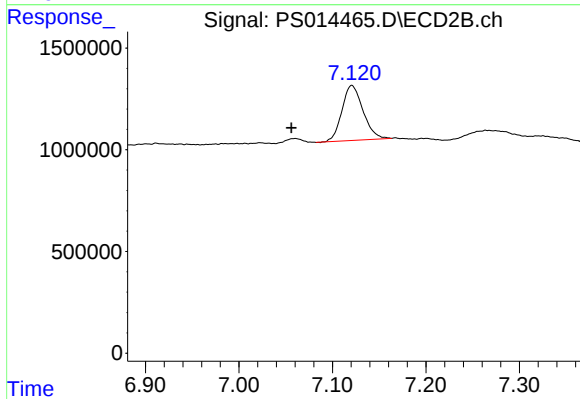

#5 DICAMBA


R.T.: 7.121 min
Delta R.T.: 0.065 min
Response: 4231841
Conc: 2.11 ng/ml

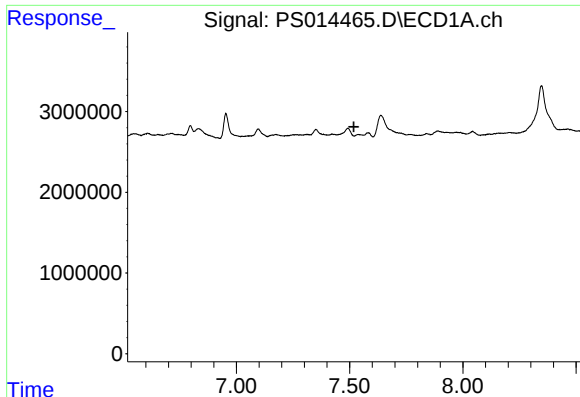

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

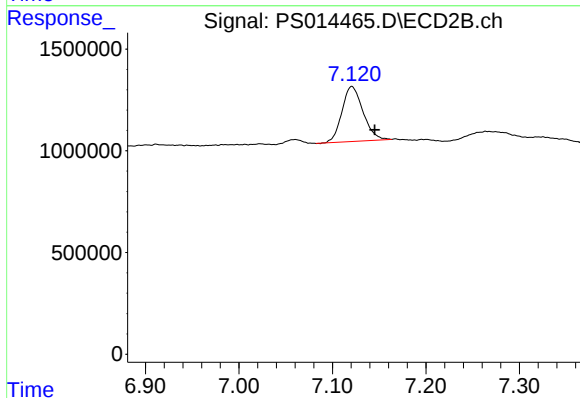


#6 MCP

R.T.: 7.121 min
Delta R.T.: -0.025 min
Response: 4231841
Conc: 2.54 ug/ml

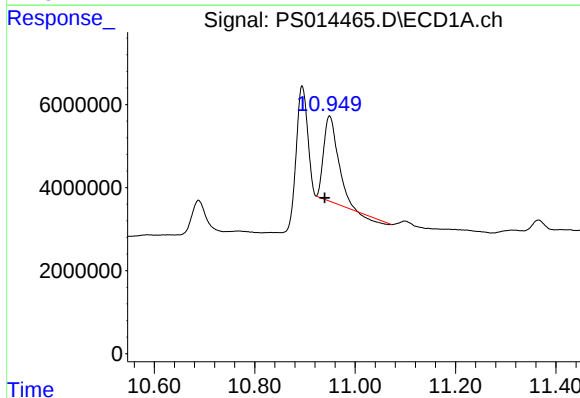

#15 Picloram

R.T.: 10.949 min
Delta R.T.: 0.010 min
Response: 39412913
Conc: 3.77 ng/ml

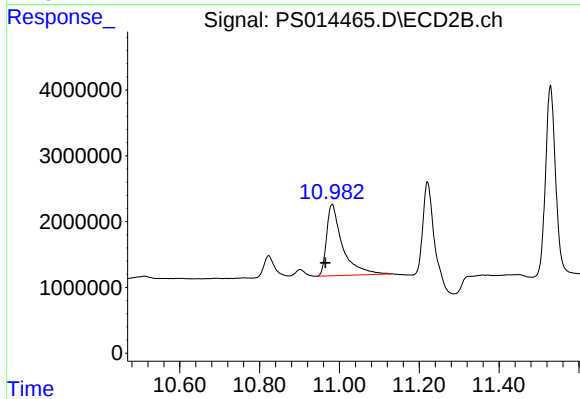

#15 Picloram

R.T.: 10.983 min
Delta R.T.: 0.018 min
Response: 29991200
Conc: 7.91 ng/ml