

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040522\
 Data File : PS018886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2022 09:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 01:10:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.808	1534.6E6	335.4E6	525.659	469.748
Target Compounds							
10) T	Pentachlo...	8.658	0.000	3630664	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.655	0	1660126	N.D.	<MDL
12) T	2,4,5-T	9.469	0.000	17481909	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.501f	0	15885768	N.D.	27.891
14) T	DINOSEB	11.200	0.000	31327401	0	1.919	N.D. #
15) T	Picloram	0.000	10.934f	0	34236683	N.D.	6.055
16) T	DCPA	11.474	0.000	4627758	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040522\
Data File : PS018886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2022 09:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 01:10:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

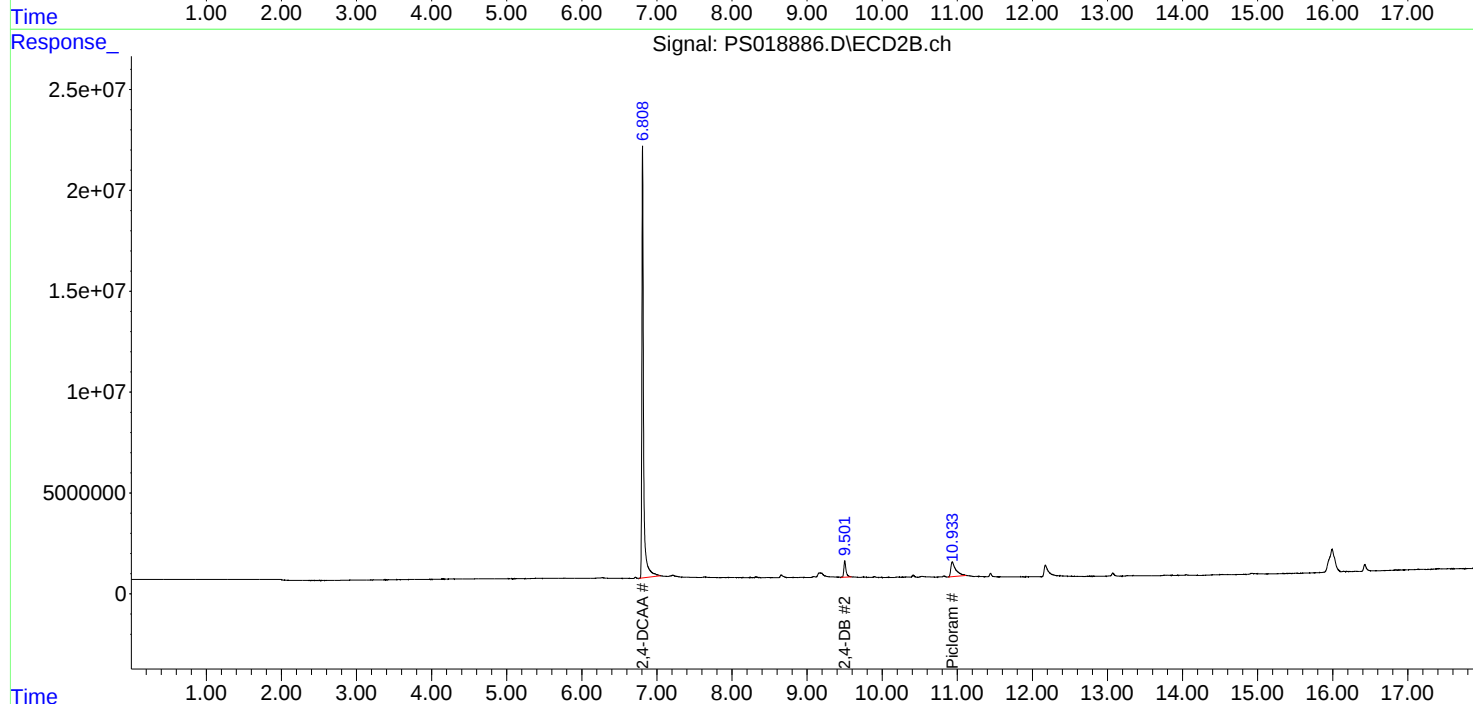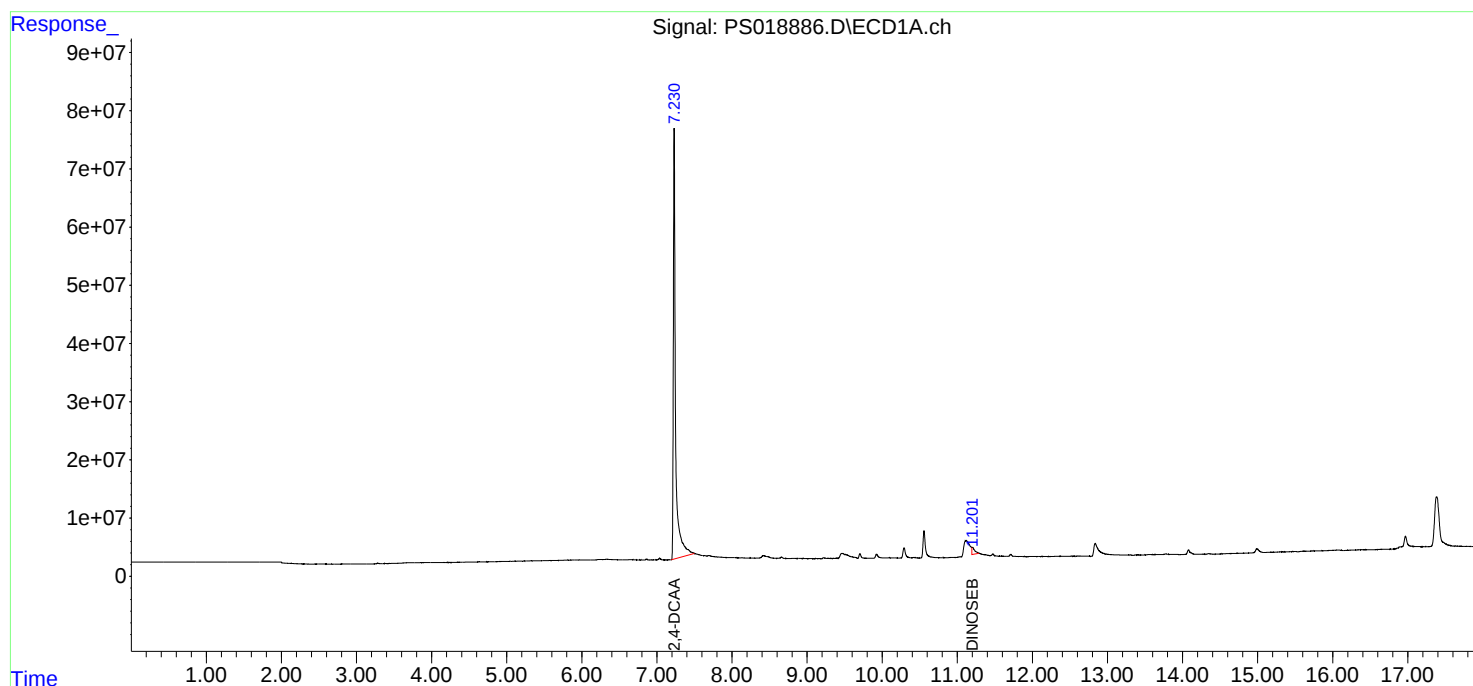


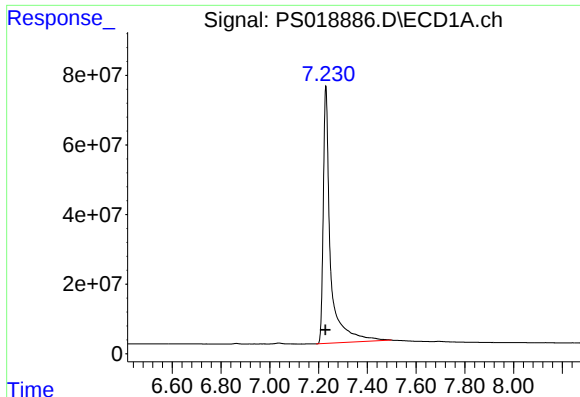

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: 0.003 min
Response: 1534639229
Conc: 525.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

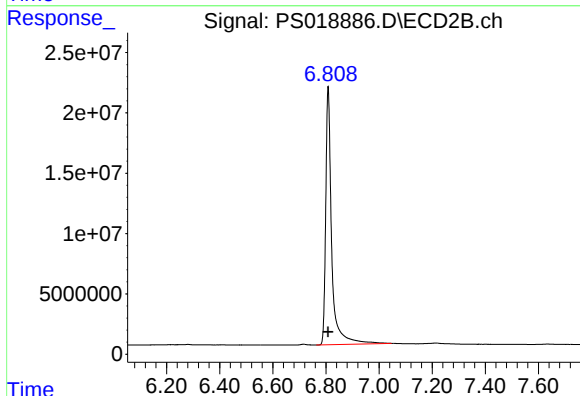


#4 2,4-DCAA

R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 335372816
Conc: 469.75 ng/ml

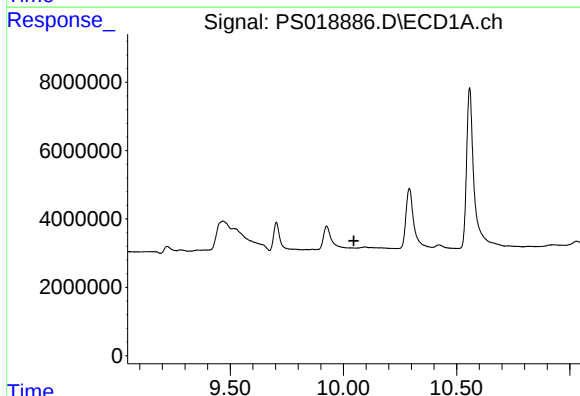


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.046 min
Response: 0
Conc: N.D.

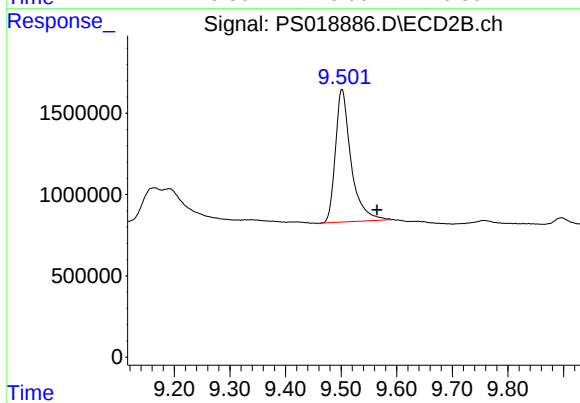

#13 2,4-DB


R.T.: 9.501 min
Delta R.T.: -0.063 min
Response: 15885768
Conc: 27.89 ng/ml

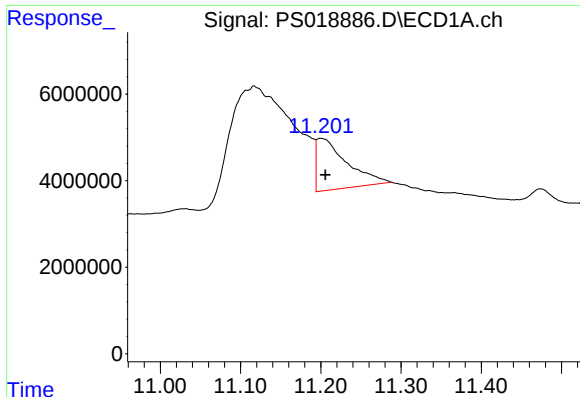

#14 DINOSEB


R.T.: 11.200 min
Delta R.T.: -0.006 min
Response: 31327401
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

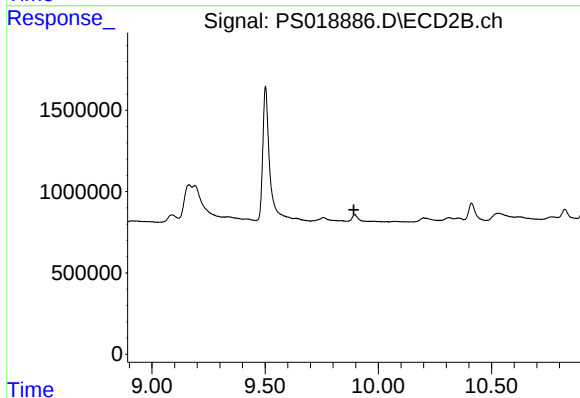


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.892 min
Response: 0
Conc: N.D.

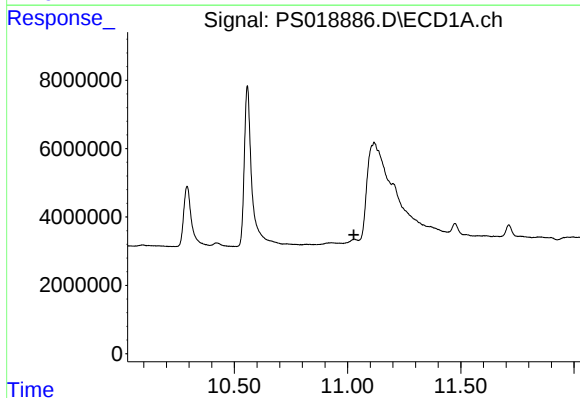

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.028 min
Response: 0
Conc: N.D.

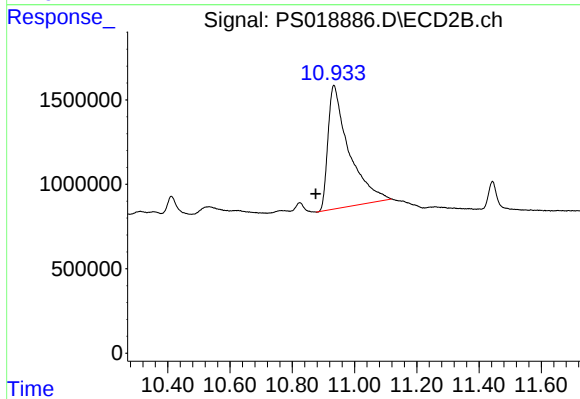

#15 Picloram

R.T.: 10.934 min
Delta R.T.: 0.059 min
Response: 34236683
Conc: 6.06 ng/ml