

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
 Data File : PS004004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2019 08:46
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:06:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.807	0	85444	N.D.	<MDL
Target Compounds							
2) T	3,5-DICHL...	0.000	8.945	0	407727	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.922	0	100910	N.D.	<MDL
5) T	DICAMBA	0.000	11.068	0	48005	N.D.	<MDL
6) T	MCP	0.000	11.269	0	405120	N.D.	<MDL
7) T	MCPA	0.000	11.595	0	2967699	N.D.	1.664
8) T	DICHLORPROP	0.000	12.212	0	113388	N.D.	<MDL
9) T	2,4-D	0.000	12.639	0	154507	N.D.	<MDL
10) T	Pentachlo...	0.000	13.153	0	1862154	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.827	0	1066177	N.D.	<MDL
12) T	2,4,5-T	0.000	14.410	0	53151	N.D.	<MDL
13) T	2,4-DB	0.000	14.983	0	3016297	N.D.	10.158
14) T	DINOSEB	0.000	15.402	0	2453201	N.D.	1.279
15) T	Picloram	0.000	16.670	0	22869547	N.D.	7.212
16) T	DCPA	0.000	16.626	0	5878597	N.D.	1.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
Data File : PS004004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2019 08:46
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:06:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

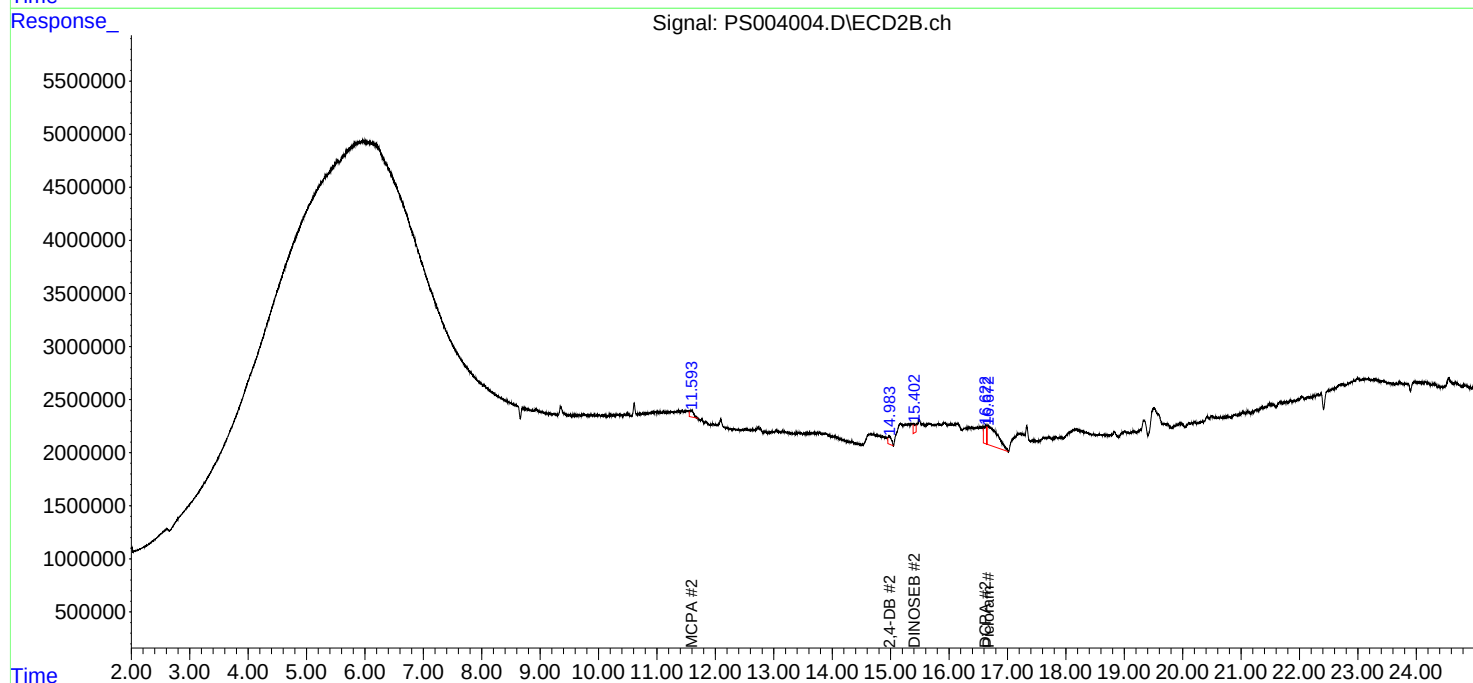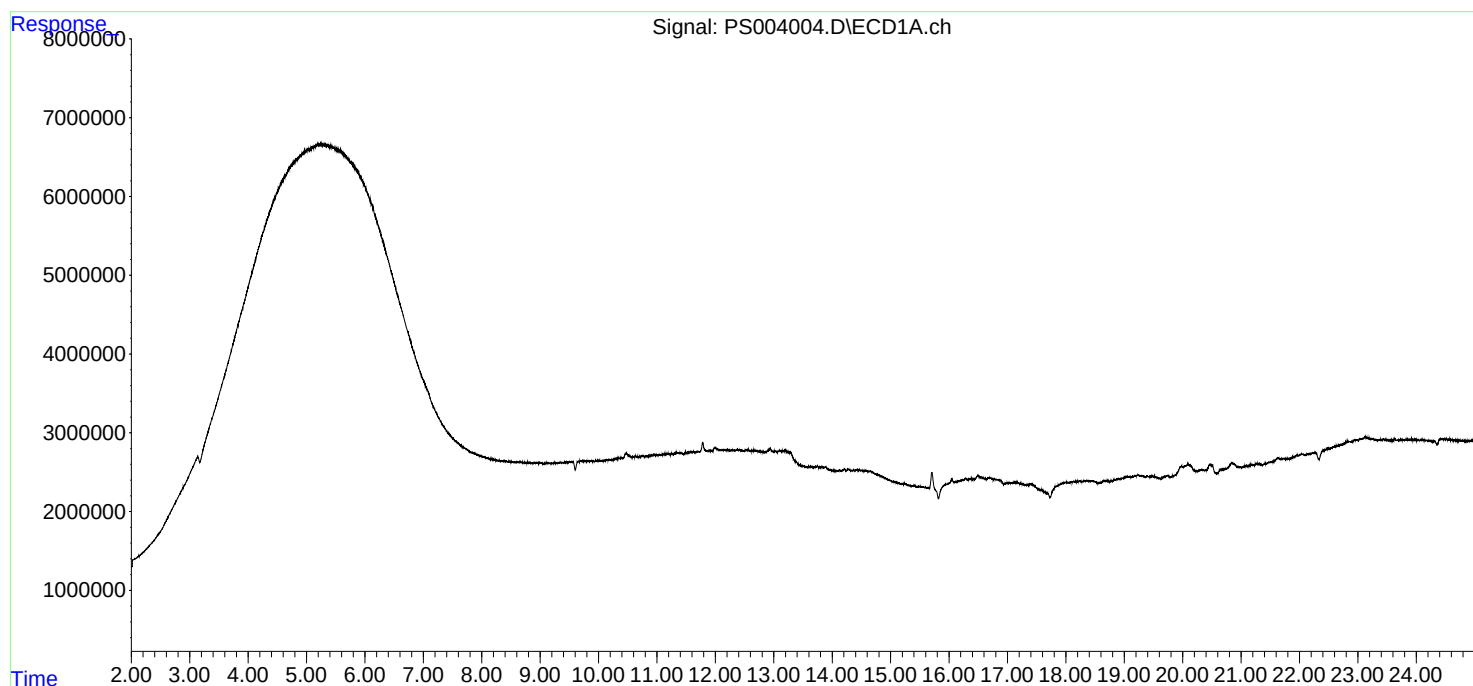


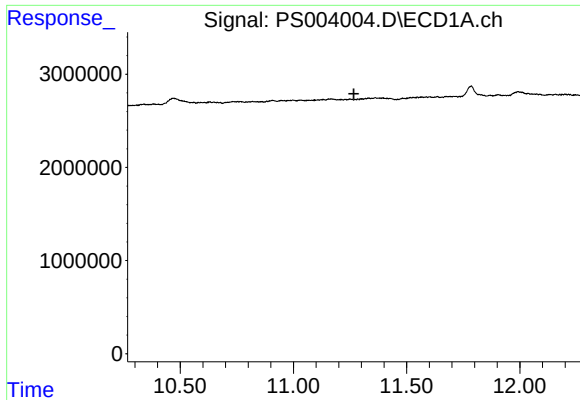

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.267 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

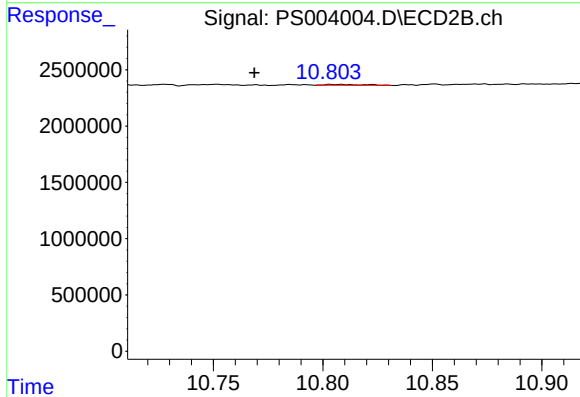


#4 2,4-DCAA

R.T.: 10.807 min
Delta R.T.: 0.038 min
Response: 85444
Conc: N.D.

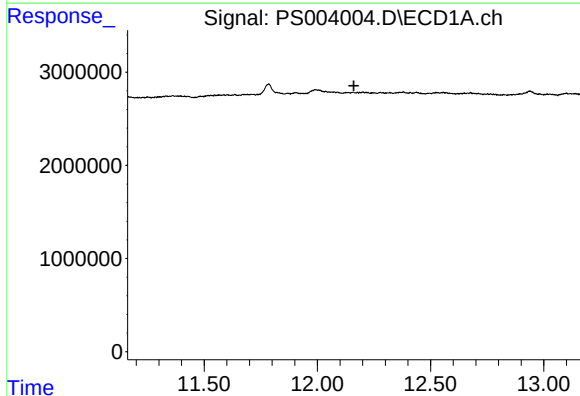


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

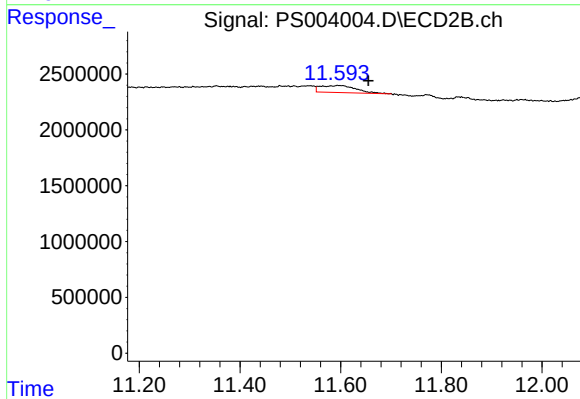

#7 MCPA


R.T.: 11.595 min
Delta R.T.: -0.060 min
Response: 2967699
Conc: 1.66 ug/ml

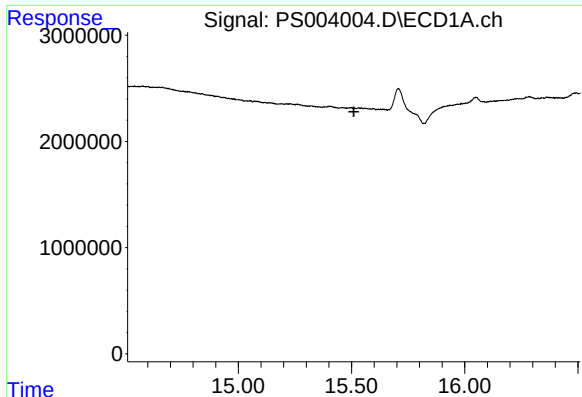

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

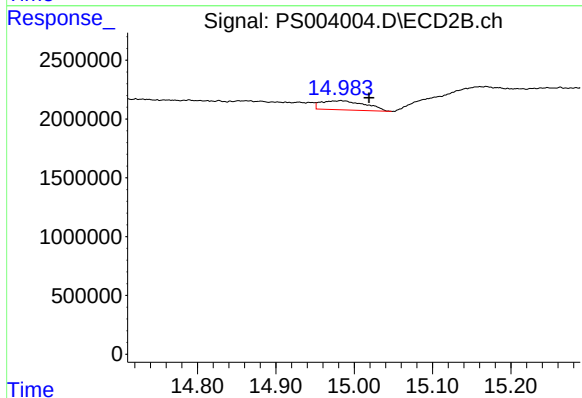


#13 2,4-DB

R.T.: 14.983 min
Delta R.T.: -0.035 min
Response: 3016297
Conc: 10.16 ng/ml

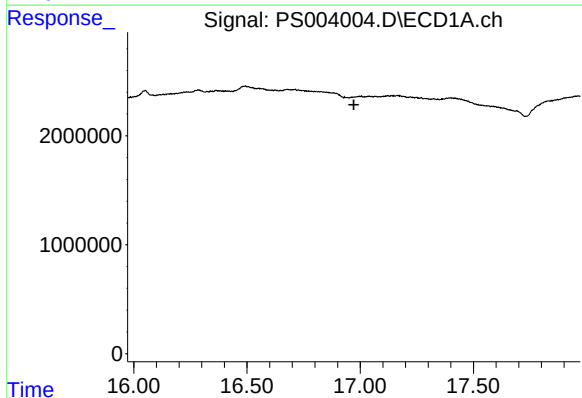


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

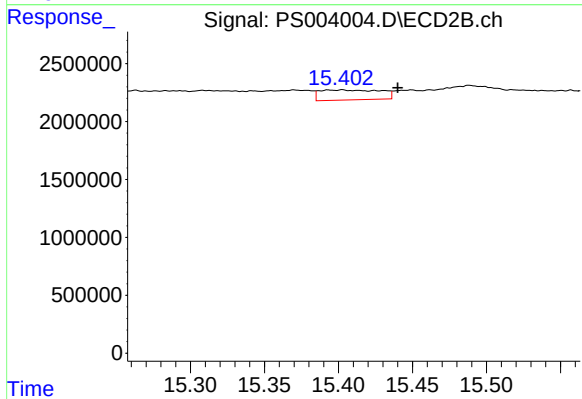

#14 DINOSEB


R.T.: 15.402 min
Delta R.T.: -0.038 min
Response: 2453201
Conc: 1.28 ng/ml

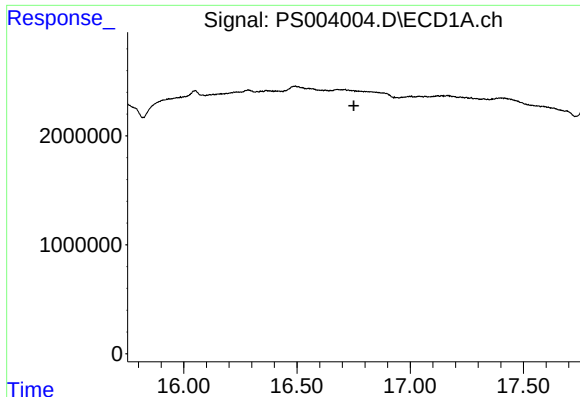

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

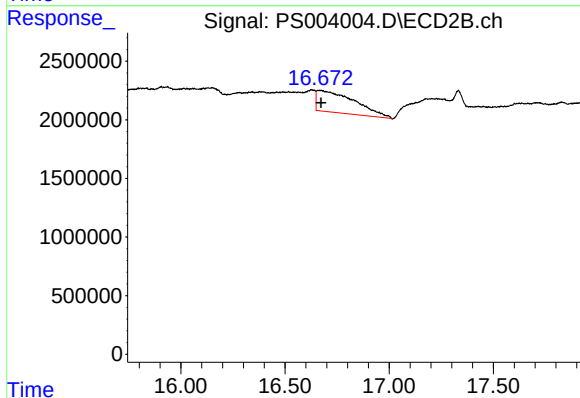


#15 Picloram

R.T.: 16.670 min
Delta R.T.: -0.003 min
Response: 22869547
Conc: 7.21 ng/ml

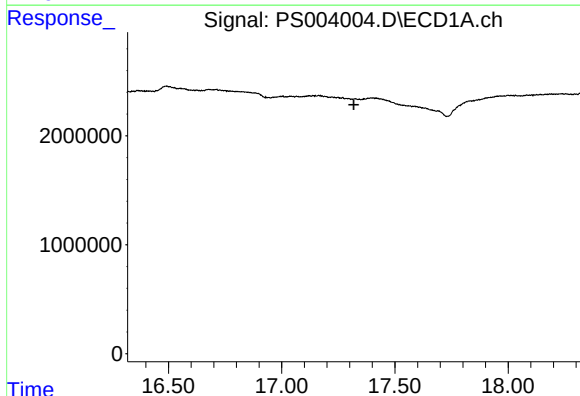

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

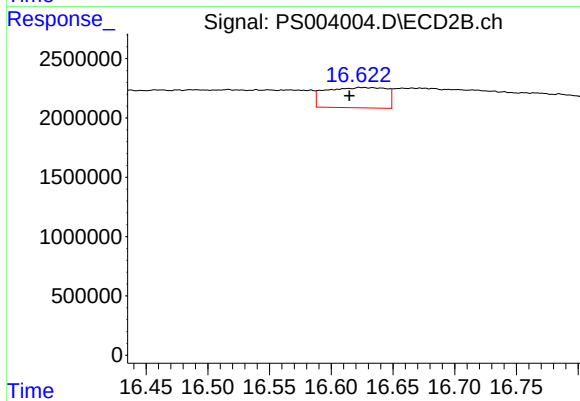

#16 DCPA

R.T.: 16.626 min
Delta R.T.: 0.011 min
Response: 5878597
Conc: 1.74 ng/ml