

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
 Data File : PS004005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2019 09:18
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:06:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.798	158.2E6	153.3E6	362.681	312.505
Target Compounds							
2) T	3,5-DICHL...	0.000	8.955	0	80528	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.888	0	59899	N.D.	<MDL
6) T	MCP	0.000	11.250	0	7677	N.D.	<MDL
7) T	MCPA	0.000	11.683	0	395583	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.152	0	5187097	N.D.	11.142
9) T	2,4-D	0.000	12.677	0	90796	N.D.	<MDL
10) T	Pentachlo...	0.000	13.148	0	316173	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.761	0	140467	N.D.	<MDL
12) T	2,4,5-T	0.000	14.354	0	99808	N.D.	<MDL
13) T	2,4-DB	0.000	14.986	0	6964937	N.D.	23.455
14) T	DINOSEB	0.000	15.398	0	3772057	N.D.	1.966
15) T	Picloram	0.000	16.647	0	1229009	N.D.	<MDL
16) T	DCPA	0.000	16.647	0	1229009	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
Data File : PS004005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2019 09:18
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:06:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

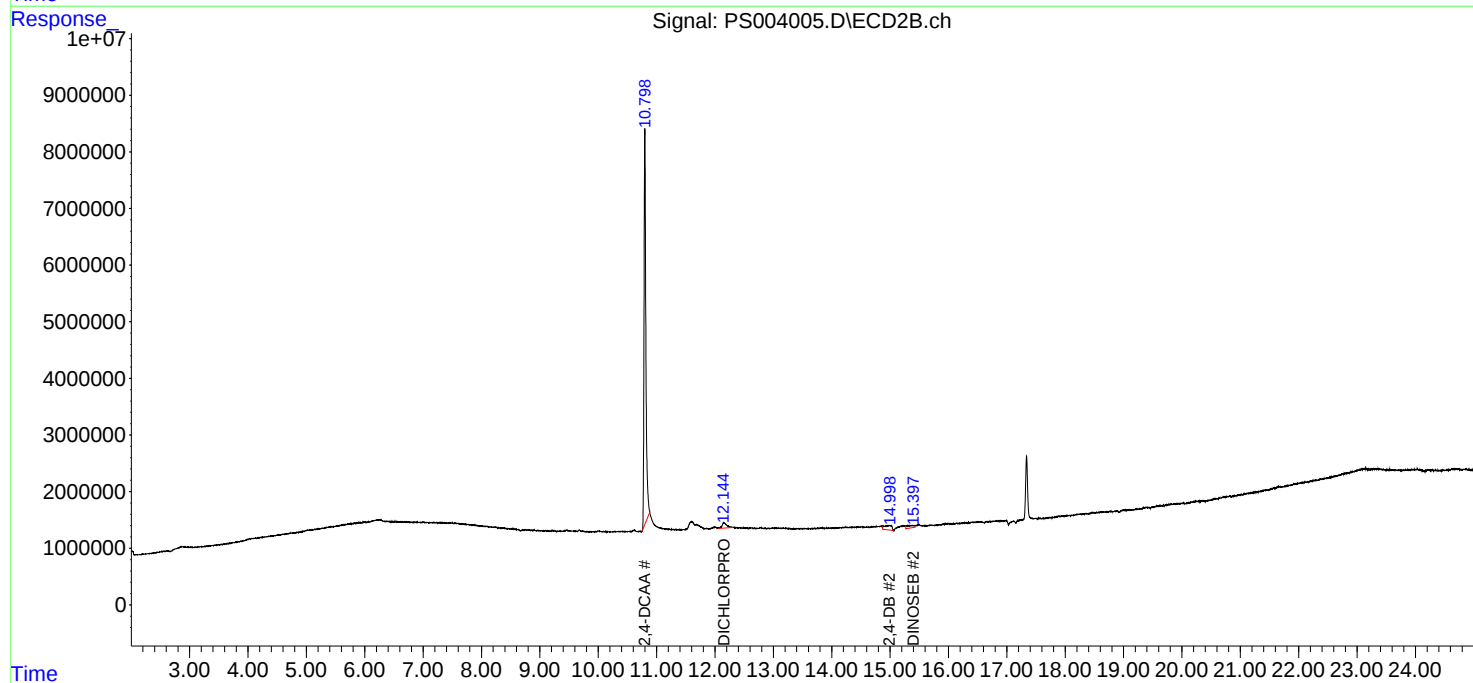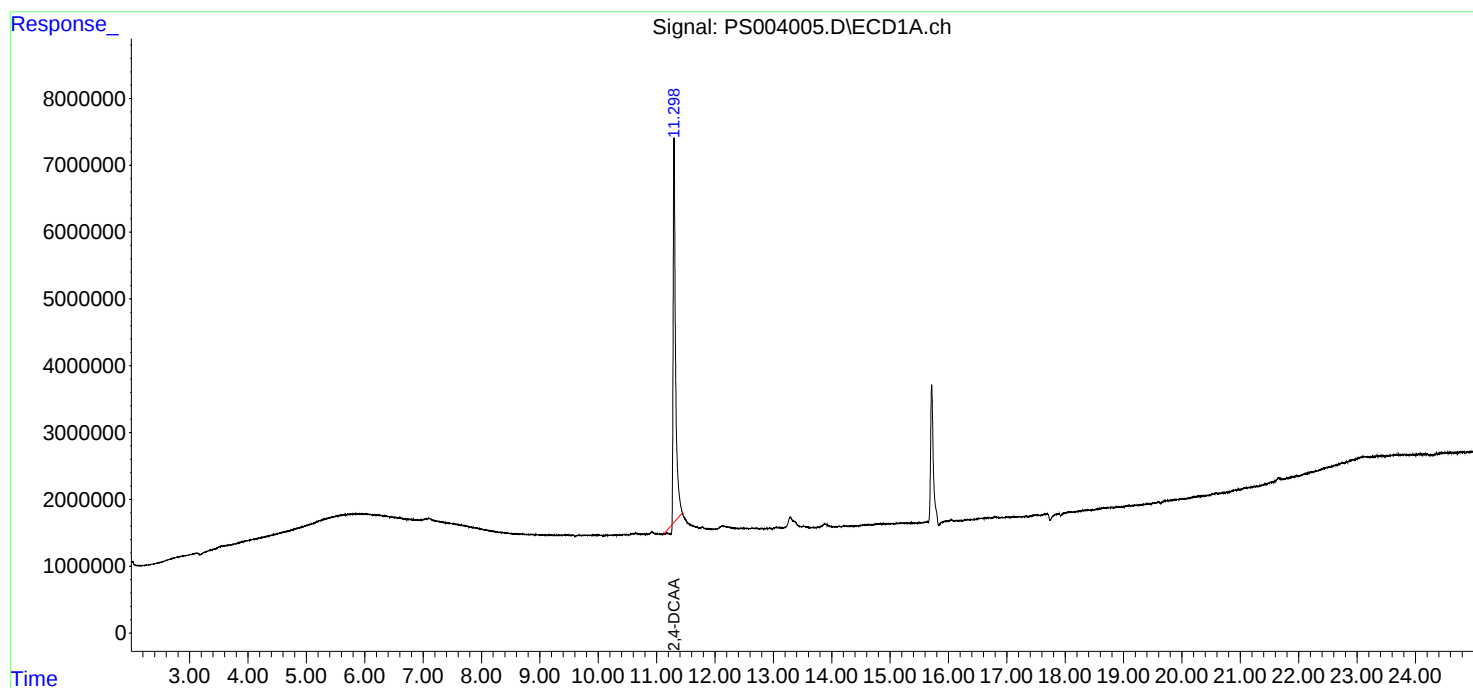


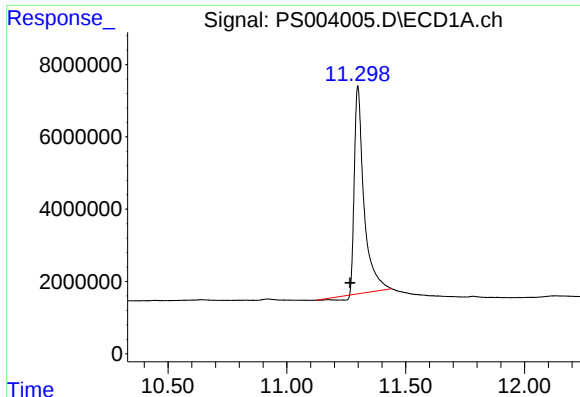

#4 2,4-DCAA


R.T.: 11.299 min
Delta R.T.: 0.032 min
Response: 158206151
Conc: 362.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

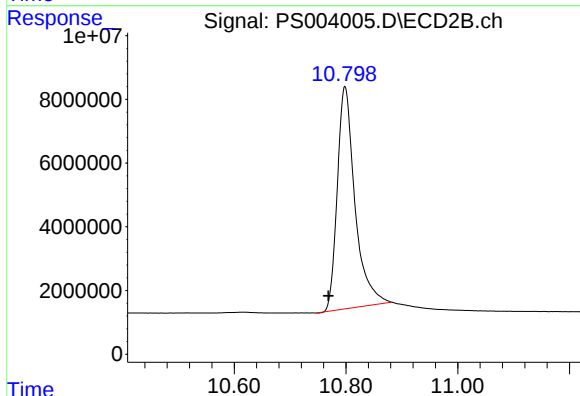


#4 2,4-DCAA

R.T.: 10.798 min
Delta R.T.: 0.030 min
Response: 153333284
Conc: 312.51 ng/ml

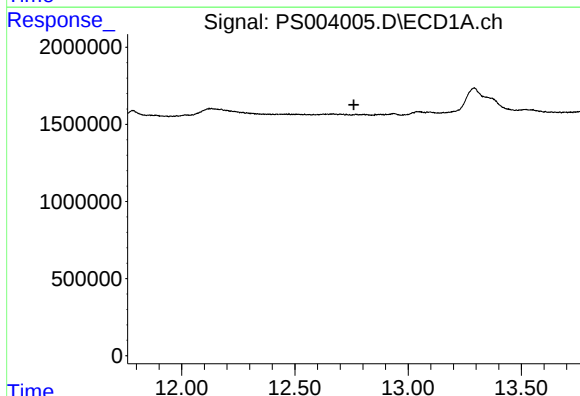


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

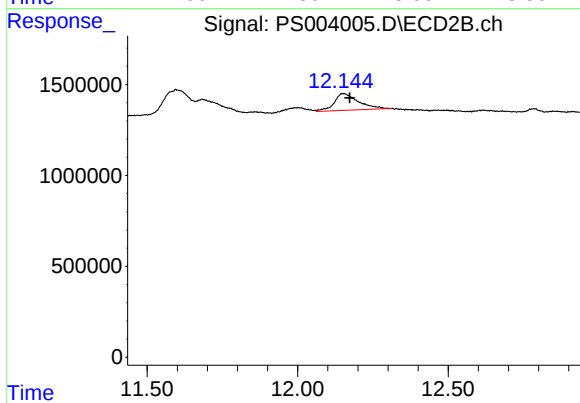

#8 DICHLORPROP


R.T.: 12.152 min
Delta R.T.: -0.021 min
Response: 5187097
Conc: 11.14 ng/ml

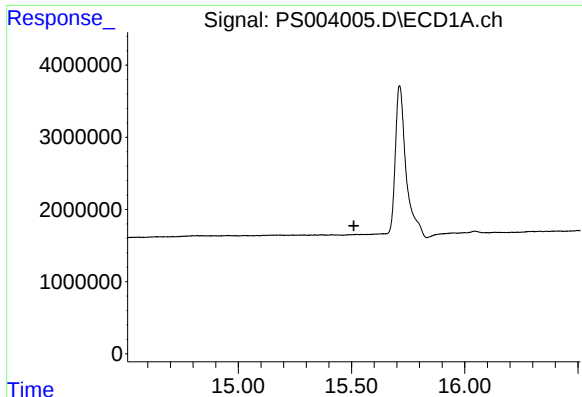

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

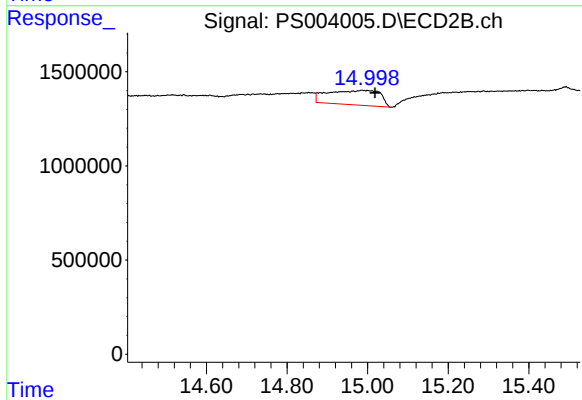


#13 2,4-DB

R.T.: 14.986 min
Delta R.T.: -0.032 min
Response: 6964937
Conc: 23.45 ng/ml

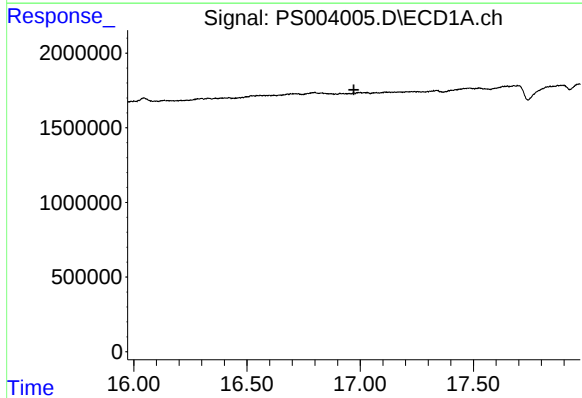

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

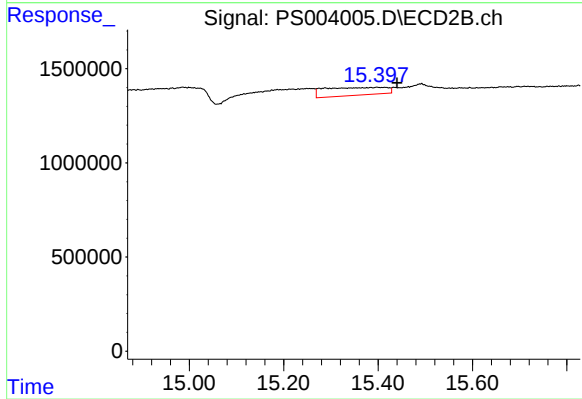

#14 DINOSEB

R.T.: 15.398 min
Delta R.T.: -0.042 min
Response: 3772057
Conc: 1.97 ng/ml