

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
 Data File : PS004012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2019 13:57
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:08:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.250	10.747	171.0E6	164.3E6	392.064	334.910
Target Compounds							
2) T	3,5-DICHL...	0.000	8.911	0	76795	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.905	0	60047	N.D.	<MDL
6) T	MCP	0.000	11.278	0	26958	N.D.	<MDL
7) T	MCPA	0.000	11.632	0	3774658	N.D.	2.117
9) T	2,4-D	0.000	12.650	0	102020	N.D.	<MDL
10) T	Pentachlo...	0.000	13.149	0	466217	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.808	0	124825	N.D.	<MDL
12) T	2,4,5-T	0.000	14.366	0	186602	N.D.	<MDL
14) T	DINOSEB	0.000	15.455	0	601992	N.D.	<MDL
15) T	Picloram	0.000	16.722	0	10972742	N.D.	3.460
16) T	DCPA	0.000	16.591	0	3080617	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
Data File : PS004012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2019 13:57
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:08:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

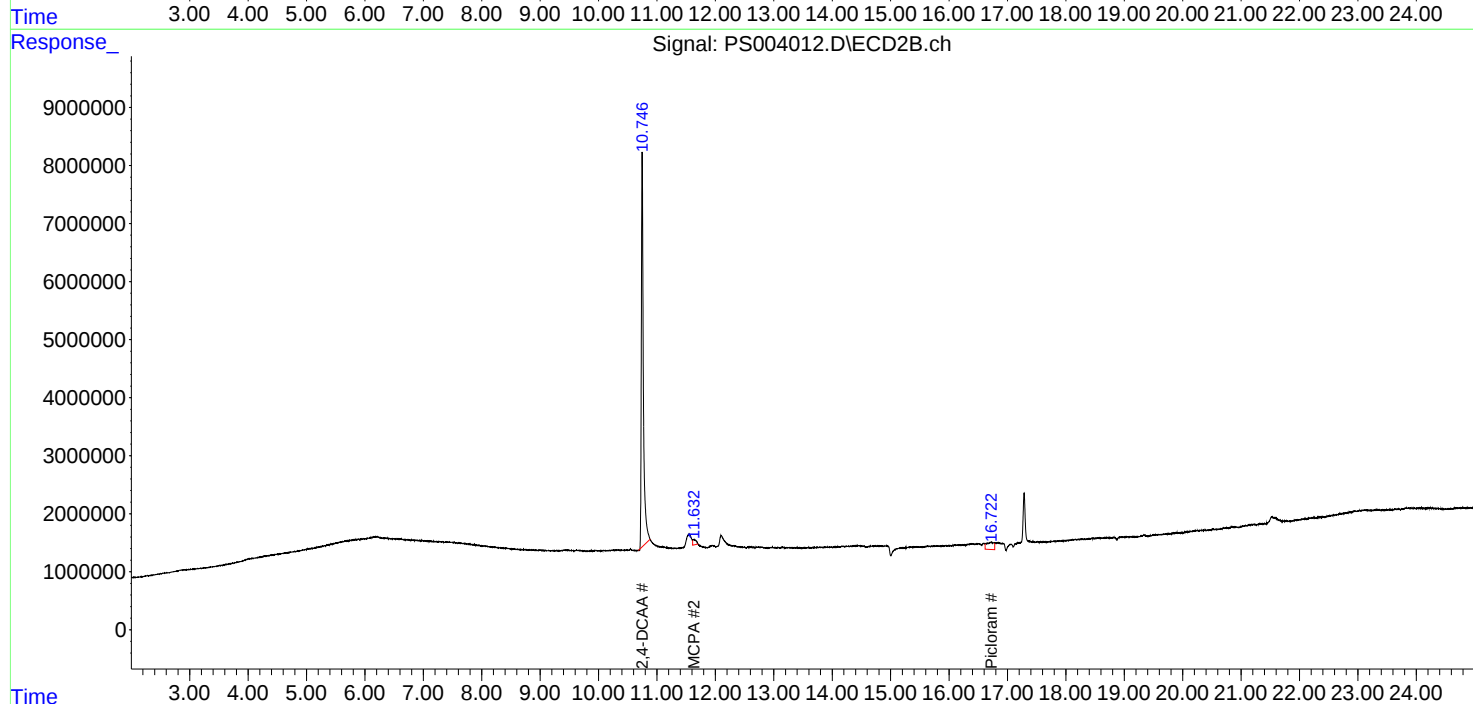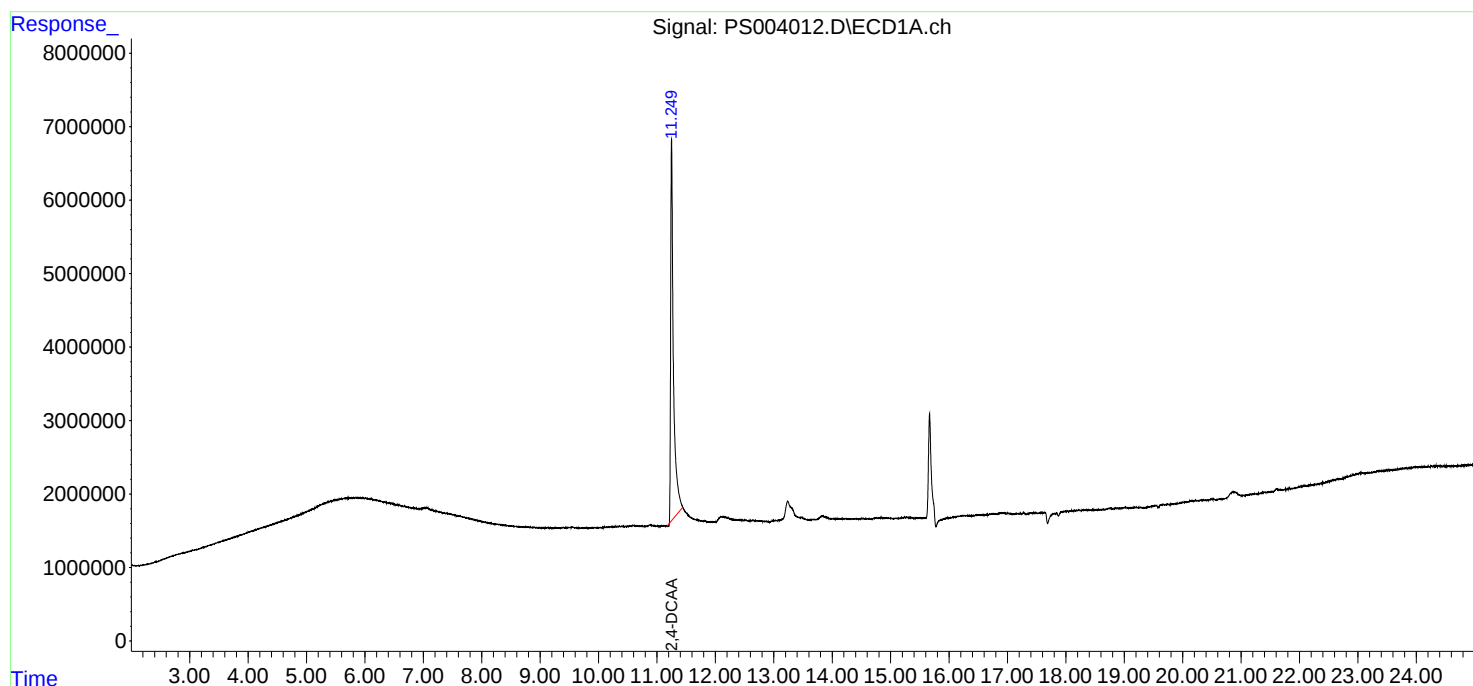


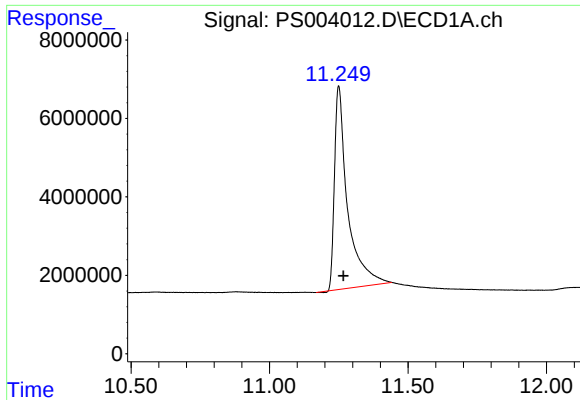

#4 2,4-DCAA


R.T.: 11.250 min
Delta R.T.: -0.017 min
Response: 171023356
Conc: 392.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

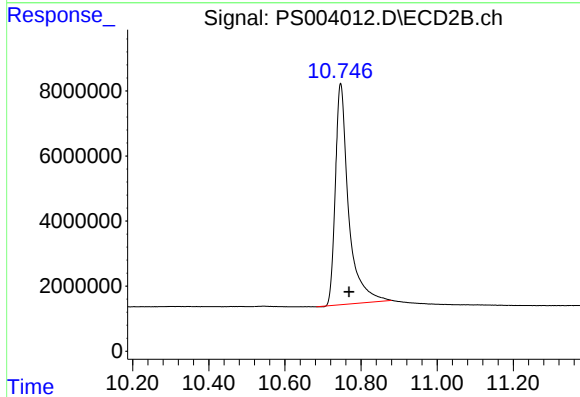


#4 2,4-DCAA

R.T.: 10.747 min
Delta R.T.: -0.022 min
Response: 164326311
Conc: 334.91 ng/ml

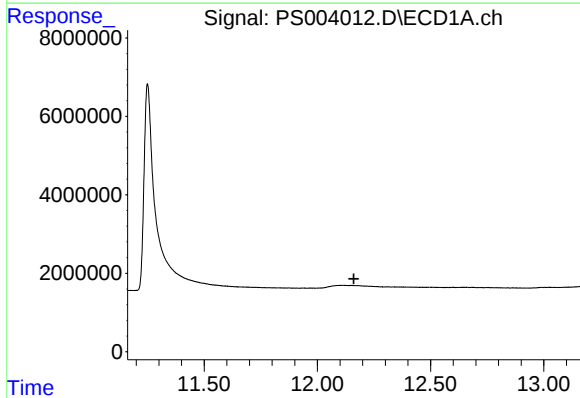


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

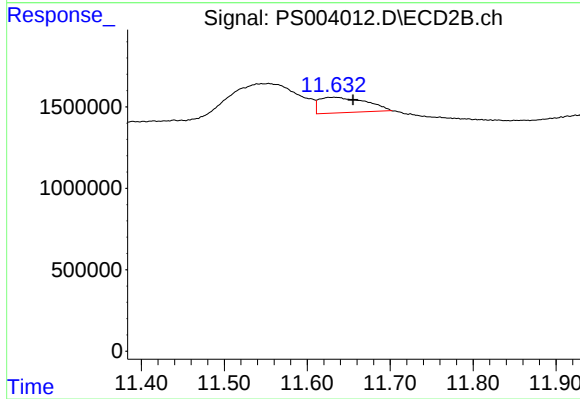

#7 MCPA


R.T.: 11.632 min
Delta R.T.: -0.023 min
Response: 3774658
Conc: 2.12 ug/ml

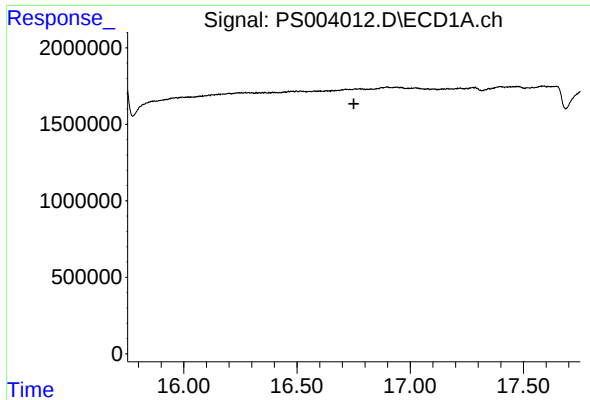

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

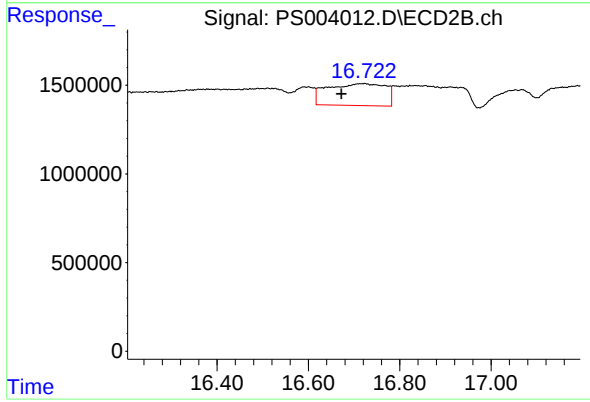

#15 Picloram

R.T.: 16.722 min
Delta R.T.: 0.050 min
Response: 10972742
Conc: 3.46 ng/ml