

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
 Data File : PS004018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2019 17:05
 Operator : EI\SJ
 Sample : K2203-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-03-040219-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:10:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.280	10.781	46029586	42380663	105.521	86.375
Target Compounds							
1) T	Dalapon	2.804	2.294	33445908	41470735	44.862	56.838 #
2) T	3,5-DICHL...	0.000	8.944	0	4508681	N.D.	7.068
3) T	4-Nitroph...	0.000	9.904	0	24538871	N.D.	108.084
5) T	DICAMBA	0.000	11.017	0	2442348	N.D.	1.313
7) T	MCPA	12.104	11.586	246.1E6	7659779	116.665	4.295 #
9) T	2,4-D	0.000	12.639	0	1001795	N.D.	1.883
10) T	Pentachlo...	0.000	13.168	0	703611	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.778	0	3502099	N.D.	1.322
12) T	2,4,5-T	0.000	14.354	0	843309	N.D.	<MDL
13) T	2,4-DB	0.000	14.962	0	11220107	N.D.	37.784
15) T	Picloram	16.735	16.696	7840527	28850403	2.308	9.098 #
16) T	DCPA	0.000	16.553	0	6683923	N.D.	1.977



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
Data File : PS004018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2019 17:05
Operator : EI\SJ
Sample : K2203-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:10:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

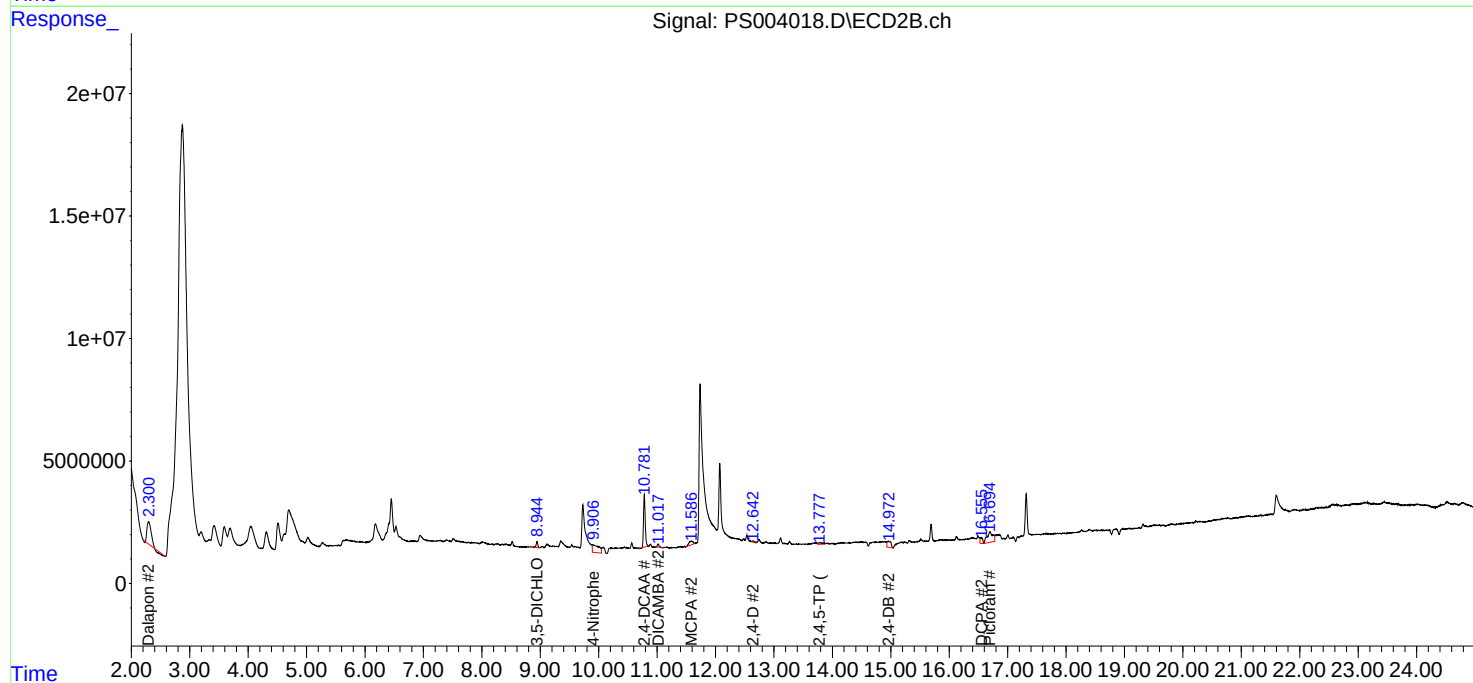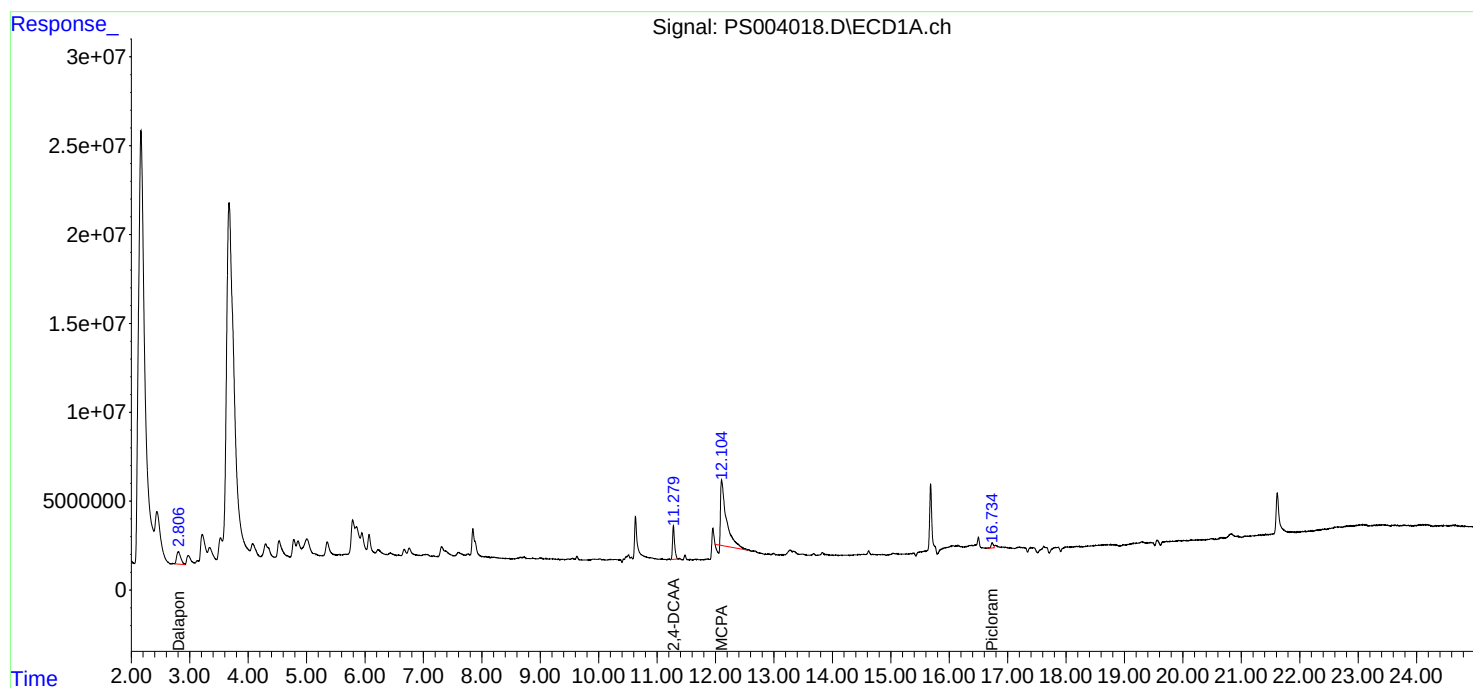


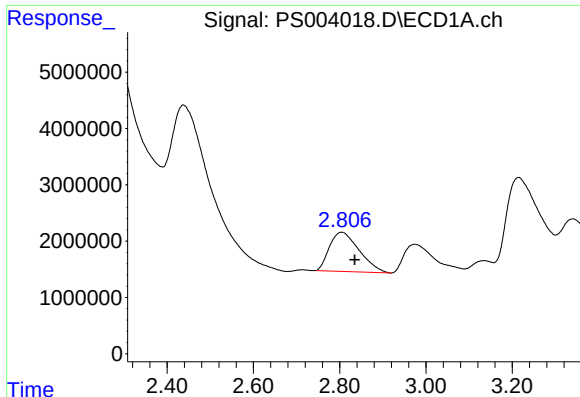

#1 Dalapon


R.T.: 2.804 min
Delta R.T.: -0.031 min
Response: 33445908
Conc: 44.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

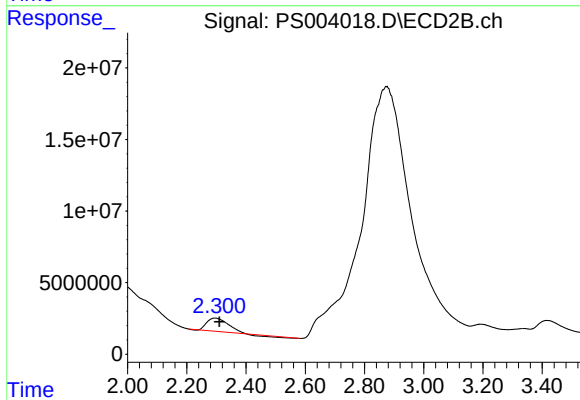


#1 Dalapon

R.T.: 2.294 min
Delta R.T.: -0.016 min
Response: 41470735
Conc: 56.84 ng/ml

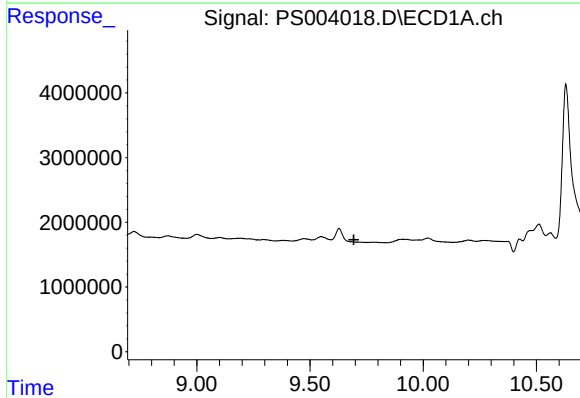


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

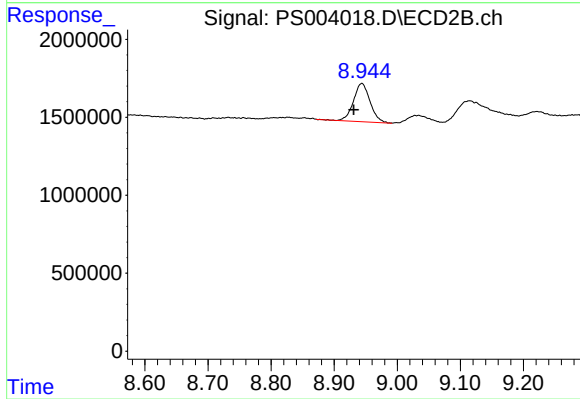

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: 0.013 min
Response: 4508681
Conc: 7.07 ng/ml

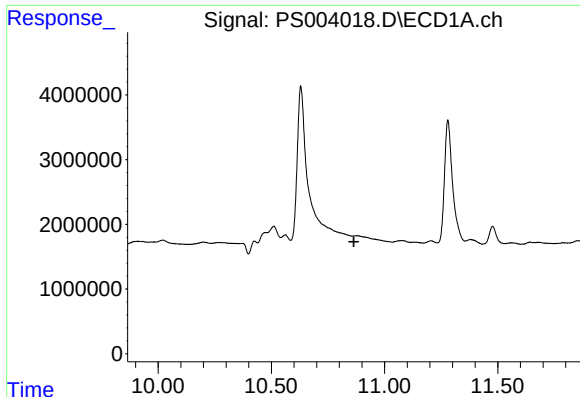

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

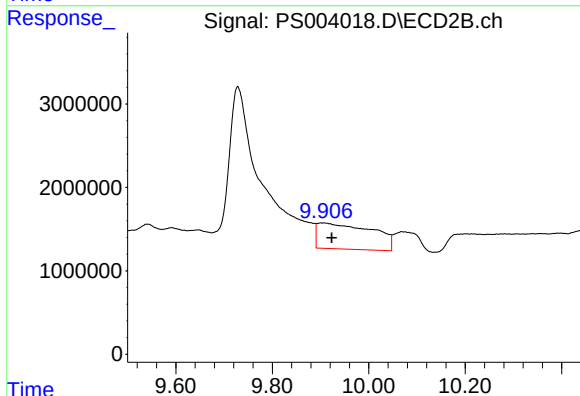


#3 4-Nitrophenol

R.T.: 9.904 min
Delta R.T.: -0.019 min
Response: 24538871
Conc: 108.08 ng/ml

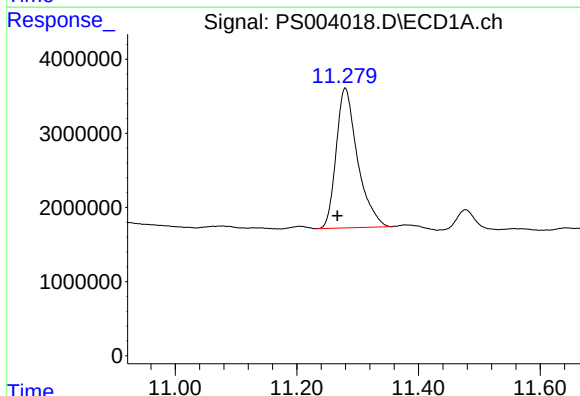


#4 2,4-DCAA

R.T.: 11.280 min
Delta R.T.: 0.013 min
Response: 46029586
Conc: 105.52 ng/ml

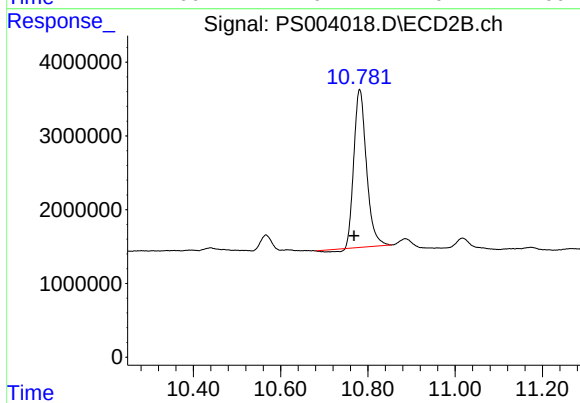

#4 2,4-DCAA


R.T.: 10.781 min
Delta R.T.: 0.013 min
Response: 42380663
Conc: 86.38 ng/ml

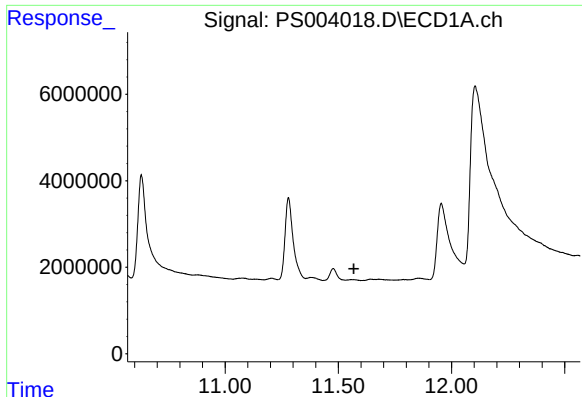

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

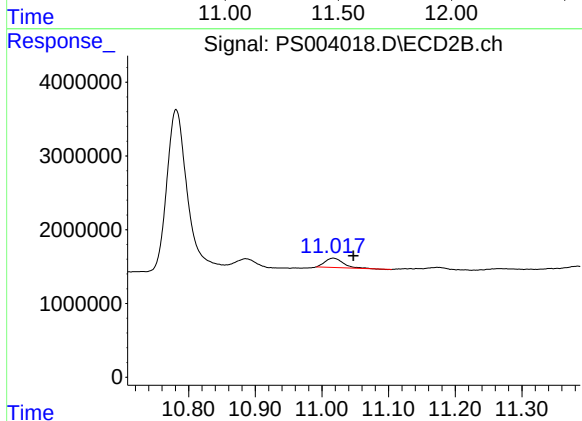


#5 DICAMBA

R.T.: 11.017 min
Delta R.T.: -0.030 min
Response: 2442348
Conc: 1.31 ng/ml

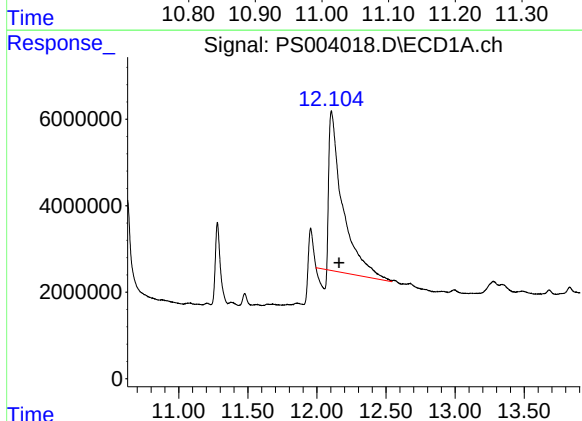


#7 MCPA

R.T.: 12.104 min
Delta R.T.: -0.057 min
Response: 246137597
Conc: 116.66 ug/ml

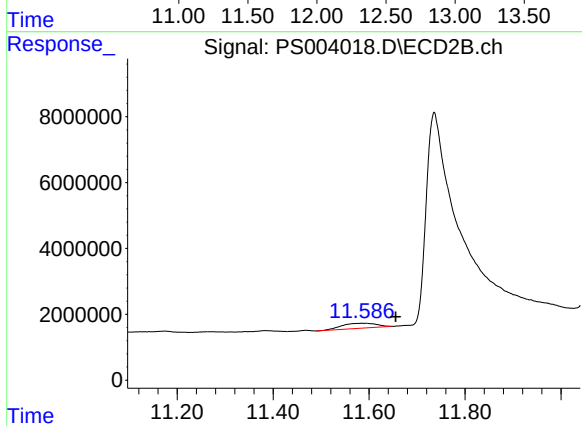

#7 MCPA


R.T.: 11.586 min
Delta R.T.: -0.069 min
Response: 7659779
Conc: 4.30 ug/ml

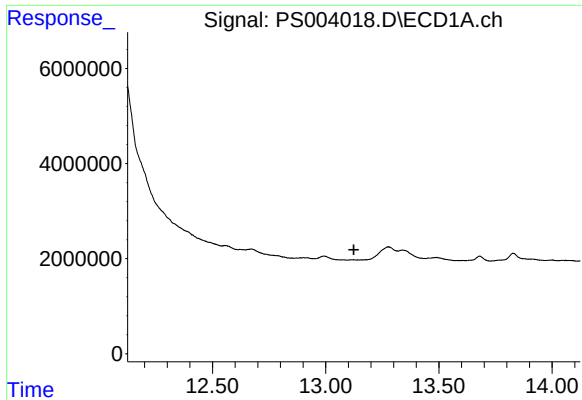

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

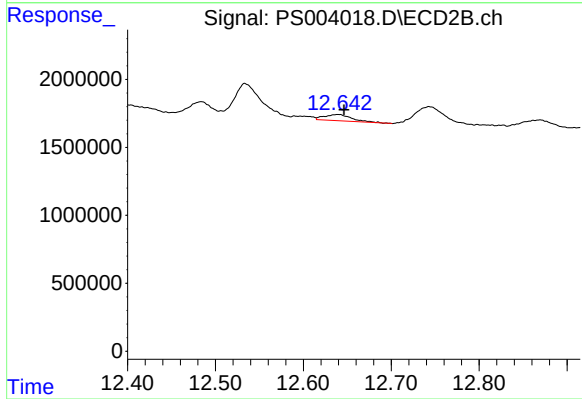


#9 2,4-D

R.T.: 12.639 min
Delta R.T.: -0.007 min
Response: 1001795
Conc: 1.88 ng/ml

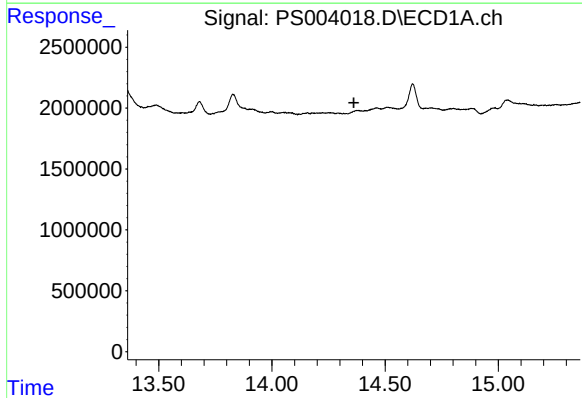


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

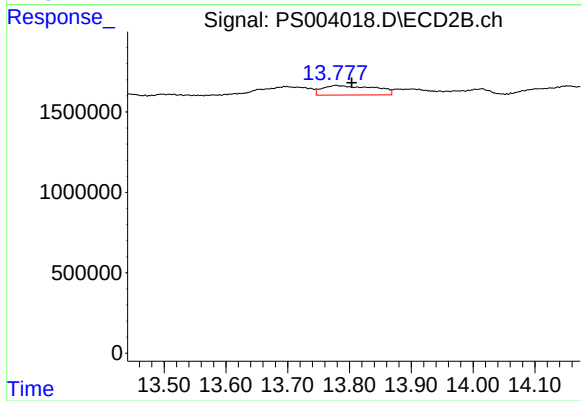

#11 2,4,5-TP (SILVEX)


R.T.: 13.778 min
Delta R.T.: -0.025 min
Response: 3502099
Conc: 1.32 ng/ml

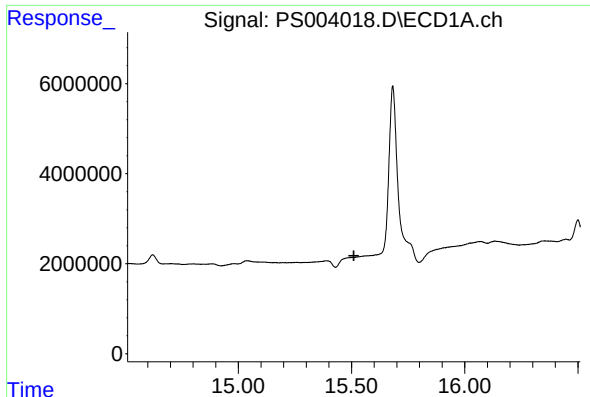

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

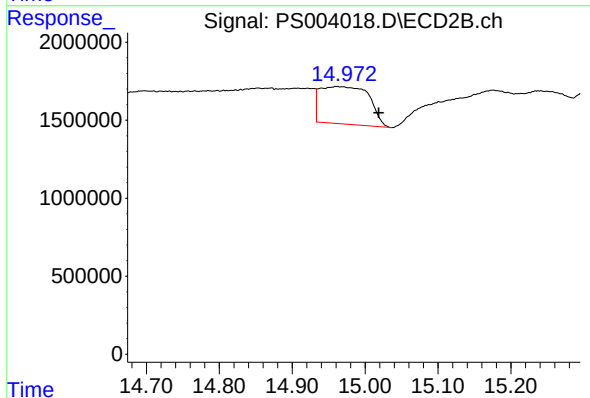


#13 2,4-DB

R.T.: 14.962 min
Delta R.T.: -0.057 min
Response: 11220107
Conc: 37.78 ng/ml

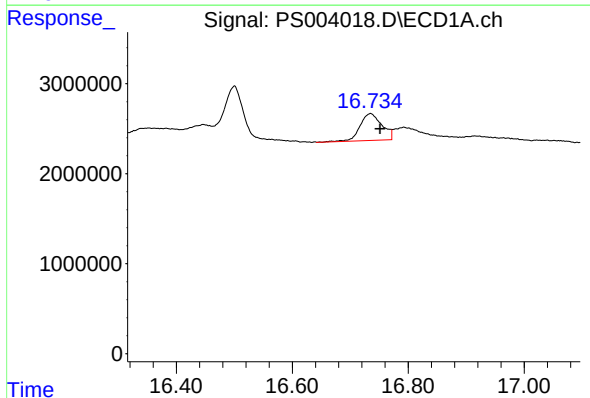


#15 Picloram

R.T.: 16.735 min
Delta R.T.: -0.017 min
Response: 7840527
Conc: 2.31 ng/ml

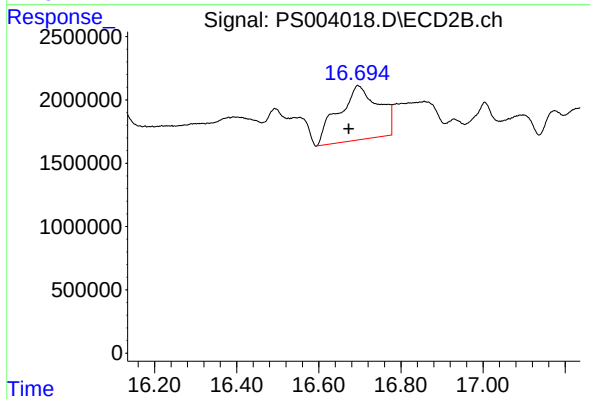

#15 Picloram


R.T.: 16.696 min
Delta R.T.: 0.023 min
Response: 28850403
Conc: 9.10 ng/ml

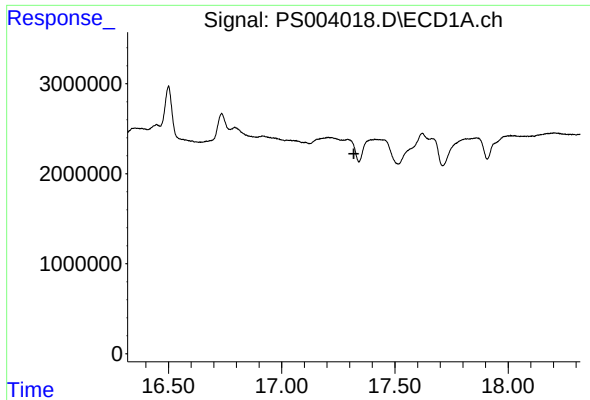

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-040219-A

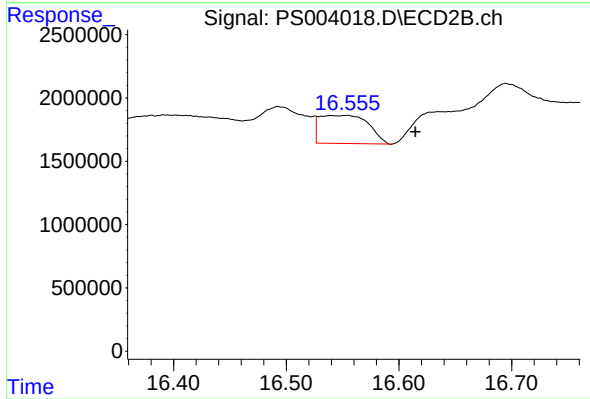

#16 DCPA

R.T.: 16.553 min
Delta R.T.: -0.062 min
Response: 6683923
Conc: 1.98 ng/ml