

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
 Data File : PS004020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2019 18:07
 Operator : EI\SJ
 Sample : K2221-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S2B(2-10)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:11:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.271	10.776	534.2E6	468.6E6	1224.689	955.021
Target Compounds							
1) T	Dalapon	2.798	2.300	65621065	213.4E6	88.019	292.486 #
2) T	3,5-DICHL...	0.000	8.943	0	2130588	N.D.	3.340
5) T	DICAMBA	0.000	11.017	0	4322554	N.D.	2.324
6) T	MCP	11.970	11.259	4694667	-270372	3.375	N.D. #
7) T	MCPA	12.112	0.000	314.2E6	0	148.937	N.D. #
9) T	2,4-D	0.000	12.638	0	2460087	N.D.	4.625
10) T	Pentachlo...	0.000	13.184	0	1513899	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.804	0	4087853	N.D.	1.544
12) T	2,4,5-T	0.000	14.361	0	1272938	N.D.	<MDL
13) T	2,4-DB	0.000	14.970	0	7705337	N.D.	25.948
15) T	Picloram	16.771	16.699	6293082	25202003	1.853	7.947 #
16) T	DCPA	0.000	16.636	0	8008399	N.D.	2.369



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
Data File : PS004020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2019 18:07
Operator : EI\SJ
Sample : K2221-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:11:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

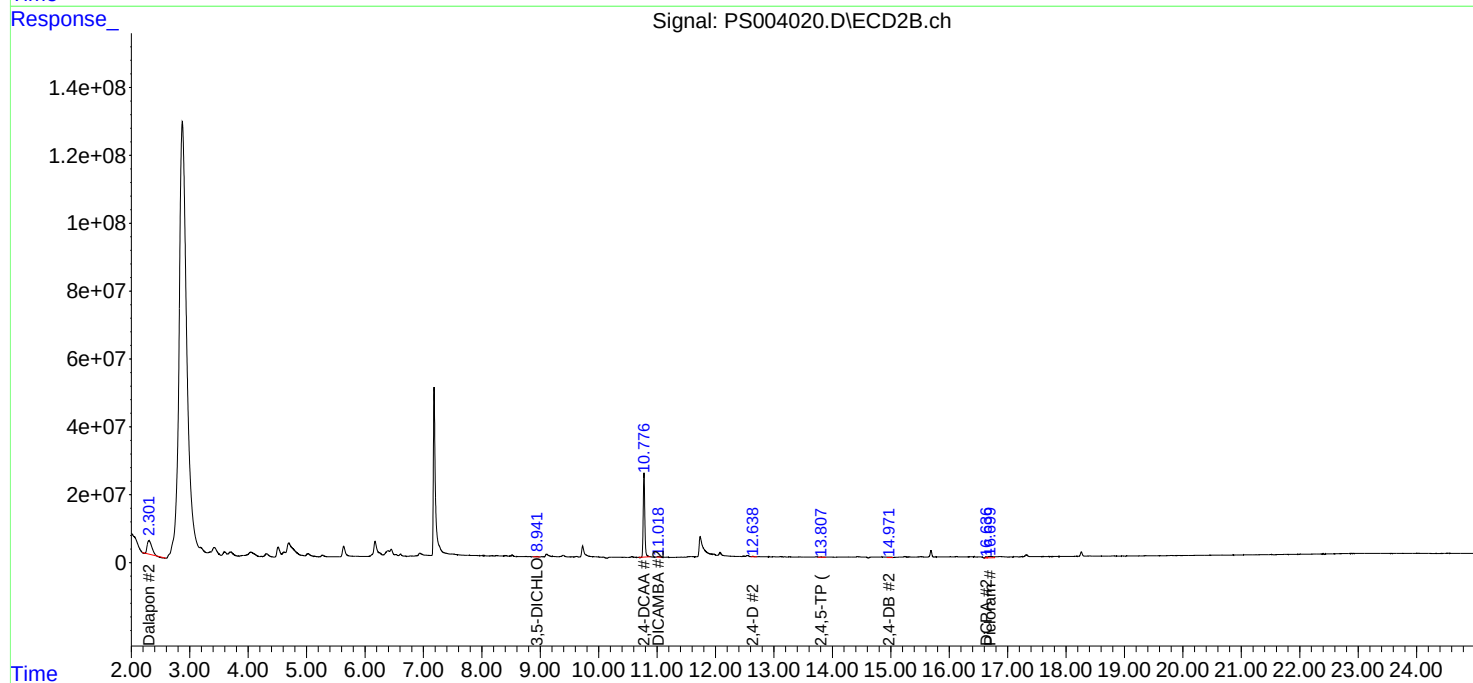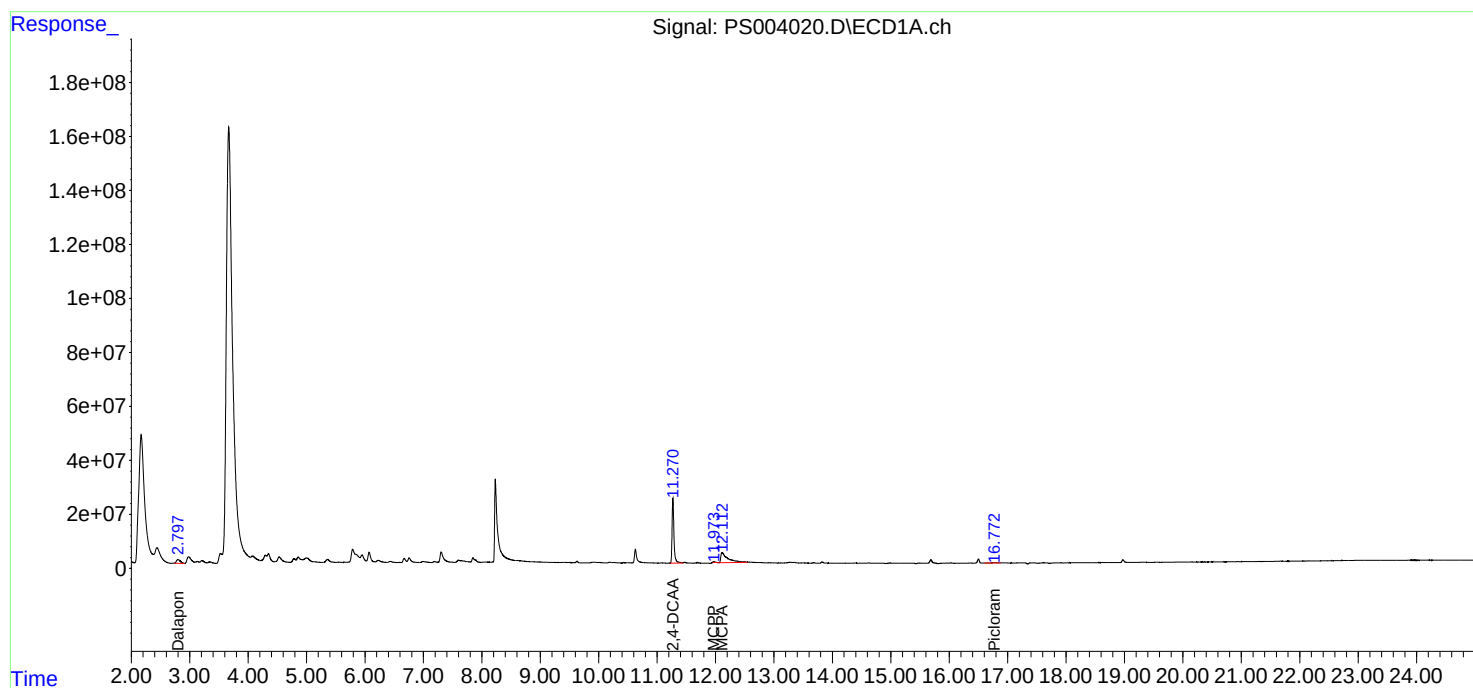


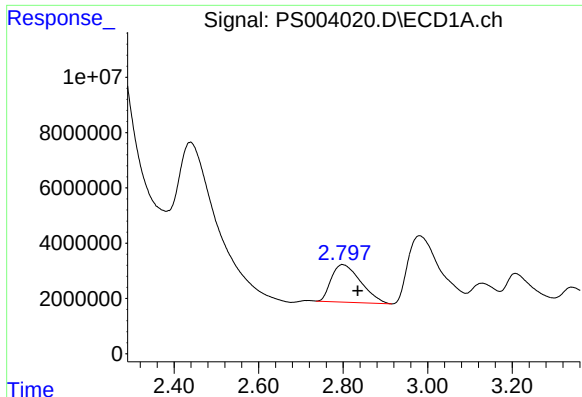

#1 Dalapon


R.T.: 2.798 min
Delta R.T.: -0.037 min
Response: 65621065
Conc: 88.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

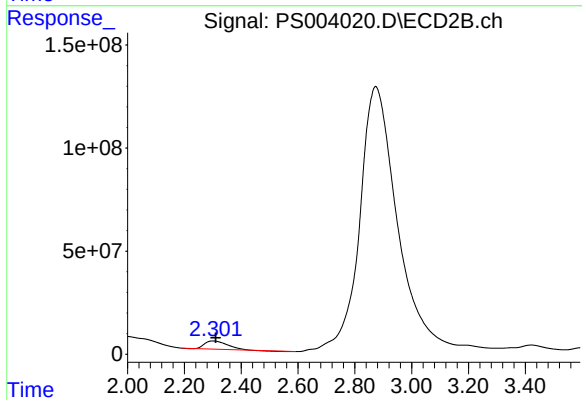


#1 Dalapon

R.T.: 2.300 min
Delta R.T.: -0.010 min
Response: 213405862
Conc: 292.49 ng/ml

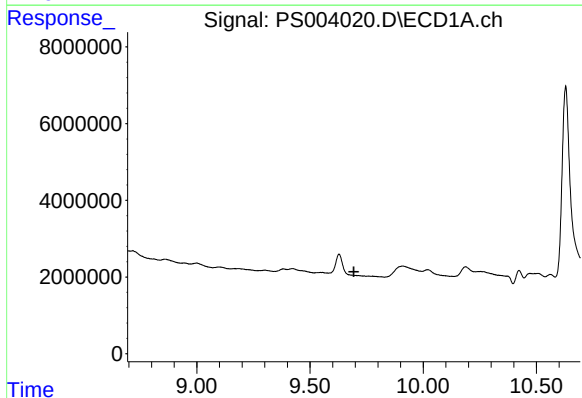


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

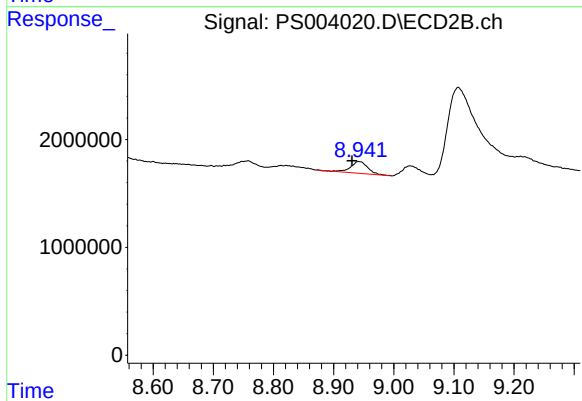

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.943 min
Delta R.T.: 0.012 min
Response: 2130588
Conc: 3.34 ng/ml

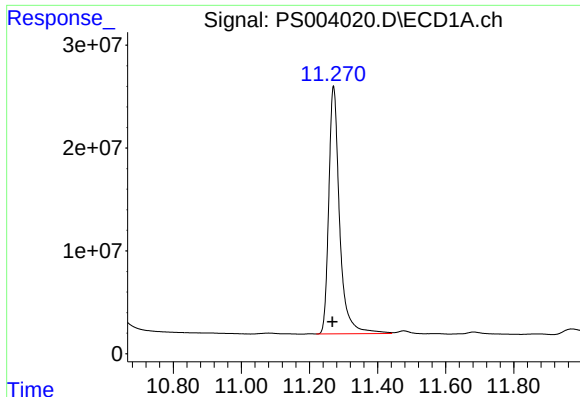

#4 2,4-DCAA


R.T.: 11.271 min
Delta R.T.: 0.004 min
Response: 534224359
Conc: 1224.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

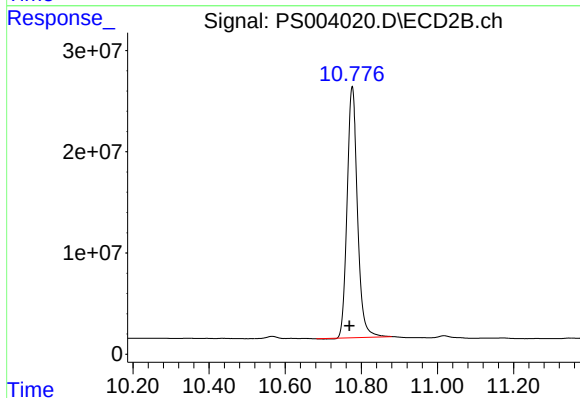


#4 2,4-DCAA

R.T.: 10.776 min
Delta R.T.: 0.007 min
Response: 468589015
Conc: 955.02 ng/ml

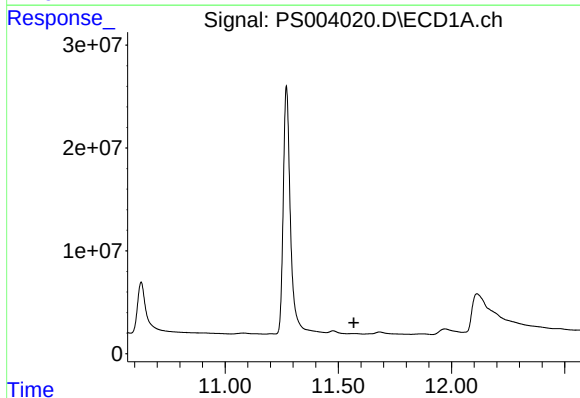


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.569 min
Response: 0
Conc: N.D.

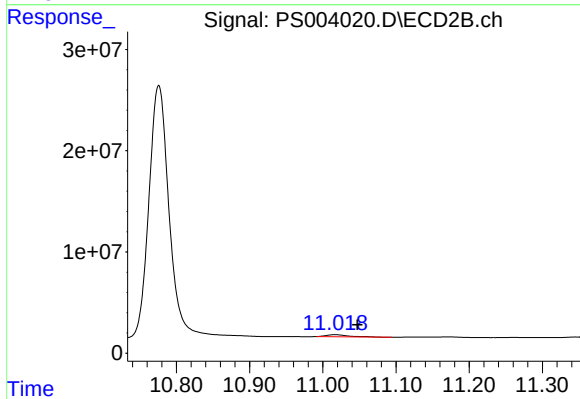

#5 DICAMBA


R.T.: 11.017 min
Delta R.T.: -0.030 min
Response: 4322554
Conc: 2.32 ng/ml

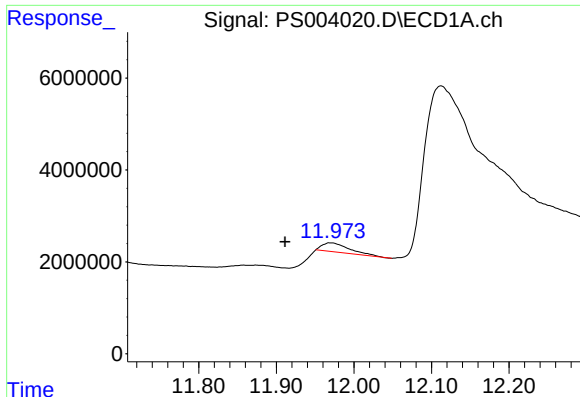

#6 MCPP


R.T.: 11.970 min
Delta R.T.: 0.059 min
Response: 4694667
Conc: 3.37 ug/ml

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

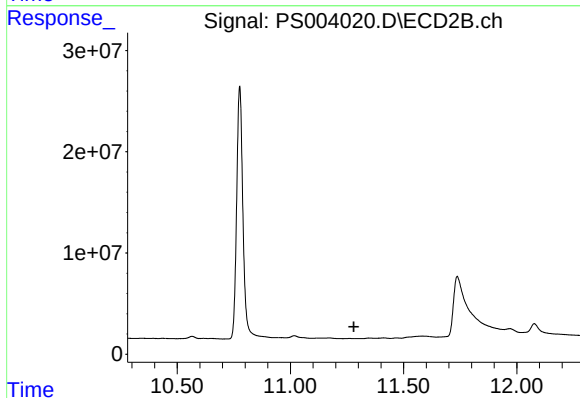


#6 MCPP

R.T.: 11.259 min
Delta R.T.: -0.021 min
Response: -270372
Conc: N.D.

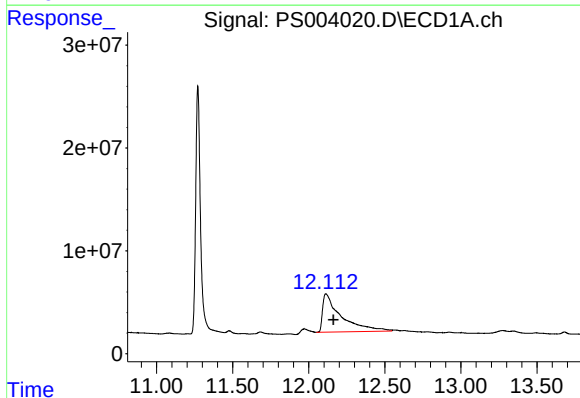


#7 MCPA

R.T.: 12.112 min
Delta R.T.: -0.049 min
Response: 314225535
Conc: 148.94 ug/ml

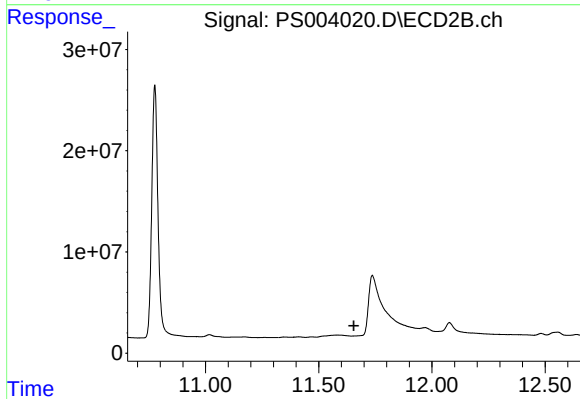

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

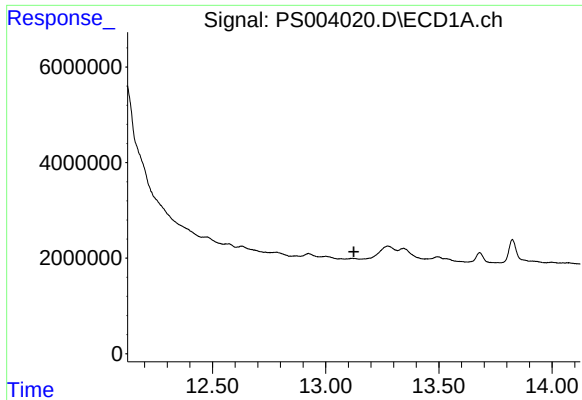

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

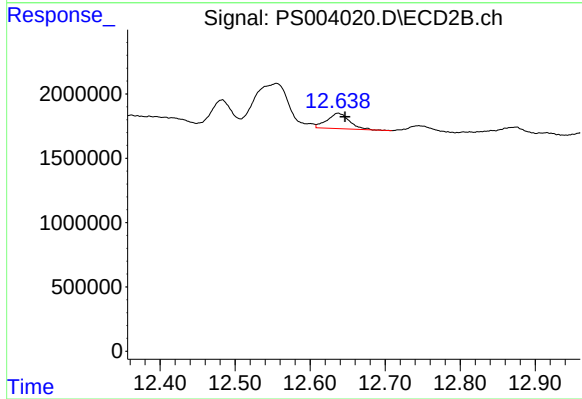


#9 2,4-D

R.T.: 12.638 min
Delta R.T.: -0.009 min
Response: 2460087
Conc: 4.63 ng/ml

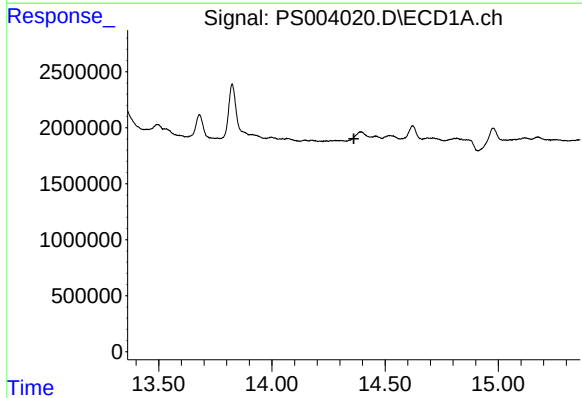


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

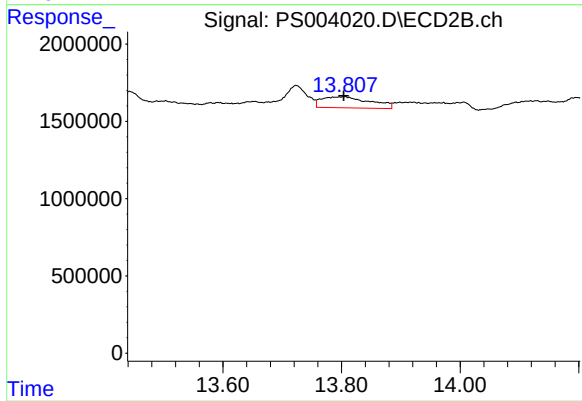

#11 2,4,5-TP (SILVEX)


R.T.: 13.804 min
Delta R.T.: 0.000 min
Response: 4087853
Conc: 1.54 ng/ml

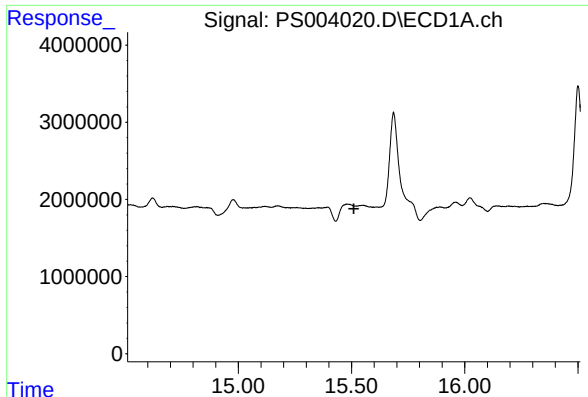

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

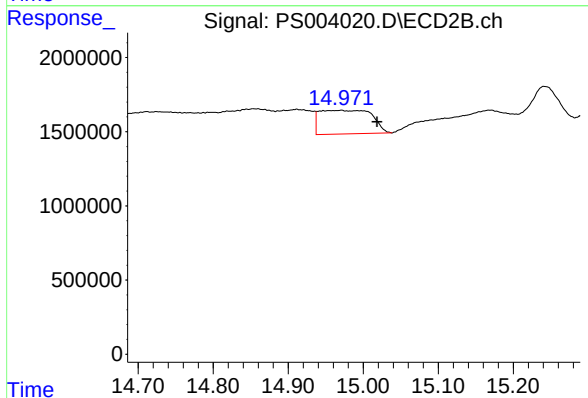


#13 2,4-DB

R.T.: 14.970 min
Delta R.T.: -0.049 min
Response: 7705337
Conc: 25.95 ng/ml

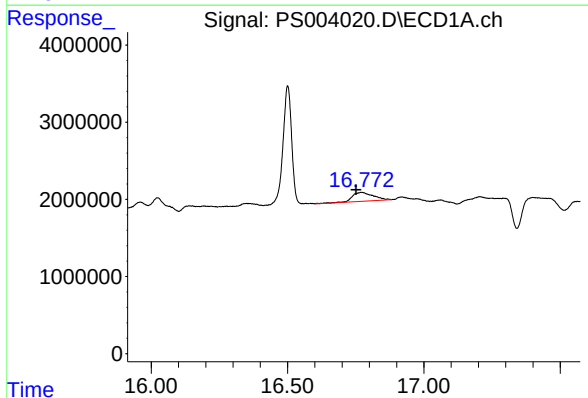


#15 Picloram

R.T.: 16.771 min
Delta R.T.: 0.020 min
Response: 6293082
Conc: 1.85 ng/ml

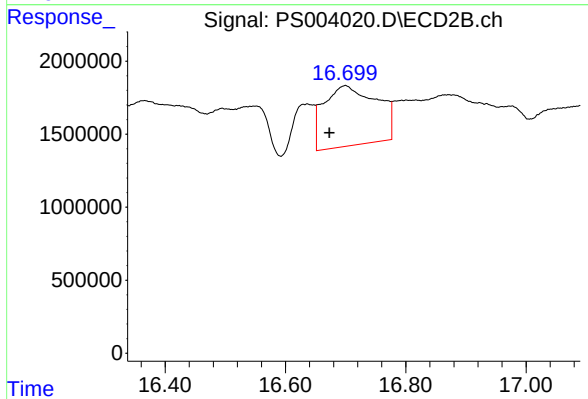

#15 Picloram


R.T.: 16.699 min
Delta R.T.: 0.027 min
Response: 25202003
Conc: 7.95 ng/ml

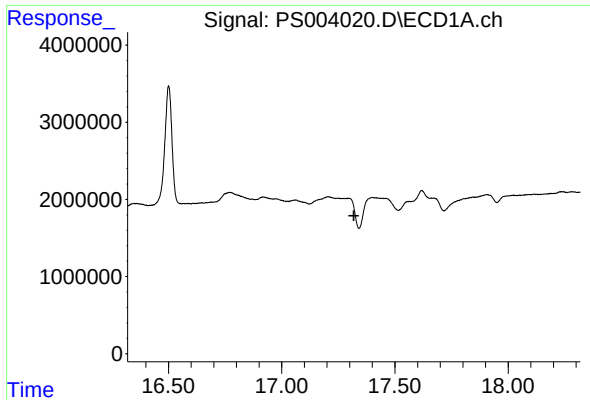

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S2B(2-10)COMP

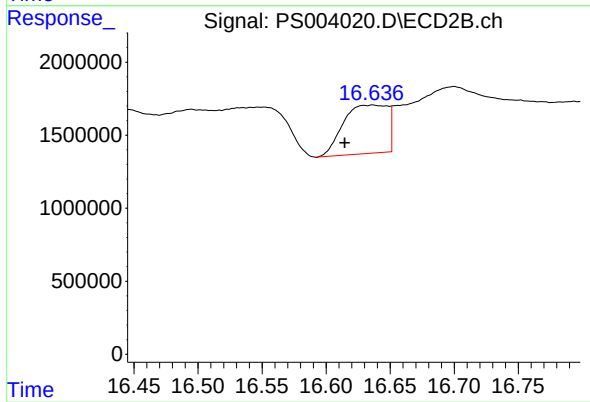

#16 DCPA

R.T.: 16.636 min
Delta R.T.: 0.021 min
Response: 8008399
Conc: 2.37 ng/ml