

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
 Data File : PS004023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2019 19:41
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:12:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.301	10.801	169.1E6	154.3E6	387.715	314.384
Target Compounds							
2) T	3,5-DICHL...	0.000	8.979	0	56655	N.D.	<MDL
3) T	4-Nitroph...	0.000	9.904	0	66319	N.D.	<MDL
7) T	MCPA	0.000	11.680	0	342514	N.D.	<MDL
8) T	DICHLORPROP	0.000	12.154	0	7282585	N.D.	15.644
9) T	2,4-D	0.000	12.654	0	280373	N.D.	<MDL
10) T	Pentachlo...	0.000	13.180	0	130772	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	13.813	0	114174	N.D.	<MDL
12) T	2,4,5-T	0.000	14.325	0	73900	N.D.	<MDL
13) T	2,4-DB	0.000	15.021	0	1301386	N.D.	4.383
14) T	DINOSEB	0.000	15.471	0	810440	N.D.	<MDL
15) T	Picloram	0.000	16.660	0	856785	N.D.	<MDL
16) T	DCPA	0.000	16.660	0	856785	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040619\
Data File : PS004023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2019 19:41
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:12:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

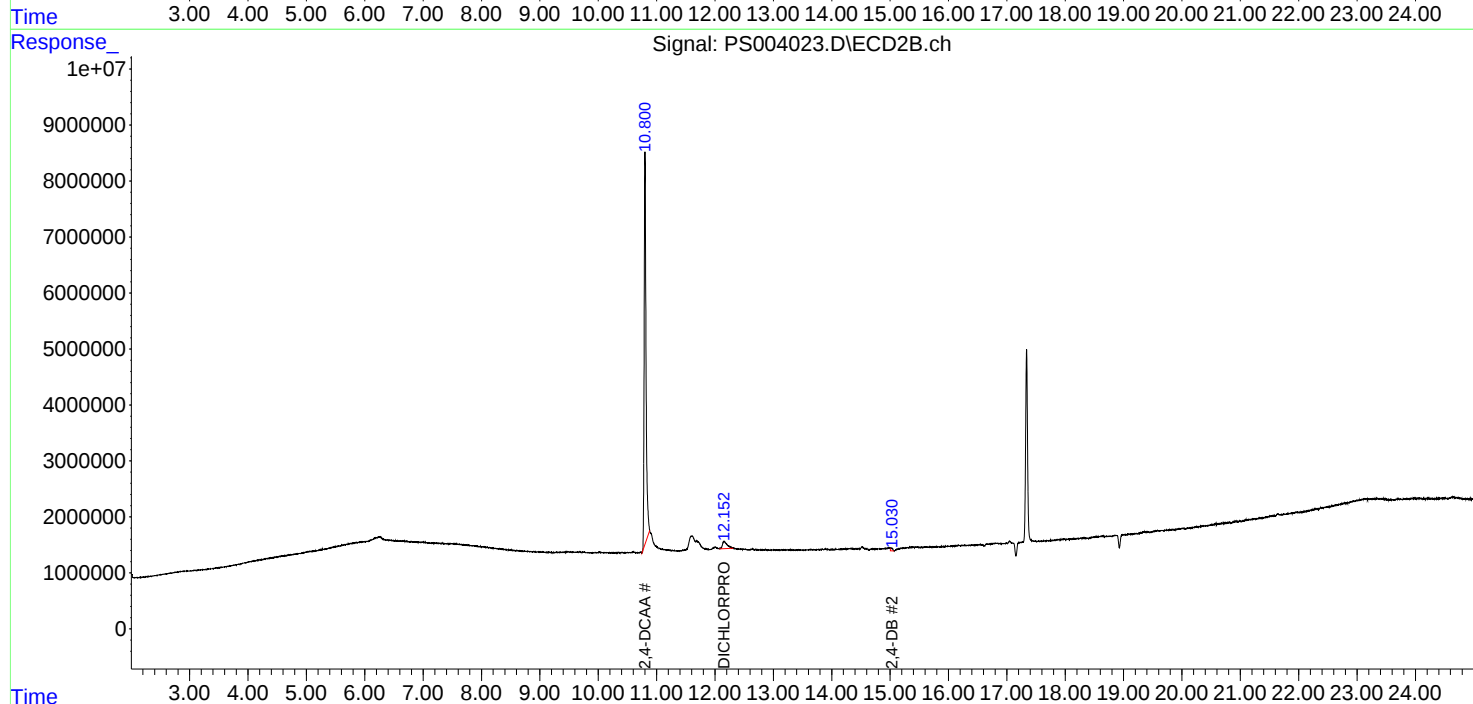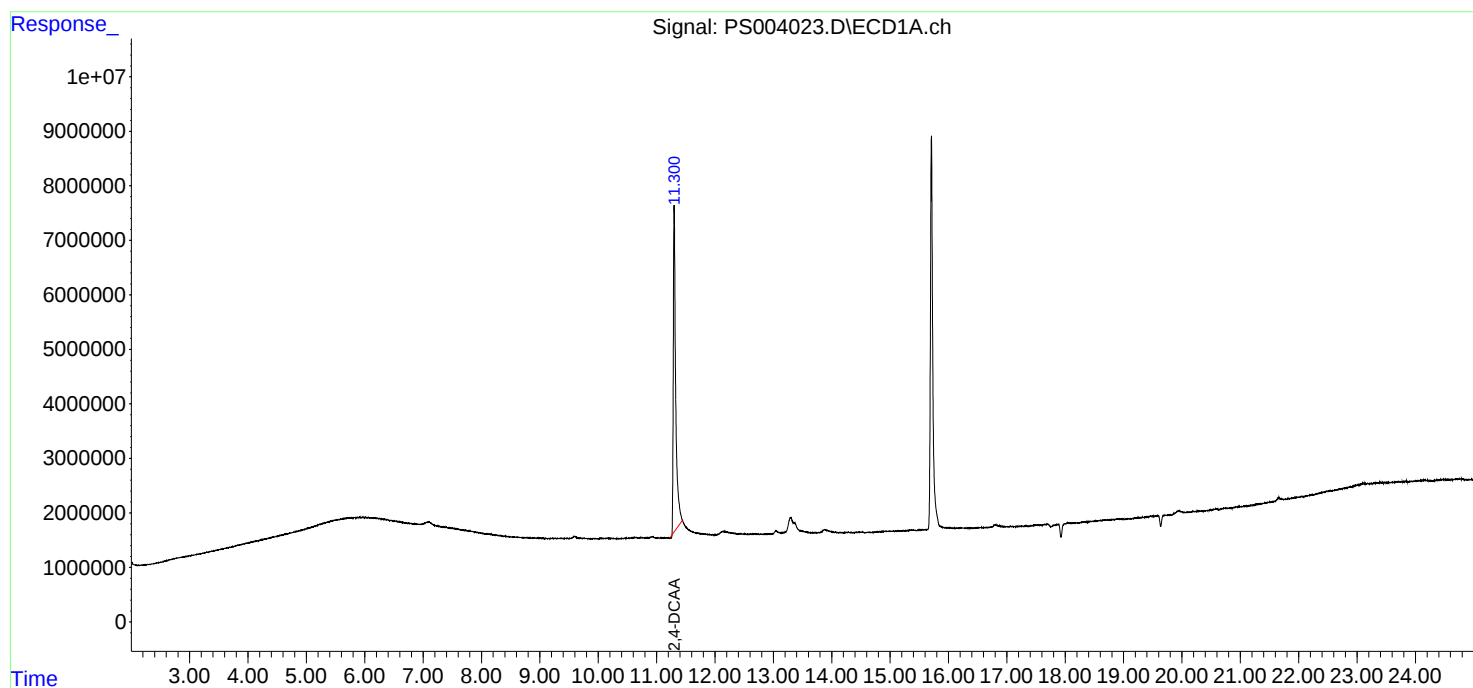


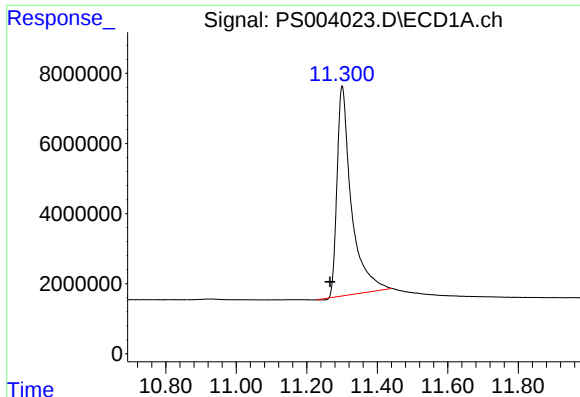

#4 2,4-DCAA


R.T.: 11.301 min
Delta R.T.: 0.034 min
Response: 169126278
Conc: 387.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

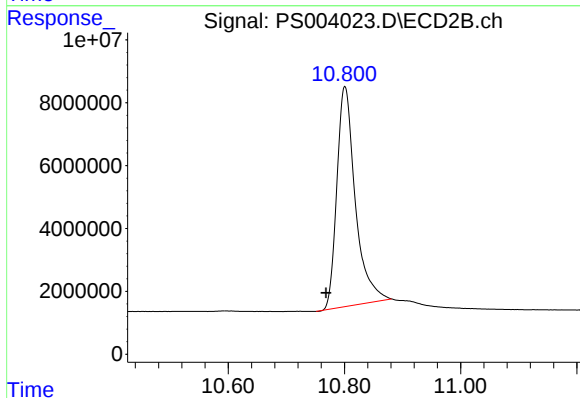


#4 2,4-DCAA

R.T.: 10.801 min
Delta R.T.: 0.032 min
Response: 154255186
Conc: 314.38 ng/ml

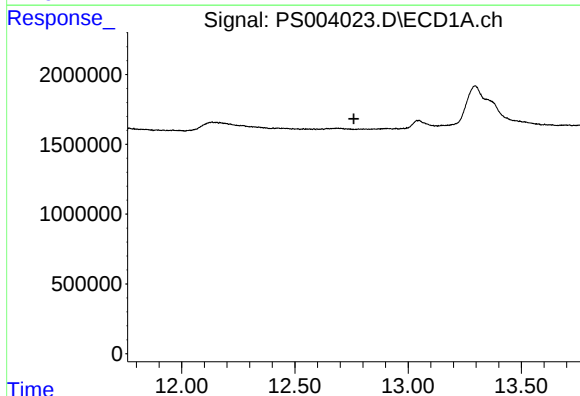


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

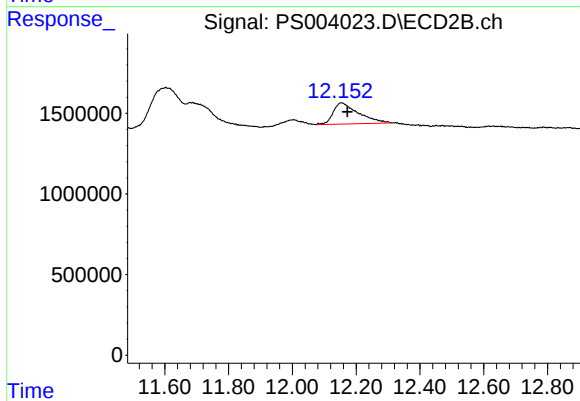

#8 DICHLORPROP


R.T.: 12.154 min
Delta R.T.: -0.019 min
Response: 7282585
Conc: 15.64 ng/ml

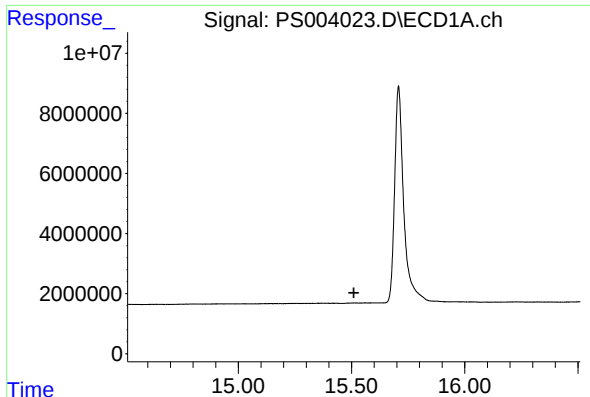

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

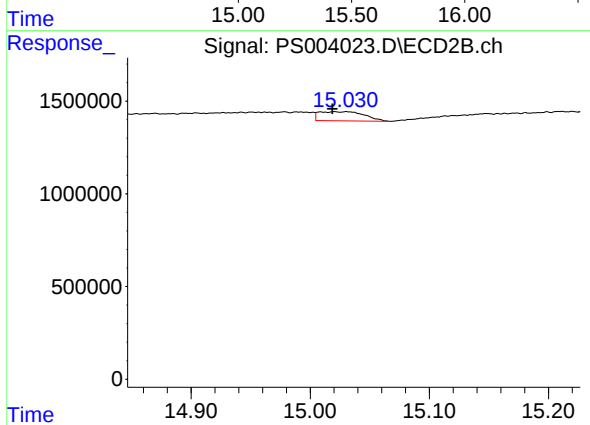

#13 2,4-DB

R.T.: 15.021 min
Delta R.T.: 0.002 min
Response: 1301386
Conc: 4.38 ng/ml