

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040620\
 Data File : PS009609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 00:19
 Operator : DD\AJ
 Sample : PB128000BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 07:28:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.929	530.5E6	491.6E6	958.978	895.186
Target Compounds							
1) T	Dalapon	3.008	2.591	15461270	20080409	19.826	25.503 #
2) T	3,5-DICHL...	0.000	6.106	0	18463879	N.D.	22.702
7) T	MCPA	7.733	7.396	10047753	21441173	3.299	7.945 #
8) T	DICHLORPROP	0.000	7.748	0	1934983	N.D.	3.488
11) T	2,4,5-TP ...	0.000	8.857	0	8600982	N.D.	2.885
12) T	2,4,5-T	9.449	9.253	40899459	8665132	16.078	2.935 #
13) T	2,4-DB	10.096	9.640	4875521	4832644	14.093	12.730
14) T	DINOSEB	11.185	10.044	17597329	15678580	8.609	7.138
15) T	Picloram	11.032	11.017	15630615	22290290	5.150	5.474
16) T	DCPA	0.000	11.017	0	22290290	N.D.	5.755



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040620\
Data File : PS009609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 00:19
Operator : DD\AJ
Sample : PB128000BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 07:28:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

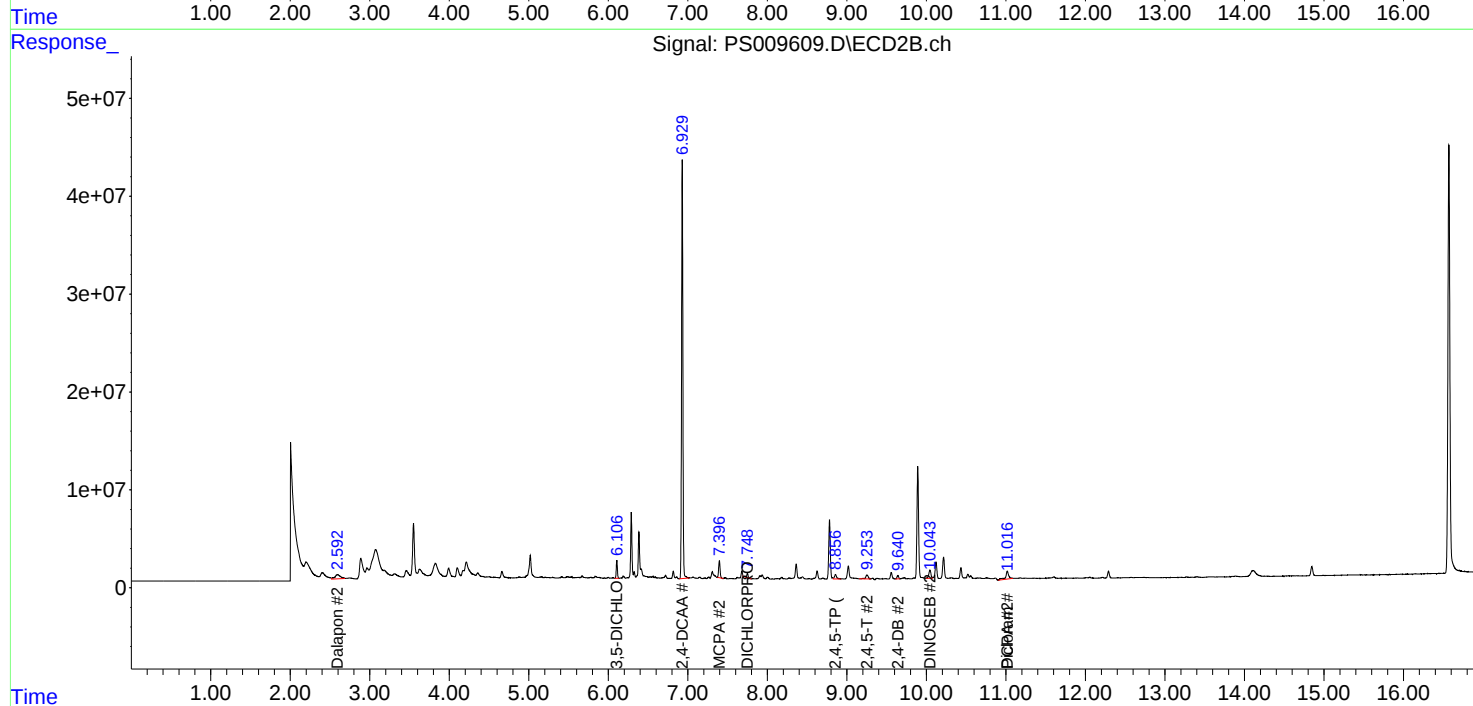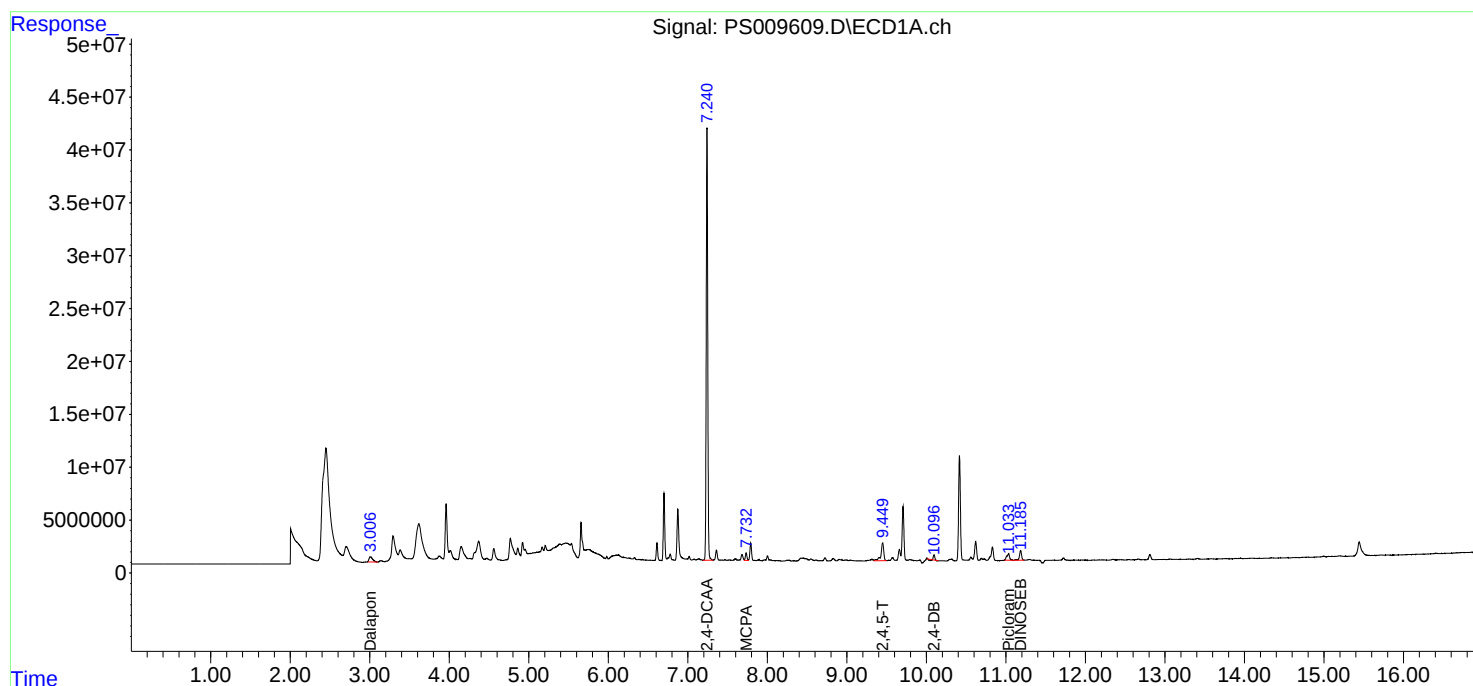


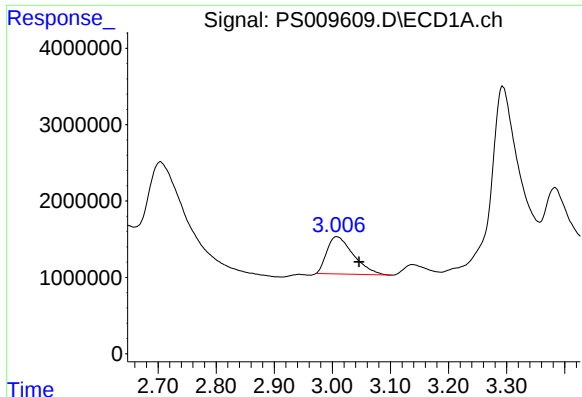

#1 Dalapon


R.T.: 3.008 min
Delta R.T.: -0.038 min
Response: 15461270
Conc: 19.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

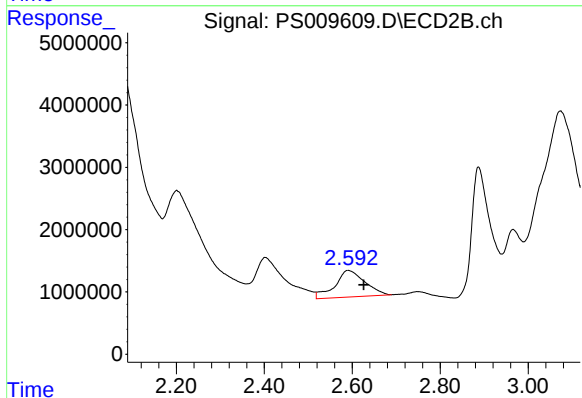


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.036 min
Response: 20080409
Conc: 25.50 ng/ml

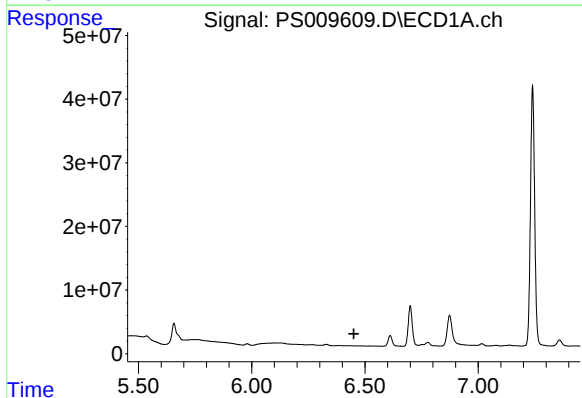


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

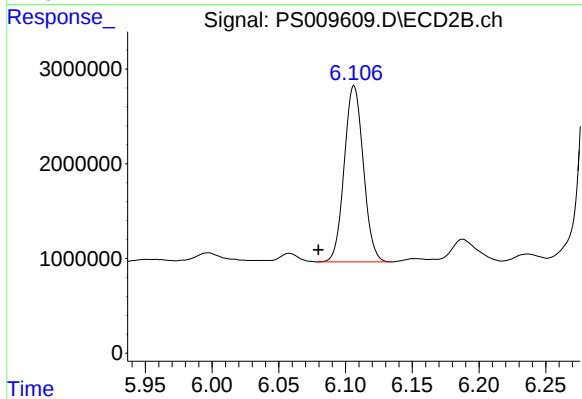

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.106 min
Delta R.T.: 0.027 min
Response: 18463879
Conc: 22.70 ng/ml

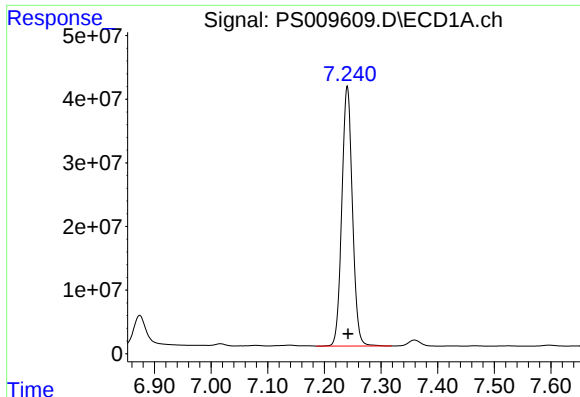

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 530478124
Conc: 958.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

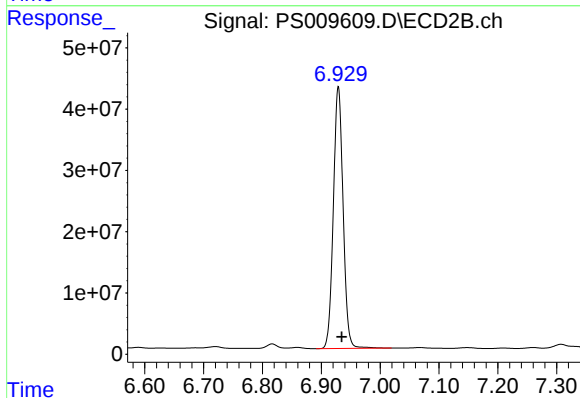


#4 2,4-DCAA

R.T.: 6.929 min
Delta R.T.: -0.006 min
Response: 491634130
Conc: 895.19 ng/ml

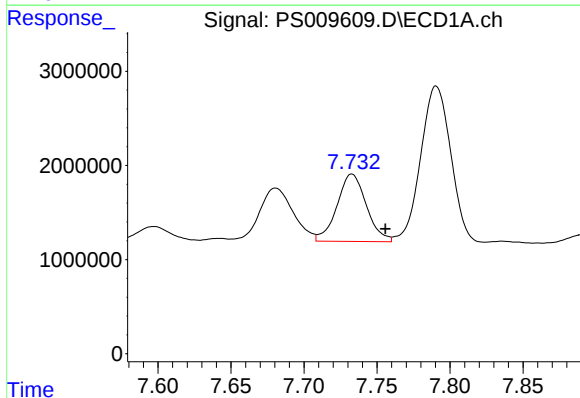


#7 MCPA

R.T.: 7.733 min
Delta R.T.: -0.023 min
Response: 10047753
Conc: 3.30 ug/ml

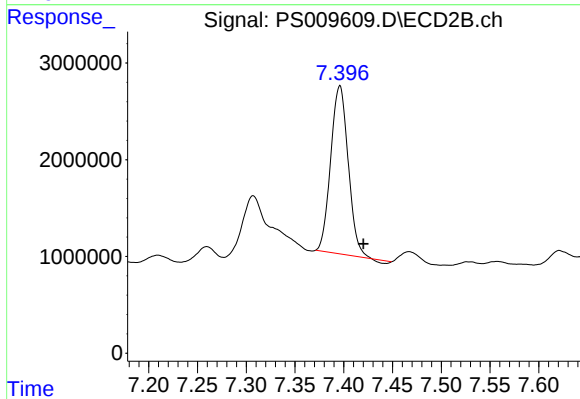

#7 MCPA


R.T.: 7.396 min
Delta R.T.: -0.024 min
Response: 21441173
Conc: 7.95 ug/ml

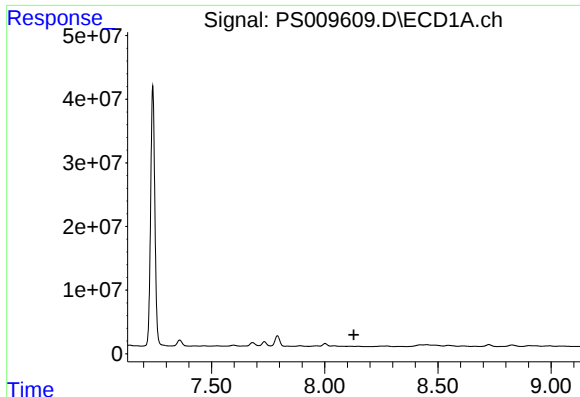

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

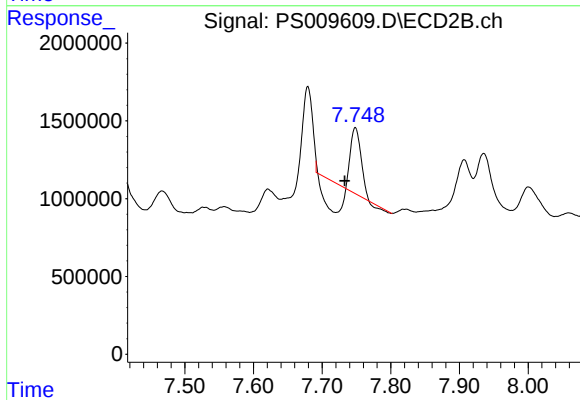


#8 DICHLORPROP

R.T.: 7.748 min
Delta R.T.: 0.015 min
Response: 1934983
Conc: 3.49 ng/ml

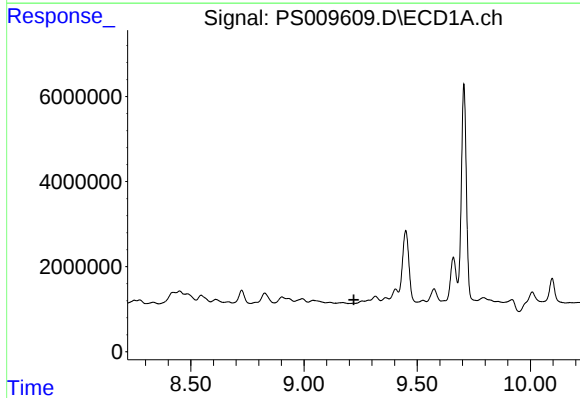


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

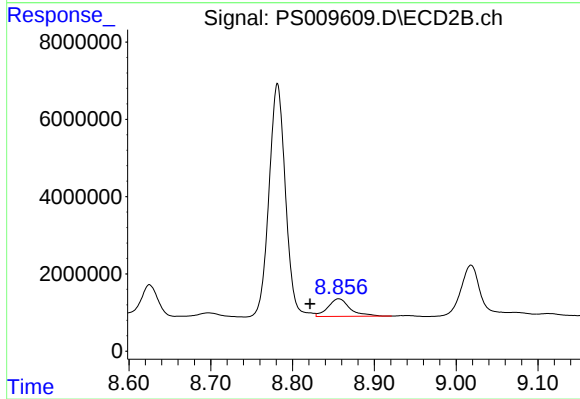

#11 2,4,5-TP (SILVEX)


R.T.: 8.857 min
Delta R.T.: 0.035 min
Response: 8600982
Conc: 2.89 ng/ml

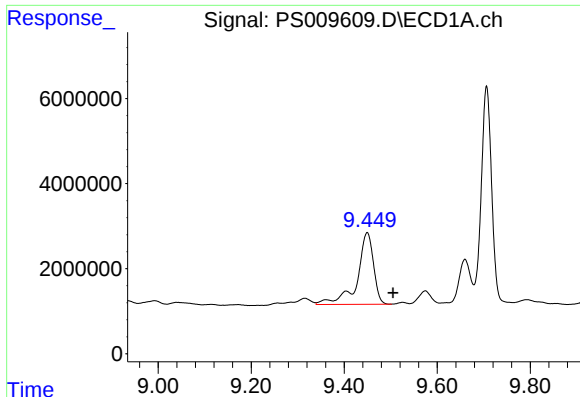

#12 2,4,5-T


R.T.: 9.449 min
Delta R.T.: -0.056 min
Response: 40899459
Conc: 16.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

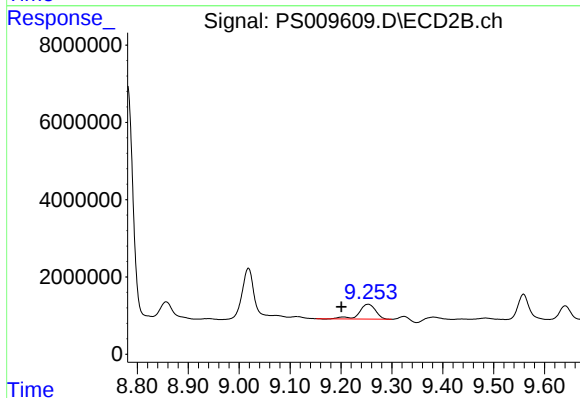


#12 2,4,5-T

R.T.: 9.253 min
Delta R.T.: 0.052 min
Response: 8665132
Conc: 2.94 ng/ml

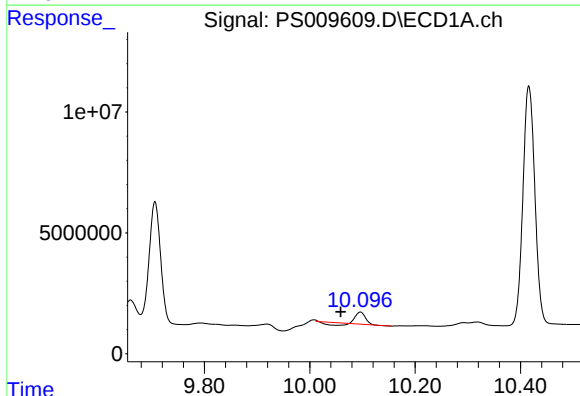


#13 2,4-DB

R.T.: 10.096 min
Delta R.T.: 0.037 min
Response: 4875521
Conc: 14.09 ng/ml

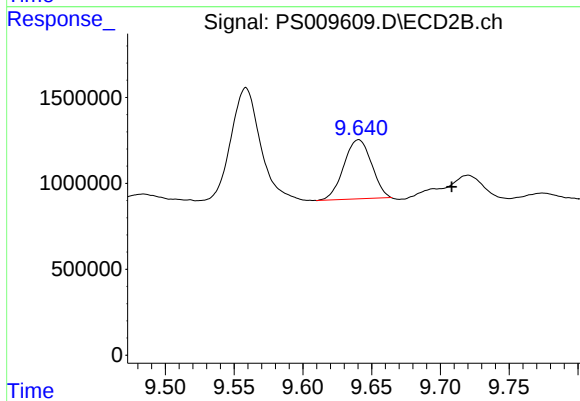

#13 2,4-DB


R.T.: 9.640 min
Delta R.T.: -0.068 min
Response: 4832644
Conc: 12.73 ng/ml

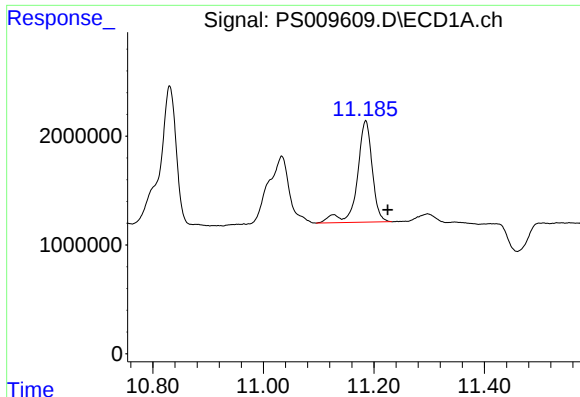

#14 DINOSEB


R.T.: 11.185 min
Delta R.T.: -0.040 min
Response: 17597329
Conc: 8.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

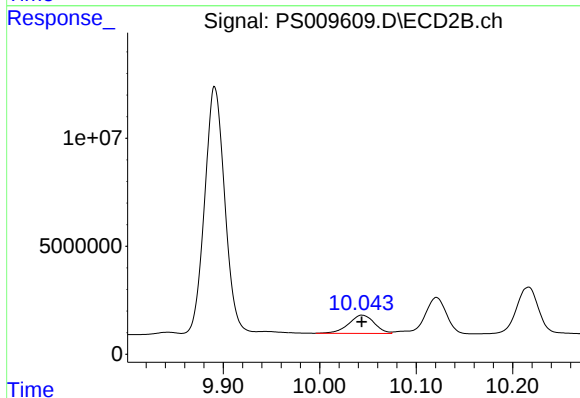


#14 DINOSEB

R.T.: 10.044 min
Delta R.T.: 0.000 min
Response: 15678580
Conc: 7.14 ng/ml

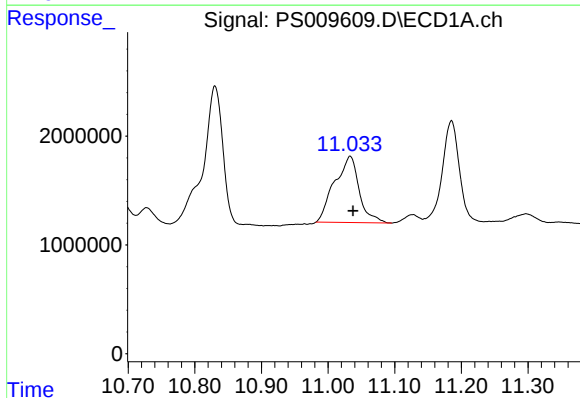


#15 Picloram

R.T.: 11.032 min
Delta R.T.: -0.005 min
Response: 15630615
Conc: 5.15 ng/ml

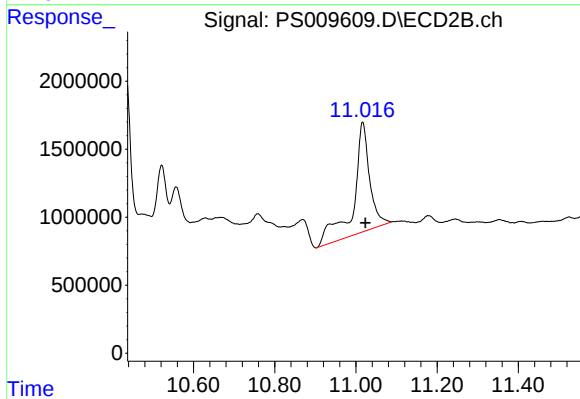

#15 Picloram


R.T.: 11.017 min
Delta R.T.: -0.007 min
Response: 22290290
Conc: 5.47 ng/ml

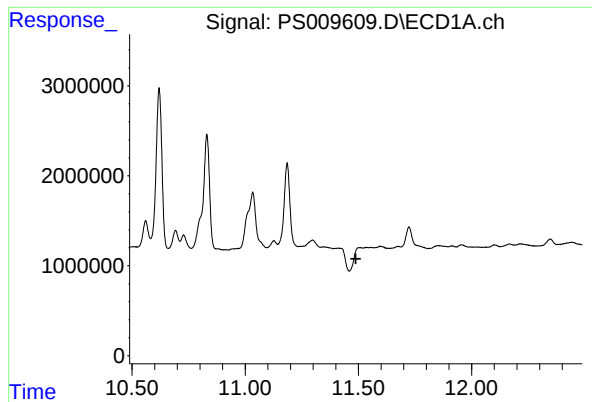

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

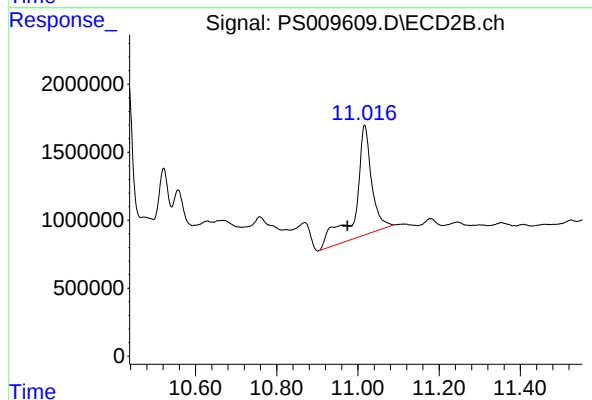

#16 DCPA

R.T.: 11.017 min
Delta R.T.: 0.043 min
Response: 22290290
Conc: 5.76 ng/ml