

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040620\
 Data File : PS009615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 02:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 07:30:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.929	294.2E6	276.9E6	531.872	504.213
Target Compounds							
8) T	DICHLORPROP	0.000	7.751	0	3317082	N.D.	5.979
9) T	2,4-D	0.000	8.059	0	3939065	N.D.	5.992
12) T	2,4,5-T	0.000	9.246	0	4629121	N.D.	1.568
15) T	Picloram	0.000	11.017	0	3873297	N.D.	<MDL
16) T	DCPA	0.000	11.017	0	3873297	N.D.	1.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040620\
Data File : PS009615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 02:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 07:30:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

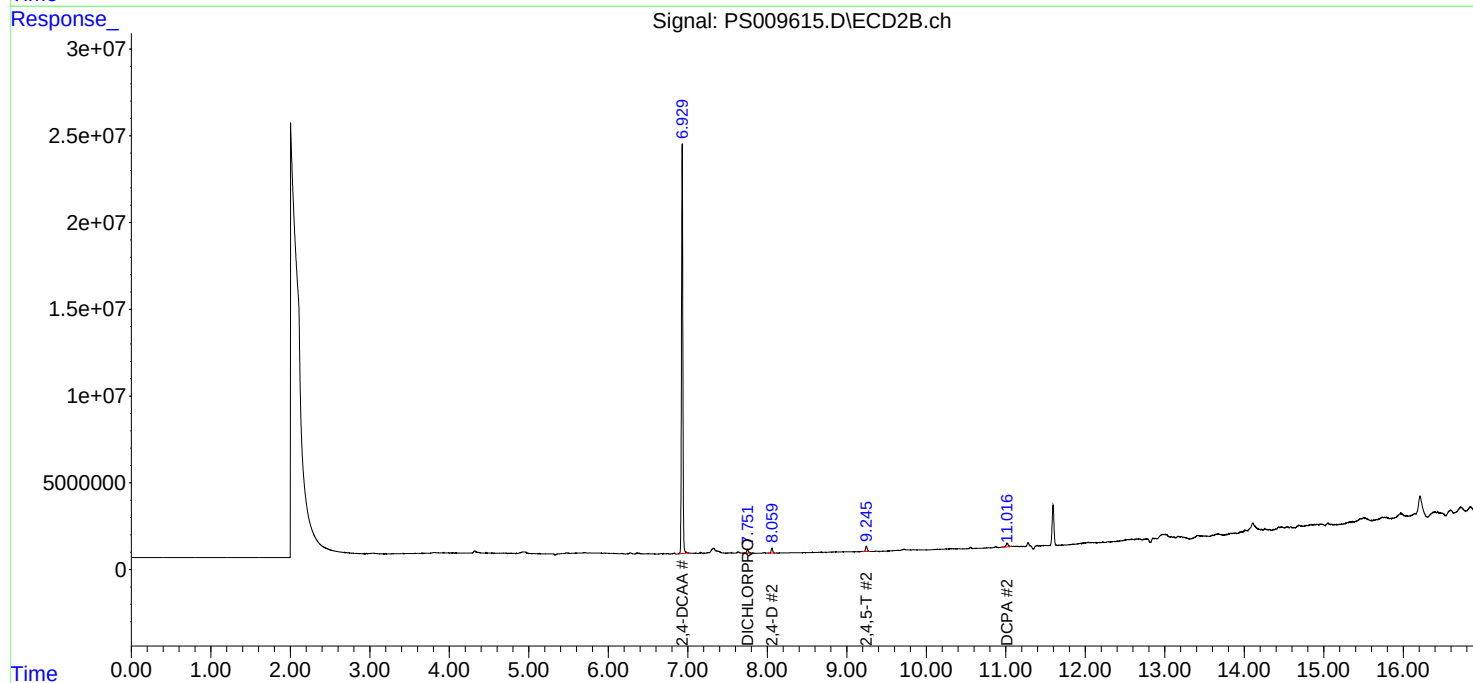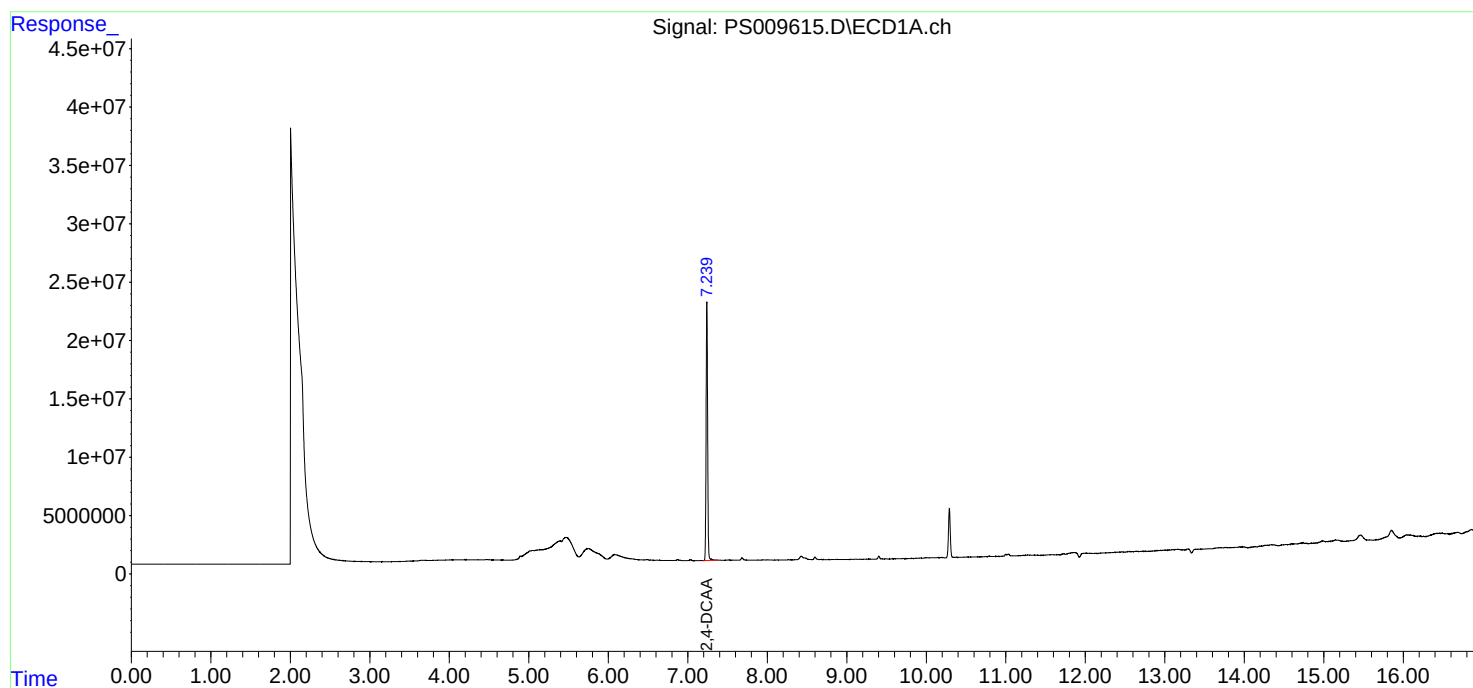


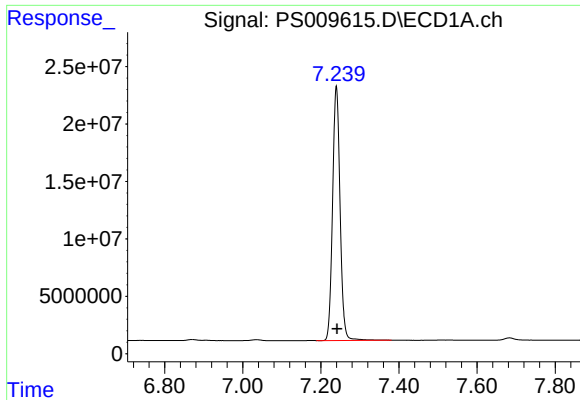

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 294215712
Conc: 531.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

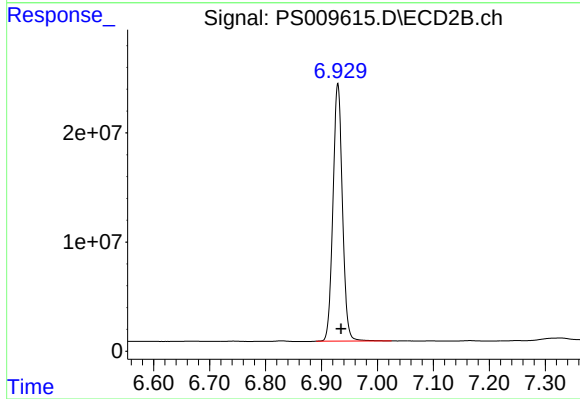


#4 2,4-DCAA

R.T.: 6.929 min
Delta R.T.: -0.006 min
Response: 276912348
Conc: 504.21 ng/ml

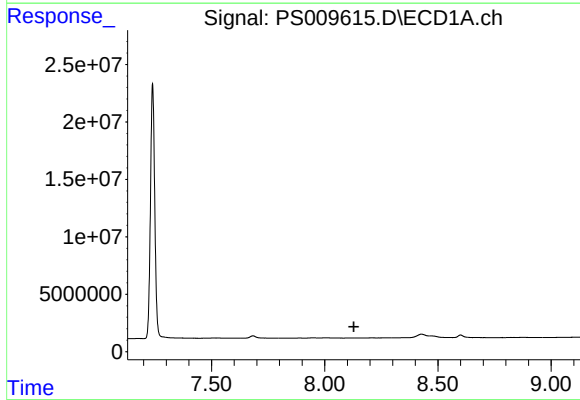


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

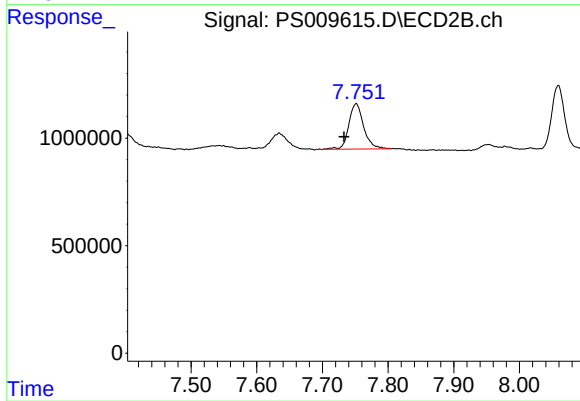

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 3317082
Conc: 5.98 ng/ml

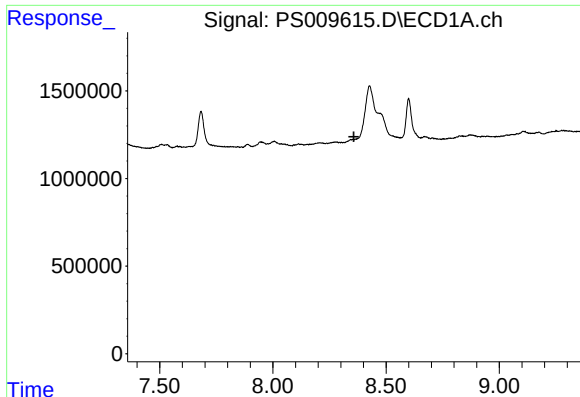

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.358 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

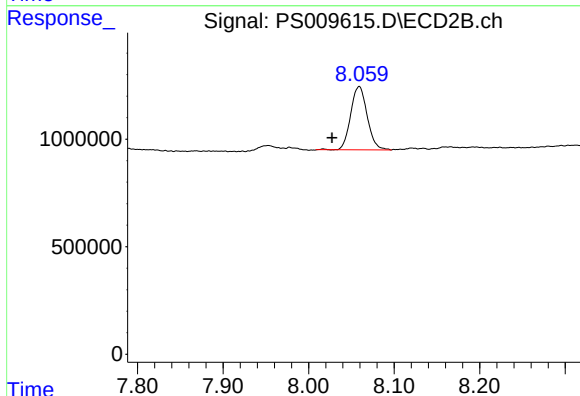


#9 2,4-D

R.T.: 8.059 min
Delta R.T.: 0.032 min
Response: 3939065
Conc: 5.99 ng/ml

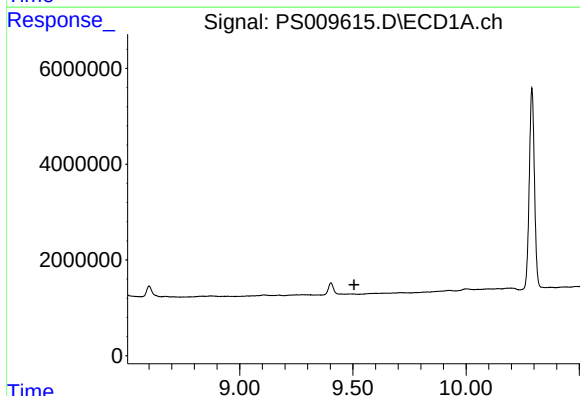


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.505 min
Response: 0
Conc: N.D.

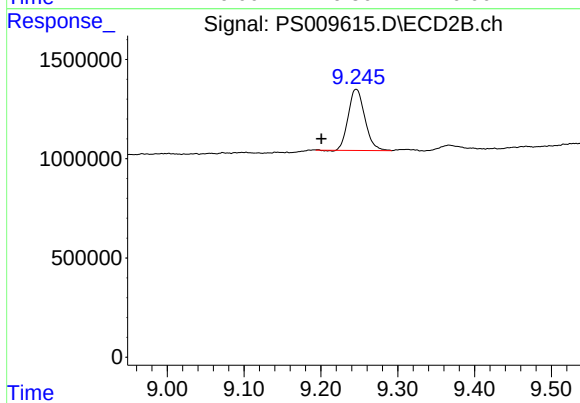

#12 2,4,5-T


R.T.: 9.246 min
Delta R.T.: 0.045 min
Response: 4629121
Conc: 1.57 ng/ml

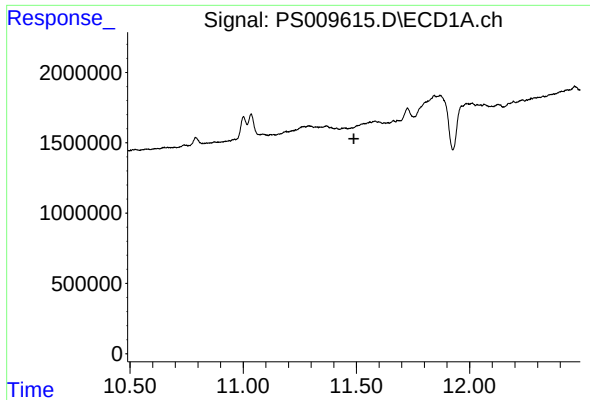

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

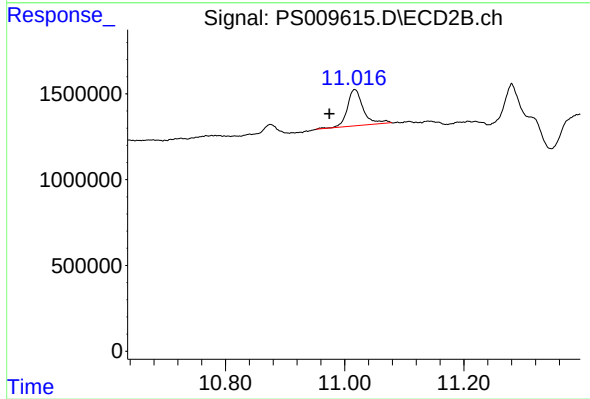

#16 DCPA

R.T.: 11.017 min
Delta R.T.: 0.043 min
Response: 3873297
Conc: 1.00 ng/ml