

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
 Data File : PS014486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 19:02
 Operator : DD\AJ
 Sample : M1909-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:10:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.886	537.0E6	190.3E6	375.834	403.367
Target Compounds							
1) T	Dalapon	2.976	2.581	43331124	5981157	27.839	10.101 #
2) T	3,5-DICHL...	0.000	6.076	0	54580327	N.D.	73.305
3) T	4-Nitroph...	7.000	6.522	5296853	4362929	7.093	14.363 #
5) T	DICAMBA	7.342	7.023	17935813	23112038	3.335	11.537 #
6) T	MCPD	7.508	7.160	12899143	3249360	3.102	1.951 #
7) T	MCPA	7.645	7.346	30323320	31066504	5.271	12.750 #
8) T	DICHLORPROP	8.035	7.709	2901075	13430282	2.191	26.359 #
9) T	2,4-D	8.221f	7.945	14672357	12514159	9.954	20.958 #
10) T	Pentachlo...	8.568	8.399	18689929	9770891	<MDL	1.431 #
11) T	2,4,5-TP ...	9.112	8.729	10831463	97617128	1.406	35.880 #
12) T	2,4,5-T	9.414	9.141	50434292	8742001	6.482	3.279 #
13) T	2,4-DB	9.984	9.696f	65398770	2744672	42.291	7.740 #
14) T	DINOSEB	11.067f	9.988	187.2E6	44062589	32.748	24.383 #
15) T	Picloram	10.930	10.966	241.4E6	95957330	23.113	25.294
16) T	DCPA	11.372	10.899	12956630	14455500	1.100	3.524 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
Data File : PS014486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 19:02
Operator : DD\AJ
Sample : M1909-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:10:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

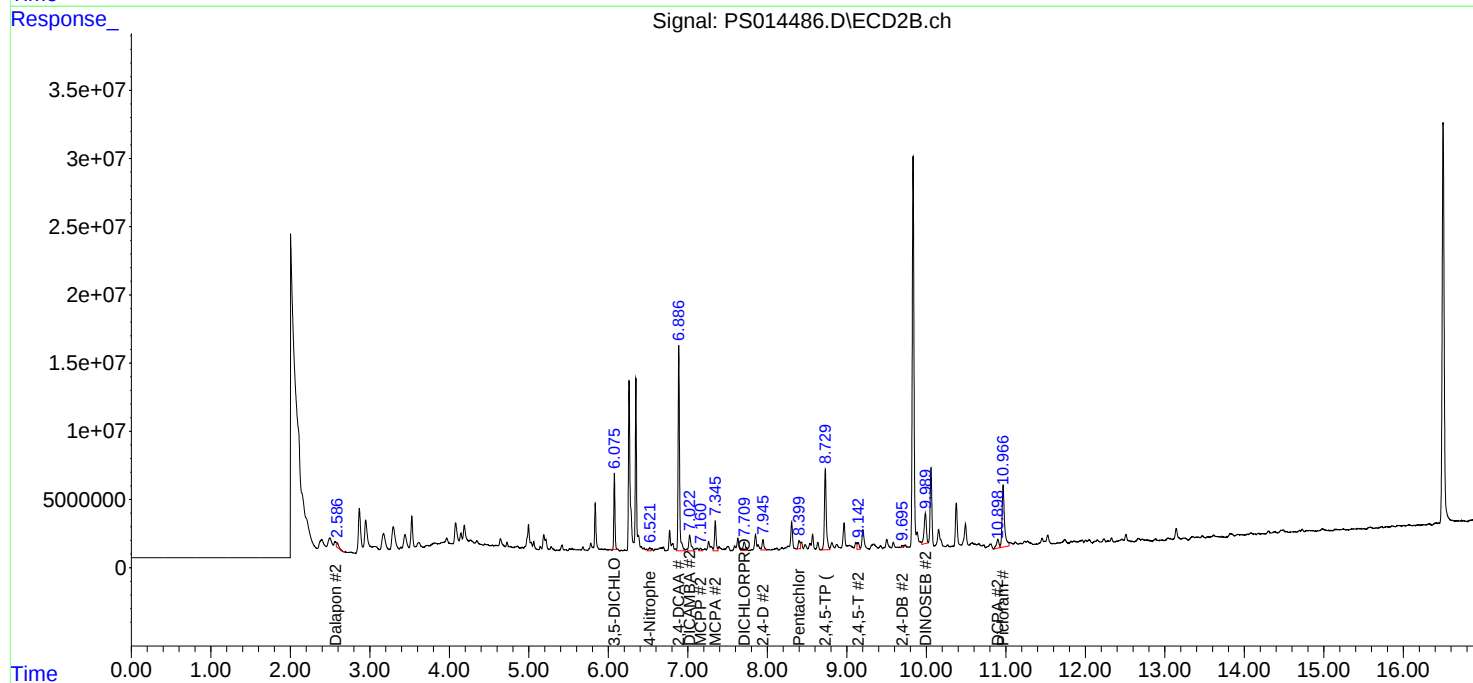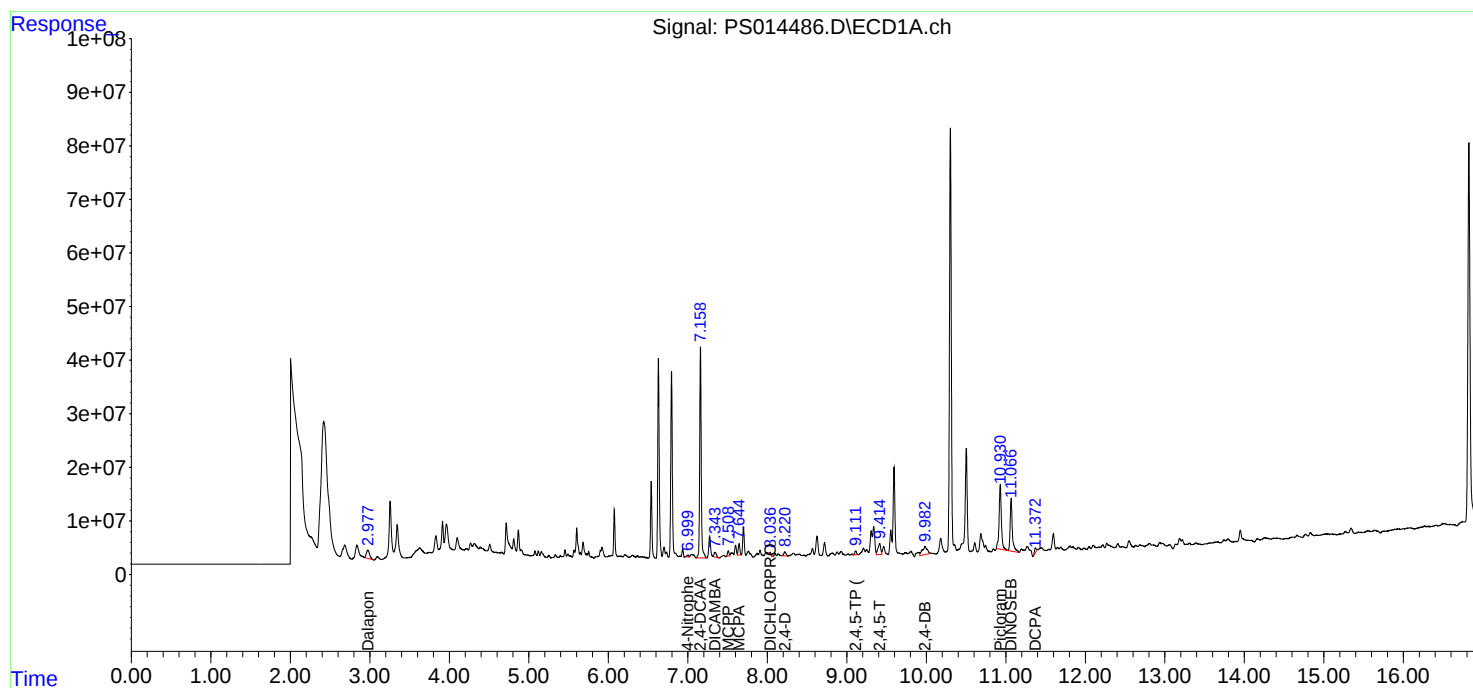


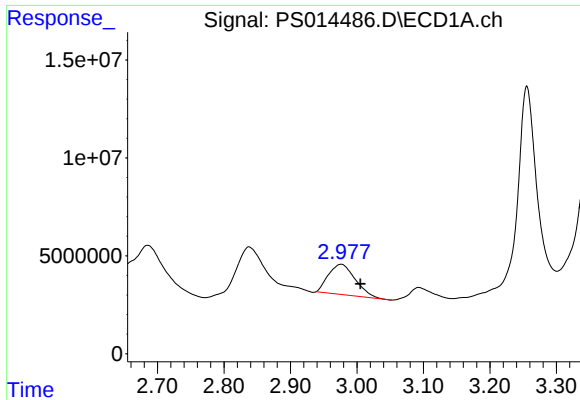

#1 Dalapon


R.T.: 2.976 min
Delta R.T.: -0.029 min
Response: 43331124
Conc: 27.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

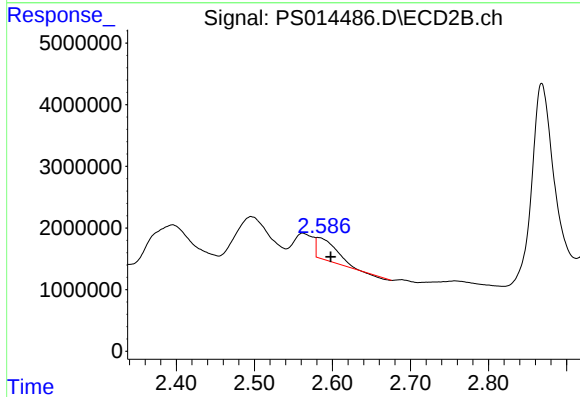


#1 Dalapon

R.T.: 2.581 min
Delta R.T.: -0.017 min
Response: 5981157
Conc: 10.10 ng/ml

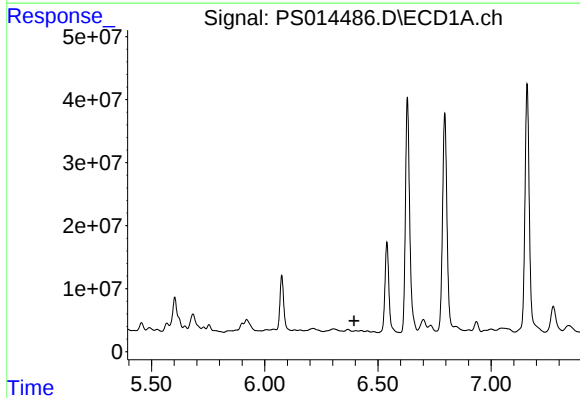


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

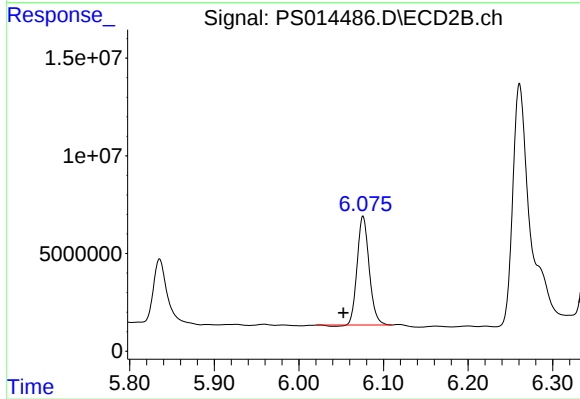

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.076 min
Delta R.T.: 0.023 min
Response: 54580327
Conc: 73.30 ng/ml

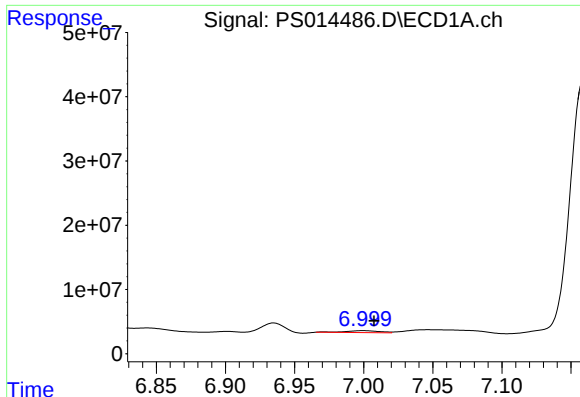

#3 4-Nitrophenol


R.T.: 7.000 min
Delta R.T.: -0.008 min
Response: 5296853
Conc: 7.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

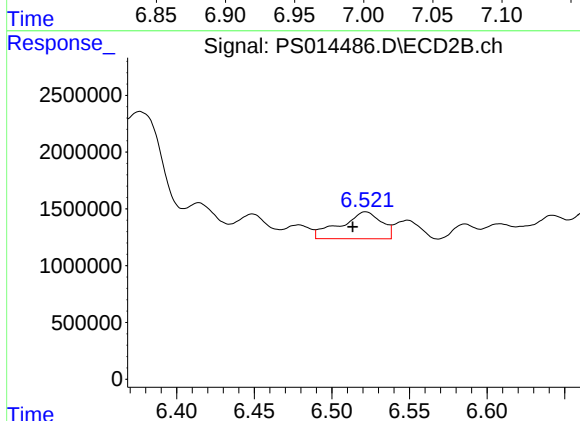


#3 4-Nitrophenol

R.T.: 6.522 min
Delta R.T.: 0.008 min
Response: 4362929
Conc: 14.36 ng/ml

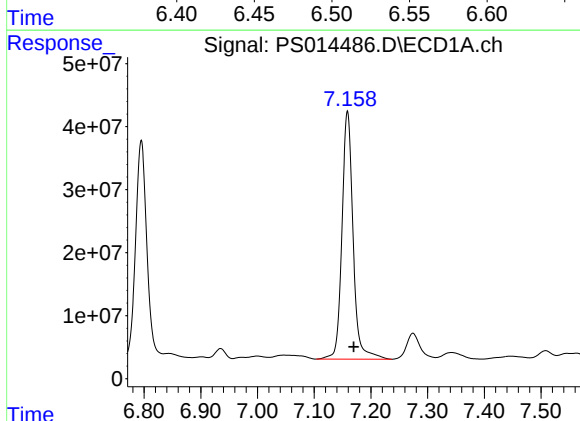


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: -0.011 min
Response: 537008057
Conc: 375.83 ng/ml

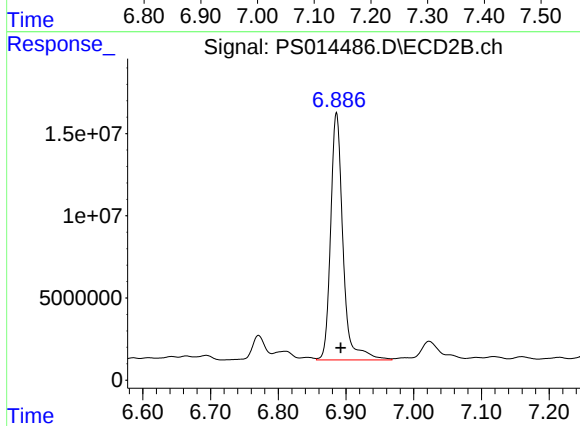

#4 2,4-DCAA


R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 190295876
Conc: 403.37 ng/ml

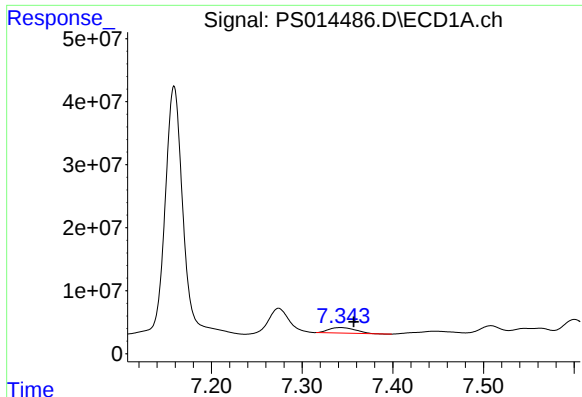

#5 DICAMBA


R.T.: 7.342 min
Delta R.T.: -0.015 min
Response: 17935813
Conc: 3.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

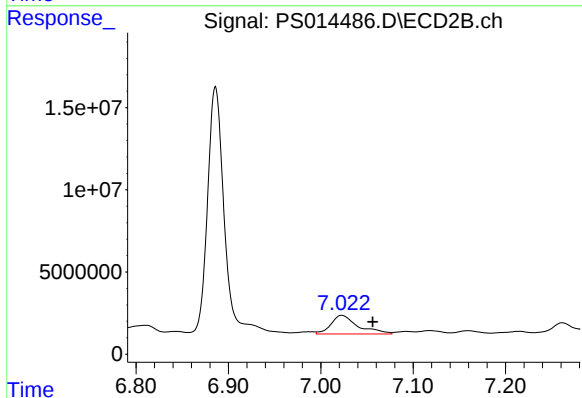


#5 DICAMBA

R.T.: 7.023 min
Delta R.T.: -0.033 min
Response: 23112038
Conc: 11.54 ng/ml

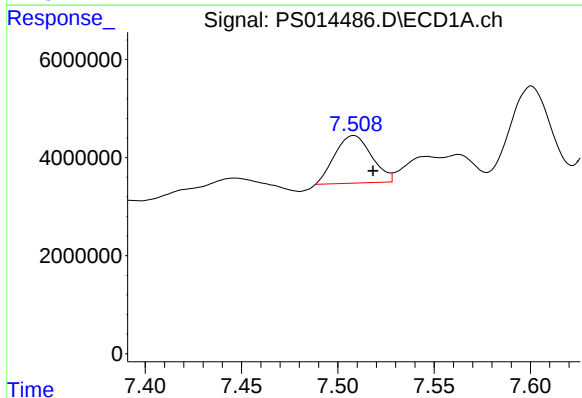


#6 MCP

R.T.: 7.508 min
Delta R.T.: -0.010 min
Response: 12899143
Conc: 3.10 ug/ml

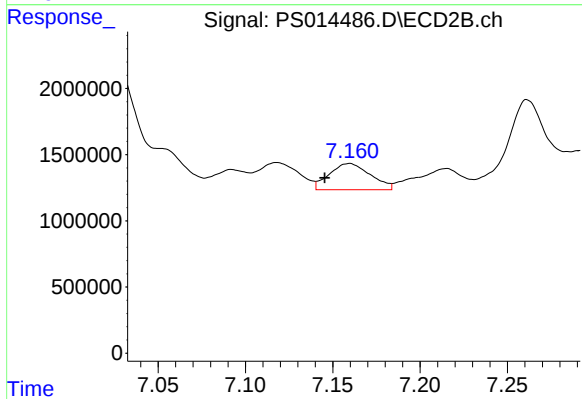

#6 MCP


R.T.: 7.160 min
Delta R.T.: 0.014 min
Response: 3249360
Conc: 1.95 ug/ml

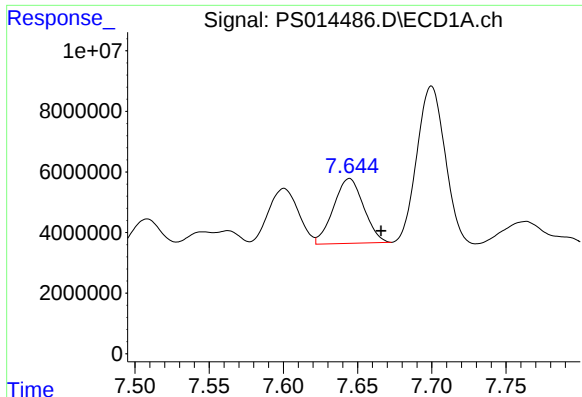

#7 MCPA


R.T.: 7.645 min
Delta R.T.: -0.021 min
Response: 30323320
Conc: 5.27 ug/ml

Instrument :
ECD_S
ClientSampleId :

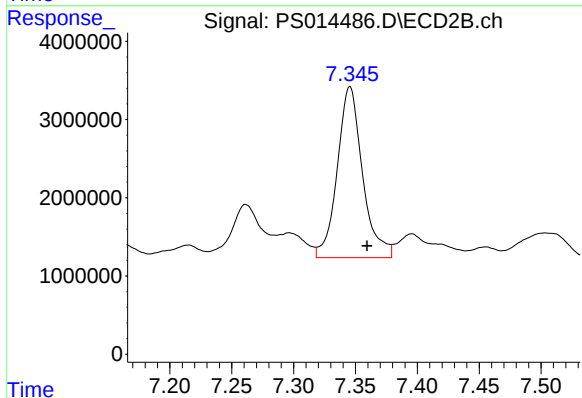


#7 MCPA

R.T.: 7.346 min
Delta R.T.: -0.014 min
Response: 31066504
Conc: 12.75 ug/ml

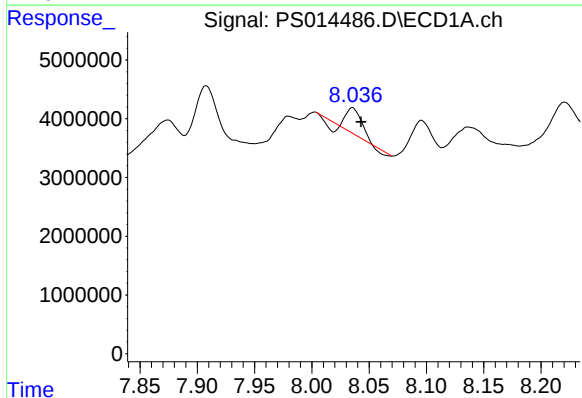


#8 DICHLORPROP

R.T.: 8.035 min
Delta R.T.: -0.008 min
Response: 2901075
Conc: 2.19 ng/ml

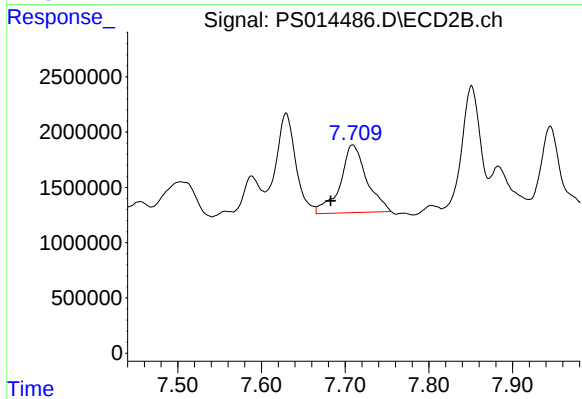

#8 DICHLORPROP


R.T.: 7.709 min
Delta R.T.: 0.026 min
Response: 13430282
Conc: 26.36 ng/ml

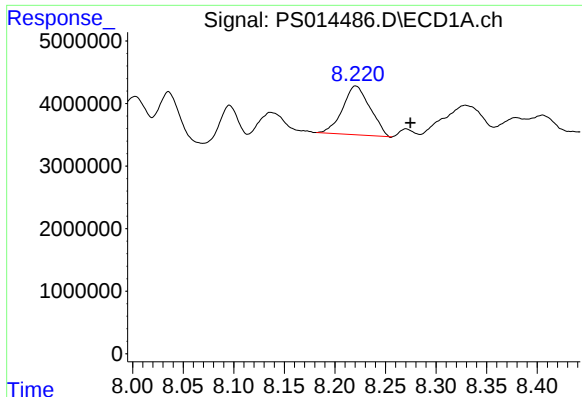

#9 2,4-D


R.T.: 8.221 min
Delta R.T.: -0.054 min
Response: 14672357
Conc: 9.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

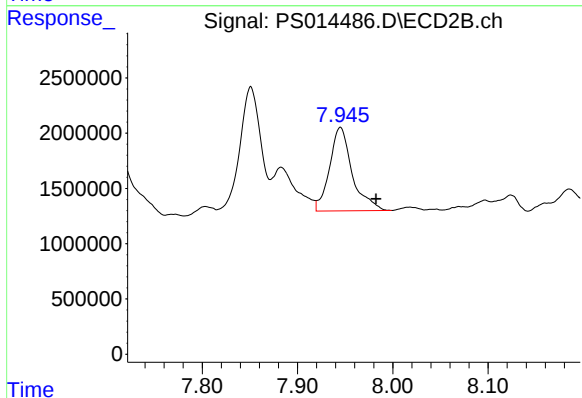


#9 2,4-D

R.T.: 7.945 min
Delta R.T.: -0.037 min
Response: 12514159
Conc: 20.96 ng/ml

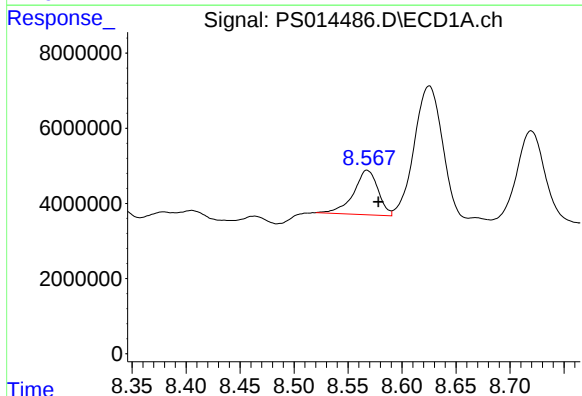


#10 Pentachlorophenol

R.T.: 8.568 min
Delta R.T.: -0.010 min
Response: 18689929
Conc: N.D.

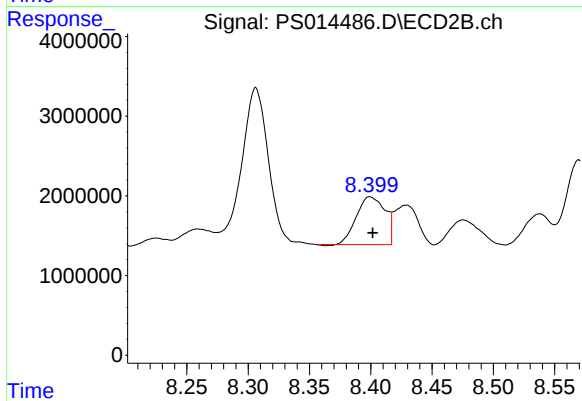

#10 Pentachlorophenol


R.T.: 8.399 min
Delta R.T.: -0.002 min
Response: 9770891
Conc: 1.43 ng/ml

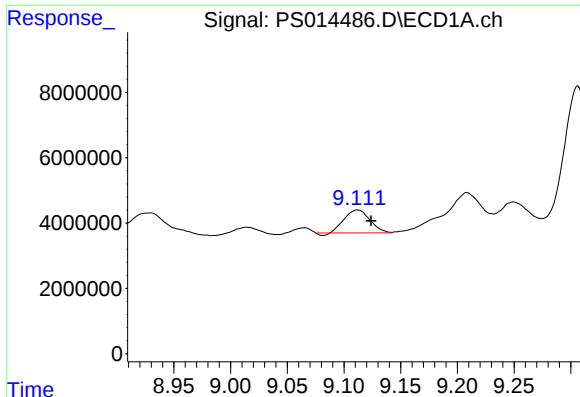

#11 2,4,5-TP (SILVEX)


R.T.: 9.112 min
Delta R.T.: -0.012 min
Response: 10831463
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

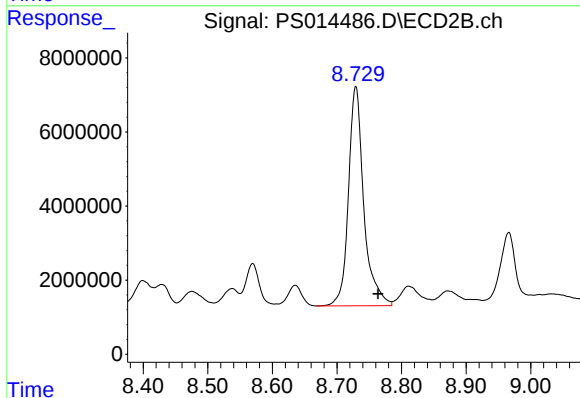


#11 2,4,5-TP (SILVEX)

R.T.: 8.729 min
Delta R.T.: -0.034 min
Response: 97617128
Conc: 35.88 ng/ml

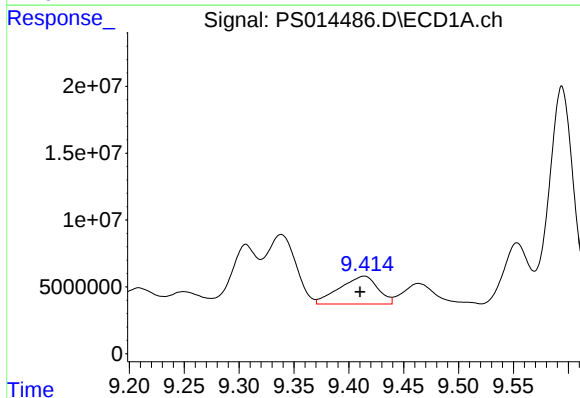


#12 2,4,5-T

R.T.: 9.414 min
Delta R.T.: 0.004 min
Response: 50434292
Conc: 6.48 ng/ml

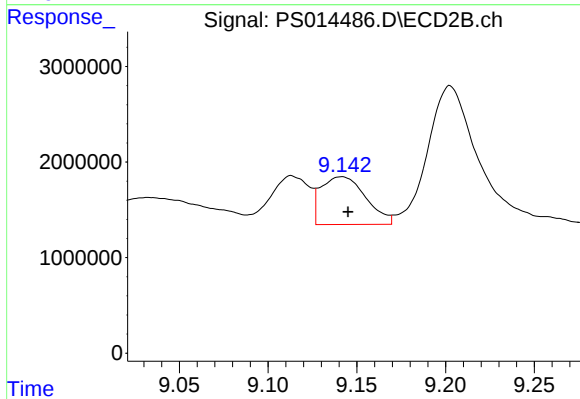

#12 2,4,5-T


R.T.: 9.141 min
Delta R.T.: -0.004 min
Response: 8742001
Conc: 3.28 ng/ml

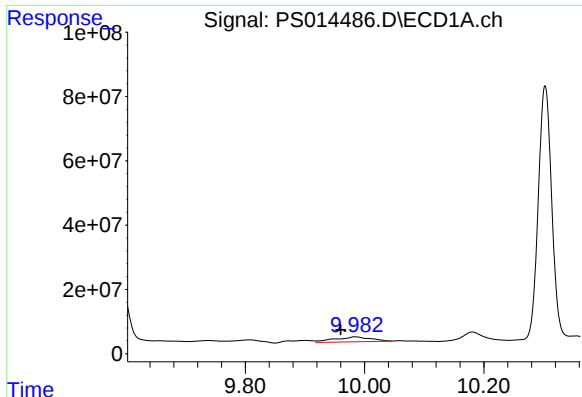

#13 2,4-DB


R.T.: 9.984 min
Delta R.T.: 0.024 min
Response: 65398770
Conc: 42.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

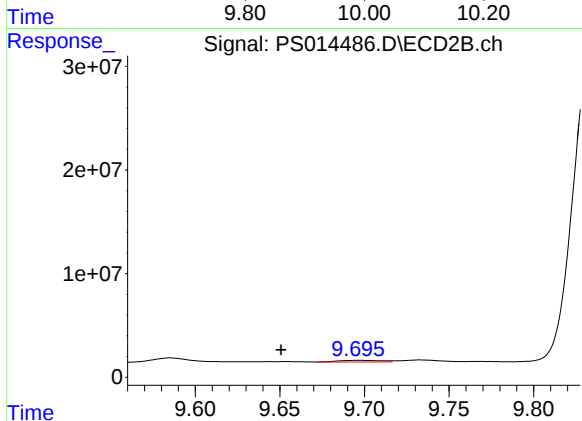


#13 2,4-DB

R.T.: 9.696 min
Delta R.T.: 0.045 min
Response: 2744672
Conc: 7.74 ng/ml

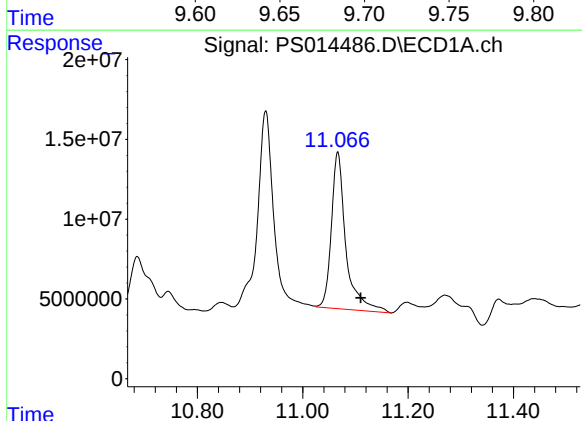


#14 DINOSEB

R.T.: 11.067 min
Delta R.T.: -0.044 min
Response: 187176047
Conc: 32.75 ng/ml

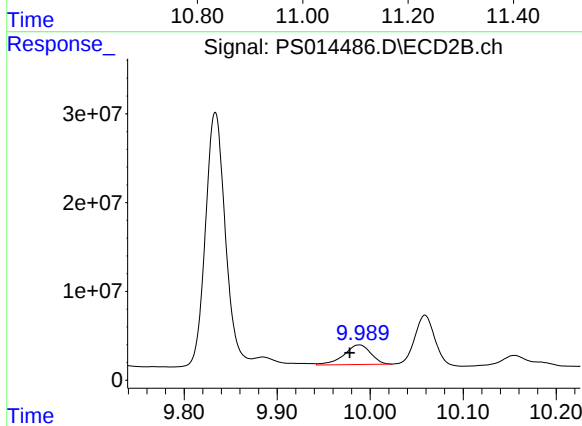

#14 DINOSEB


R.T.: 9.988 min
Delta R.T.: 0.010 min
Response: 44062589
Conc: 24.38 ng/ml

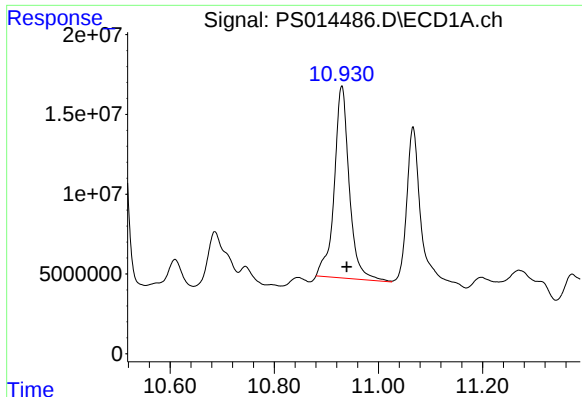

#15 Picloram


R.T.: 10.930 min
Delta R.T.: -0.010 min
Response: 241356424
Conc: 23.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

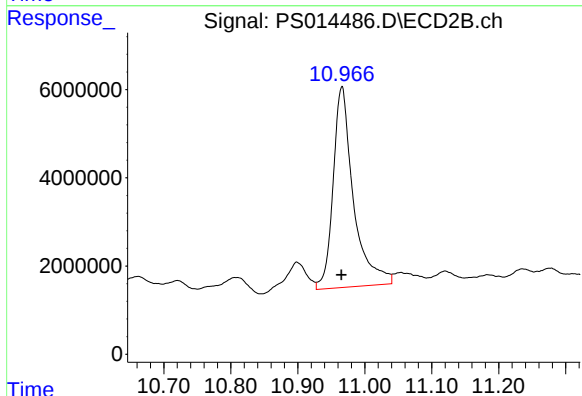


#15 Picloram

R.T.: 10.966 min
Delta R.T.: 0.001 min
Response: 95957330
Conc: 25.29 ng/ml

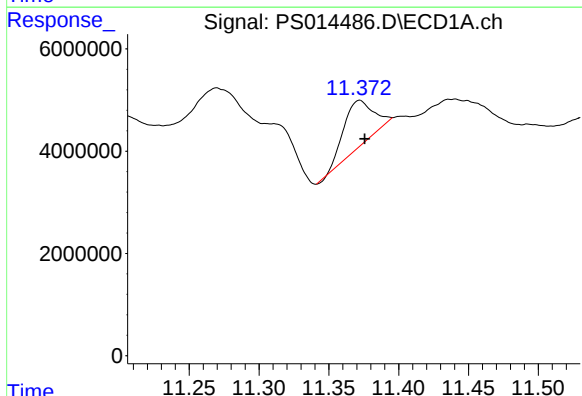

#16 DCPA

R.T.: 11.372 min
Delta R.T.: -0.004 min
Response: 12956630
Conc: 1.10 ng/ml

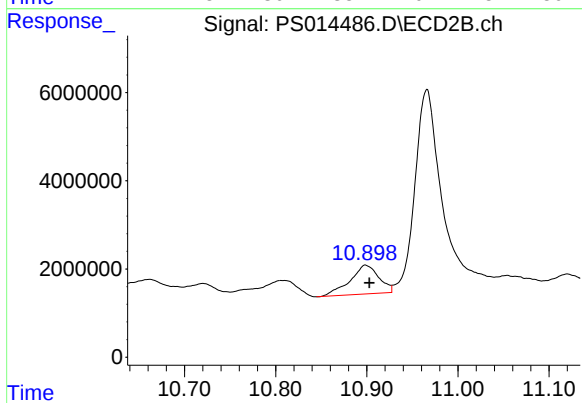

#16 DCPA

R.T.: 10.899 min
Delta R.T.: -0.005 min
Response: 14455500
Conc: 3.52 ng/ml