

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
 Data File : PS014491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 20:57
 Operator : DD\AJ
 Sample : M1932-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:12:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.885	712.4E6	251.0E6	498.585	531.964
Target Compounds							
1) T	Dalapon	2.977	2.562	45457706	419371	29.205	<MDL #
2) T	3,5-DICHL...	6.452f	6.076	6145409	78896007	3.183	105.962 #
3) T	4-Nitroph...	7.061f	6.522	30470798	8152488	40.802	26.838 #
5) T	DICAMBA	7.337	7.058	21439733	2477029	3.987	1.236 #
6) T	MCPD	7.514	7.128	24929623	4290029	5.996	2.576 #
7) T	MCPA	7.645	7.345	210.1E6	41388981	36.523	16.986 #
8) T	DICHLORPROP	7.982f	7.670	15118879	3177922	11.417	6.237 #
9) T	2,4-D	8.268	7.949	14079038	25972343	9.552	43.498 #
10) T	Pentachlo...	8.626f	8.406	56635833	6787704	2.845	<MDL #
11) T	2,4,5-TP ...	9.068f	8.728	7384307	98979888	<MDL	36.381 #
12) T	2,4,5-T	9.417	9.131	10302827	34946856	1.324	13.108 #
13) T	2,4-DB	10.010f	9.667	103.8E6	8547353	67.152	24.103 #
14) T	DINOSEB	11.066f	9.987	232.1E6	41373210	40.600	22.895 #
15) T	Picloram	10.945	10.983	19214432	7584336	1.840	1.999
16) T	DCPA	0.000	10.877	0	6264837	N.D.	1.527



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
Data File : PS014491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 20:57
Operator : DD\AJ
Sample : M1932-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:12:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

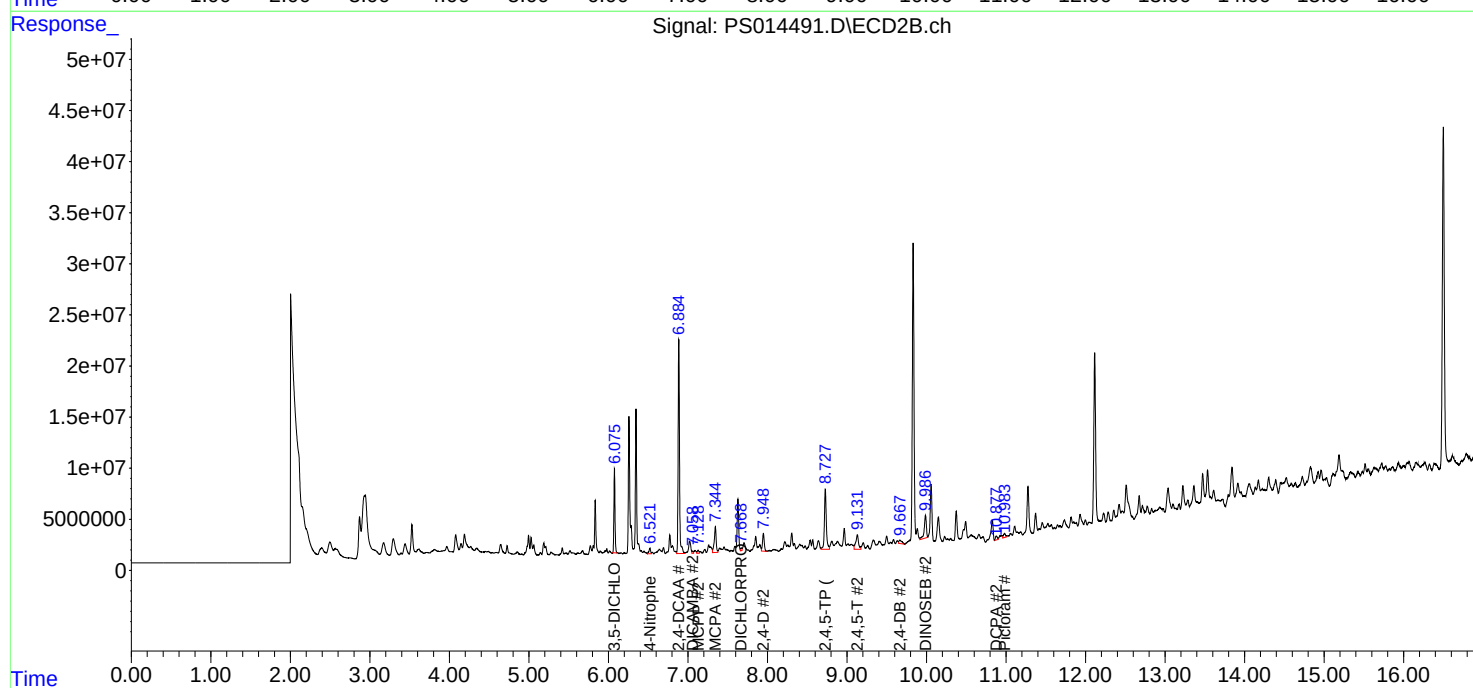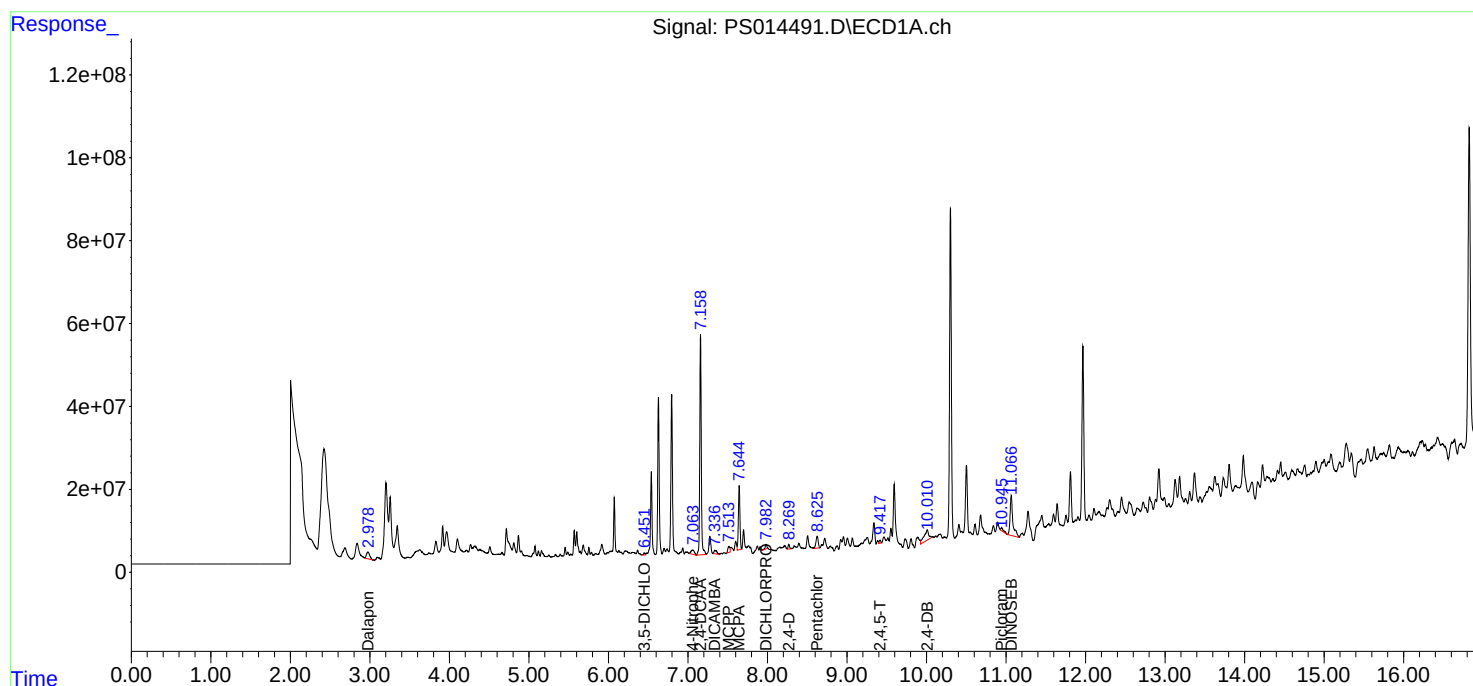


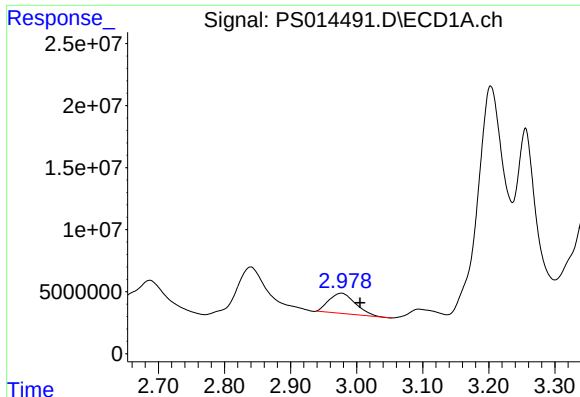

#1 Dalapon


R.T.: 2.977 min
Delta R.T.: -0.028 min
Response: 45457706
Conc: 29.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

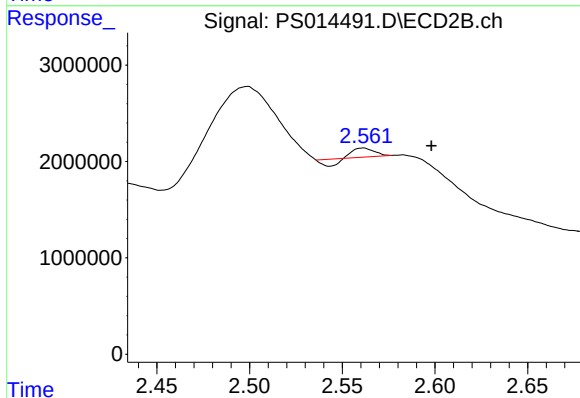


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: -0.036 min
Response: 419371
Conc: N.D.

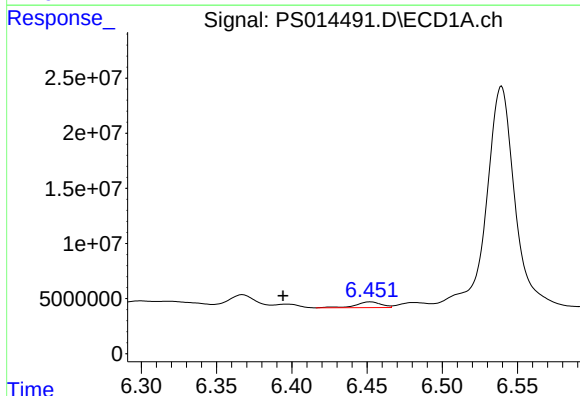


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.452 min
Delta R.T.: 0.058 min
Response: 6145409
Conc: 3.18 ng/ml

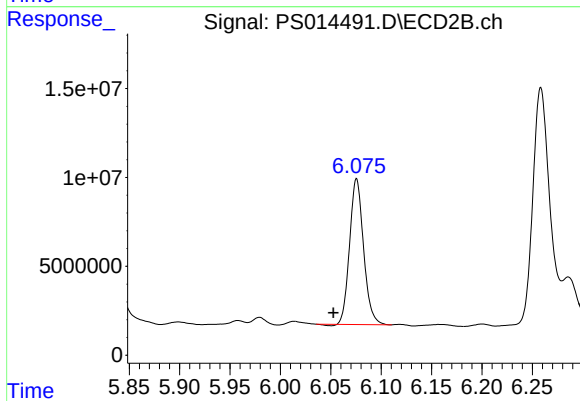

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.076 min
Delta R.T.: 0.023 min
Response: 78896007
Conc: 105.96 ng/ml

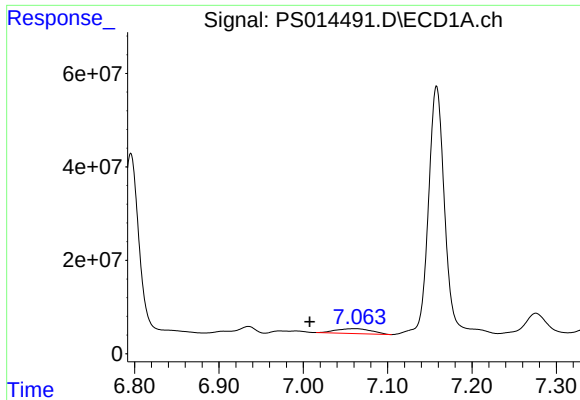

#3 4-Nitrophenol


R.T.: 7.061 min
Delta R.T.: 0.053 min
Response: 30470798
Conc: 40.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

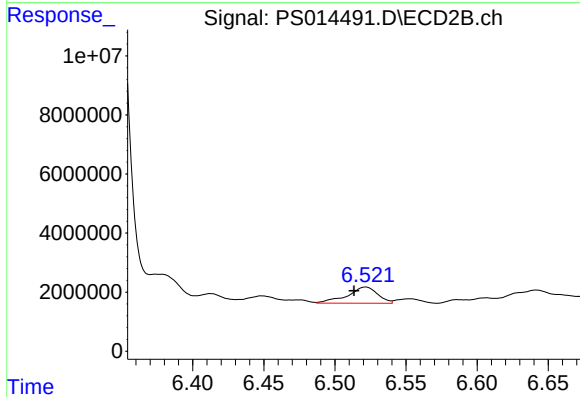


#3 4-Nitrophenol

R.T.: 6.522 min
Delta R.T.: 0.008 min
Response: 8152488
Conc: 26.84 ng/ml

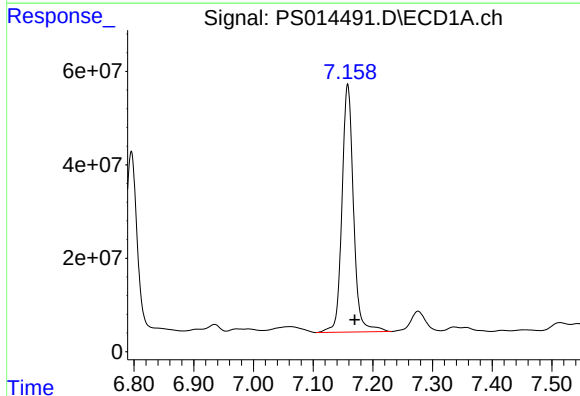


#4 2,4-DCAA

R.T.: 7.158 min
Delta R.T.: -0.012 min
Response: 712399794
Conc: 498.59 ng/ml

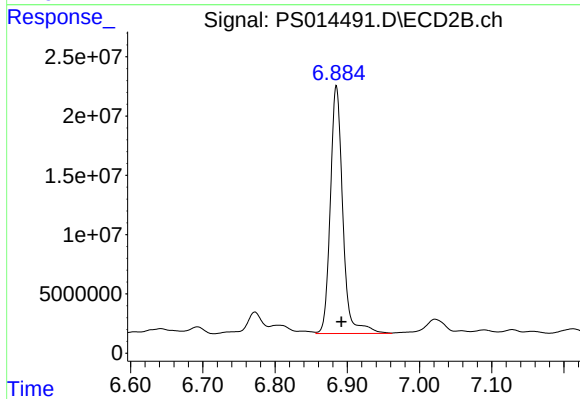

#4 2,4-DCAA


R.T.: 6.885 min
Delta R.T.: -0.007 min
Response: 250963942
Conc: 531.96 ng/ml

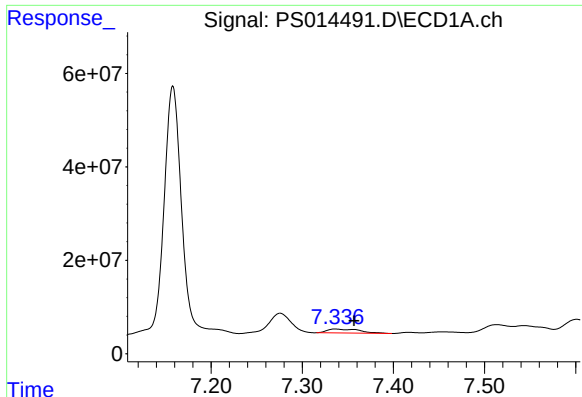

#5 DICAMBA


R.T.: 7.337 min
Delta R.T.: -0.021 min
Response: 21439733
Conc: 3.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

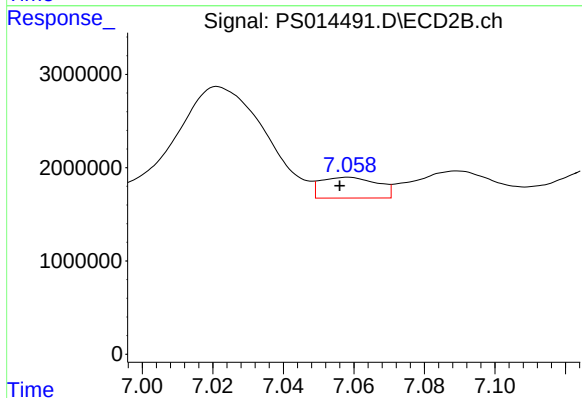


#5 DICAMBA

R.T.: 7.058 min
Delta R.T.: 0.002 min
Response: 2477029
Conc: 1.24 ng/ml

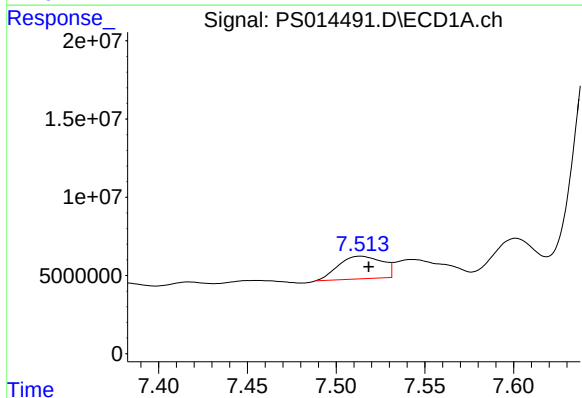


#6 MCP

R.T.: 7.514 min
Delta R.T.: -0.005 min
Response: 24929623
Conc: 6.00 ug/ml

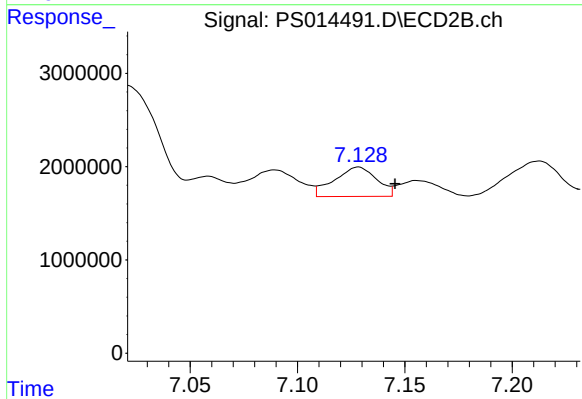

#6 MCP


R.T.: 7.128 min
Delta R.T.: -0.017 min
Response: 4290029
Conc: 2.58 ug/ml

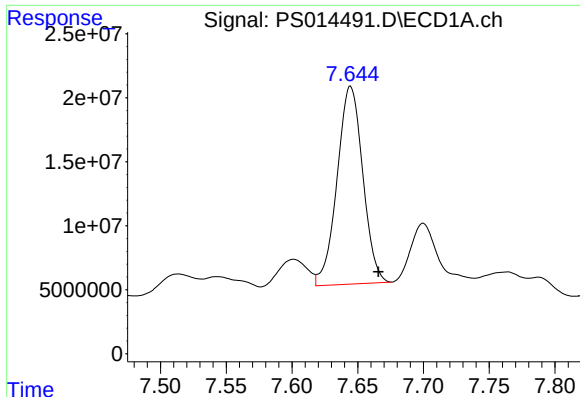

#7 MCPA


R.T.: 7.645 min
Delta R.T.: -0.021 min
Response: 210120370
Conc: 36.52 ug/ml

Instrument :
ECD_S
ClientSampleId :

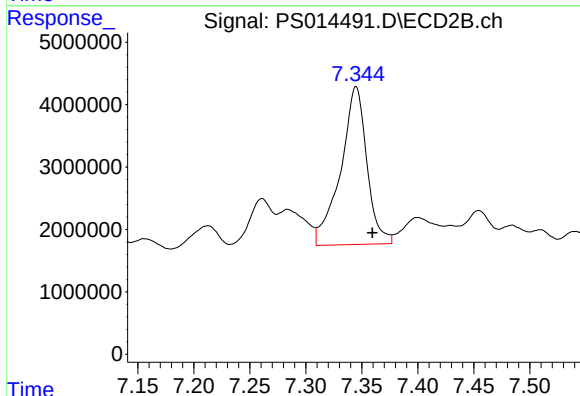


#7 MCPA

R.T.: 7.345 min
Delta R.T.: -0.014 min
Response: 41388981
Conc: 16.99 ug/ml

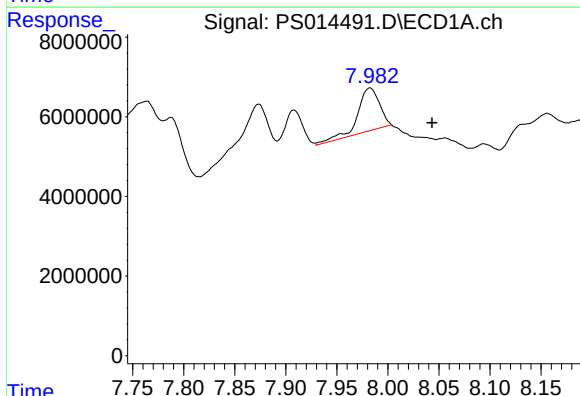


#8 DICHLORPROP

R.T.: 7.982 min
Delta R.T.: -0.061 min
Response: 15118879
Conc: 11.42 ng/ml

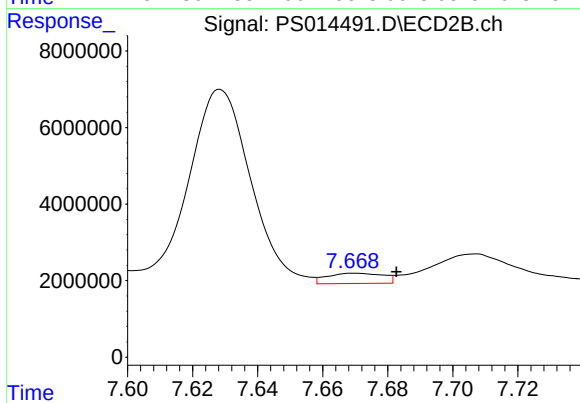

#8 DICHLORPROP


R.T.: 7.670 min
Delta R.T.: -0.013 min
Response: 3177922
Conc: 6.24 ng/ml

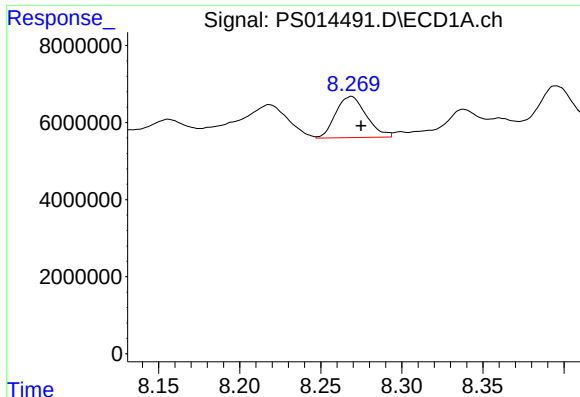

#9 2,4-D


R.T.: 8.268 min
Delta R.T.: -0.006 min
Response: 14079038
Conc: 9.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

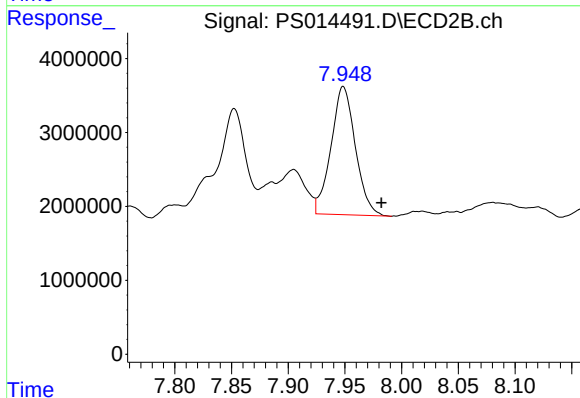


#9 2,4-D

R.T.: 7.949 min
Delta R.T.: -0.034 min
Response: 25972343
Conc: 43.50 ng/ml

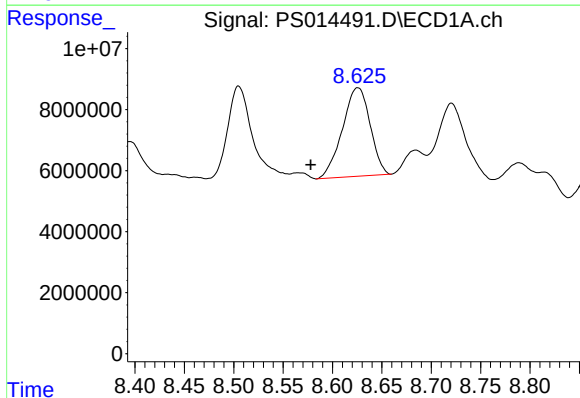


#10 Pentachlorophenol

R.T.: 8.626 min
Delta R.T.: 0.048 min
Response: 56635833
Conc: 2.85 ng/ml

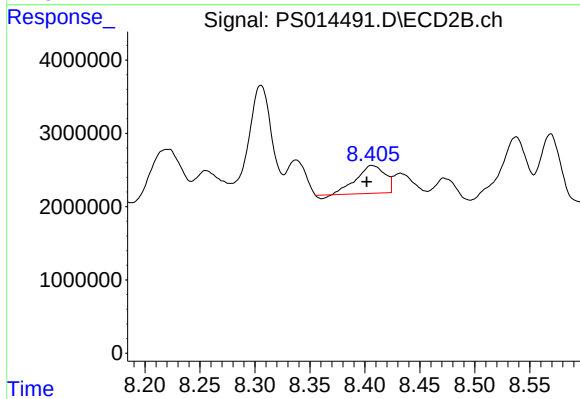

#10 Pentachlorophenol


R.T.: 8.406 min
Delta R.T.: 0.005 min
Response: 6787704
Conc: N.D.

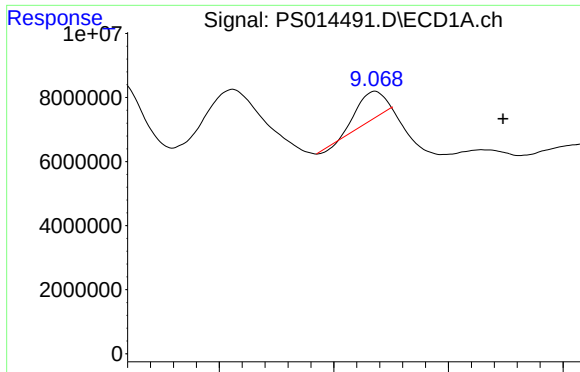

#11 2,4,5-TP (SILVEX)


R.T.: 9.068 min
Delta R.T.: -0.056 min
Response: 7384307
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

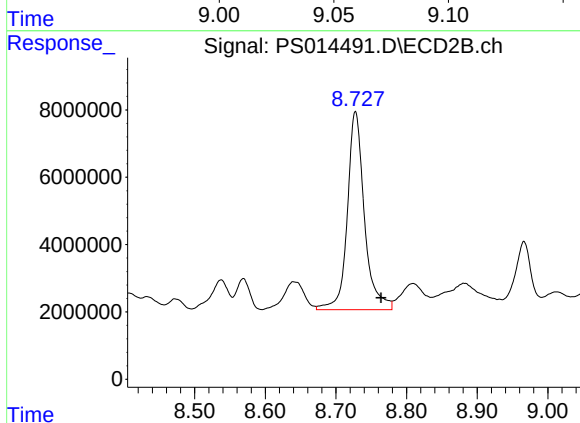


#11 2,4,5-TP (SILVEX)

R.T.: 8.728 min
Delta R.T.: -0.036 min
Response: 98979888
Conc: 36.38 ng/ml

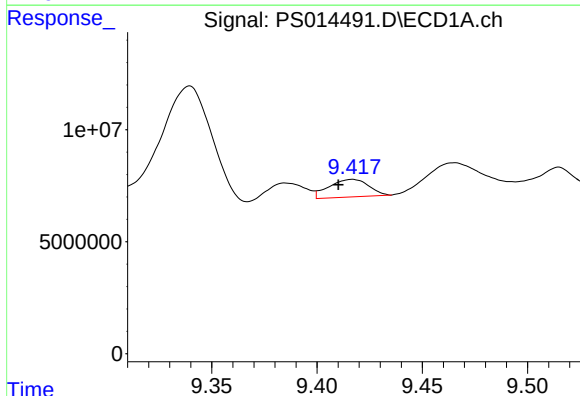


#12 2,4,5-T

R.T.: 9.417 min
Delta R.T.: 0.006 min
Response: 10302827
Conc: 1.32 ng/ml

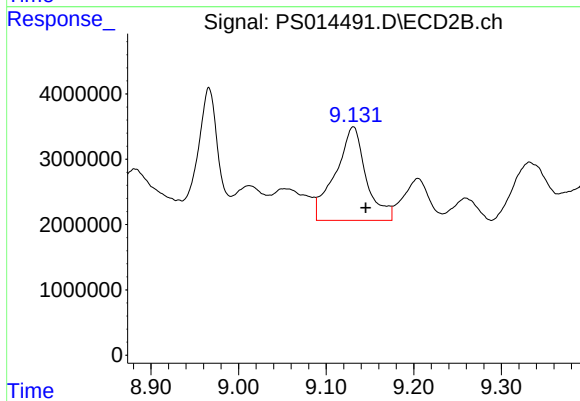

#12 2,4,5-T


R.T.: 9.131 min
Delta R.T.: -0.014 min
Response: 34946856
Conc: 13.11 ng/ml

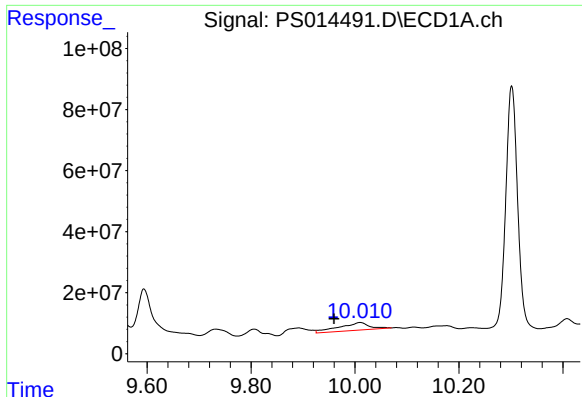

#13 2,4-DB


R.T.: 10.010 min
Delta R.T.: 0.050 min
Response: 103843445
Conc: 67.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

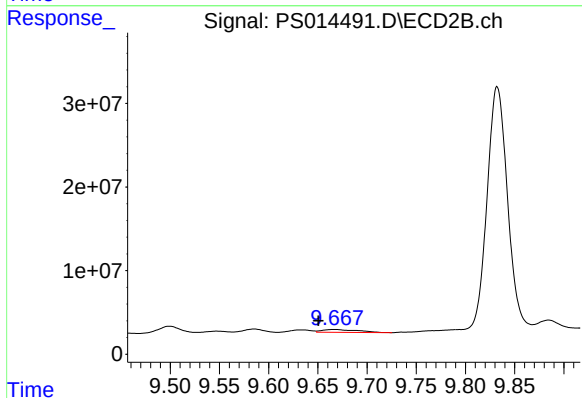


#13 2,4-DB

R.T.: 9.667 min
Delta R.T.: 0.016 min
Response: 8547353
Conc: 24.10 ng/ml

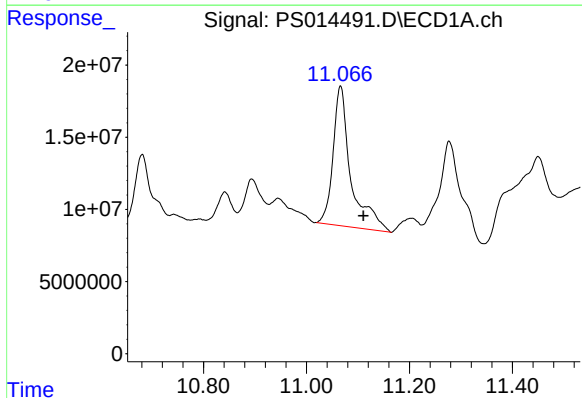


#14 DINOSEB

R.T.: 11.066 min
Delta R.T.: -0.044 min
Response: 232060178
Conc: 40.60 ng/ml

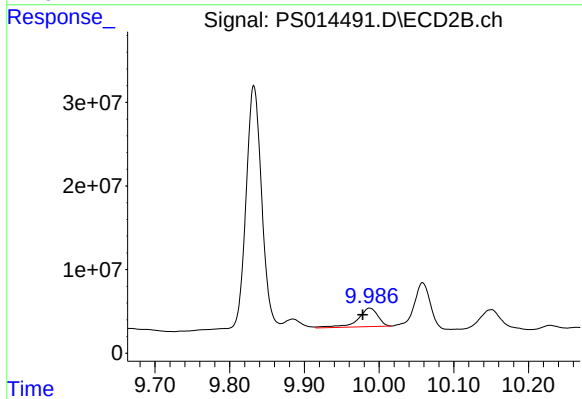

#14 DINOSEB


R.T.: 9.987 min
Delta R.T.: 0.009 min
Response: 41373210
Conc: 22.90 ng/ml

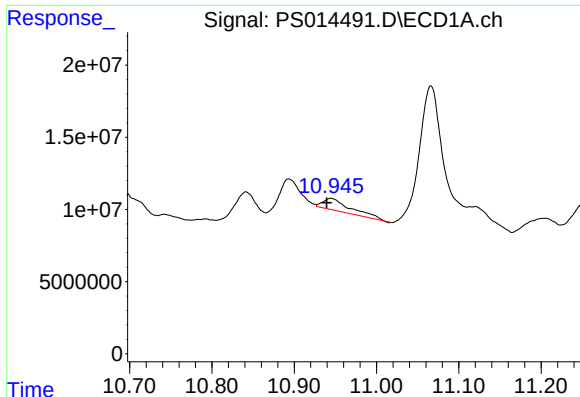

#15 Picloram


R.T.: 10.945 min
Delta R.T.: 0.006 min
Response: 19214432
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

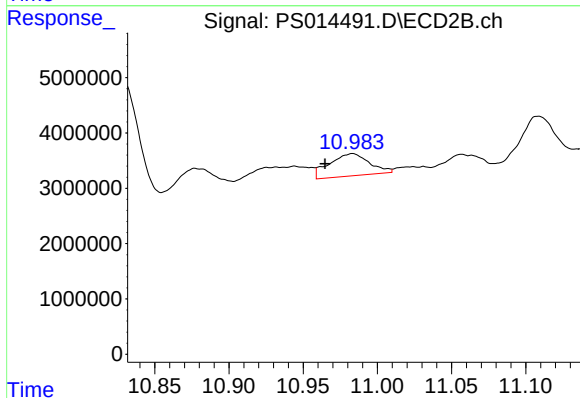


#15 Picloram

R.T.: 10.983 min
Delta R.T.: 0.019 min
Response: 7584336
Conc: 2.00 ng/ml

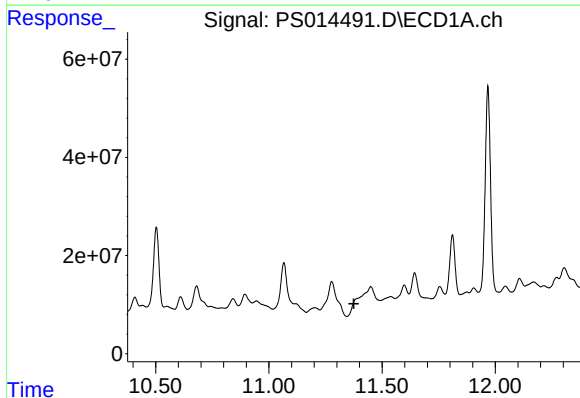

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.376 min
Response: 0
Conc: N.D.

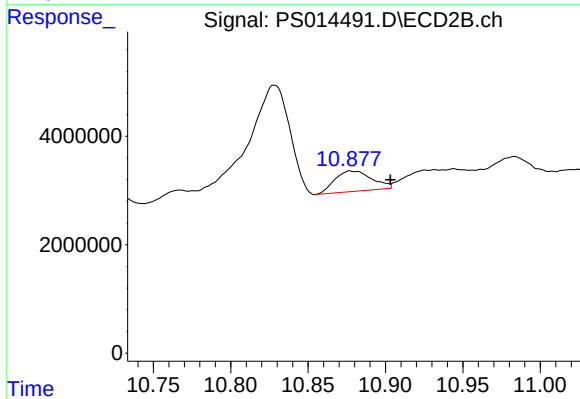

#16 DCPA

R.T.: 10.877 min
Delta R.T.: -0.026 min
Response: 6264837
Conc: 1.53 ng/ml