

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
 Data File : PS014494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 22:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:13:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.887	739.0E6	267.4E6	517.222	566.892
Target Compounds							
7) T	MCPA	7.627	7.290f	5624551	2869540	<MDL	1.178 #
9) T	2,4-D	8.333f	0.000	651177	0	<MDL	N.D. #
13) T	2,4-DB	9.896f	0.000	1447646	0	<MDL	N.D. #
14) T	DINOSEB	11.079	0.000	15083754	0	2.639	N.D. #
15) T	Picloram	10.952	10.979	11575647	589652	1.109	<MDL #
16) T	DCPA	0.000	10.909	0	1582020	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
Data File : PS014494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 22:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:13:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

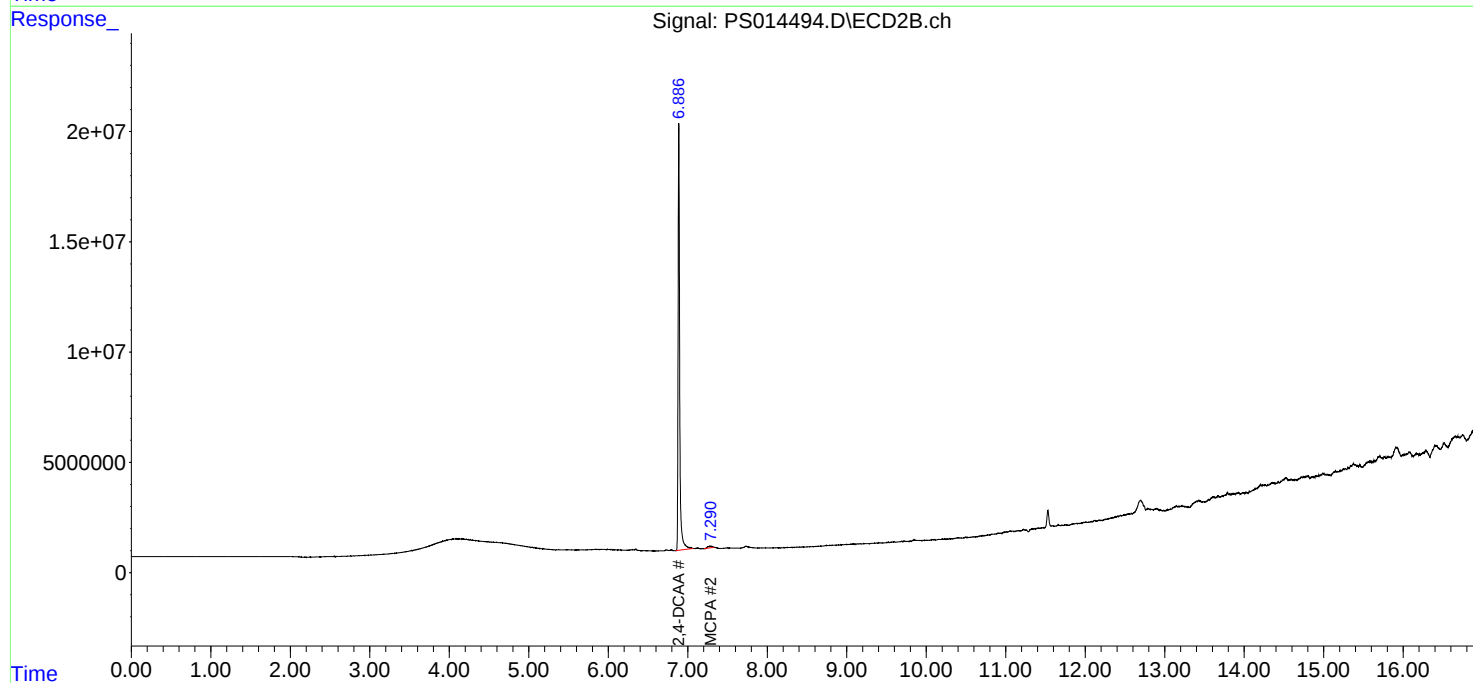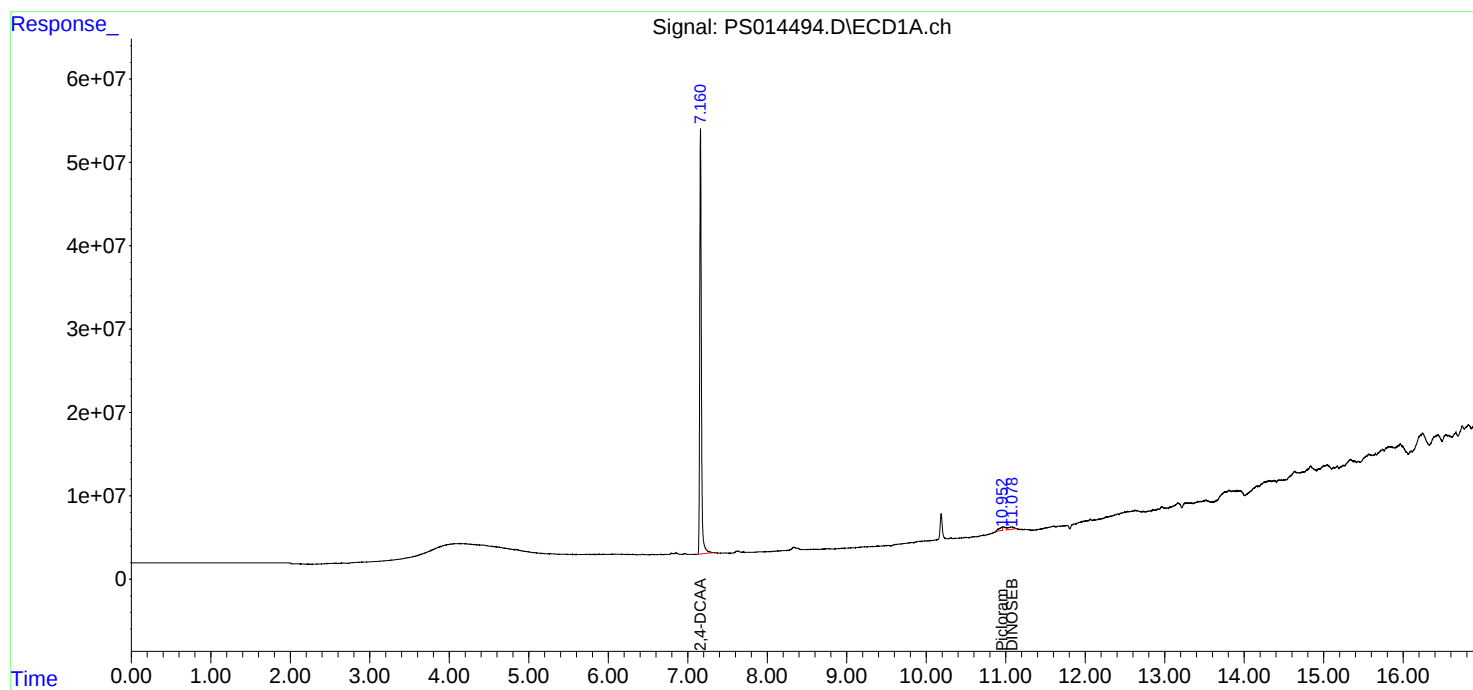


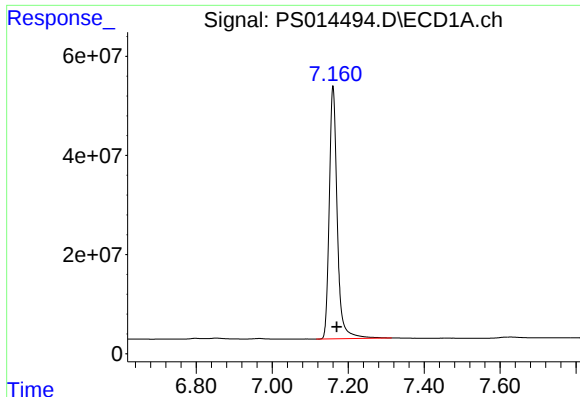

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: -0.010 min
Response: 739028460
Conc: 517.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

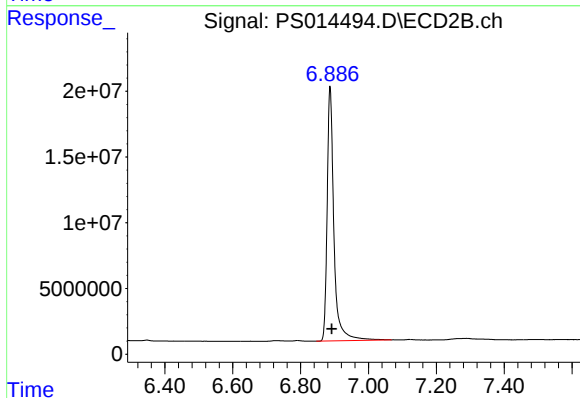


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: -0.005 min
Response: 267441778
Conc: 566.89 ng/ml

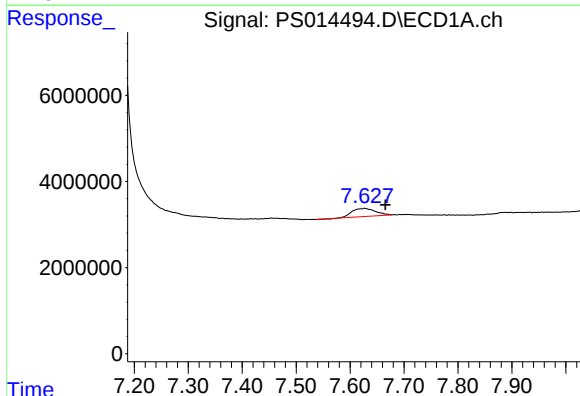


#7 MCPA

R.T.: 7.627 min
Delta R.T.: -0.039 min
Response: 5624551
Conc: N.D.

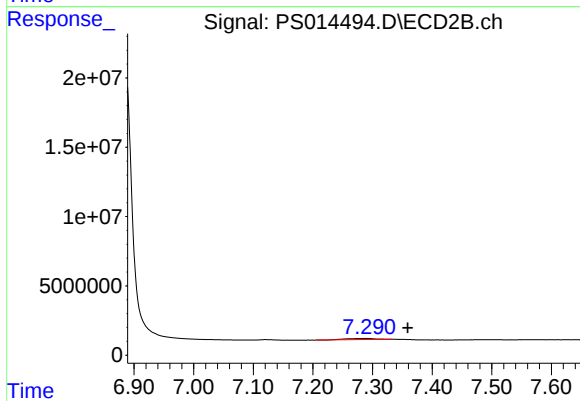

#7 MCPA


R.T.: 7.290 min
Delta R.T.: -0.069 min
Response: 2869540
Conc: 1.18 ug/ml

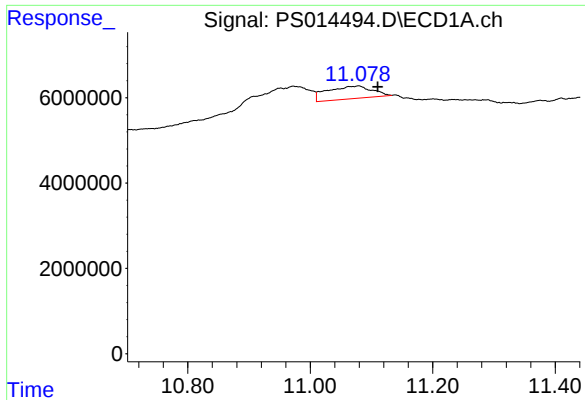

#14 DINOSEB


R.T.: 11.079 min
Delta R.T.: -0.031 min
Response: 15083754
Conc: 2.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

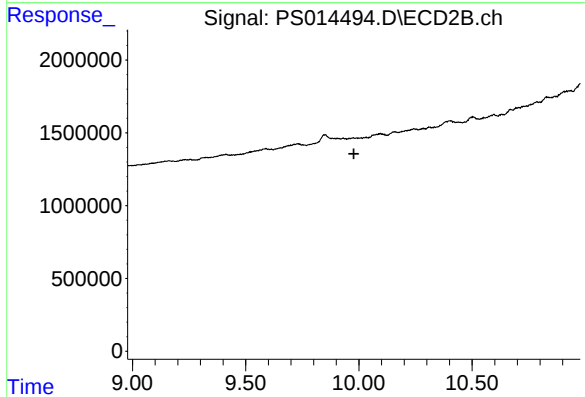


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.978 min
Response: 0
Conc: N.D.

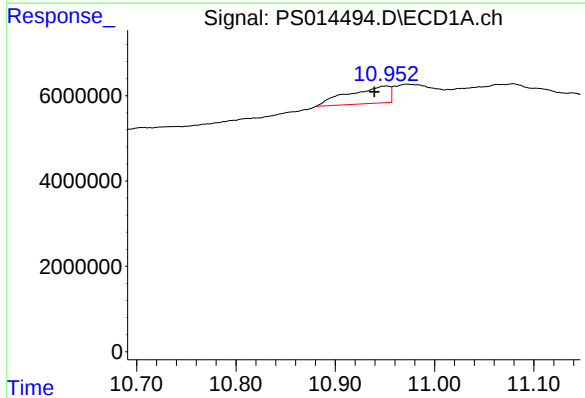

#15 Picloram

R.T.: 10.952 min
Delta R.T.: 0.013 min
Response: 11575647
Conc: 1.11 ng/ml

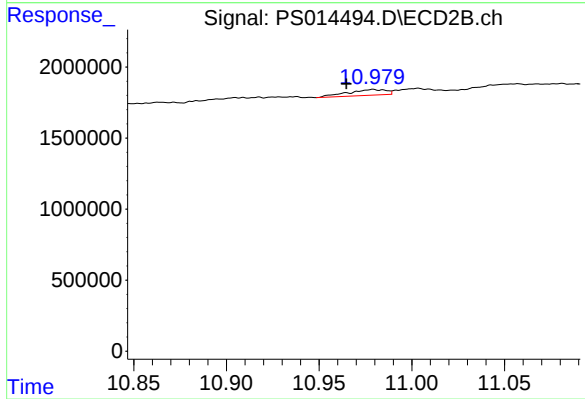

#15 Picloram

R.T.: 10.979 min
Delta R.T.: 0.014 min
Response: 589652
Conc: N.D.