

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
 Data File : PS014500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 00:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.886	740.7E6	267.2E6	518.394	566.286
Target Compounds							
2) T	3,5-DICHL...	6.429	0.000	5639709	0	2.921	N.D. #
5) T	DICAMBA	0.000	7.054	0	1558851	N.D.	<MDL
6) T	MCP	0.000	7.121	0	2252370	N.D.	1.353
7) T	MCPA	7.623f	0.000	6234722	0	1.084	N.D. #
8) T	DICHLORPROP	0.000	7.732f	0	1335053	N.D.	2.620
9) T	2,4-D	8.342f	0.000	18915162	0	12.833	N.D. #
10) T	Pentachlo...	8.571	8.399	8001946	2770857	<MDL	<MDL #
11) T	2,4,5-TP ...	9.118	8.762	4067637	1756451	<MDL	<MDL #
12) T	2,4,5-T	9.414	0.000	4085256	0	<MDL	N.D. #
15) T	Picloram	10.949	10.987	8512714	3164400	<MDL	<MDL #
16) T	DCPA	11.365	10.900	5784966	2254328	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040621\
Data File : PS014500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 00:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:15:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

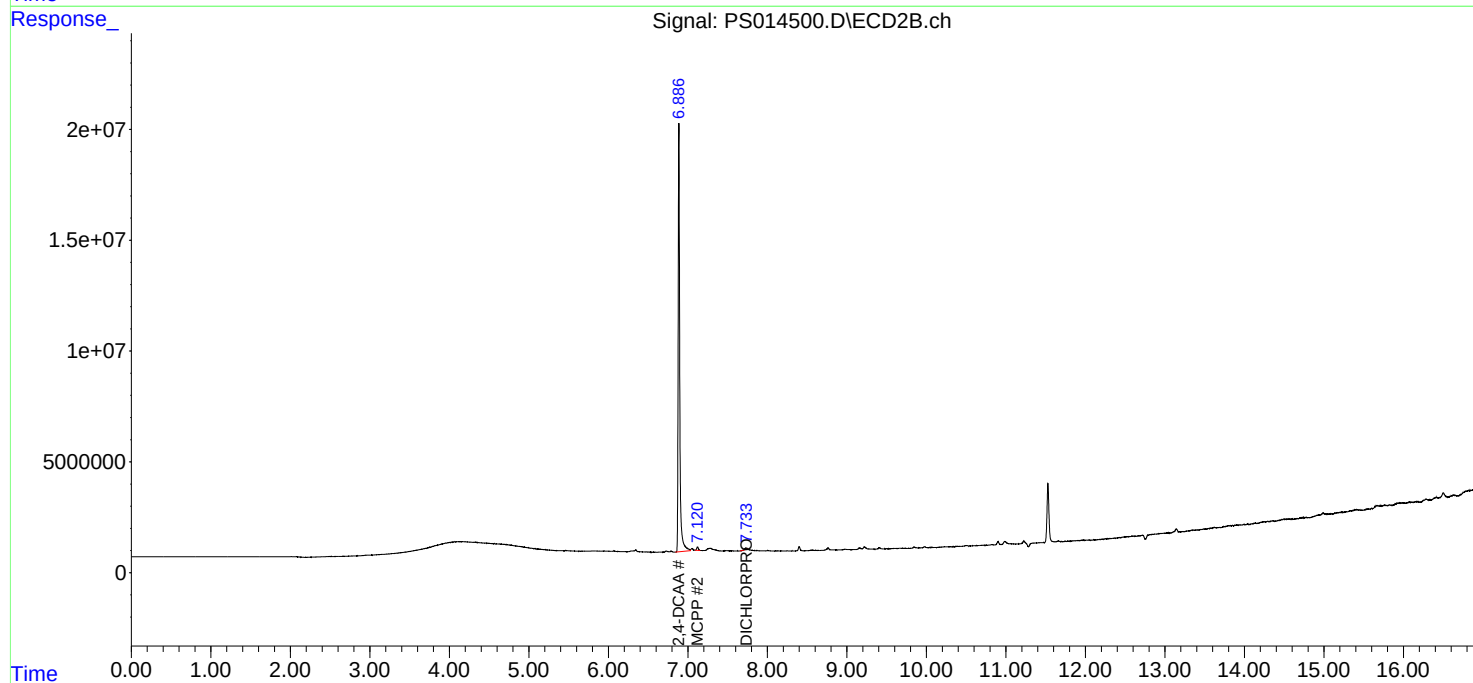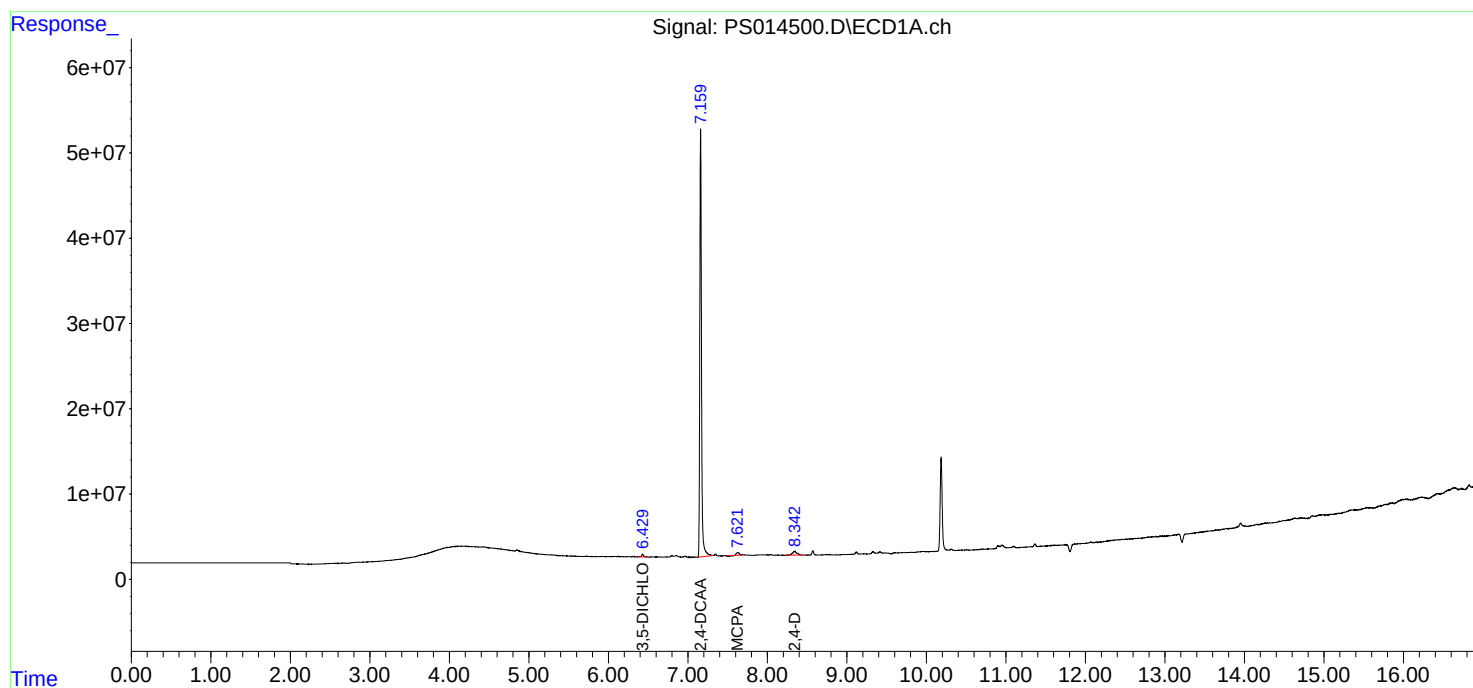


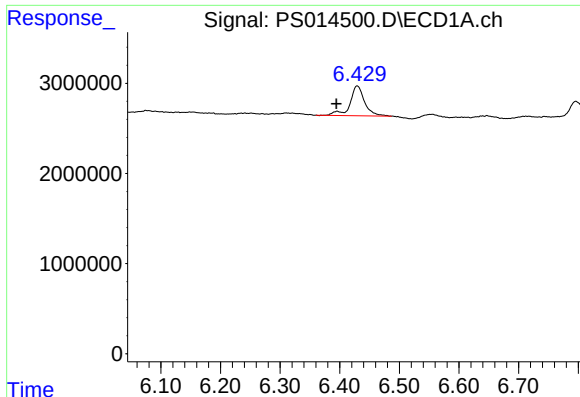

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.429 min
Delta R.T.: 0.035 min
Response: 5639709
Conc: 2.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

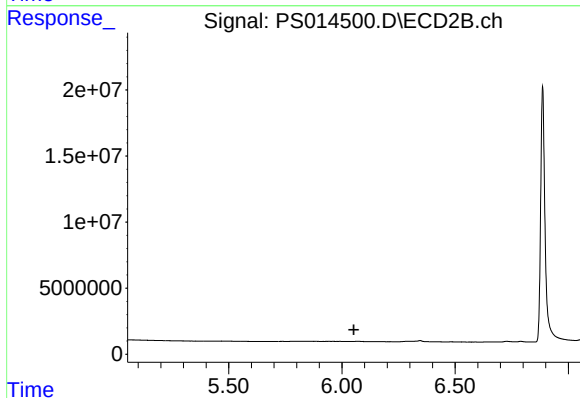


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

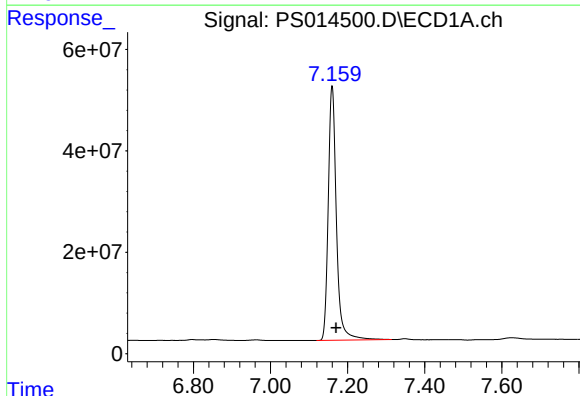


#4 2,4-DCAA

R.T.: 7.160 min
Delta R.T.: -0.010 min
Response: 740703085
Conc: 518.39 ng/ml

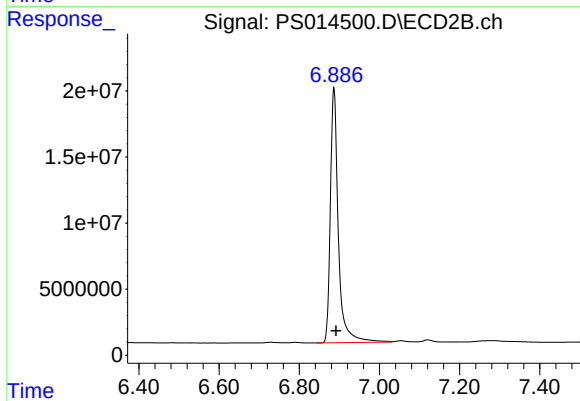

#4 2,4-DCAA


R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 267156117
Conc: 566.29 ng/ml

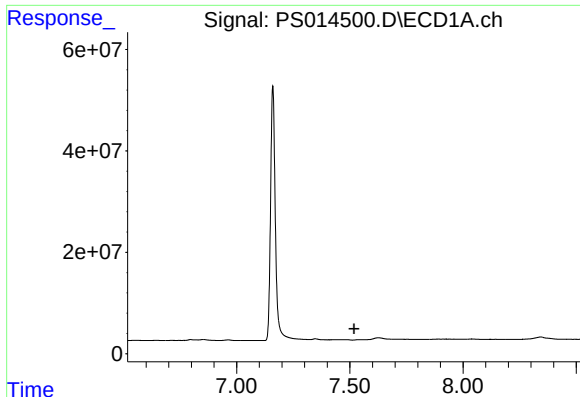

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

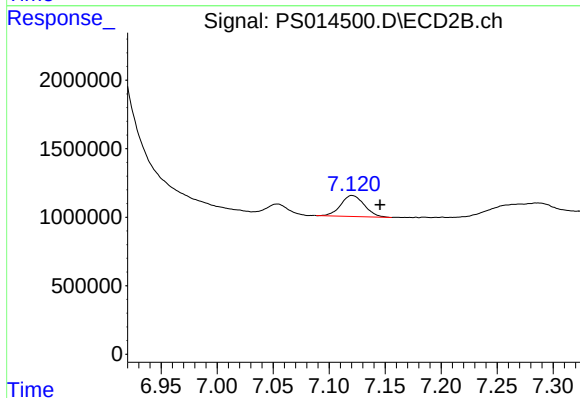


#6 MCPP

R.T.: 7.121 min
Delta R.T.: -0.025 min
Response: 2252370
Conc: 1.35 ug/ml

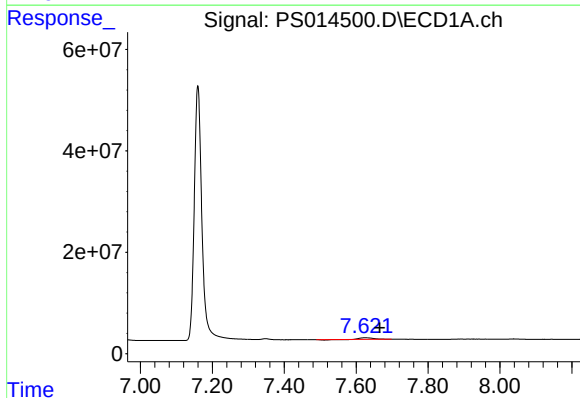


#7 MCPA

R.T.: 7.623 min
Delta R.T.: -0.043 min
Response: 6234722
Conc: 1.08 ug/ml

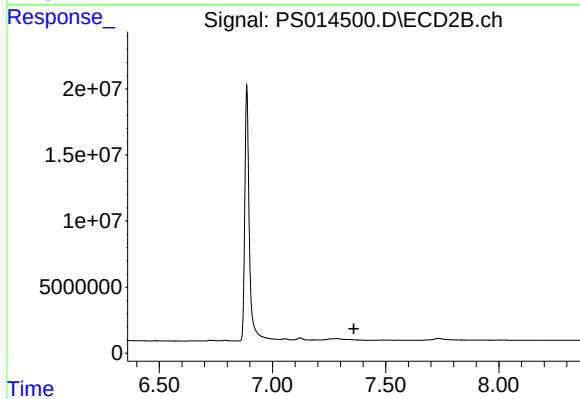

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.359 min
Response: 0
Conc: N.D.

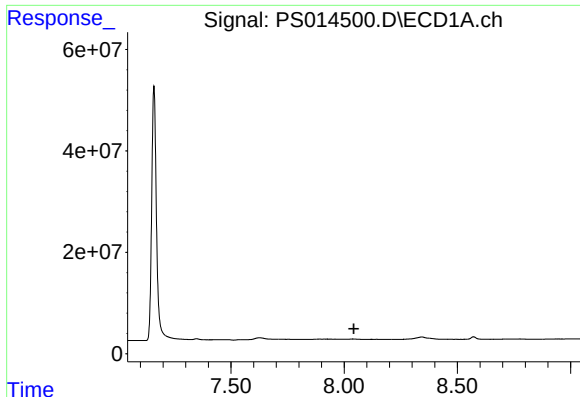

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

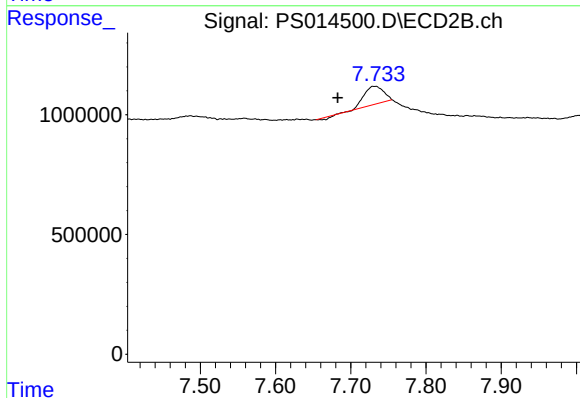


#8 DICHLORPROP

R.T.: 7.732 min
Delta R.T.: 0.050 min
Response: 1335053
Conc: 2.62 ng/ml

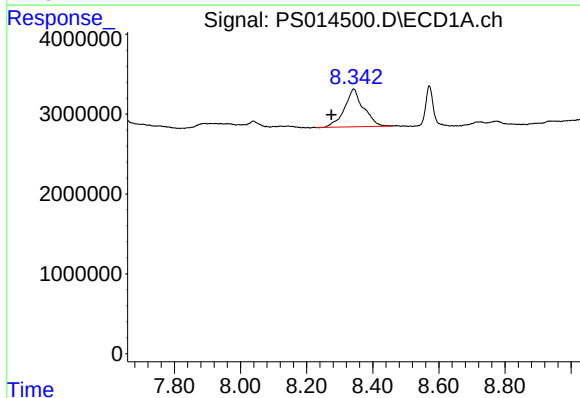

#9 2,4-D

R.T.: 8.342 min
Delta R.T.: 0.067 min
Response: 18915162
Conc: 12.83 ng/ml

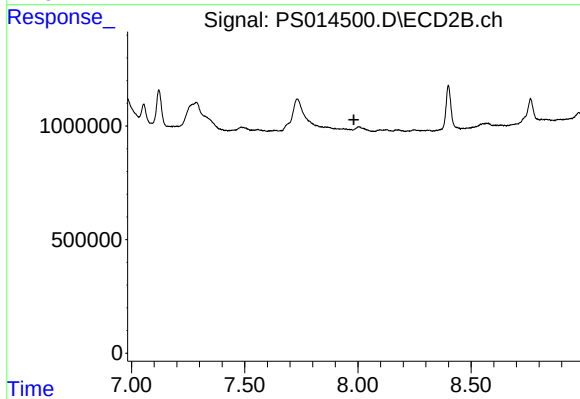

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.