

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040622\
 Data File : PS018910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2022 08:40
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 23:59:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	7.020f	0.000	8332255	0	7.299 N.D. #
5) T	DICAMBA	0.000	7.037f	0	29720870	N.D. 9.336
6) T	MCP	0.000	7.037	0	29720870	N.D. 11.617
8) T	DICHLORPROP	0.000	7.646f	0	3446341	N.D. 4.191
11) T	2,4,5-TP ...	0.000	8.648	0	6698832	N.D. 1.465
12) T	2,4,5-T	9.520	0.000	9791565	0	<MDL N.D. #
13) T	2,4-DB	0.000	9.499f	0	16891001	N.D. 29.655
15) T	Picloram	11.004	10.909	307.8E6	19817426	11.002 3.505 #
16) T	DCPA	11.476	0.000	4538927	0	<MDL N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040622\
Data File : PS018910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2022 08:40
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 23:59:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

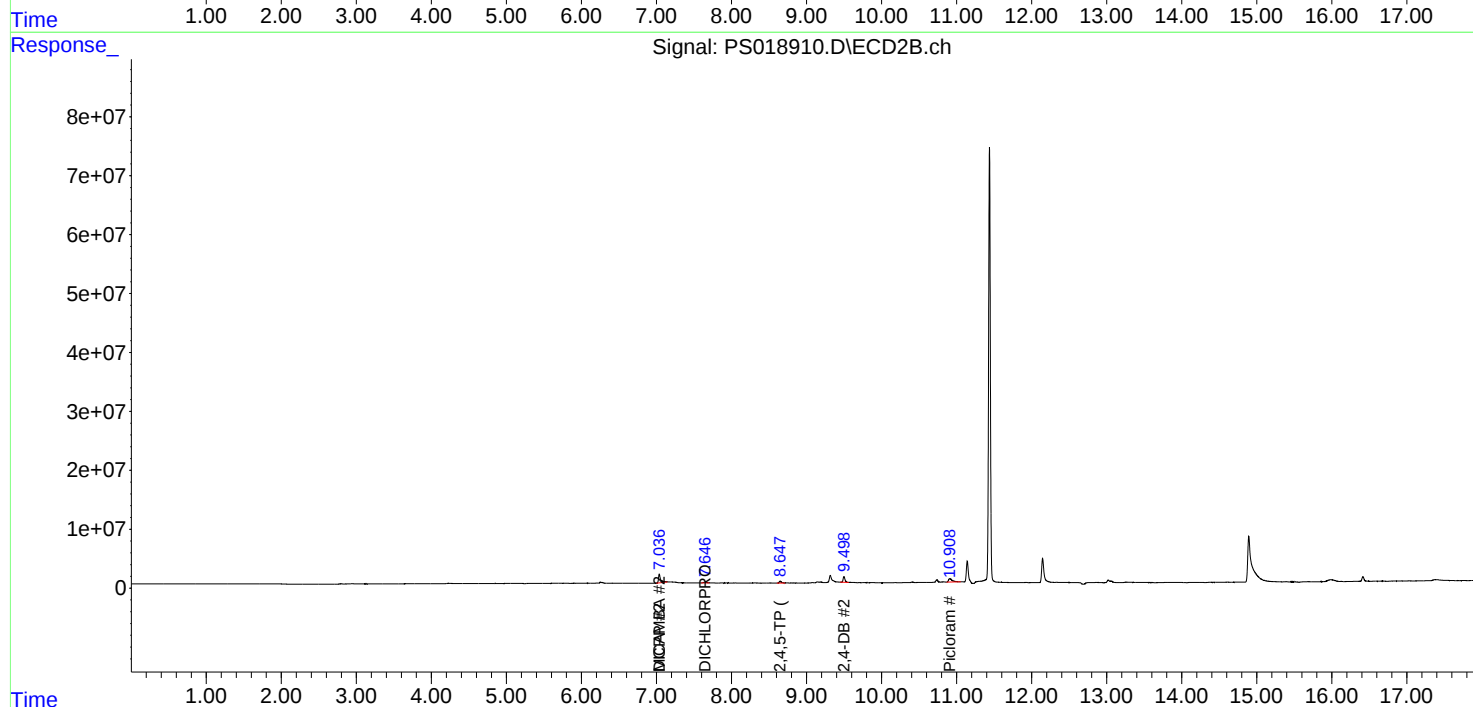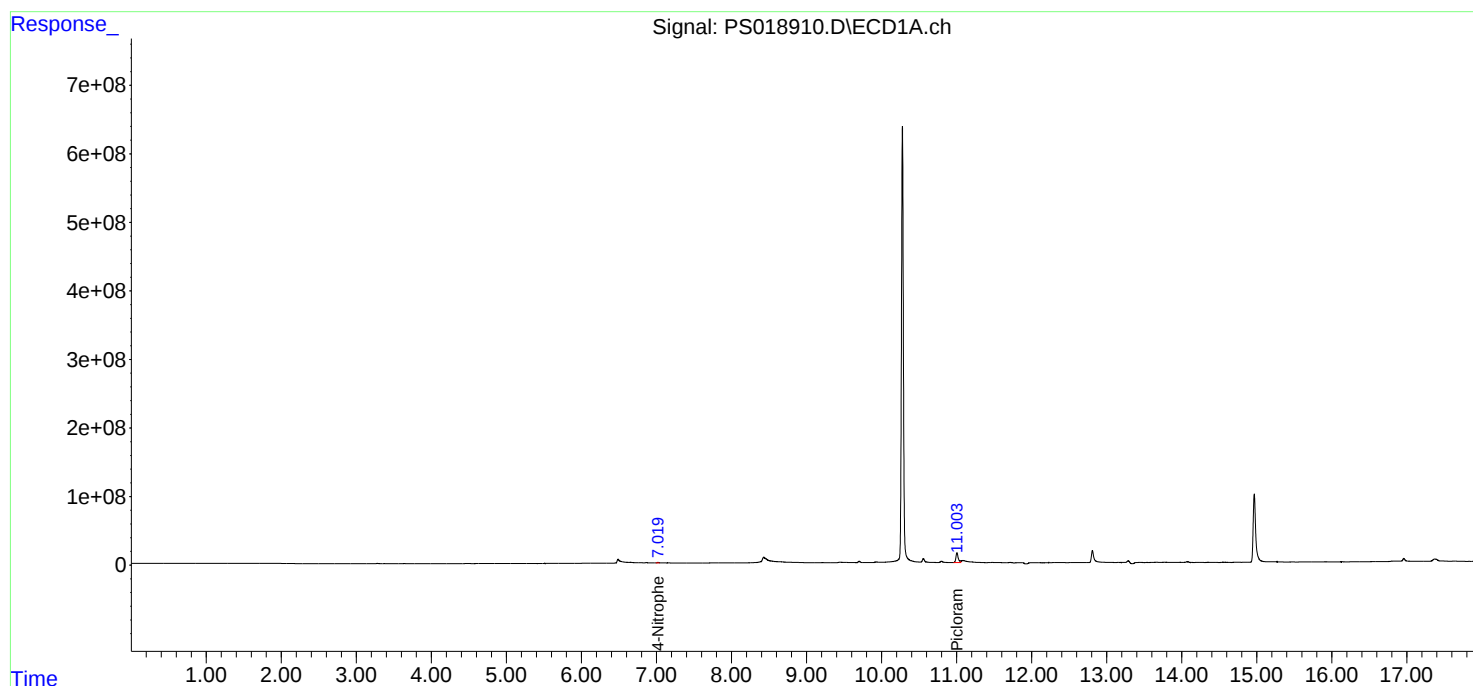


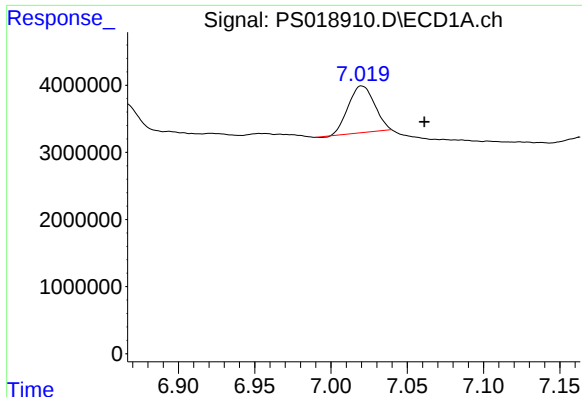

#3 4-Nitrophenol


R.T.: 7.020 min
Delta R.T.: -0.041 min
Response: 8332255
Conc: 7.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

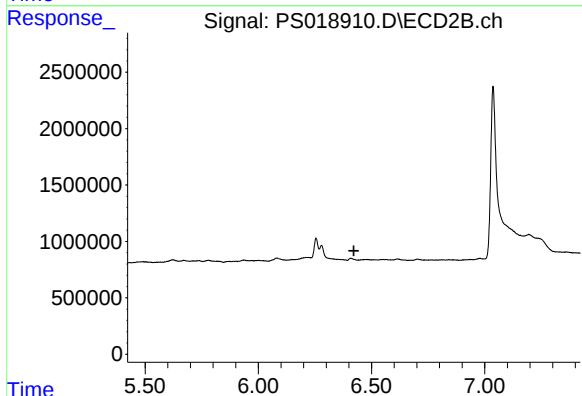


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

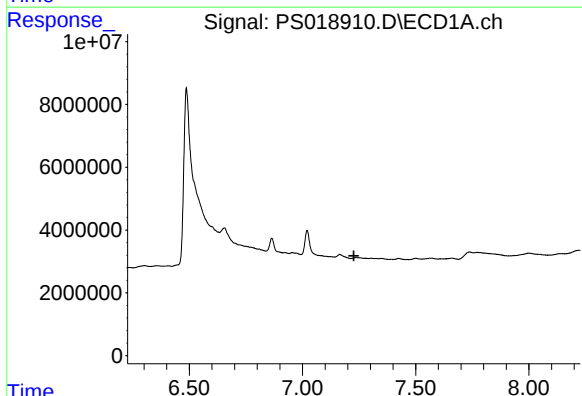


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.227 min
Response: 0
Conc: N.D.

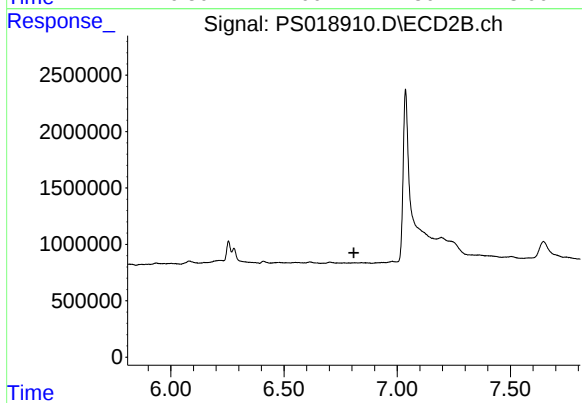

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

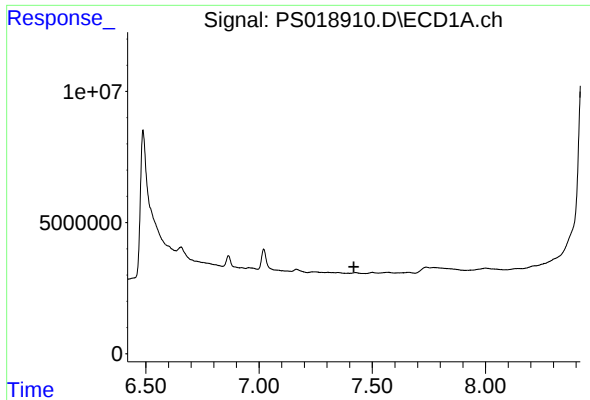

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

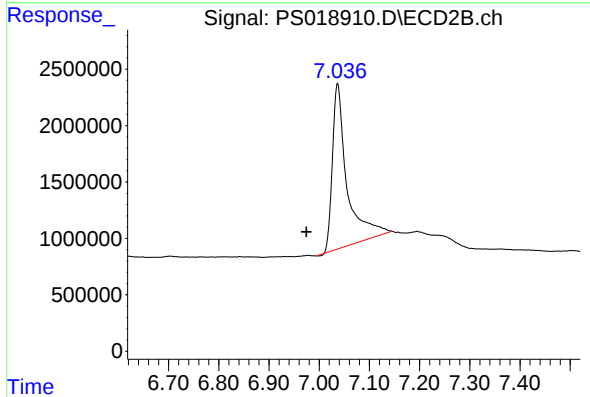


#5 DICAMBA

R.T.: 7.037 min
Delta R.T.: 0.062 min
Response: 29720870
Conc: 9.34 ng/ml

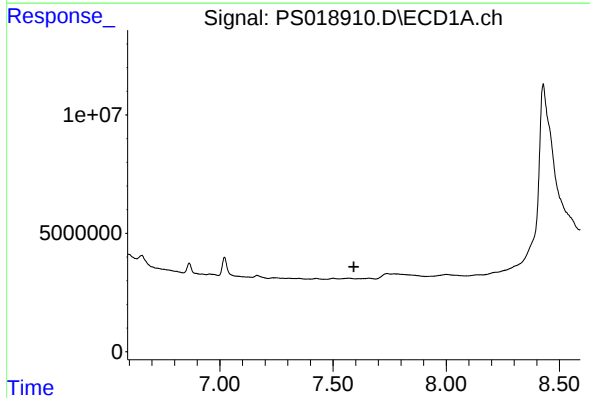


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.592 min
Response: 0
Conc: N.D.

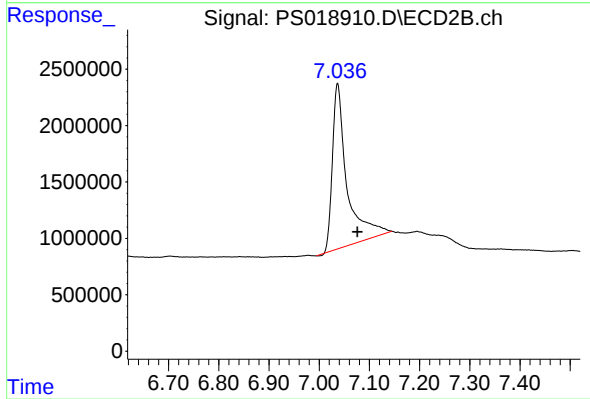

#6 MCP


R.T.: 7.037 min
Delta R.T.: -0.039 min
Response: 29720870
Conc: 11.62 ug/ml

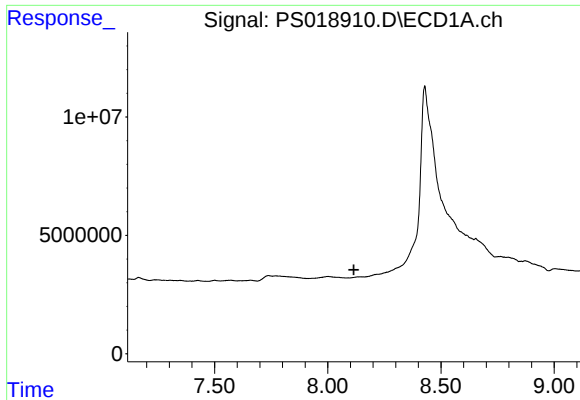

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

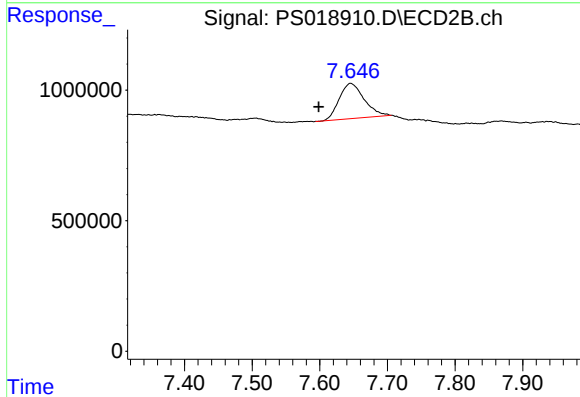


#8 DICHLORPROP

R.T.: 7.646 min
Delta R.T.: 0.047 min
Response: 3446341
Conc: 4.19 ng/ml

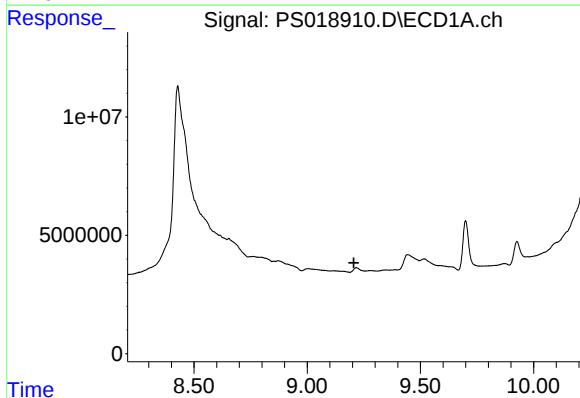


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.206 min
Response: 0
Conc: N.D.

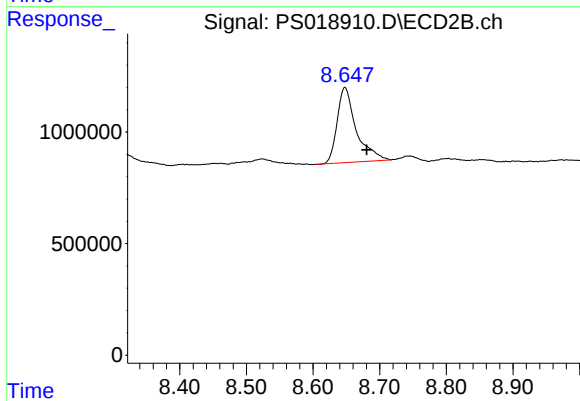

#11 2,4,5-TP (SILVEX)


R.T.: 8.648 min
Delta R.T.: -0.033 min
Response: 6698832
Conc: 1.47 ng/ml

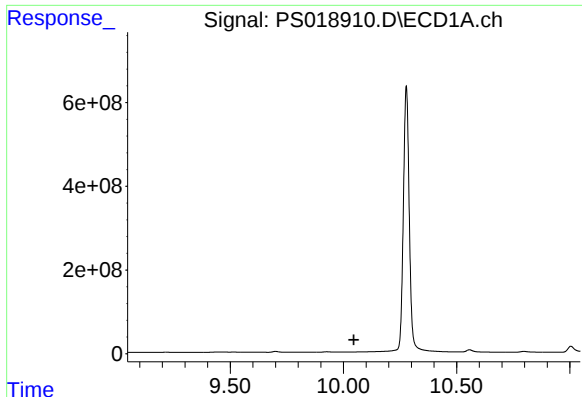

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

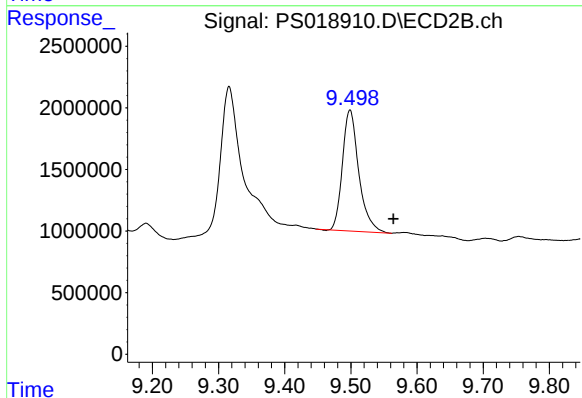


#13 2,4-DB

R.T.: 9.499 min
Delta R.T.: -0.066 min
Response: 16891001
Conc: 29.66 ng/ml

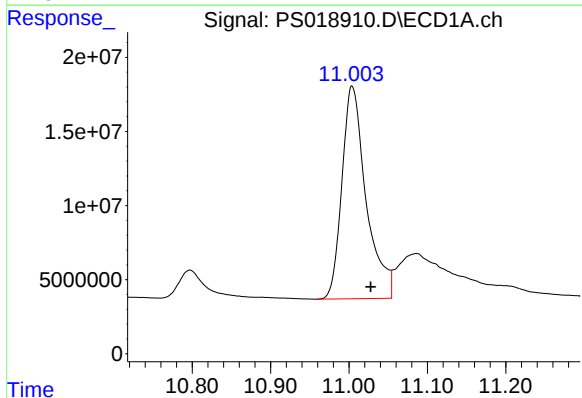

#15 Picloram

R.T.: 11.004 min
Delta R.T.: -0.024 min
Response: 307804101
Conc: 11.00 ng/ml

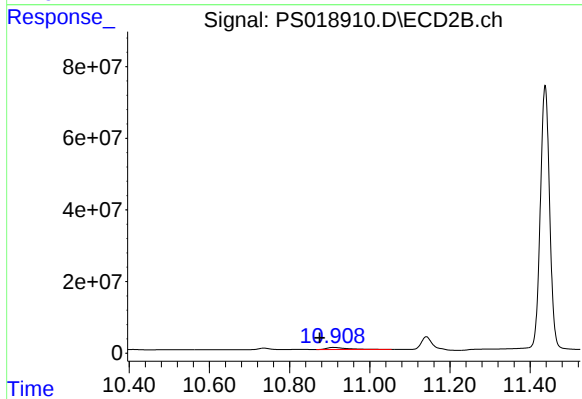

#15 Picloram

R.T.: 10.909 min
Delta R.T.: 0.034 min
Response: 19817426
Conc: 3.50 ng/ml