

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040622\
 Data File : PS018915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2022 17:07
 Operator : AJ\MA
 Sample : PB143919BD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 00:00:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.806	1912.7E6	390.1E6	655.143	546.405
Target Compounds							
1) T	Dalapon	3.028	2.532	1794.9E6	383.7E6	392.372	413.682
2) T	3,5-DICHL...	6.436	5.979	2375.3E6	566.9E6	592.111	514.131
3) T	4-Nitroph...	7.064	6.421	561.5E6	208.1E6	491.923	489.988
5) T	DICAMBA	7.418	6.972	7547.6E6	1682.4E6	600.297	528.496
6) T	MCPD	7.587	7.068	587.6E6	130.9E6	57.589	51.145
7) T	MCPA	7.735	7.281	807.6E6	181.6E6	56.739	50.696
8) T	DICHLORPROP	8.112	7.595	1897.2E6	428.2E6	569.124	520.697
9) T	2,4-D	8.344	7.889	2210.0E6	482.9E6	553.017	522.520
10) T	Pentachlo...	8.651	8.315	26057.0E6	5839.6E6	582.390	554.928
11) T	2,4,5-TP ...	9.205	8.677	10562.1E6	2489.8E6	516.192	544.667
12) T	2,4,5-T	9.490	9.056	10344.8E6	2281.1E6	504.590	547.785
13) T	2,4-DB	10.045	9.562	1605.4E6	303.9E6	472.896	533.518
14) T	DINOSEB	11.203	9.889	7426.5E6	1715.9E6	454.881	532.078
15) T	Picloram	11.026	10.872	12656.3E6	2865.2E6	452.365	506.741
16) T	DCPA	11.470	10.820	11982.7E6	3048.6E6	476.074	559.318



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040622\
Data File : PS018915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2022 17:07
Operator : AJ\MA
Sample : PB143919BD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 00:00:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

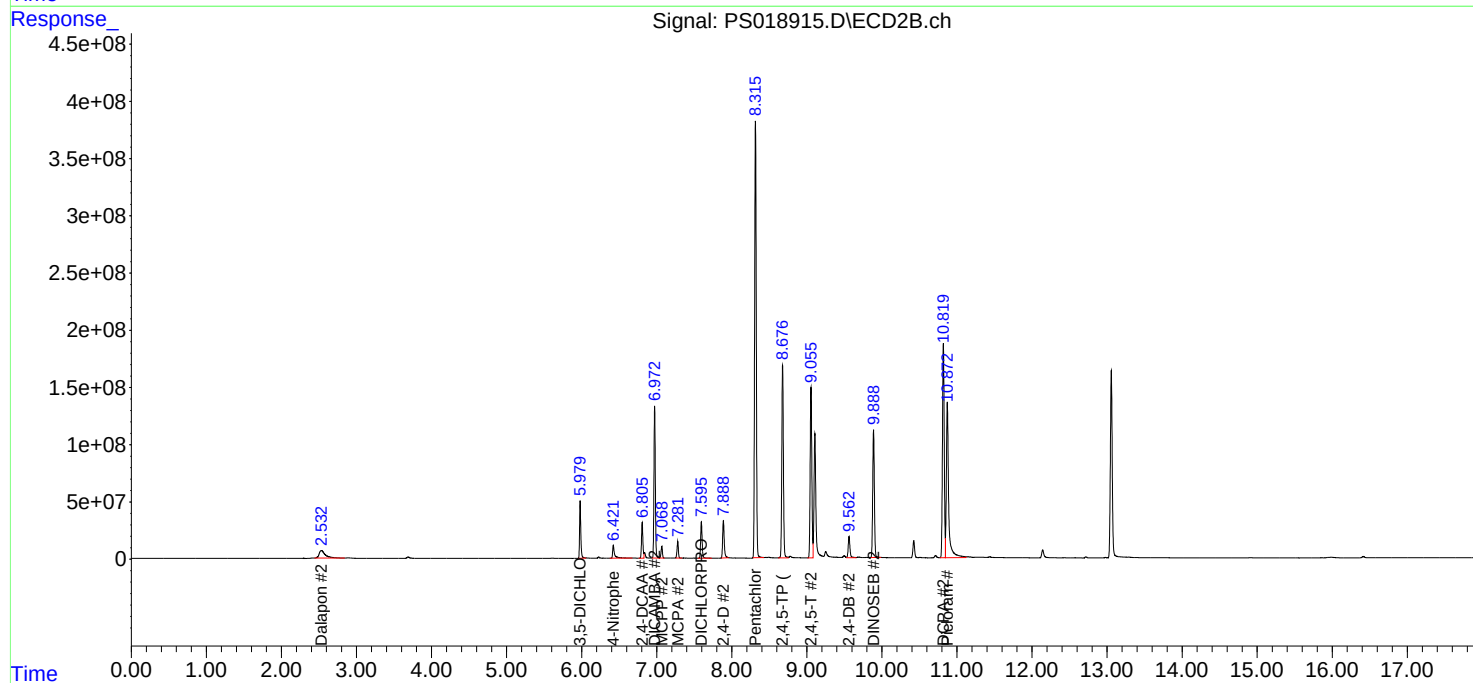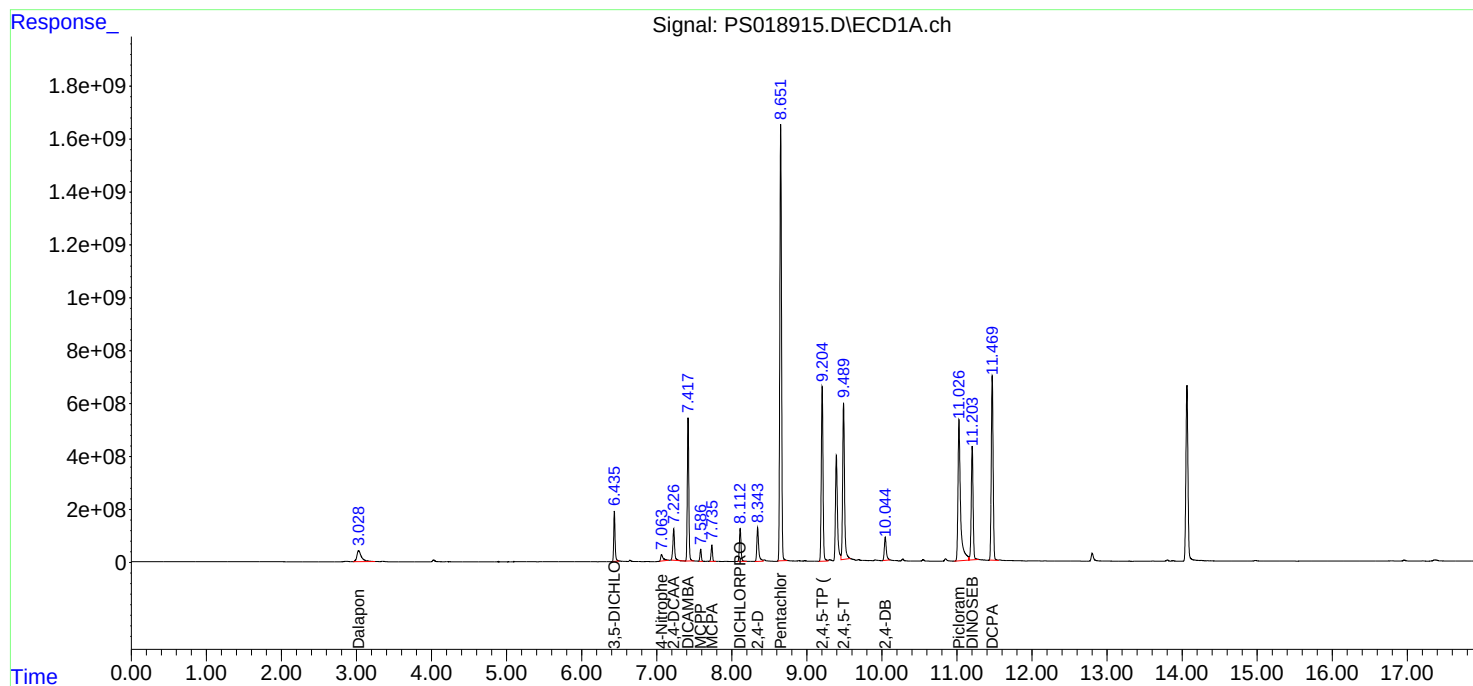


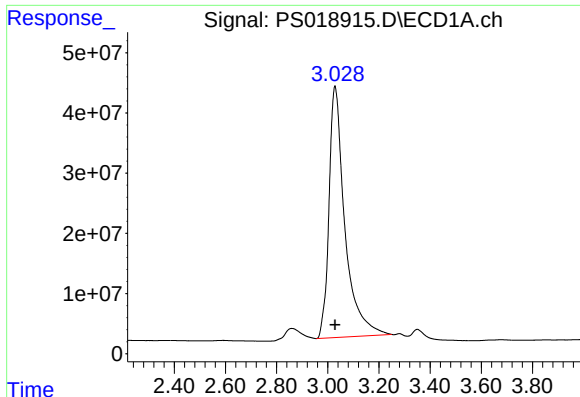

#1 Dalapon


R.T.: 3.028 min
Delta R.T.: -0.001 min
Response: 1794891935
Conc: 392.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

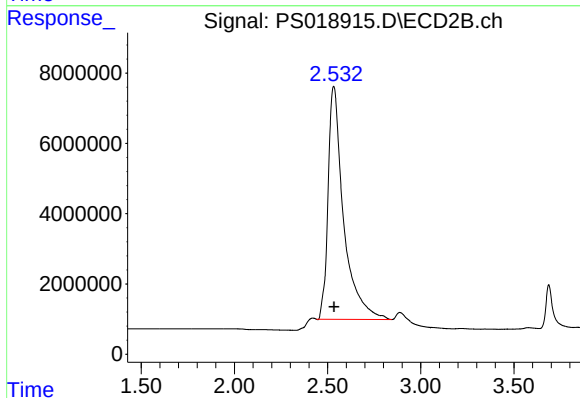


#1 Dalapon

R.T.: 2.532 min
Delta R.T.: -0.002 min
Response: 383699684
Conc: 413.68 ng/ml

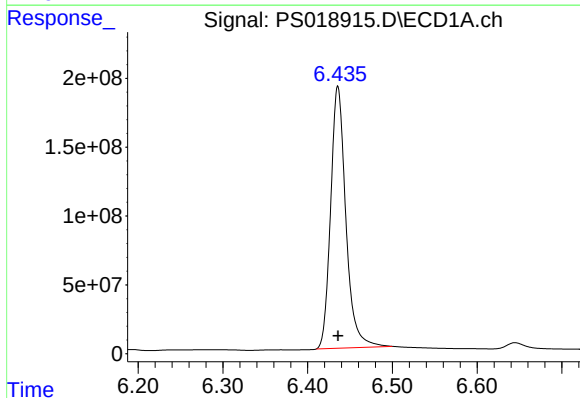


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 2375341131
Conc: 592.11 ng/ml

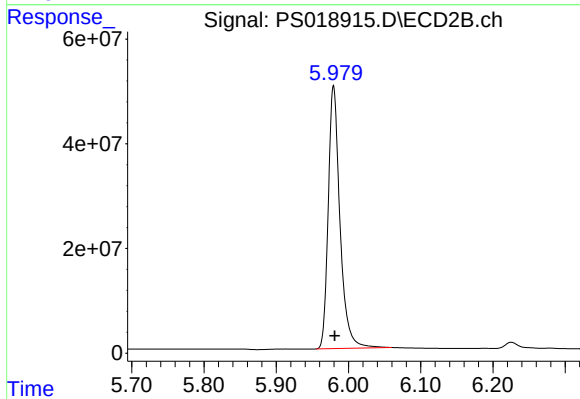

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.979 min
Delta R.T.: -0.002 min
Response: 566893312
Conc: 514.13 ng/ml

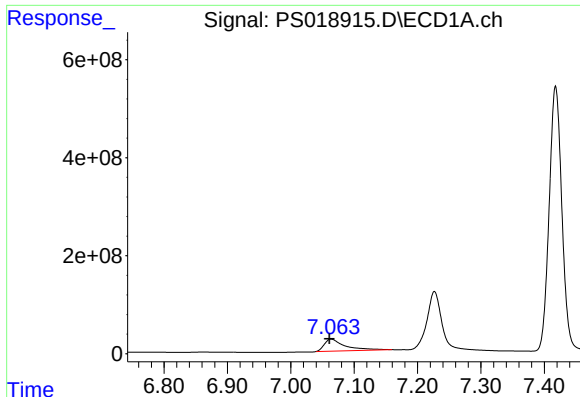

#3 4-Nitrophenol


R.T.: 7.064 min
Delta R.T.: 0.003 min
Response: 561531596
Conc: 491.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

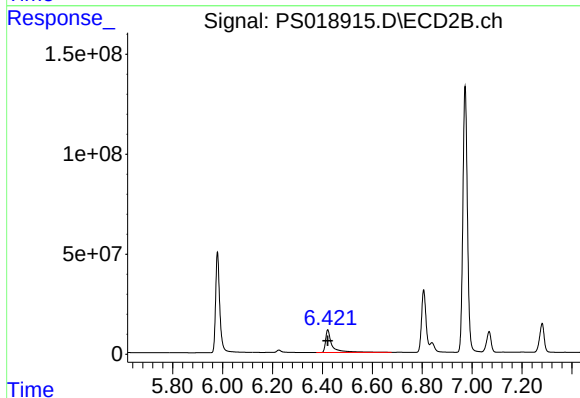


#3 4-Nitrophenol

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 208132272
Conc: 489.99 ng/ml

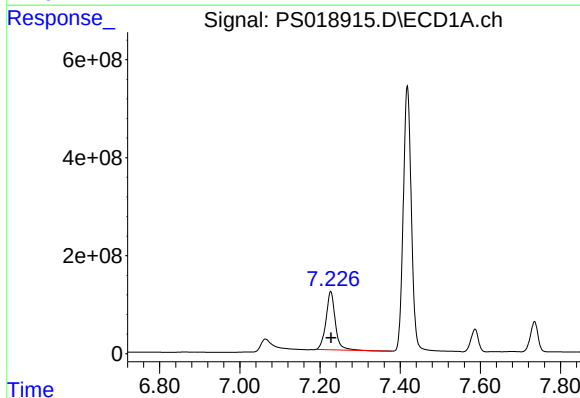


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 1912664235
Conc: 655.14 ng/ml

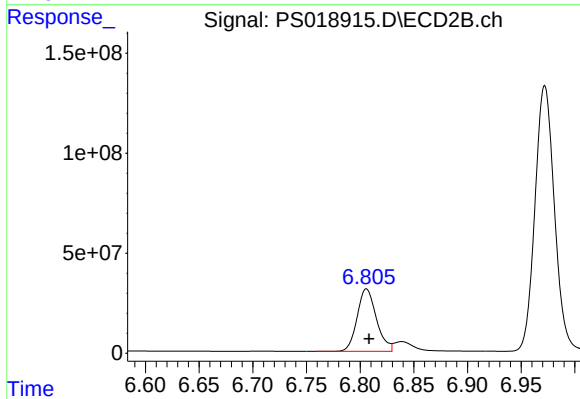

#4 2,4-DCAA


R.T.: 6.806 min
Delta R.T.: -0.003 min
Response: 390101990
Conc: 546.41 ng/ml

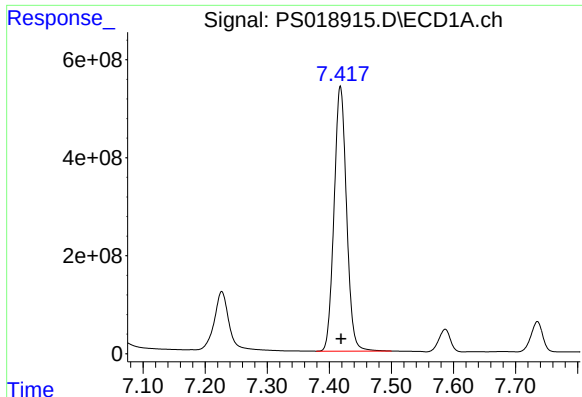

#5 DICAMBA


R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 7547574157
Conc: 600.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

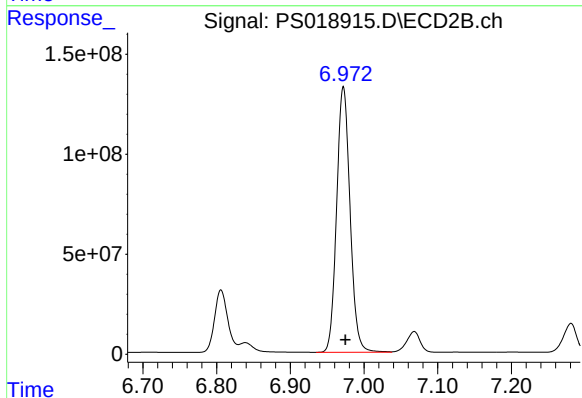


#5 DICAMBA

R.T.: 6.972 min
Delta R.T.: -0.003 min
Response: 1682421992
Conc: 528.50 ng/ml

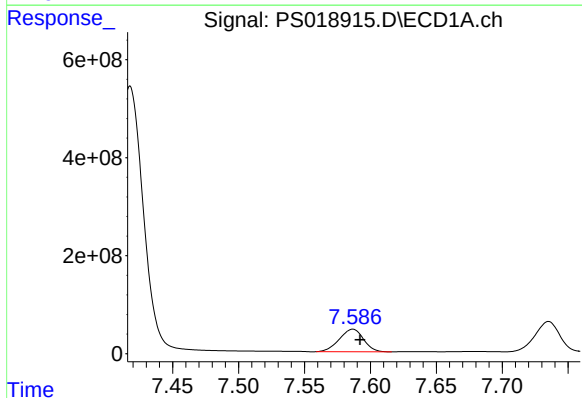


#6 MCP

R.T.: 7.587 min
Delta R.T.: -0.006 min
Response: 587562611
Conc: 57.59 ug/ml

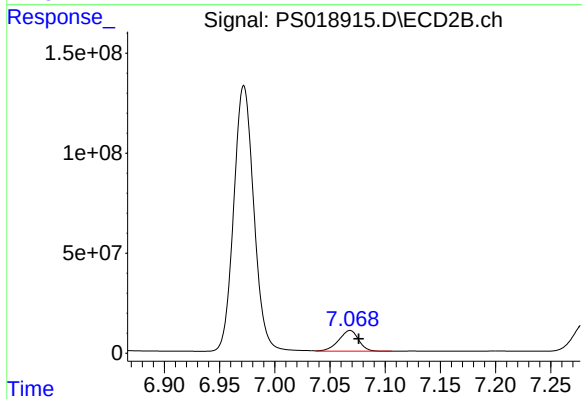

#6 MCP


R.T.: 7.068 min
Delta R.T.: -0.008 min
Response: 130852714
Conc: 51.14 ug/ml

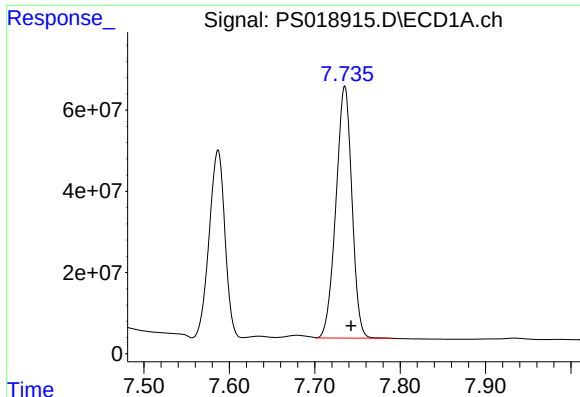

#7 MCPA


R.T.: 7.735 min
Delta R.T.: -0.007 min
Response: 807627900
Conc: 56.74 ug/ml

Instrument :
ECD_S
ClientSampleId :

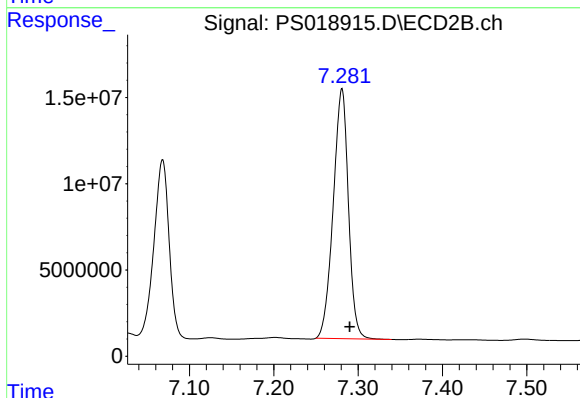


#7 MCPA

R.T.: 7.281 min
Delta R.T.: -0.009 min
Response: 181630611
Conc: 50.70 ug/ml

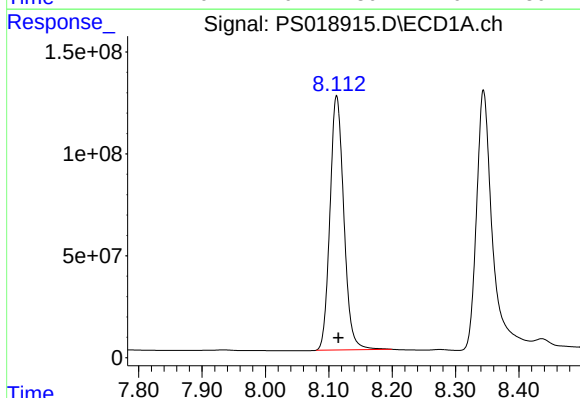


#8 DICHLORPROP

R.T.: 8.112 min
Delta R.T.: -0.003 min
Response: 1897179225
Conc: 569.12 ng/ml

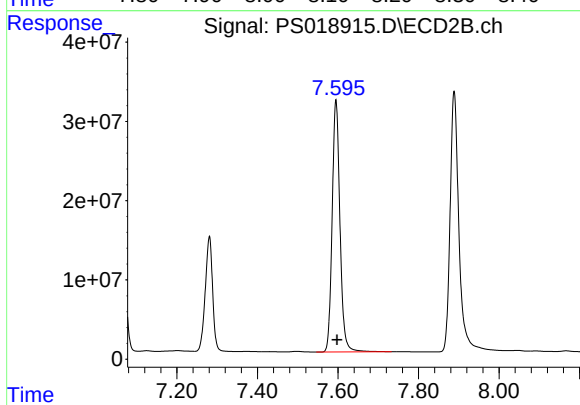

#8 DICHLORPROP


R.T.: 7.595 min
Delta R.T.: -0.003 min
Response: 428198473
Conc: 520.70 ng/ml

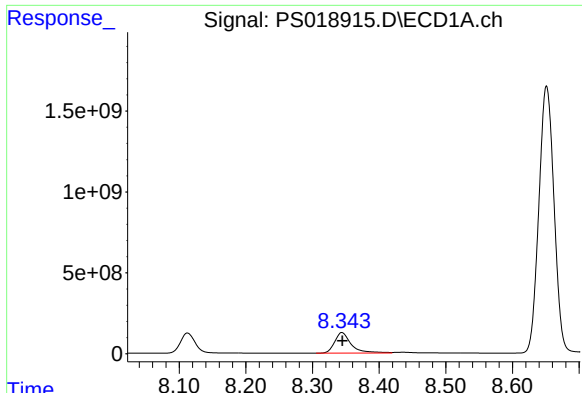

#9 2,4-D


R.T.: 8.344 min
Delta R.T.: 0.000 min
Response: 2209980827
Conc: 553.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

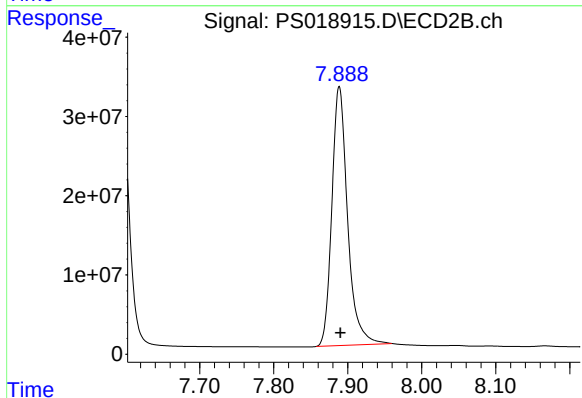


#9 2,4-D

R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 482928957
Conc: 522.52 ng/ml

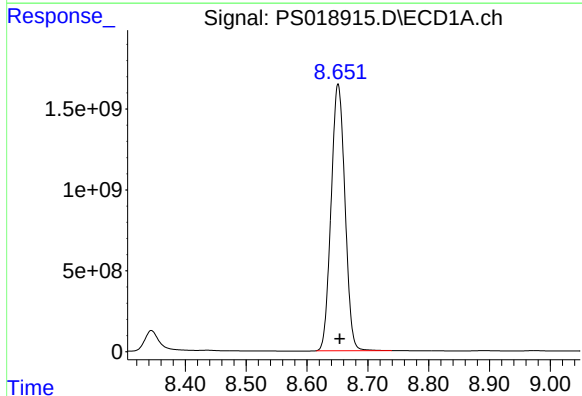


#10 Pentachlorophenol

R.T.: 8.651 min
Delta R.T.: -0.003 min
Response: 26057041978
Conc: 582.39 ng/ml

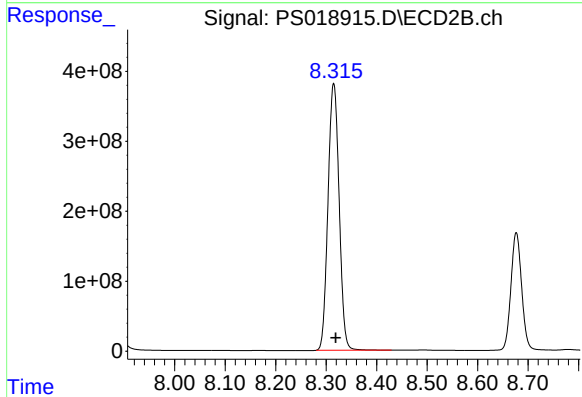

#10 Pentachlorophenol


R.T.: 8.315 min
Delta R.T.: -0.004 min
Response: 5839586771
Conc: 554.93 ng/ml

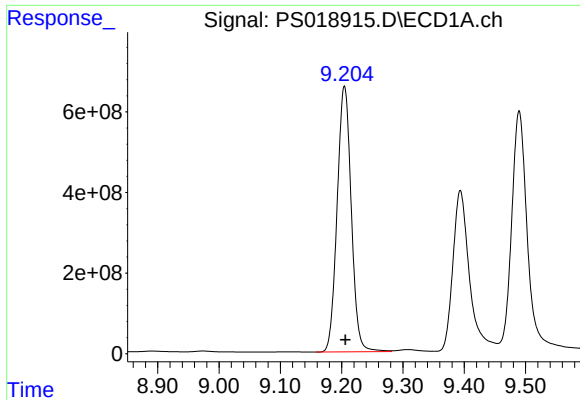

#11 2,4,5-TP (SILVEX)


R.T.: 9.205 min
Delta R.T.: -0.002 min
Response: 10562084421
Conc: 516.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

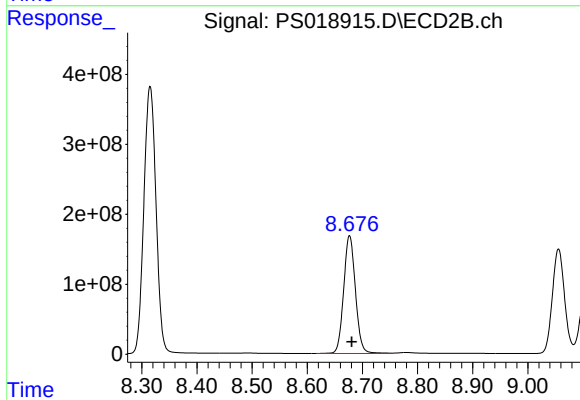


#11 2,4,5-TP (SILVEX)

R.T.: 8.677 min
Delta R.T.: -0.004 min
Response: 2489840353
Conc: 544.67 ng/ml

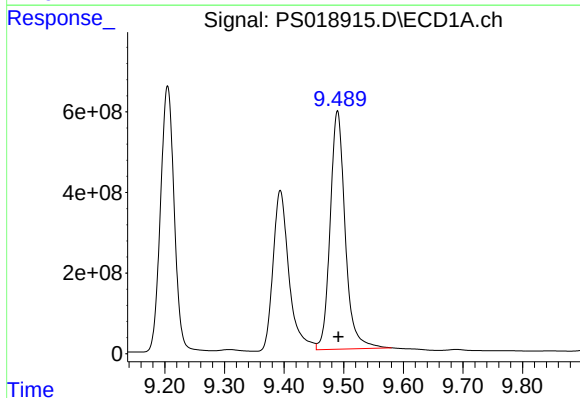


#12 2,4,5-T

R.T.: 9.490 min
Delta R.T.: -0.002 min
Response: 10344768011
Conc: 504.59 ng/ml

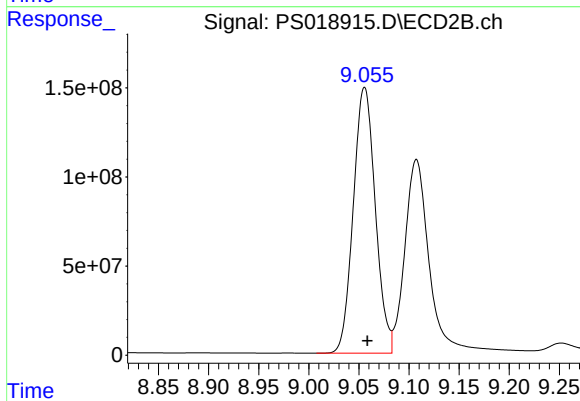

#12 2,4,5-T


R.T.: 9.056 min
Delta R.T.: -0.003 min
Response: 2281097028
Conc: 547.79 ng/ml

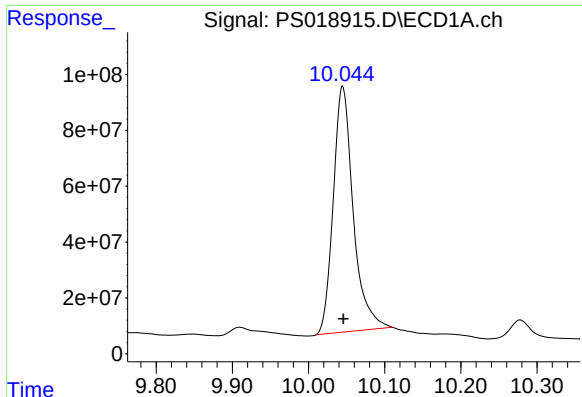

#13 2,4-DB


R.T.: 10.045 min
Delta R.T.: -0.001 min
Response: 1605429950
Conc: 472.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

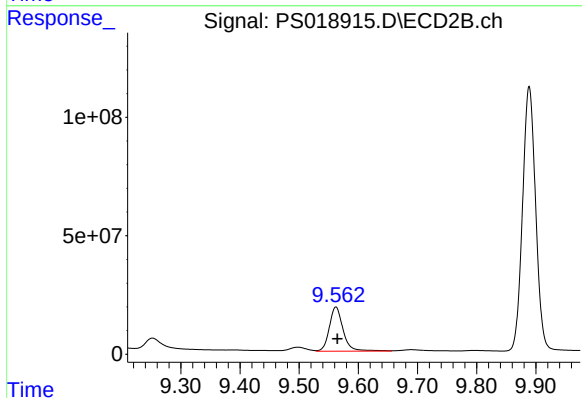


#13 2,4-DB

R.T.: 9.562 min
Delta R.T.: -0.003 min
Response: 303878135
Conc: 533.52 ng/ml

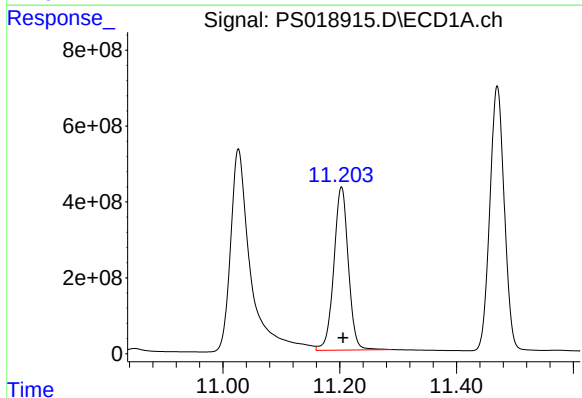


#14 DINOSEB

R.T.: 11.203 min
Delta R.T.: -0.003 min
Response: 7426545016
Conc: 454.88 ng/ml

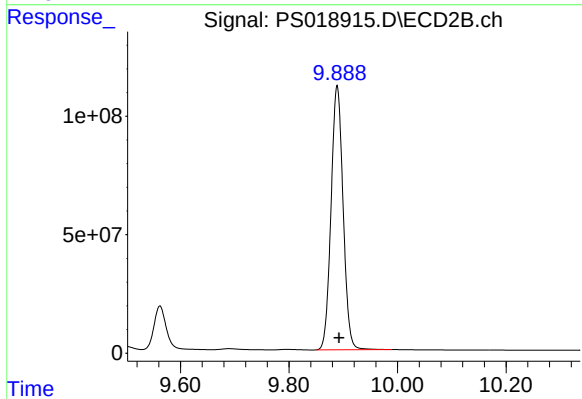

#14 DINOSEB


R.T.: 9.889 min
Delta R.T.: -0.003 min
Response: 1715855891
Conc: 532.08 ng/ml

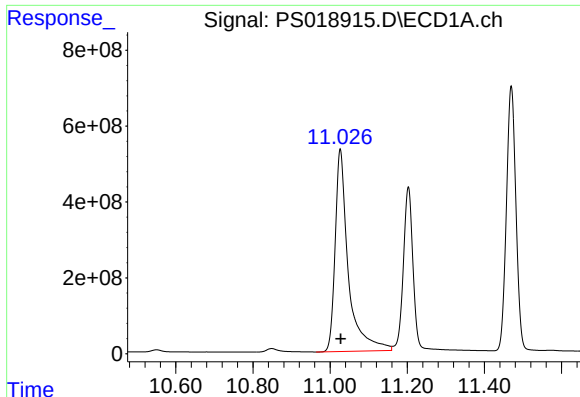

#15 Picloram


R.T.: 11.026 min
Delta R.T.: -0.001 min
Response: 12656299266
Conc: 452.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

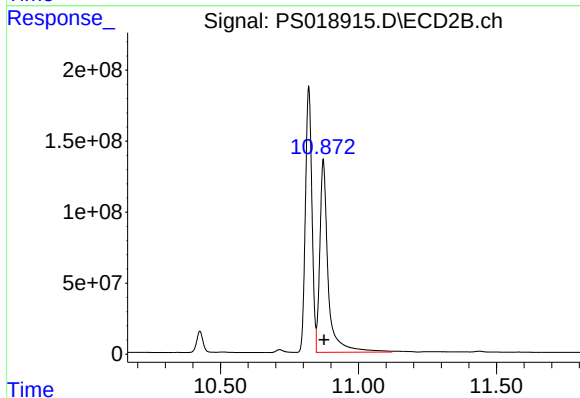


#15 Picloram

R.T.: 10.872 min
Delta R.T.: -0.003 min
Response: 2865225567
Conc: 506.74 ng/ml

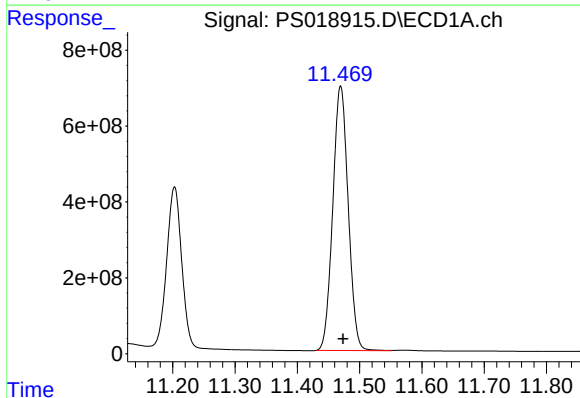

#16 DCPA

R.T.: 11.470 min
Delta R.T.: -0.004 min
Response: 11982748982
Conc: 476.07 ng/ml

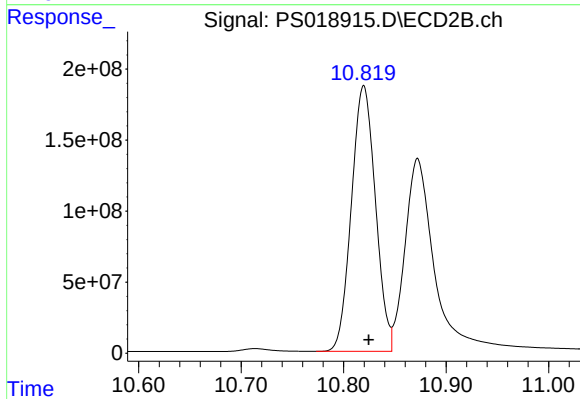

#16 DCPA

R.T.: 10.820 min
Delta R.T.: -0.005 min
Response: 3048629258
Conc: 559.32 ng/ml