

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040622\
 Data File : PS018920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2022 19:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 00:01:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.806	1591.2E6	359.4E6	545.019	503.386
Target Compounds							
3) T	4-Nitroph...	7.028	0.000	1978445	0	1.733	N.D. #
7) T	MCPA	7.679f	0.000	3596961	0	<MDL	N.D. #
9) T	2,4-D	8.411f	0.000	10579267	0	2.647	N.D. #
11) T	2,4,5-TP ...	0.000	8.638f	0	9063456	N.D.	1.983
12) T	2,4,5-T	9.499	9.126f	4091273	3031791	<MDL	<MDL #
14) T	DINOSEB	11.266f	0.000	972801	0	<MDL	N.D. #
15) T	Picloram	11.054	10.893	36168434	6461331	1.293	1.143
16) T	DCPA	0.000	10.893f	0	6461331	N.D.	1.185



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040622\
Data File : PS018920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2022 19:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 00:01:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

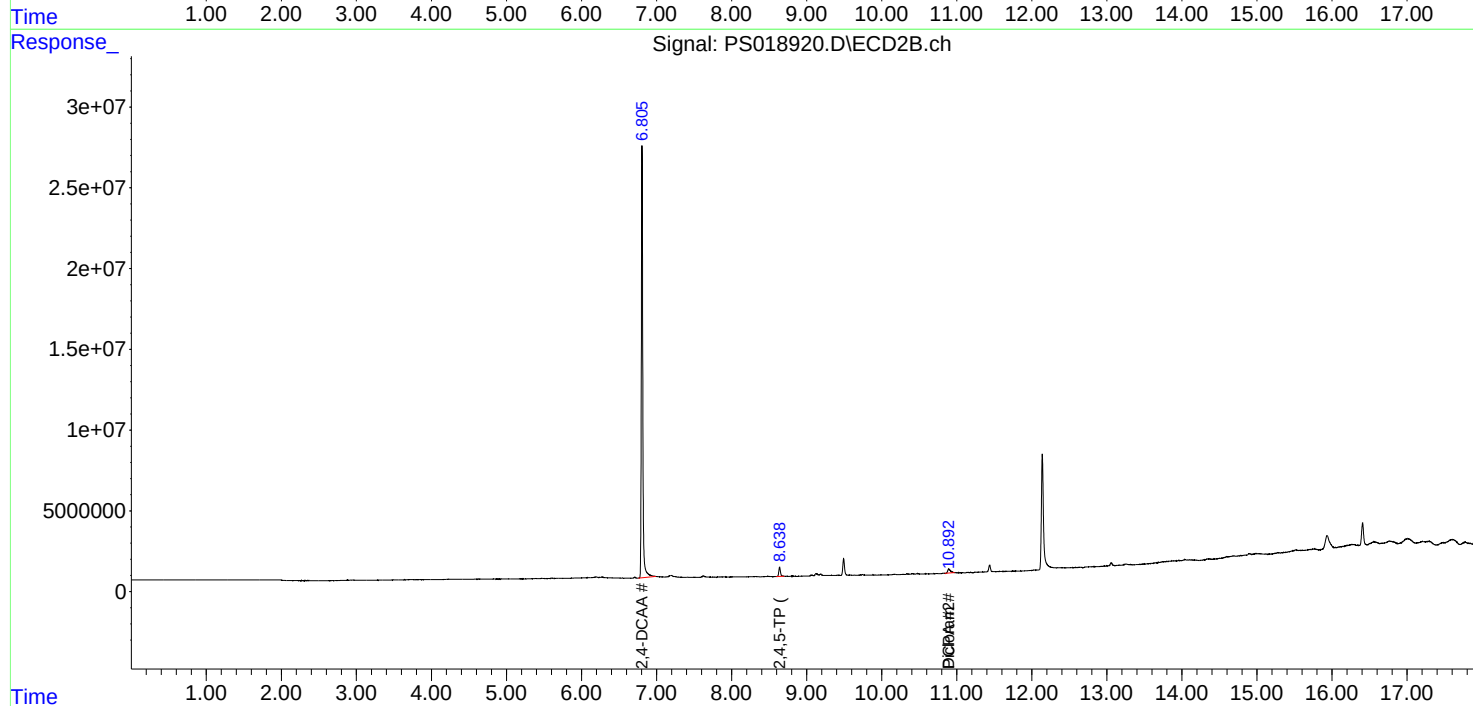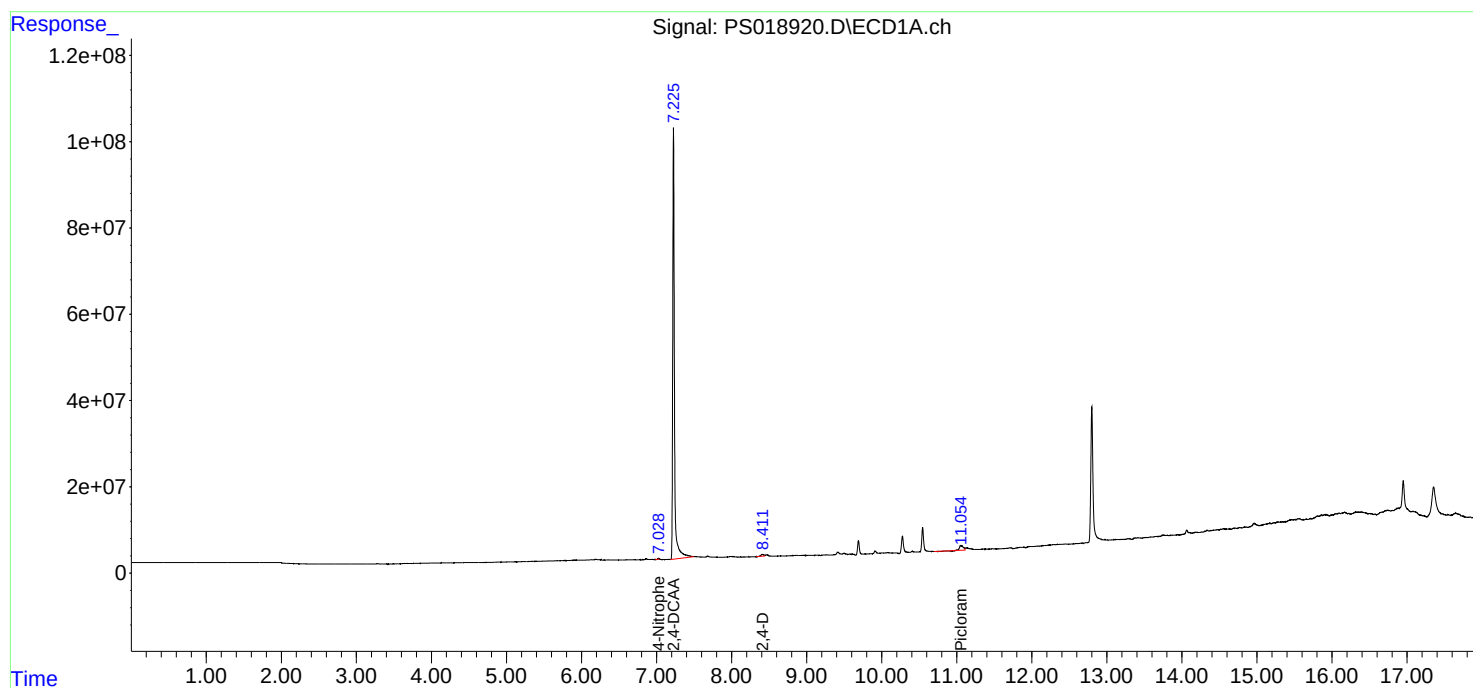


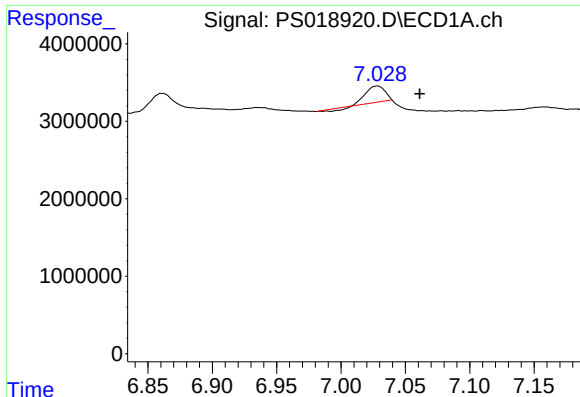

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.033 min
Response: 1978445
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

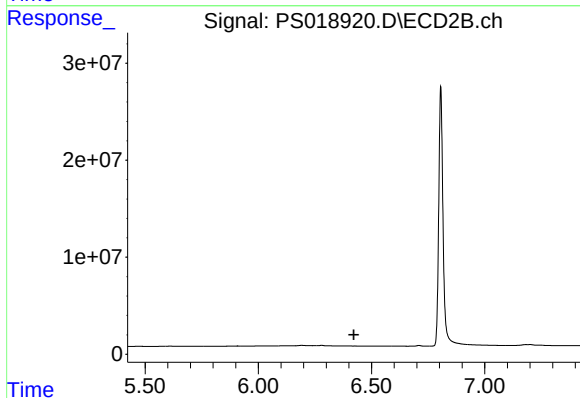


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

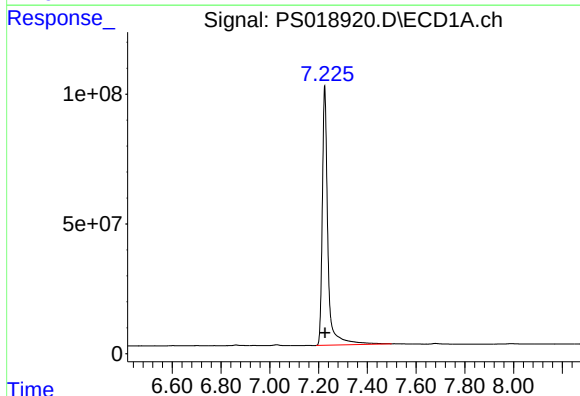


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.002 min
Response: 1591160159
Conc: 545.02 ng/ml

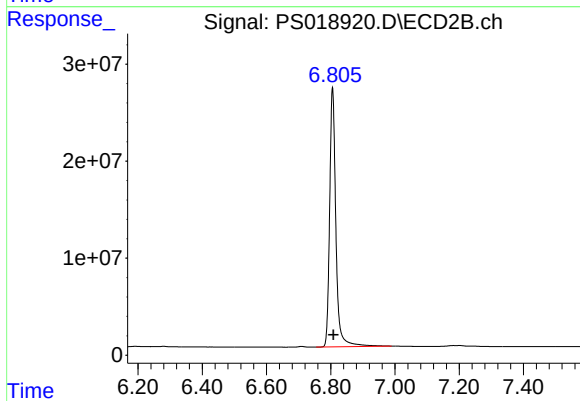

#4 2,4-DCAA


R.T.: 6.806 min
Delta R.T.: -0.003 min
Response: 359388421
Conc: 503.39 ng/ml

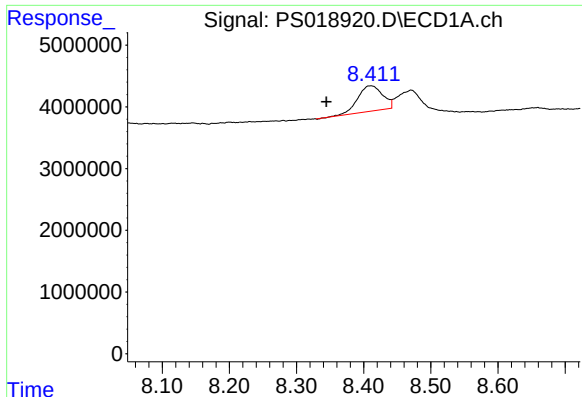

#9 2,4-D


R.T.: 8.411 min
Delta R.T.: 0.067 min
Response: 10579267
Conc: 2.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

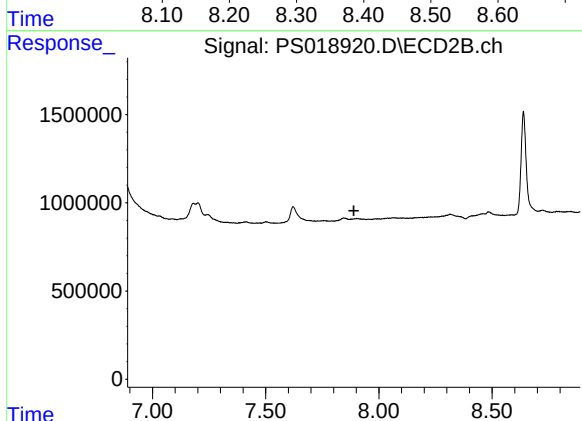


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.890 min
Response: 0
Conc: N.D.

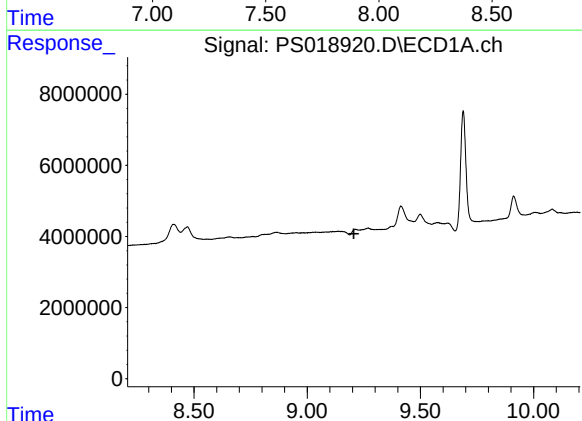


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.206 min
Response: 0
Conc: N.D.

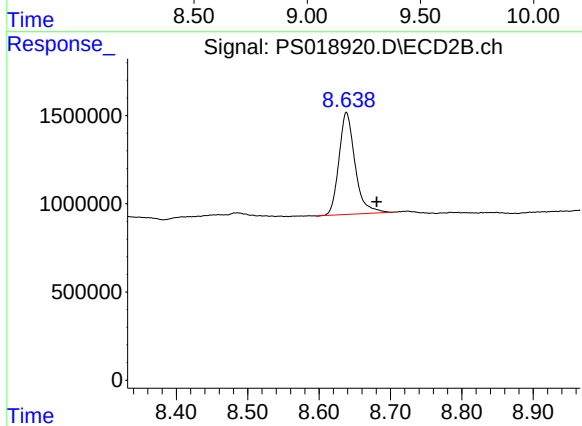

#11 2,4,5-TP (SILVEX)


R.T.: 8.638 min
Delta R.T.: -0.042 min
Response: 9063456
Conc: 1.98 ng/ml

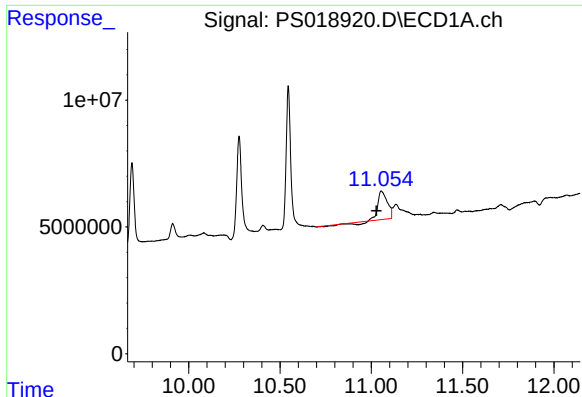

#15 Picloram


R.T.: 11.054 min
Delta R.T.: 0.027 min
Response: 36168434
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

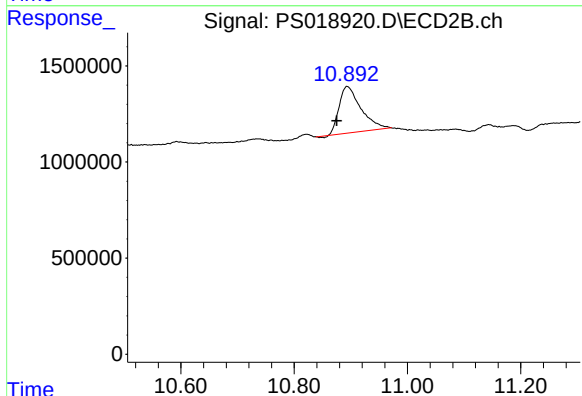


#15 Picloram

R.T.: 10.893 min
Delta R.T.: 0.018 min
Response: 6461331
Conc: 1.14 ng/ml

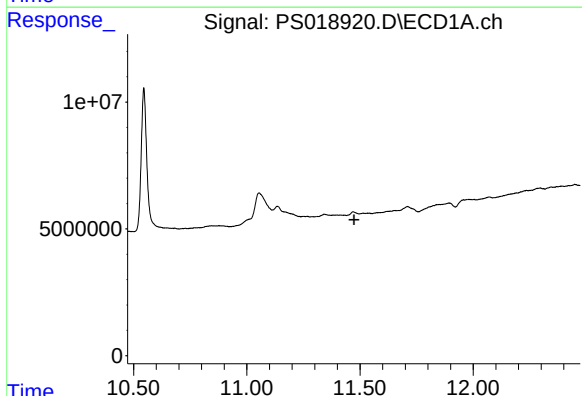

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.473 min
Response: 0
Conc: N.D.

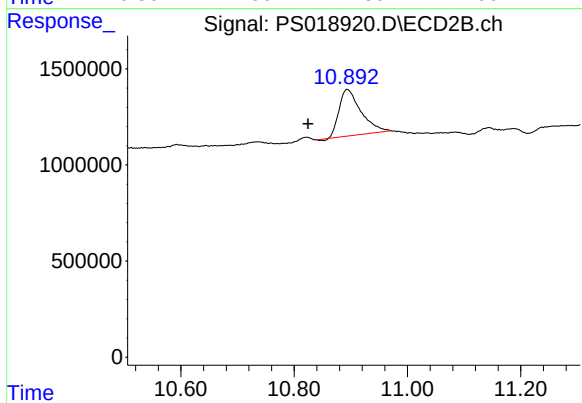

#16 DCPA

R.T.: 10.893 min
Delta R.T.: 0.069 min
Response: 6461331
Conc: 1.19 ng/ml