

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040720\
 Data File : PS009624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2020 13:09
 Operator : DD\AJ
 Sample : L2100-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:55:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.930	118.9E6	88337941	214.962	160.849 #
Target Compounds							
2) T	3,5-DICHL...	0.000	6.064	0	7308492	N.D.	8.986
5) T	DICAMBA	7.445	7.145	11107168	4132605	5.219	1.800 #
6) T	MCP	0.000	7.145	0	4132605	N.D.	2.272
7) T	MCPA	7.734	7.397	26269968	22374483	8.625	8.291
9) T	2,4-D	8.407	8.012	14170249	9199666	26.877	13.995 #
10) T	Pentachlo...	8.667	8.453	33631505	12734055	4.783	1.678 #
11) T	2,4,5-TP ...	9.217	8.813	40594150	30420059	14.809	10.204 #
12) T	2,4,5-T	9.545	9.194	67917114	20860426	26.699	7.066 #
13) T	2,4-DB	10.098	9.721	-10303427	24187506	N.D.	63.716
14) T	DINOSEB	11.186	10.046	43260431	34018149	21.163	15.488 #
15) T	Picloram	11.010	11.020	63827356	26345383	21.031	6.470 #
16) T	DCPA	0.000	11.020	0	26345383	N.D.	6.802



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040720\
Data File : PS009624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2020 13:09
Operator : DD\AJ
Sample : L2100-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 14:55:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

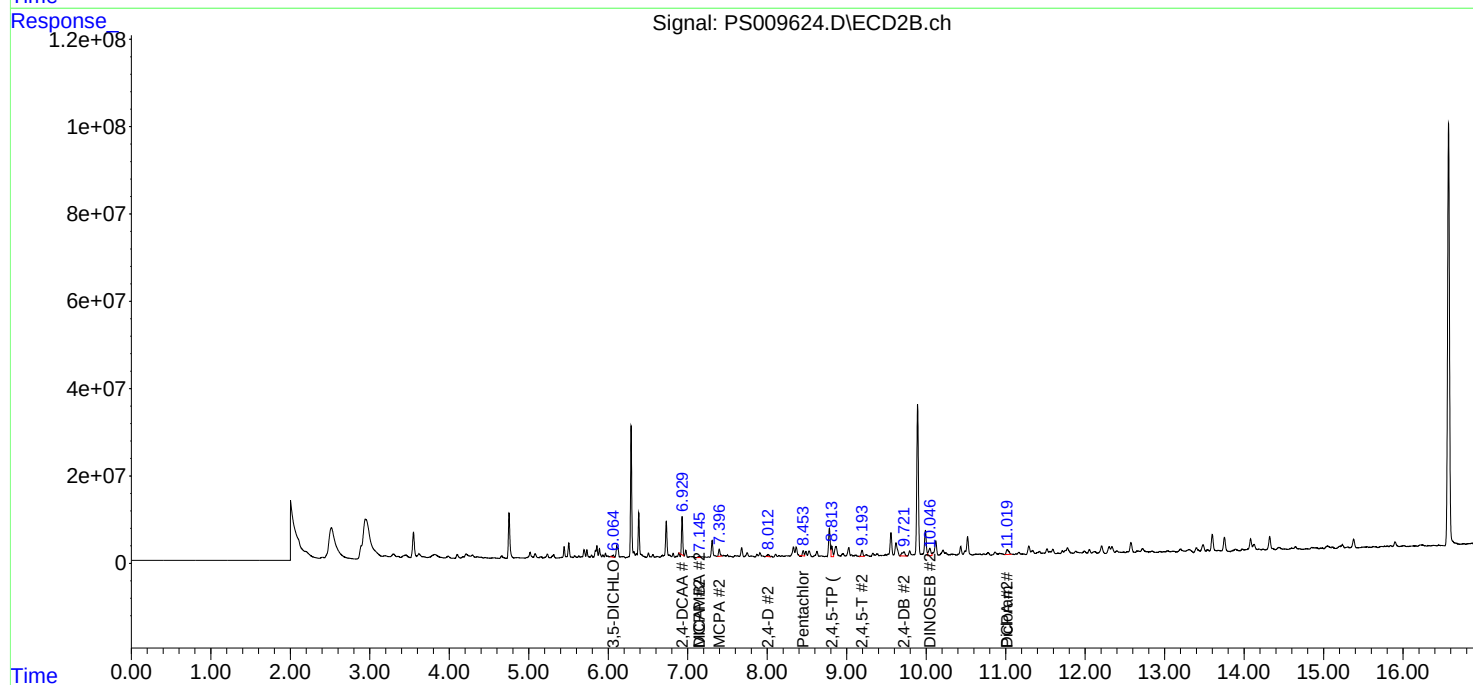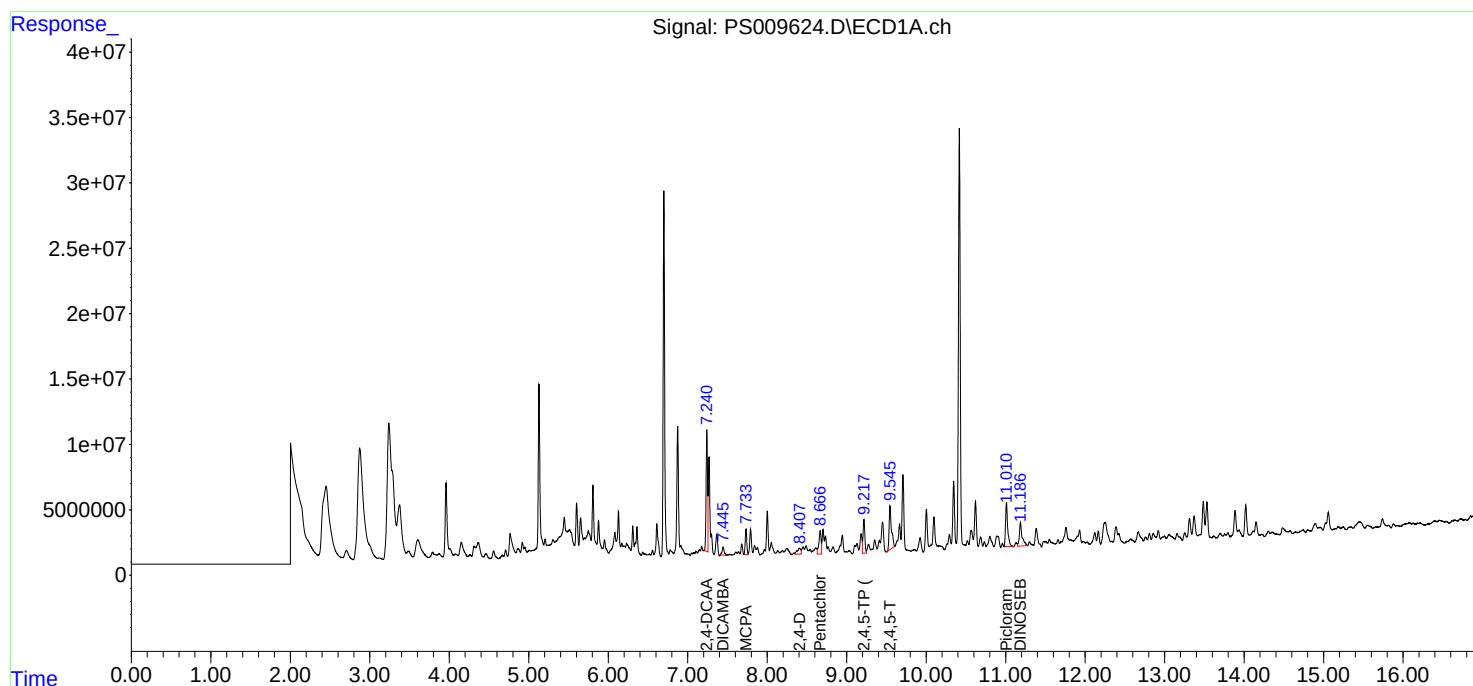


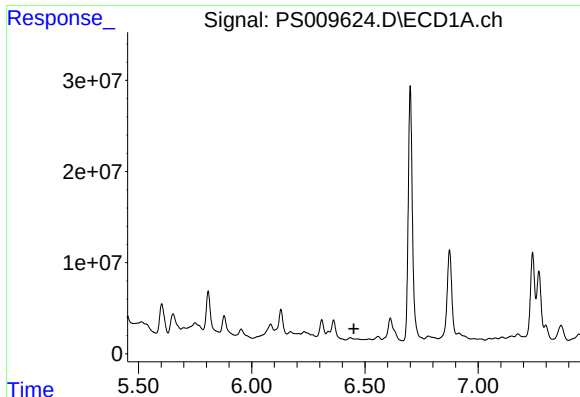

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

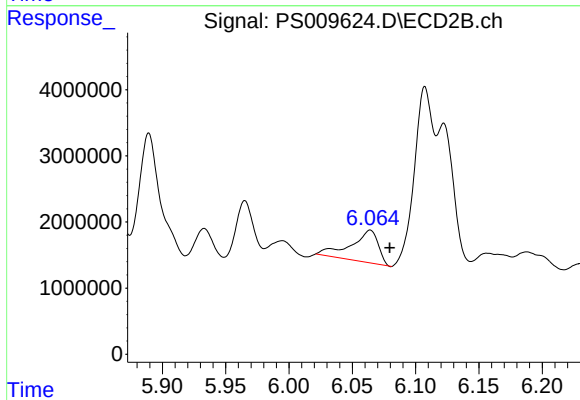


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.064 min
Delta R.T.: -0.016 min
Response: 7308492
Conc: 8.99 ng/ml

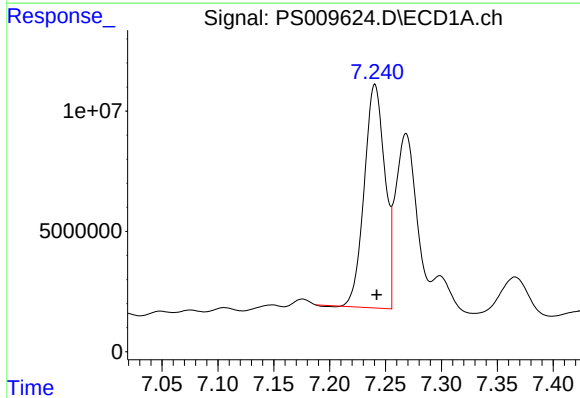


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 118910289
Conc: 214.96 ng/ml

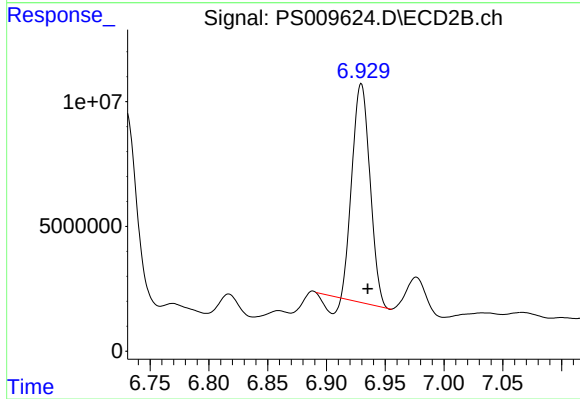

#4 2,4-DCAA


R.T.: 6.930 min
Delta R.T.: -0.006 min
Response: 88337941
Conc: 160.85 ng/ml

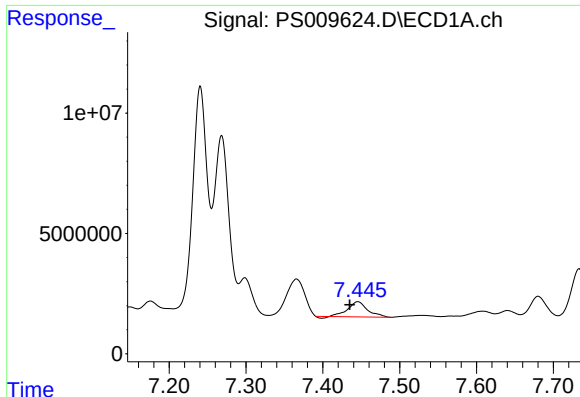

#5 DICAMBA


R.T.: 7.445 min
Delta R.T.: 0.010 min
Response: 11107168
Conc: 5.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

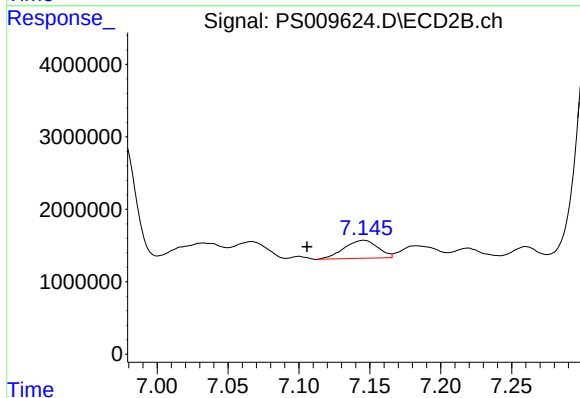


#5 DICAMBA

R.T.: 7.145 min
Delta R.T.: 0.040 min
Response: 4132605
Conc: 1.80 ng/ml

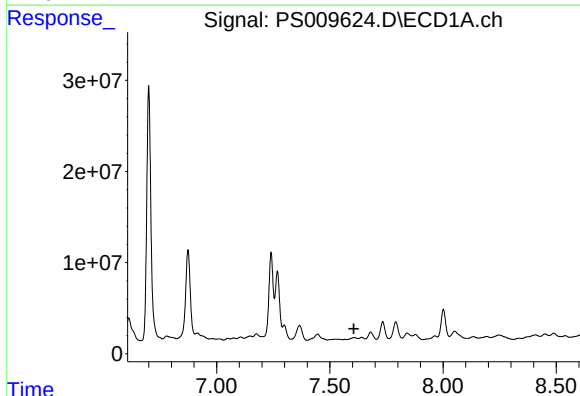


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.606 min
Response: 0
Conc: N.D.

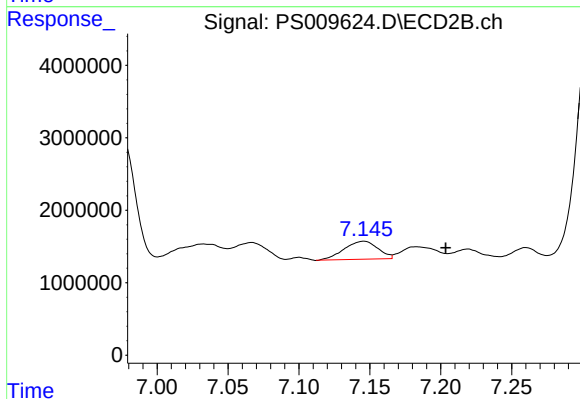

#6 MCPP


R.T.: 7.145 min
Delta R.T.: -0.058 min
Response: 4132605
Conc: 2.27 ug/ml

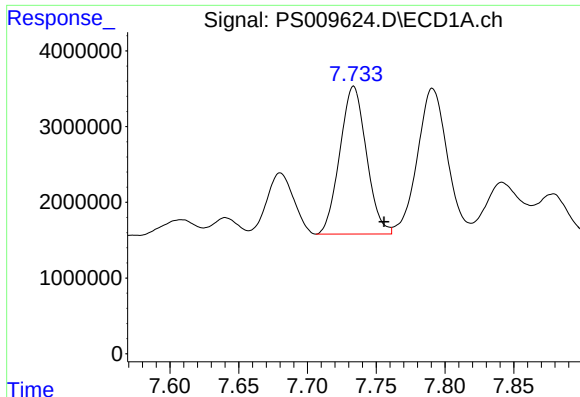

#7 MCPA


R.T.: 7.734 min
Delta R.T.: -0.022 min
Response: 26269968
Conc: 8.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

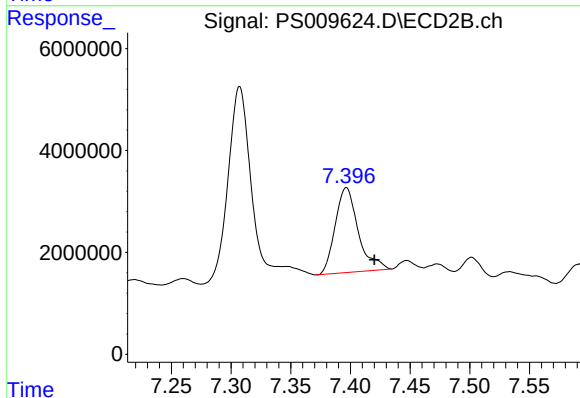


#7 MCPA

R.T.: 7.397 min
Delta R.T.: -0.023 min
Response: 22374483
Conc: 8.29 ug/ml

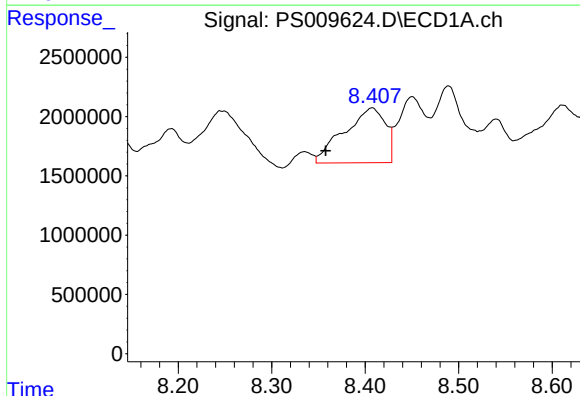


#9 2,4-D

R.T.: 8.407 min
Delta R.T.: 0.049 min
Response: 14170249
Conc: 26.88 ng/ml

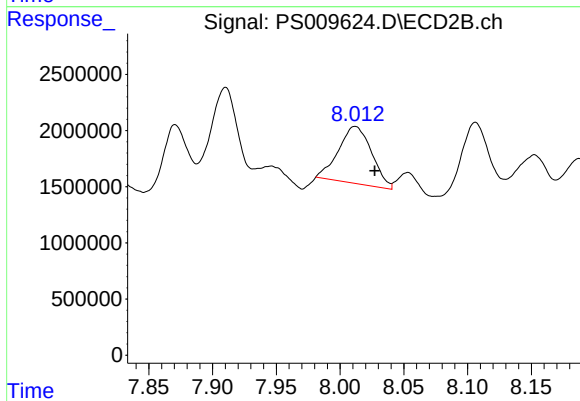

#9 2,4-D


R.T.: 8.012 min
Delta R.T.: -0.015 min
Response: 9199666
Conc: 13.99 ng/ml

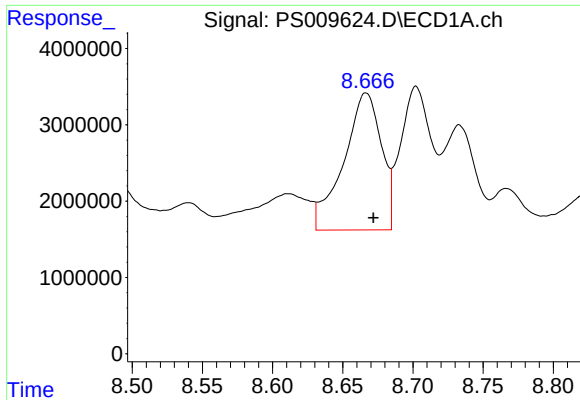

#10 Pentachlorophenol


R.T.: 8.667 min
Delta R.T.: -0.005 min
Response: 33631505
Conc: 4.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

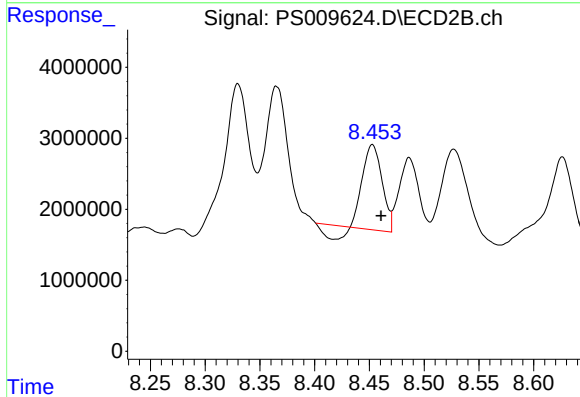


#10 Pentachlorophenol

R.T.: 8.453 min
Delta R.T.: -0.008 min
Response: 12734055
Conc: 1.68 ng/ml

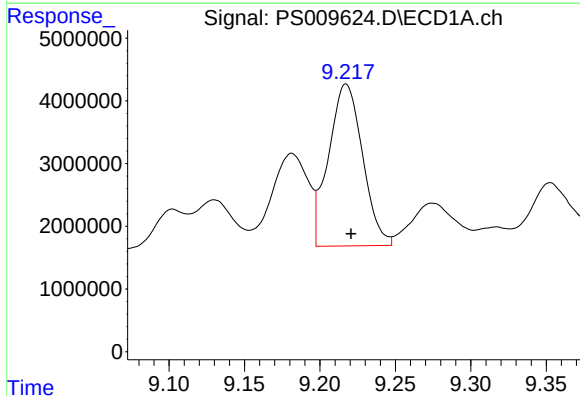


#11 2,4,5-TP (SILVEX)

R.T.: 9.217 min
Delta R.T.: -0.003 min
Response: 40594150
Conc: 14.81 ng/ml

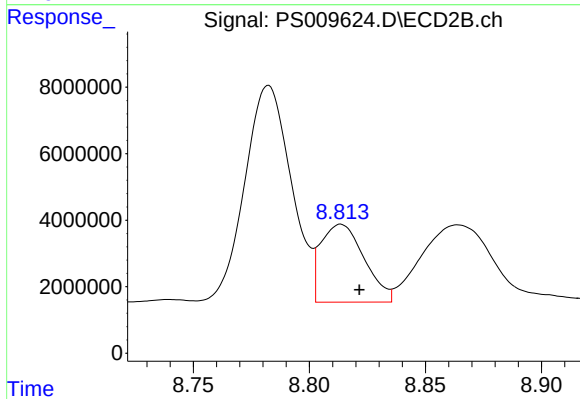

#11 2,4,5-TP (SILVEX)


R.T.: 8.813 min
Delta R.T.: -0.008 min
Response: 30420059
Conc: 10.20 ng/ml

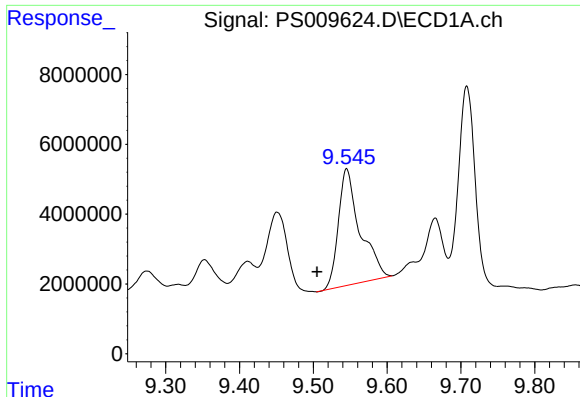

#12 2,4,5-T


R.T.: 9.545 min
Delta R.T.: 0.040 min
Response: 67917114
Conc: 26.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

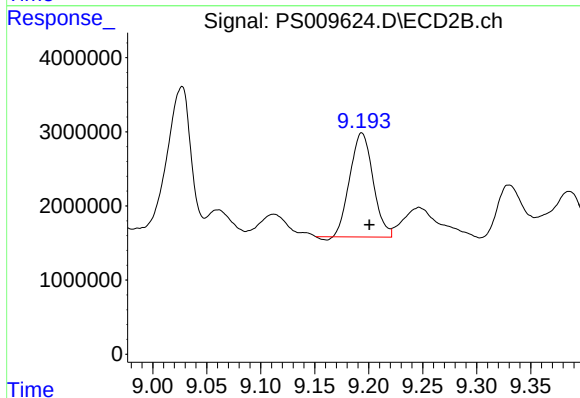


#12 2,4,5-T

R.T.: 9.194 min
Delta R.T.: -0.007 min
Response: 20860426
Conc: 7.07 ng/ml

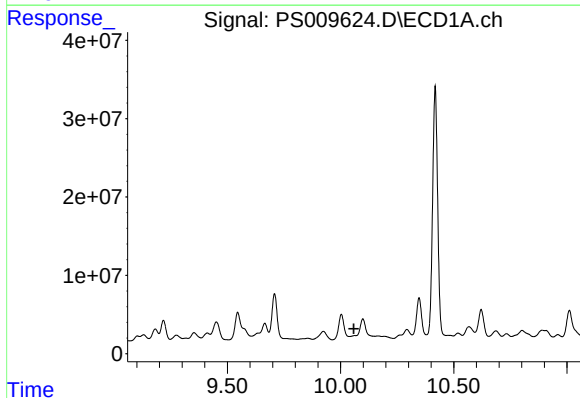


#13 2,4-DB

R.T.: 10.098 min
Delta R.T.: 0.040 min
Response: -10303427
Conc: N.D.

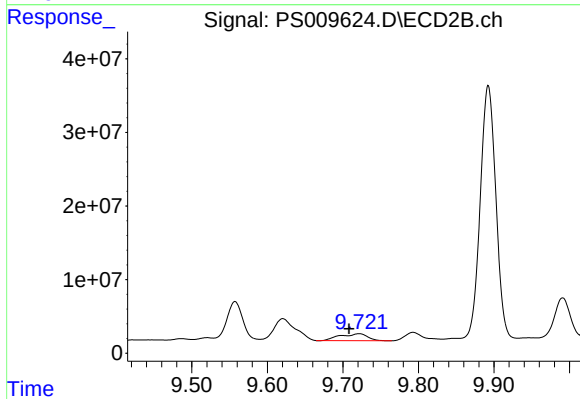

#13 2,4-DB


R.T.: 9.721 min
Delta R.T.: 0.013 min
Response: 24187506
Conc: 63.72 ng/ml

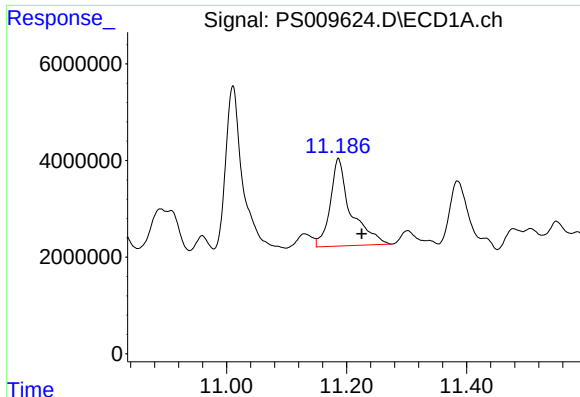

#14 DINOSEB


R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 43260431
Conc: 21.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

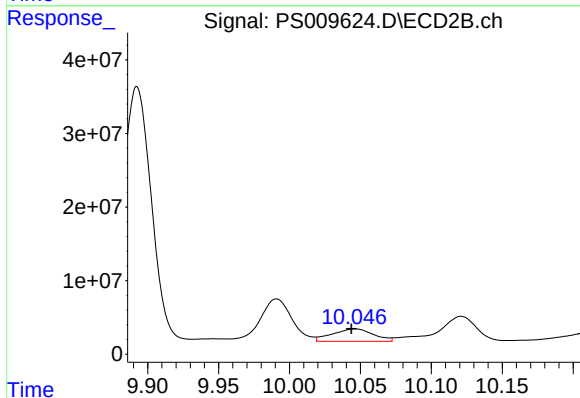


#14 DINOSEB

R.T.: 10.046 min
Delta R.T.: 0.003 min
Response: 34018149
Conc: 15.49 ng/ml

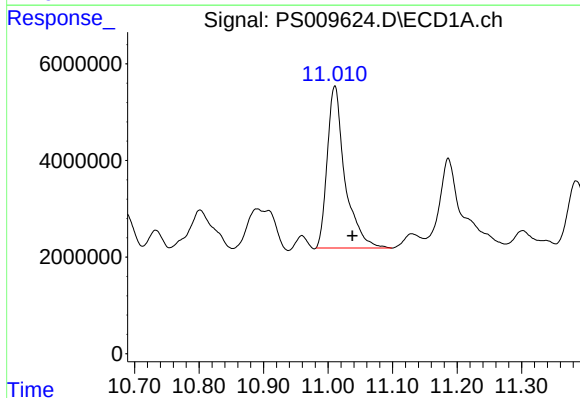


#15 Picloram

R.T.: 11.010 min
Delta R.T.: -0.027 min
Response: 63827356
Conc: 21.03 ng/ml

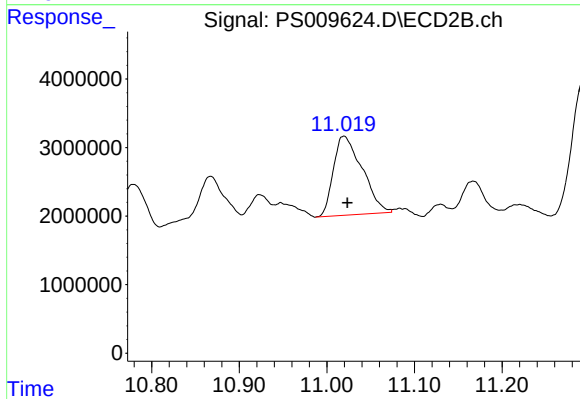

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.004 min
Response: 26345383
Conc: 6.47 ng/ml

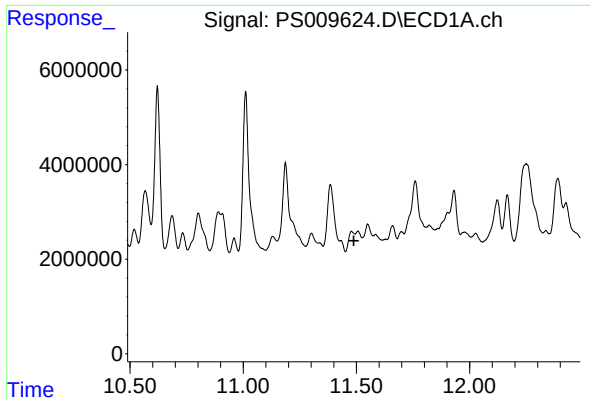

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

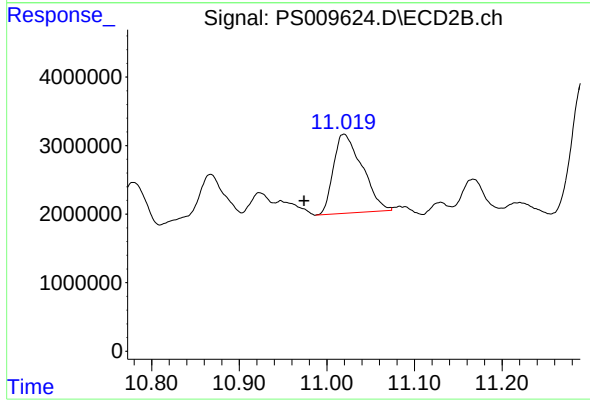

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.046 min
Response: 26345383
Conc: 6.80 ng/ml