

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040720\
 Data File : PS009662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 04:06
 Operator : DD\AJ
 Sample : L2166-13
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-52-46-COMP

Manual Integrations
 APPROVED

Sohil
 4/9/2020 10:16:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 08:20:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.239	6.929	262.9E6	247.2E6	475.277m	450.077

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040720\
Data File : PS009662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 04:06
Operator : DD\AJ
Sample : L2166-13
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-52-46-COMP


Manual Integrations
APPROVED

Sohil
4/9/2020 10:16:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 08:20:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

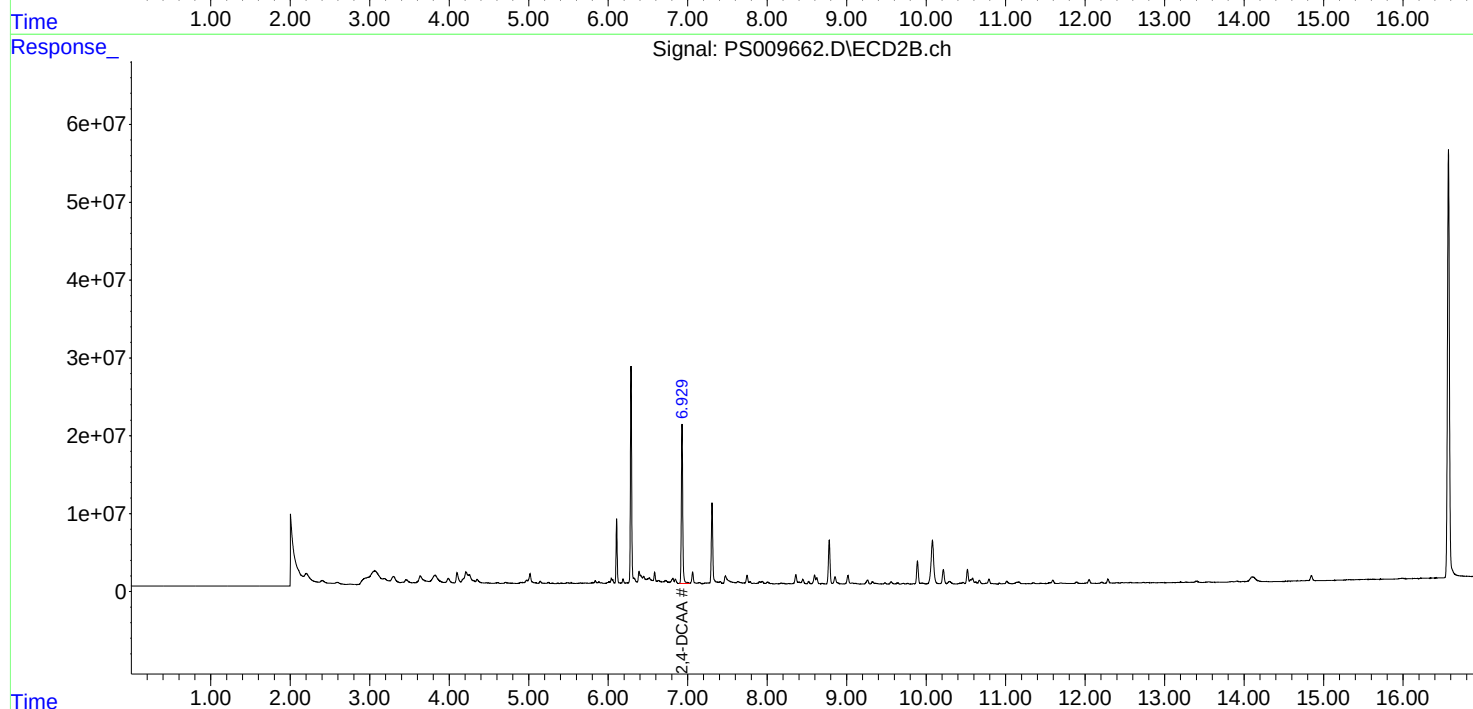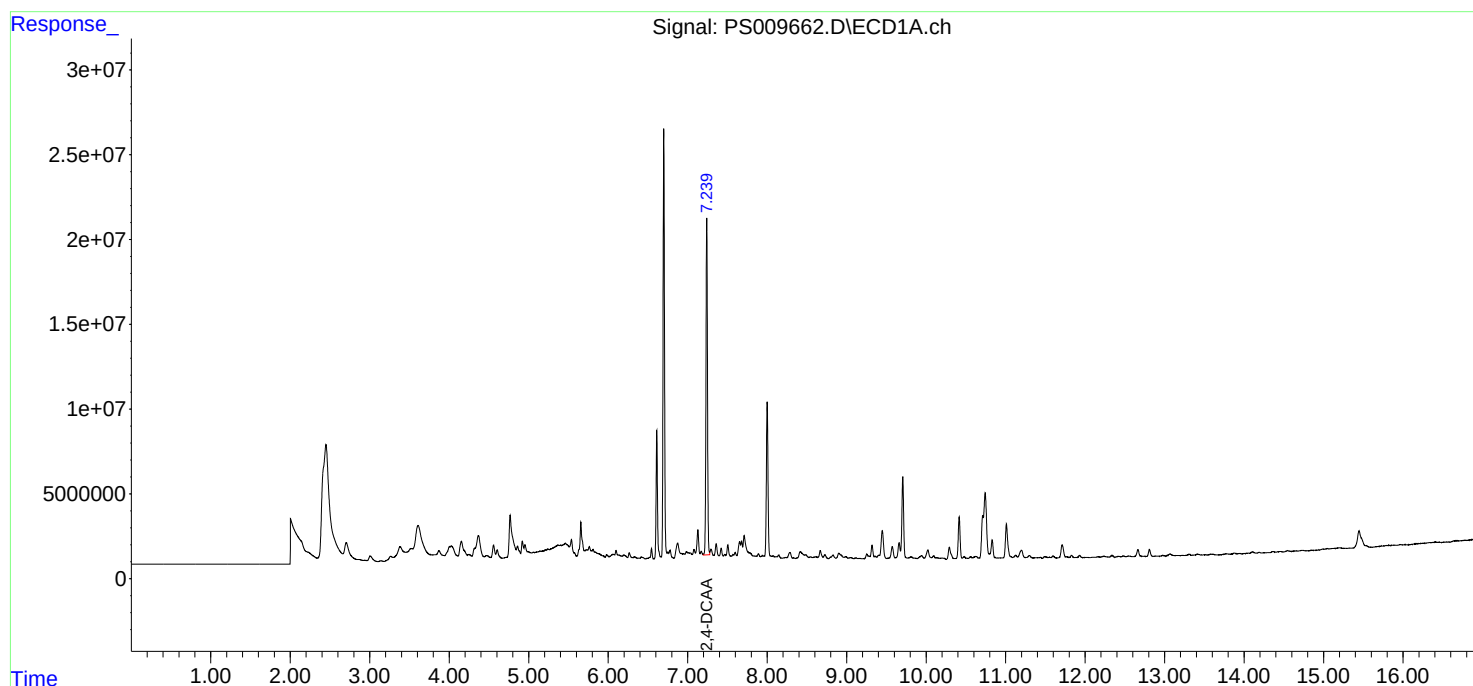

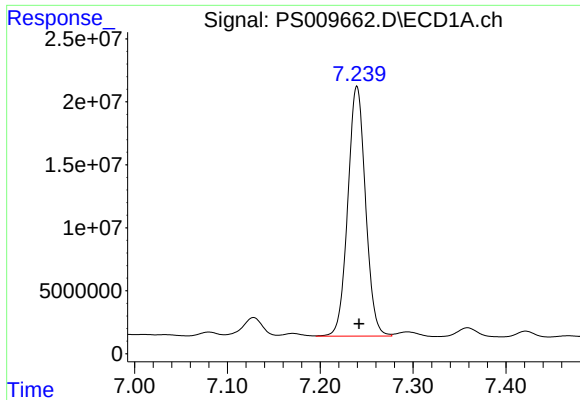


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 262908900
Conc: 475.28 ng/ml m

Instrument :
ECD_S
ClientSampleId :
TP-52-46-COMP

Manual Integrations
APPROVED

Sohil
4/9/2020 10:16:46 AM

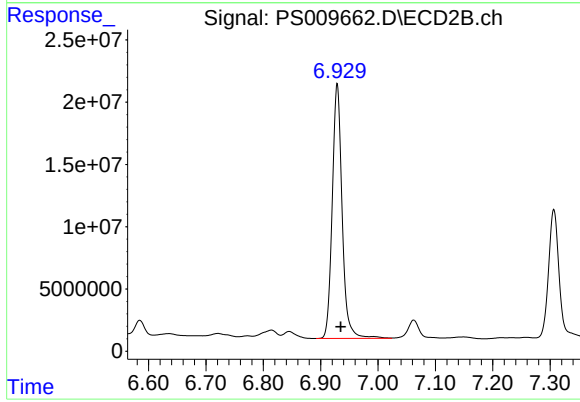

#4 2,4-DCAA

R.T.: 6.929 min
Delta R.T.: -0.006 min
Response: 247181467
Conc: 450.08 ng/ml