

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040721\
 Data File : PS014511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 14:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 15:33:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.885	682.2E6	253.4E6	477.465	537.089
Target Compounds							
7) T	MCPA	7.619f	0.000	7592409	0	1.320	N.D. #
8) T	DICHLORPROP	0.000	7.723f	0	2452736	N.D.	4.814
9) T	2,4-D	8.323f	0.000	21613970	0	14.664	N.D. #
15) T	Picloram	10.997f	0.000	6514825	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040721\
Data File : PS014511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 14:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 15:33:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

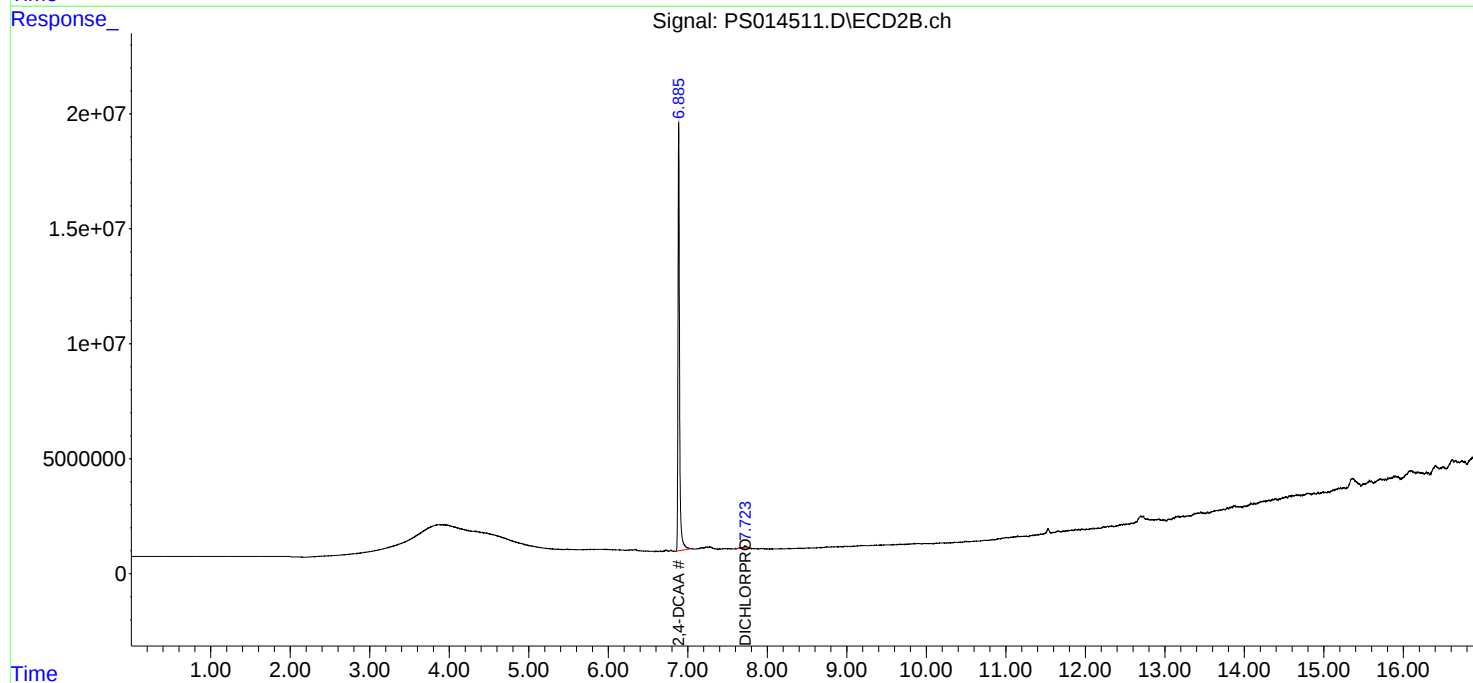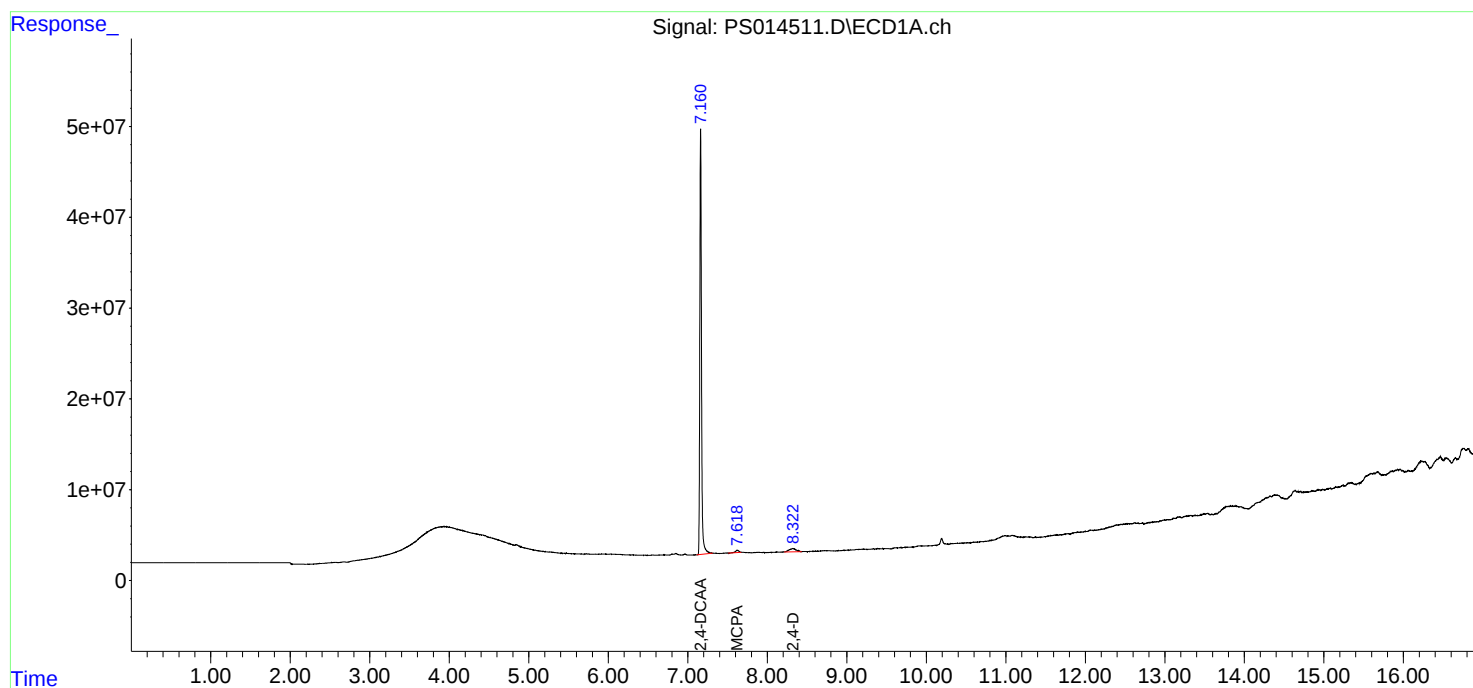


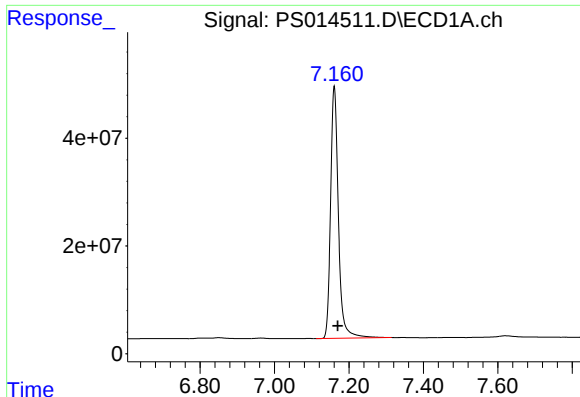

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: -0.010 min
Response: 682222704
Conc: 477.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

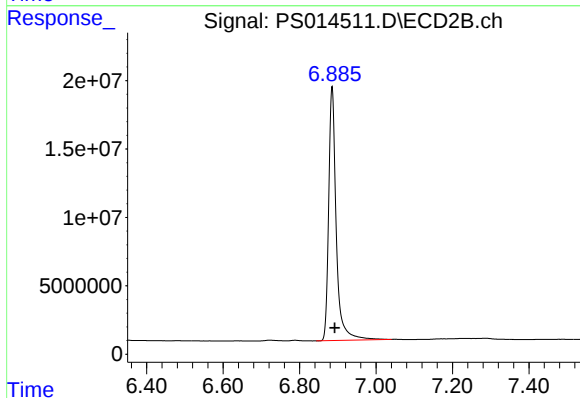


#4 2,4-DCAA

R.T.: 6.885 min
Delta R.T.: -0.007 min
Response: 253382000
Conc: 537.09 ng/ml

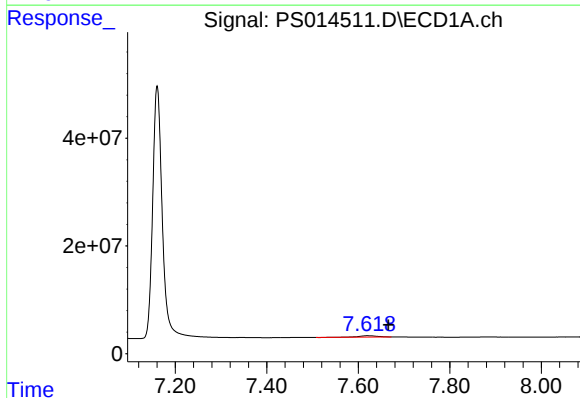


#7 MCPA

R.T.: 7.619 min
Delta R.T.: -0.047 min
Response: 7592409
Conc: 1.32 ug/ml

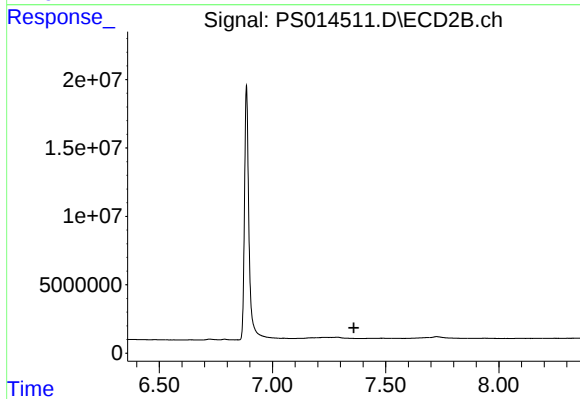

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.359 min
Response: 0
Conc: N.D.

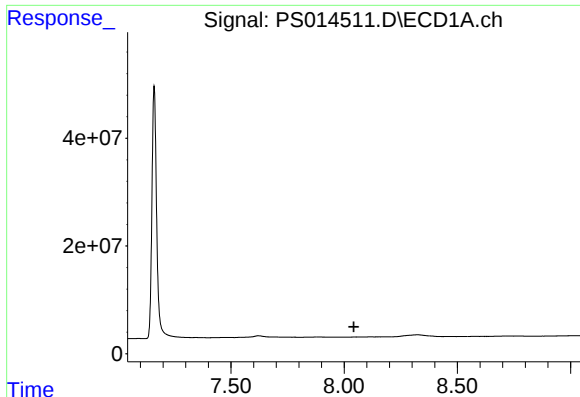

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

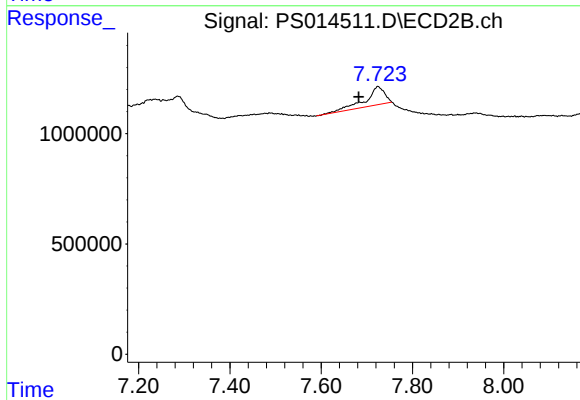


#8 DICHLORPROP

R.T.: 7.723 min
Delta R.T.: 0.041 min
Response: 2452736
Conc: 4.81 ng/ml

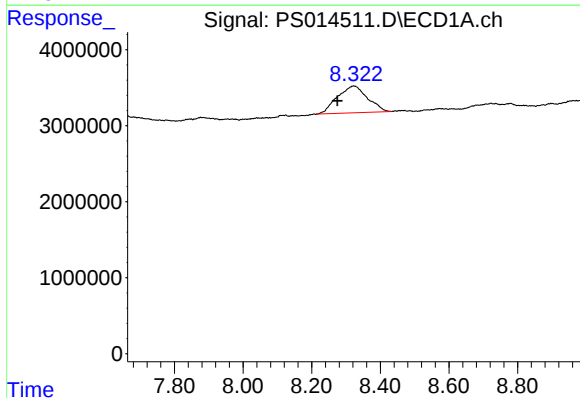

#9 2,4-D

R.T.: 8.323 min
Delta R.T.: 0.048 min
Response: 21613970
Conc: 14.66 ng/ml

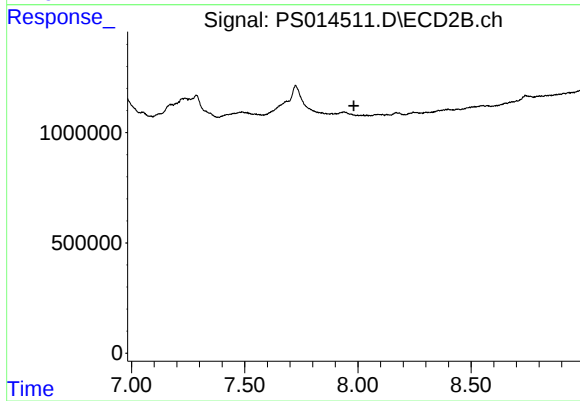

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.