

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040722\
 Data File : PS018922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2022 08:49
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:17:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.481f	0.000	63315706	0	15.783	N.D. #
3) T	4-Nitroph...	7.018f	0.000	8204054	0	7.187	N.D. #
5) T	DICAMBA	0.000	7.031f	0	46520661	N.D.	14.613
6) T	MCP	0.000	7.031f	0	46520661	N.D.	18.183
7) T	MCPA	7.683f	0.000	20646967	0	1.451	N.D. #
8) T	DICHLORPROP	0.000	7.619	0	6125038	N.D.	7.448
9) T	2,4-D	8.415f	0.000	430.2E6	0	107.659	N.D. #
10) T	Pentachlo...	8.663	0.000	6912866	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.213	8.637f	-2552704	6060276	N.D.	1.326
12) T	2,4,5-T	9.501	9.119f	10392745	6717060	<MDL	1.613 #
13) T	2,4-DB	10.086f	0.000	2758529	0	<MDL	N.D. #
15) T	Picloram	11.047	10.883	285.7E6	36509109	10.211	6.457 #
16) T	DCPA	0.000	10.824	0	3156802	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040722\
Data File : PS018922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2022 08:49
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:17:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

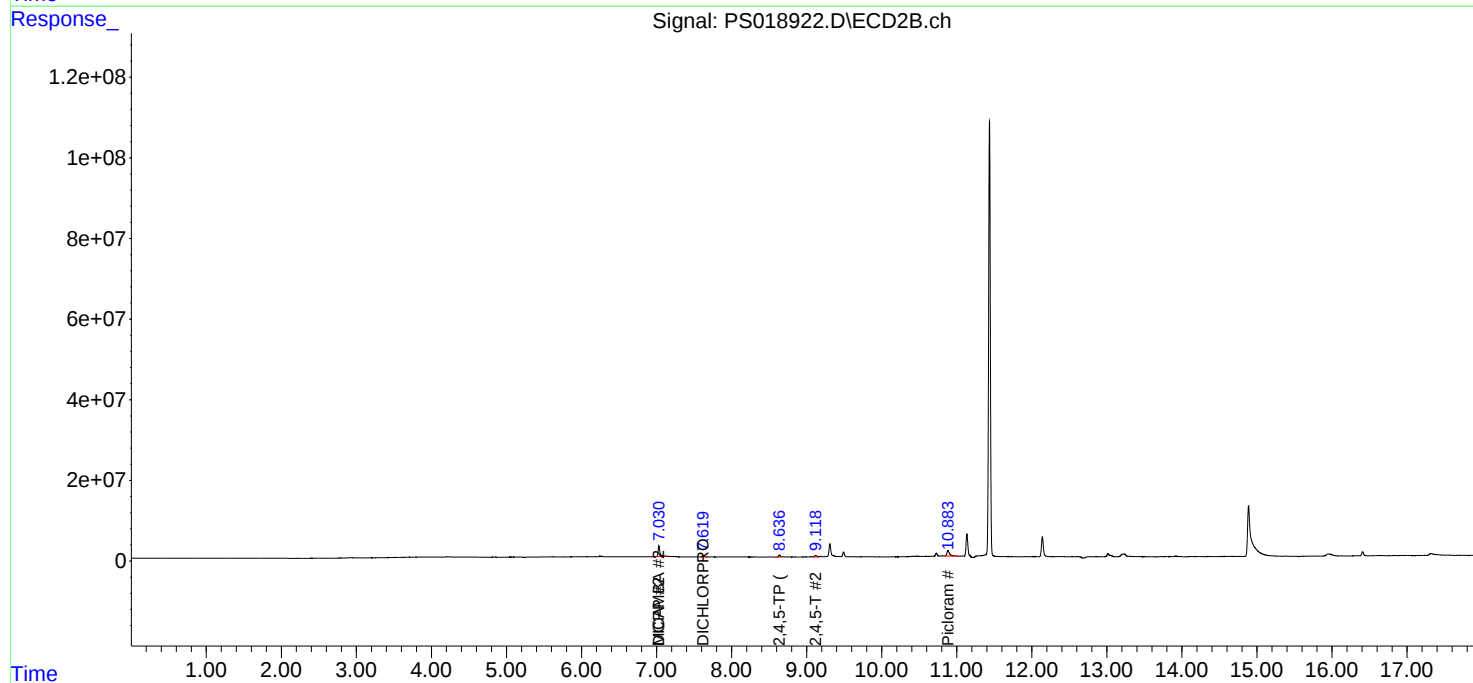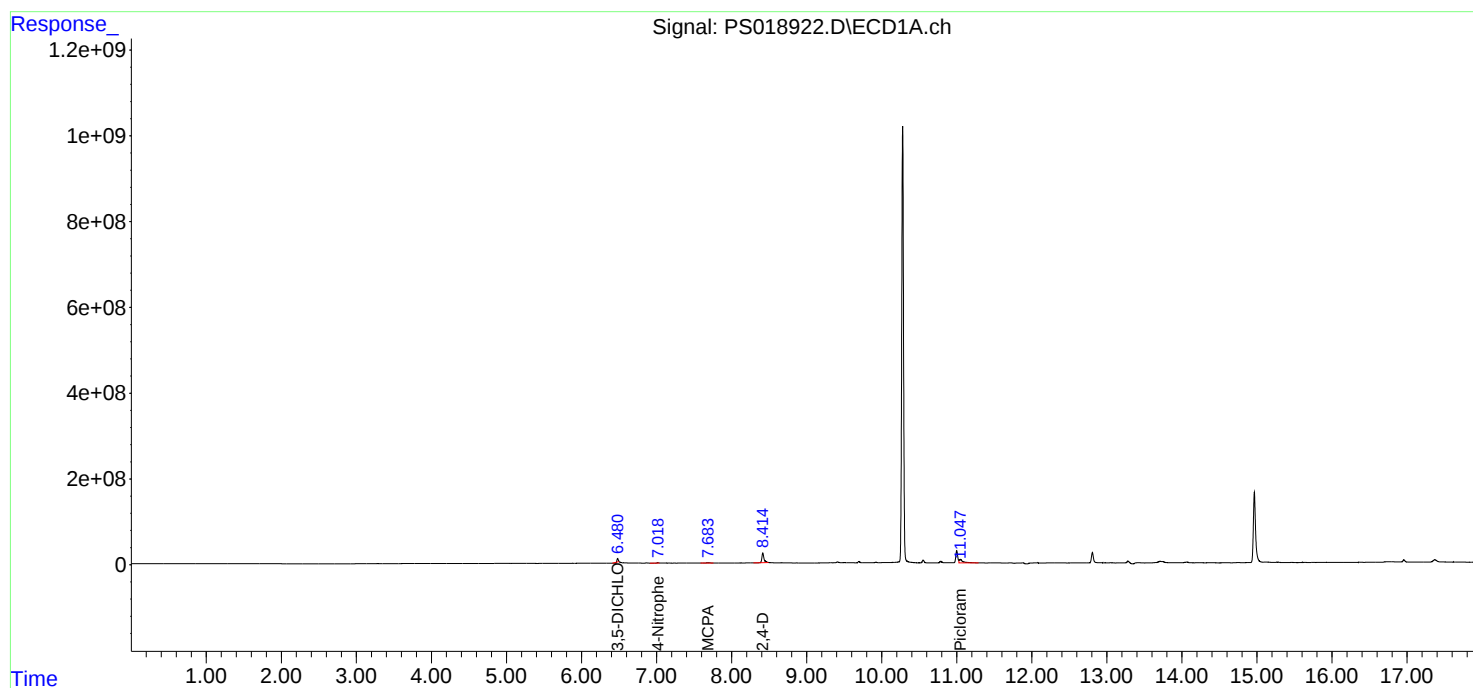


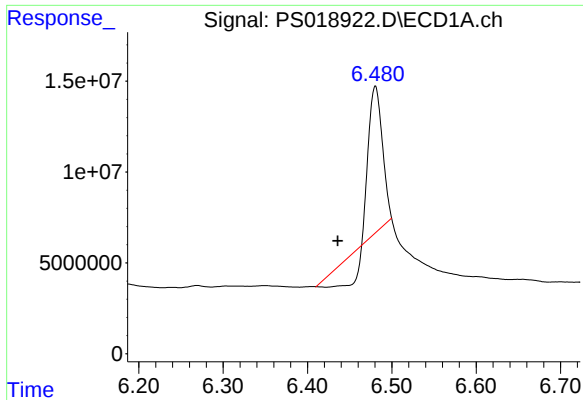

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.481 min
Delta R.T.: 0.045 min
Response: 63315706
Conc: 15.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

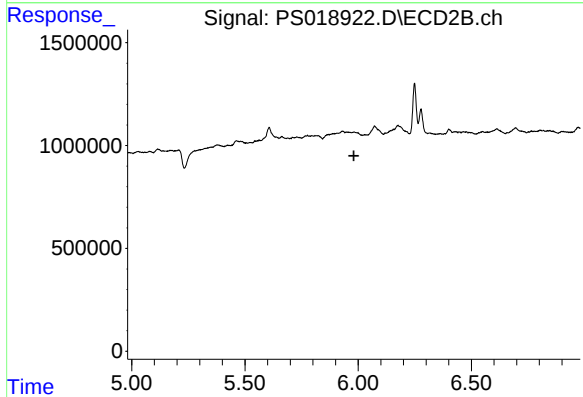


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.981 min
Response: 0
Conc: N.D.

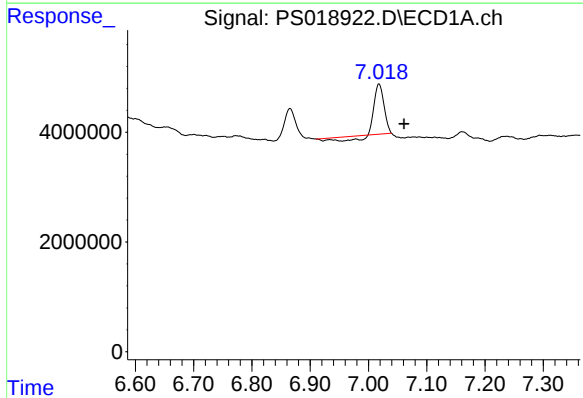


#3 4-Nitrophenol

R.T.: 7.018 min
Delta R.T.: -0.043 min
Response: 8204054
Conc: 7.19 ng/ml

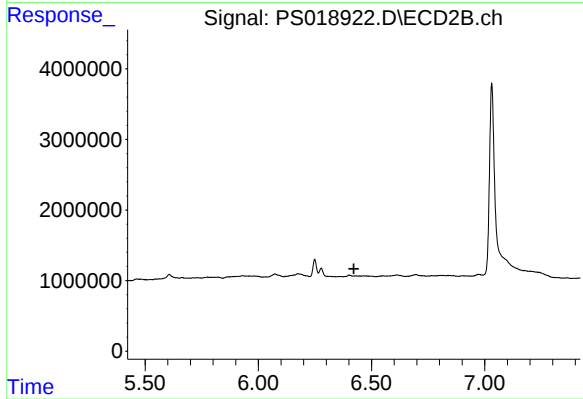

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

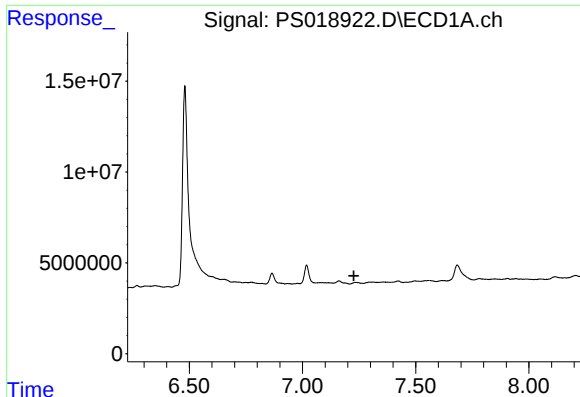

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

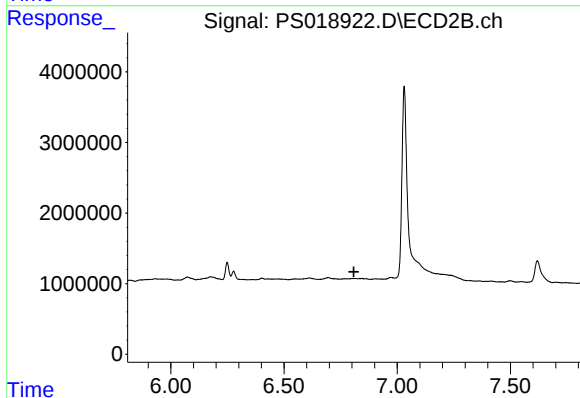


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

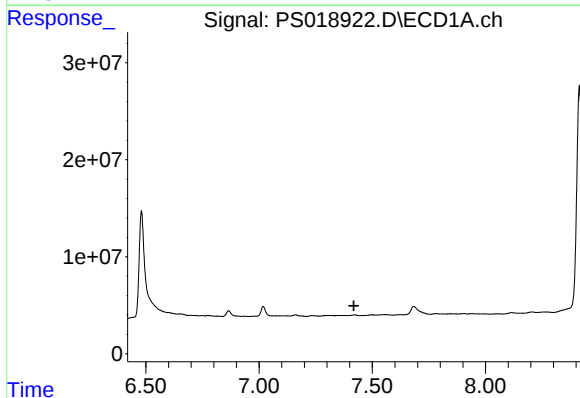


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

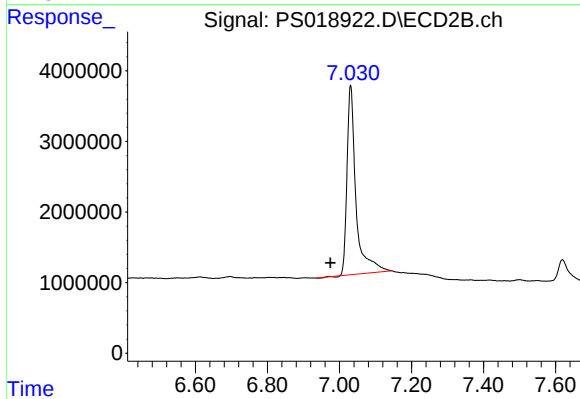

#5 DICAMBA


R.T.: 7.031 min
Delta R.T.: 0.056 min
Response: 46520661
Conc: 14.61 ng/ml

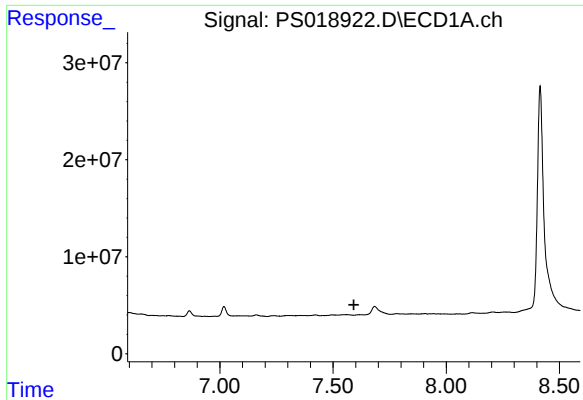

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

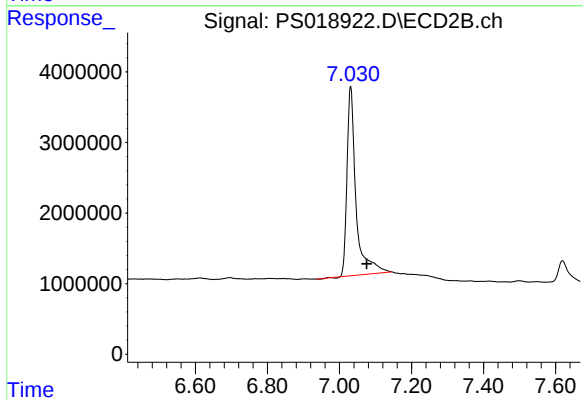


#6 MCP

R.T.: 7.031 min
Delta R.T.: -0.045 min
Response: 46520661
Conc: 18.18 ug/ml

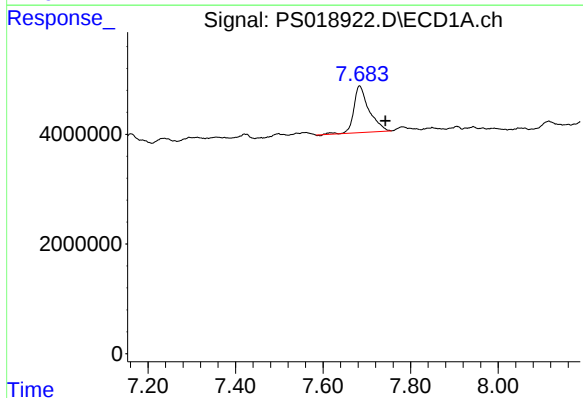


#7 MCP

R.T.: 7.683 min
Delta R.T.: -0.059 min
Response: 20646967
Conc: 1.45 ug/ml

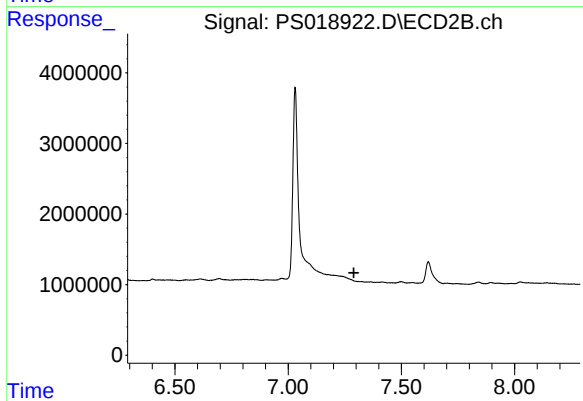

#7 MCP


R.T.: 0.000 min
Exp R.T.: 7.290 min
Response: 0
Conc: N.D.

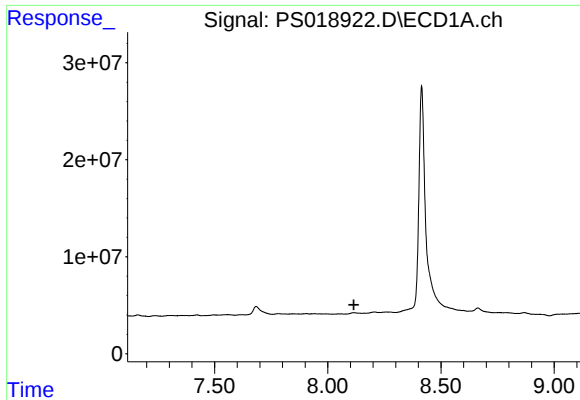

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

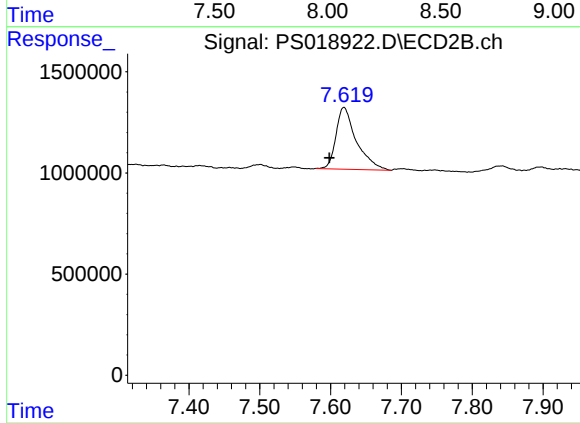


#8 DICHLORPROP

R.T.: 7.619 min
Delta R.T.: 0.021 min
Response: 6125038
Conc: 7.45 ng/ml

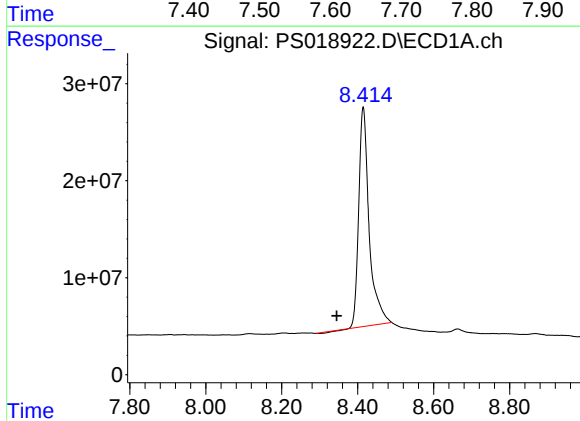


#9 2,4-D

R.T.: 8.415 min
Delta R.T.: 0.070 min
Response: 430230754
Conc: 107.66 ng/ml

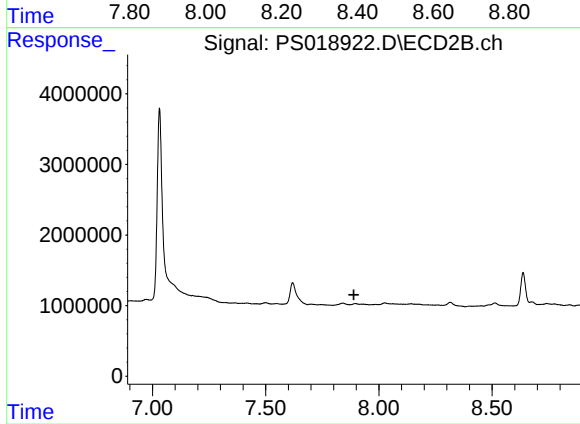

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.890 min
Response: 0
Conc: N.D.

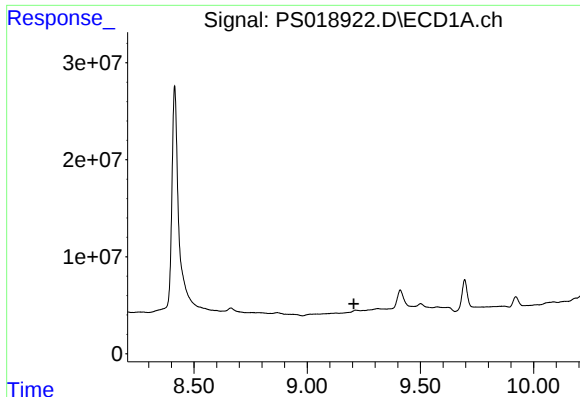

#11 2,4,5-TP (SILVEX)


R.T.: 9.213 min
Delta R.T.: 0.007 min
Response: -2552704
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

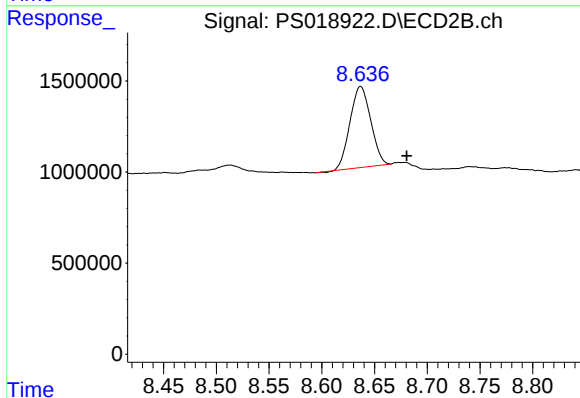


#11 2,4,5-TP (SILVEX)

R.T.: 8.637 min
Delta R.T.: -0.044 min
Response: 6060276
Conc: 1.33 ng/ml

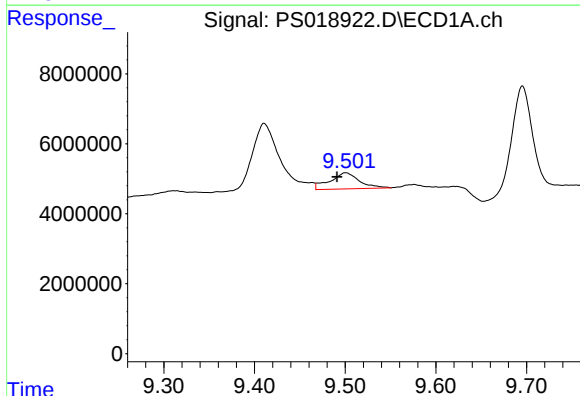


#12 2,4,5-T

R.T.: 9.501 min
Delta R.T.: 0.009 min
Response: 10392745
Conc: N.D.

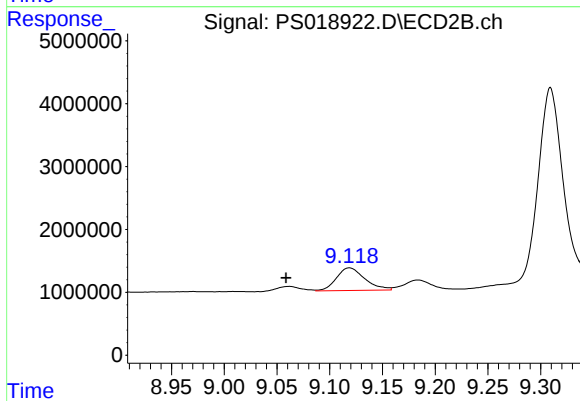

#12 2,4,5-T


R.T.: 9.119 min
Delta R.T.: 0.060 min
Response: 6717060
Conc: 1.61 ng/ml

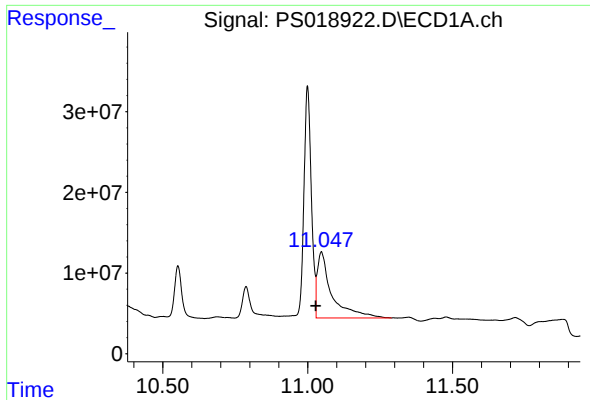

#15 Picloram

R.T.: 11.047 min
Delta R.T.: 0.019 min
Response: 285681082
Conc: 10.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

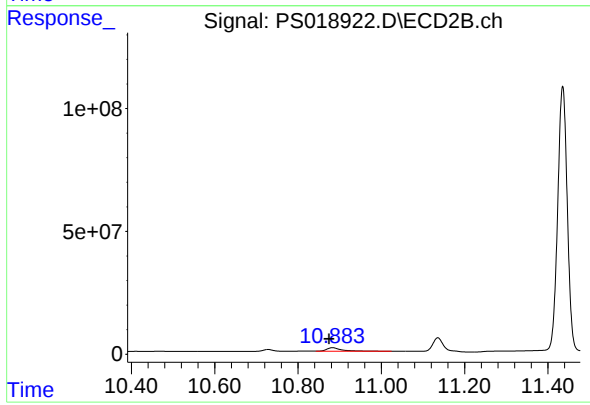

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.008 min
Response: 36509109
Conc: 6.46 ng/ml