

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040722\
 Data File : PS018935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2022 17:24
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:20:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.804	1572.1E6	343.6E6	538.499	481.262
Target Compounds							
3) T	4-Nitroph...	7.029	0.000	1749867	0	1.533	N.D. #
5) T	DICAMBA	7.486f	0.000	640844	0	<MDL	N.D. #
7) T	MCPA	7.682f	0.000	4711255	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.619	0	1739791	N.D.	2.116
11) T	2,4,5-TP ...	0.000	8.637f	0	9181589	N.D.	2.009
12) T	2,4,5-T	0.000	9.128f	0	1702930	N.D.	<MDL
14) T	DINOSEB	11.136f	0.000	18021774	0	1.104	N.D. #
15) T	Picloram	11.058	10.896	35143163	5357000	1.256	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040722\
Data File : PS018935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2022 17:24
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:20:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

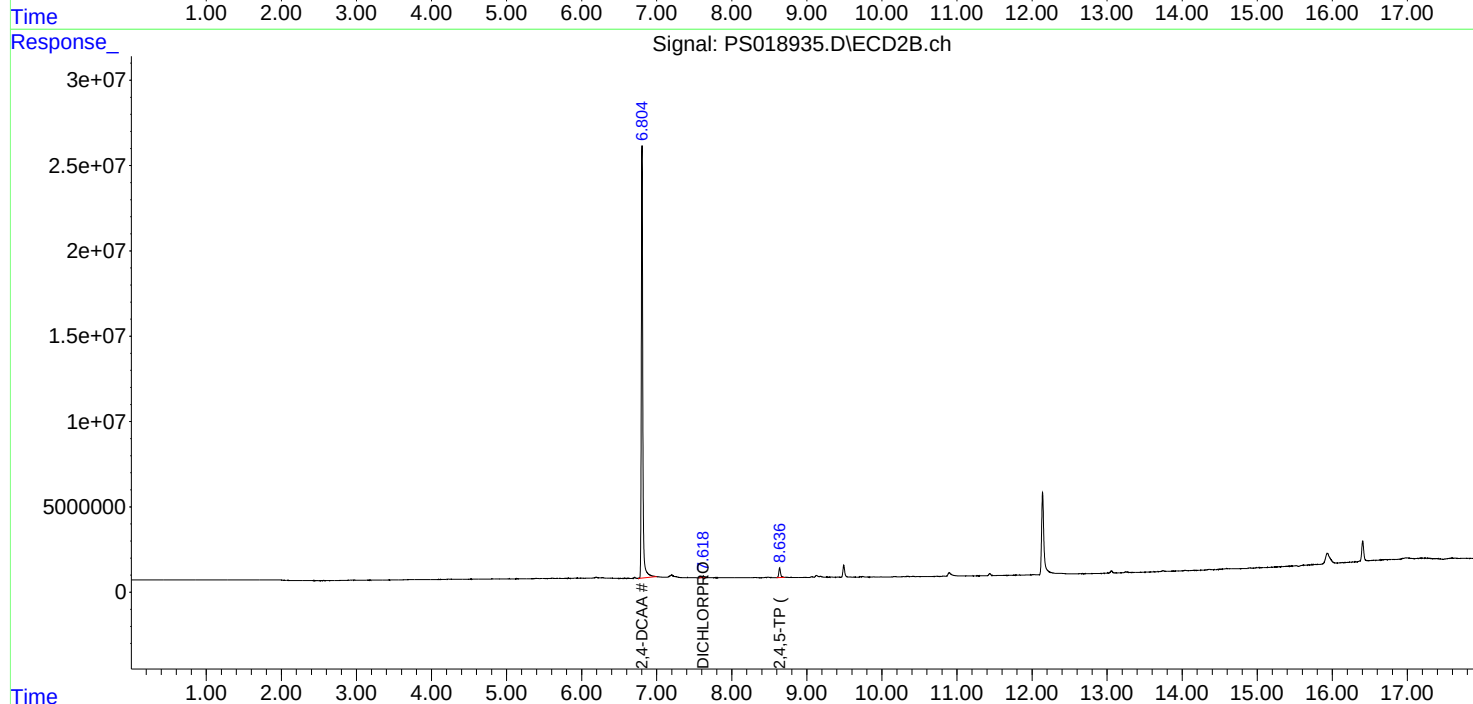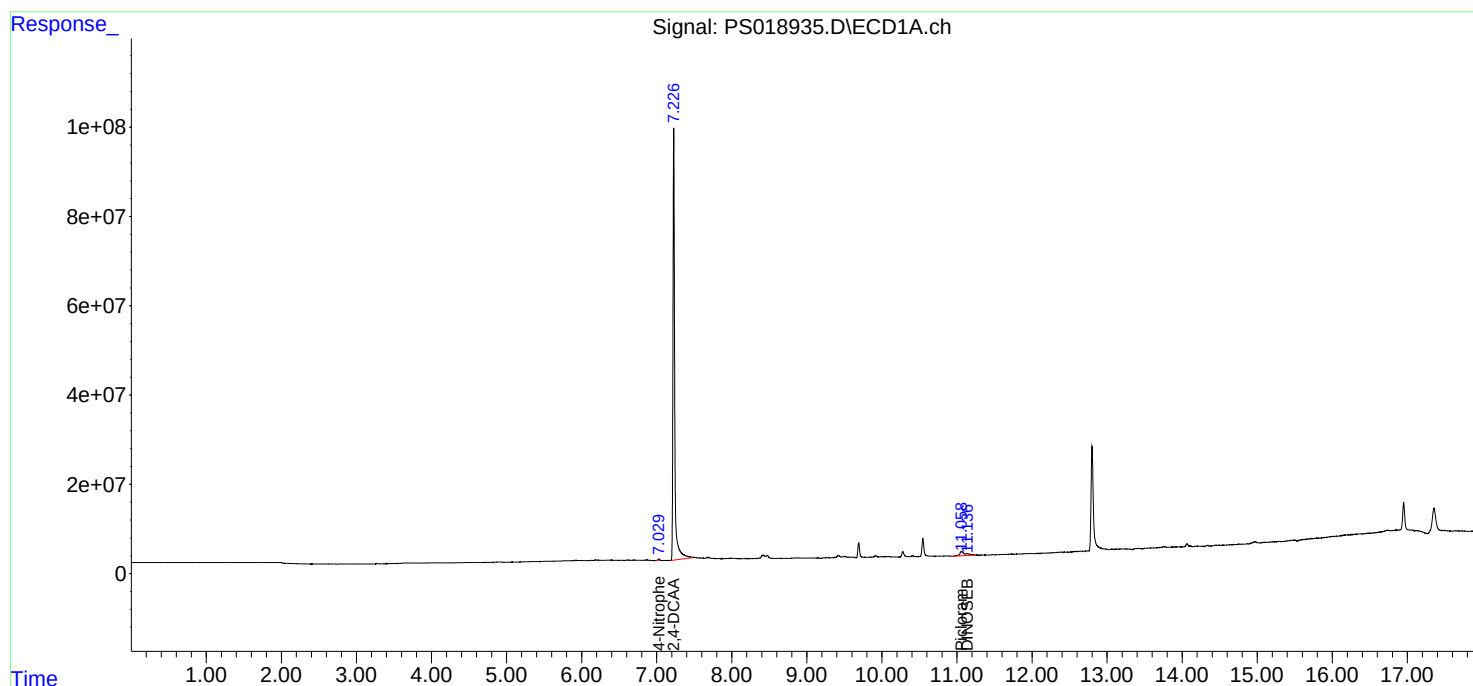


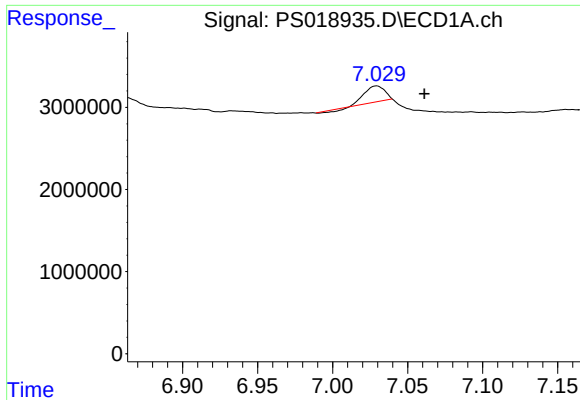

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.032 min
Response: 1749867
Conc: 1.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

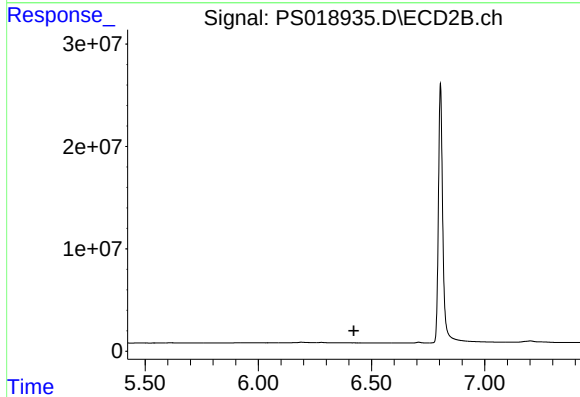


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

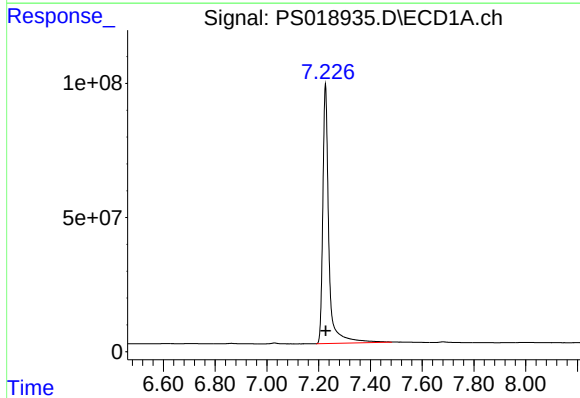


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: -0.001 min
Response: 1572125933
Conc: 538.50 ng/ml

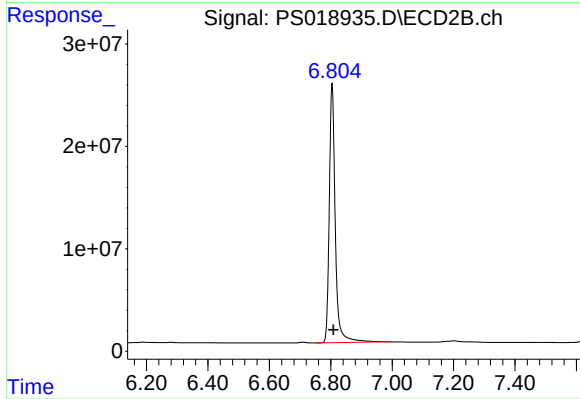

#4 2,4-DCAA


R.T.: 6.804 min
Delta R.T.: -0.004 min
Response: 343593642
Conc: 481.26 ng/ml

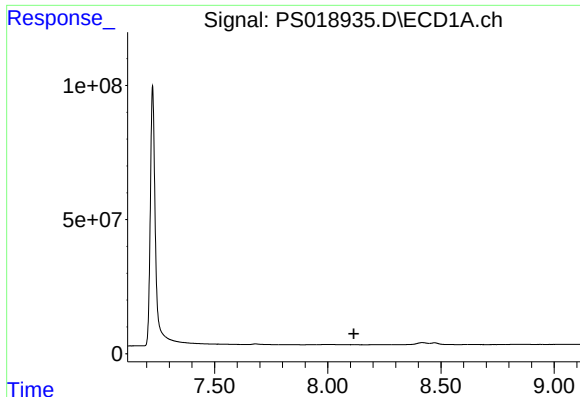

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

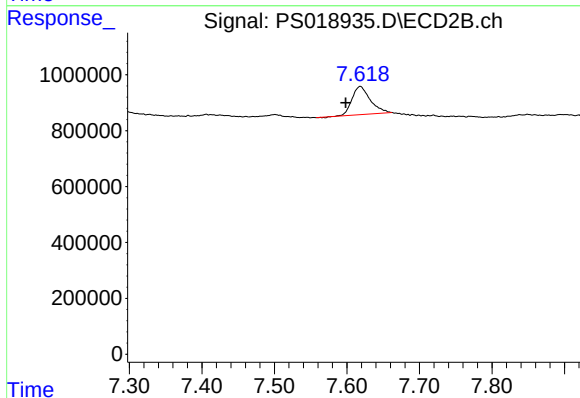


#8 DICHLORPROP

R.T.: 7.619 min
Delta R.T.: 0.020 min
Response: 1739791
Conc: 2.12 ng/ml

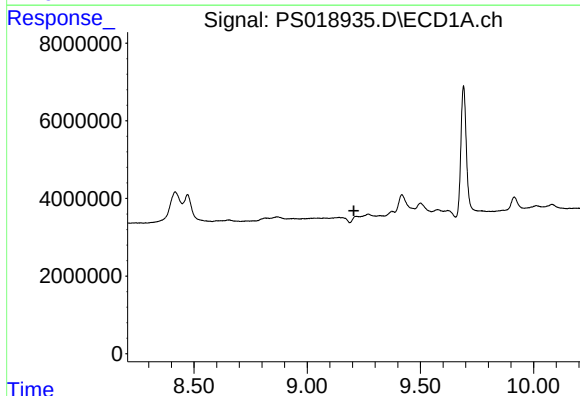


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.206 min
Response: 0
Conc: N.D.

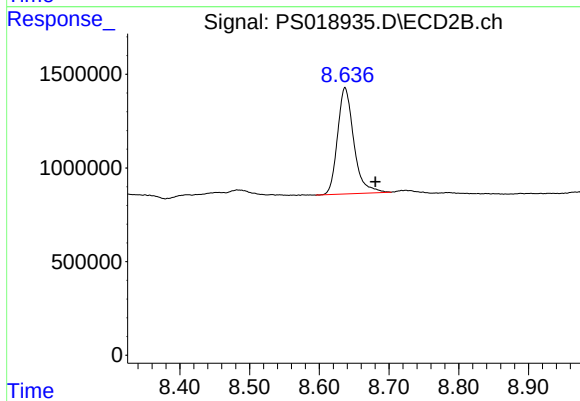

#11 2,4,5-TP (SILVEX)


R.T.: 8.637 min
Delta R.T.: -0.044 min
Response: 9181589
Conc: 2.01 ng/ml

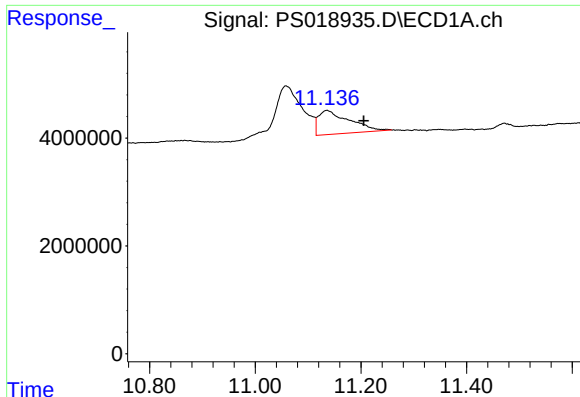

#14 DINOSEB


R.T.: 11.136 min
Delta R.T.: -0.070 min
Response: 18021774
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

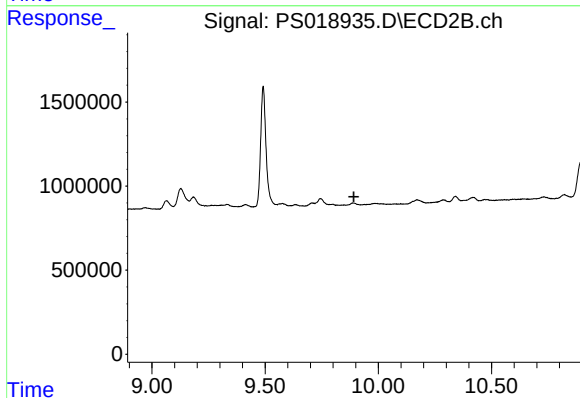


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.892 min
Response: 0
Conc: N.D.

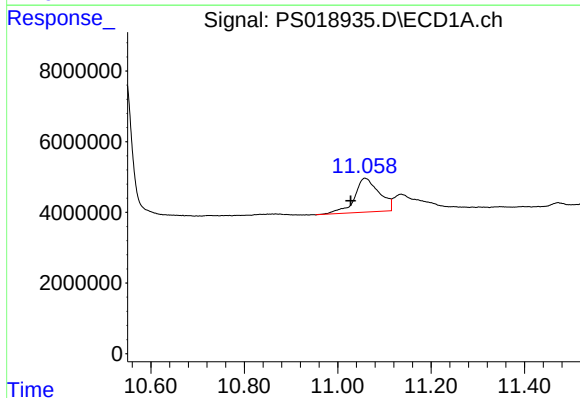

#15 Picloram

R.T.: 11.058 min
Delta R.T.: 0.030 min
Response: 35143163
Conc: 1.26 ng/ml

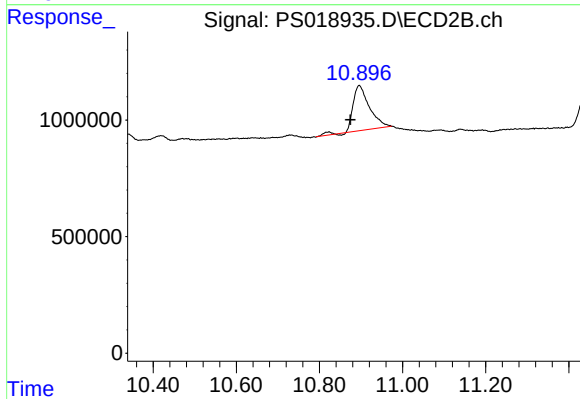

#15 Picloram

R.T.: 10.896 min
Delta R.T.: 0.021 min
Response: 5357000
Conc: N.D.