

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040722\
 Data File : PS018936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2022 17:48
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:20:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.803	2688.2E6	567.6E6	920.803	795.061
Target Compounds							
1) T	Dalapon	3.028	2.530	2919.6E6	605.5E6	638.232	652.856
2) T	3,5-DICHL...	6.434	5.978	3547.6E6	809.4E6	884.337	734.107
3) T	4-Nitroph...	7.056	6.418	609.2E6	297.4E6	533.666	700.102 #
5) T	DICAMBA	7.416	6.970	10309.2E6	2368.4E6	819.945	743.989
6) T	MCP	7.588	7.069	830.4E6	189.8E6	81.393	74.166
7) T	MCPA	7.738	7.283	1124.3E6	260.6E6	78.987	72.725
8) T	DICHLORPROP	8.110	7.592	2549.0E6	613.1E6	764.660	745.520
9) T	2,4-D	8.340	7.884	3043.3E6	701.1E6	761.531	758.591
10) T	Pentachlo...	8.650	8.313	33011.4E6	7787.1E6	737.823	739.997
11) T	2,4,5-TP ...	9.201	8.674	13818.2E6	3470.9E6	675.326	759.277
12) T	2,4,5-T	9.486	9.052	13582.0E6	3251.2E6	662.494	780.752
13) T	2,4-DB	10.039	9.558	2290.5E6	435.3E6	674.702	764.275
14) T	DINOSEB	11.201	9.887	10137.9E6	2405.0E6	620.953	745.786
15) T	Picloram	11.020	10.867	18087.6E6	4081.8E6	646.492	721.912
16) T	DCPA	11.468	10.818	16549.1E6	4190.8E6	657.497	768.858



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040722\
Data File : PS018936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2022 17:48
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:20:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

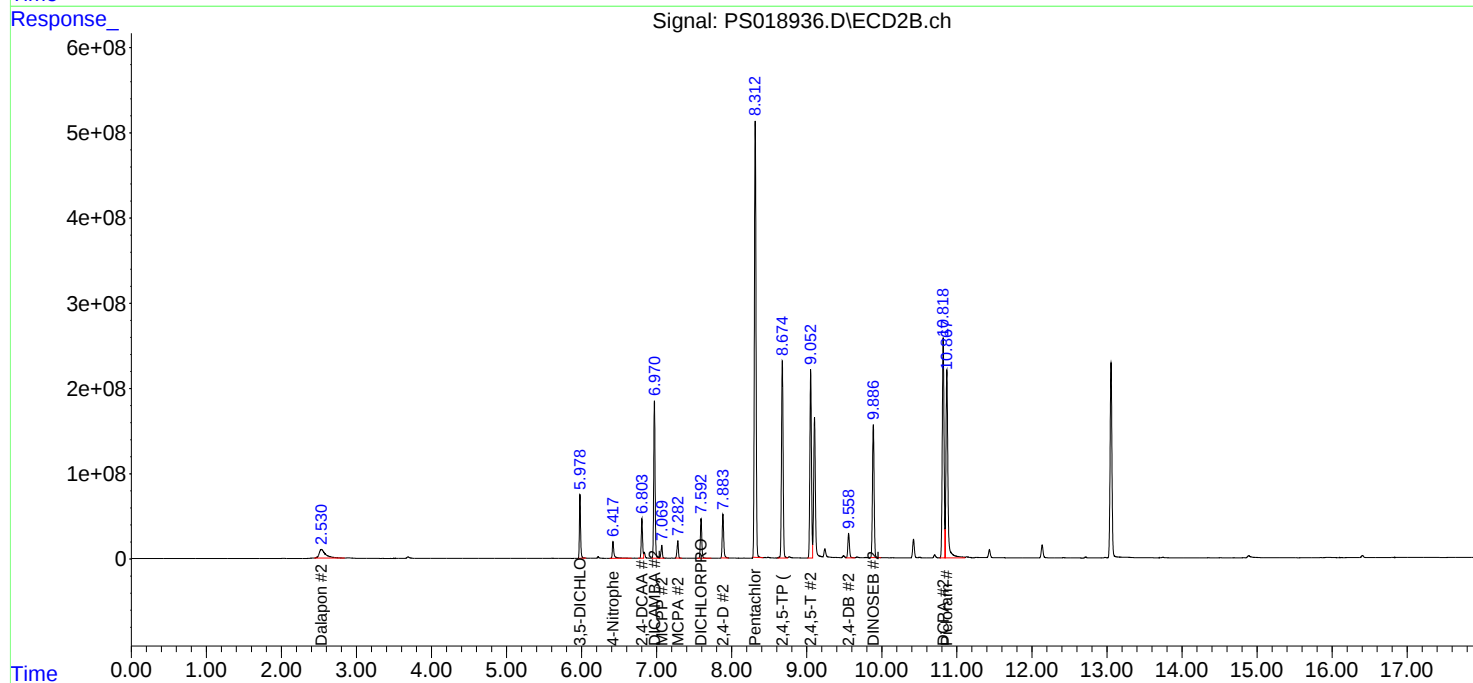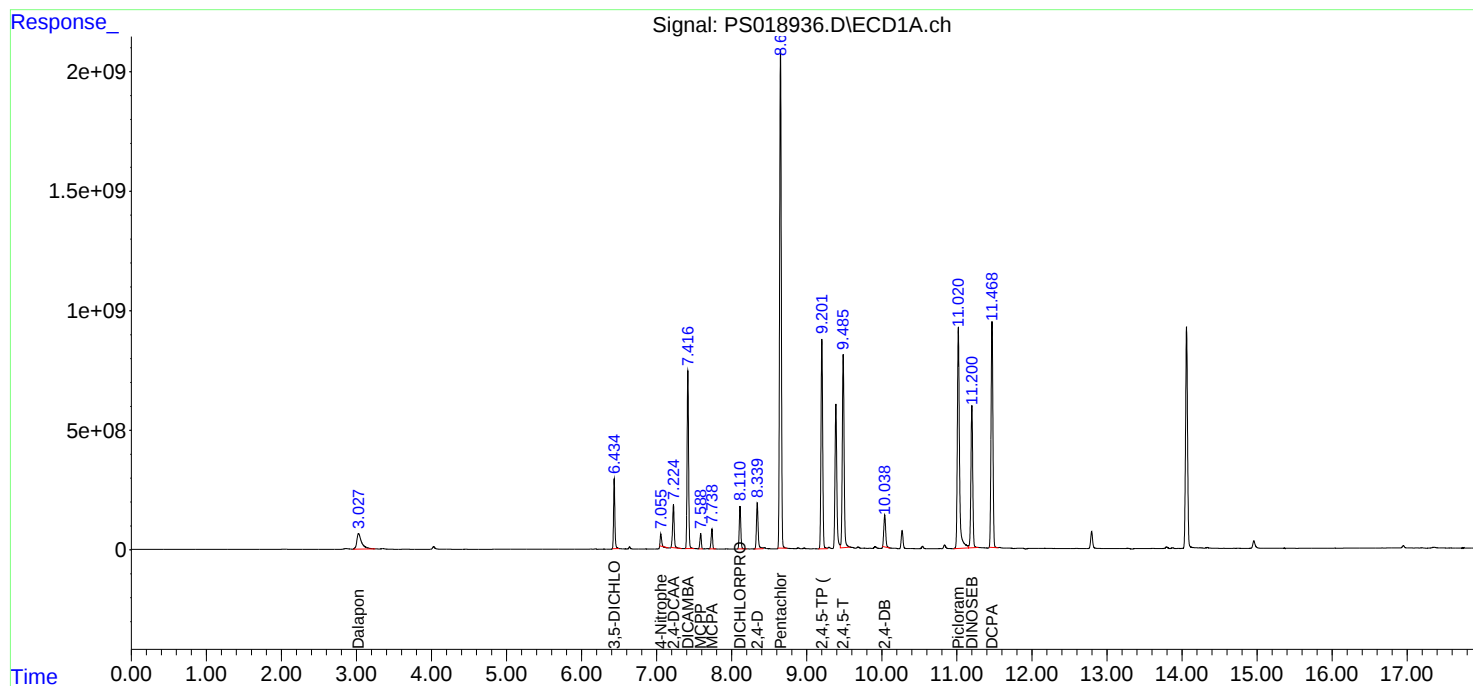


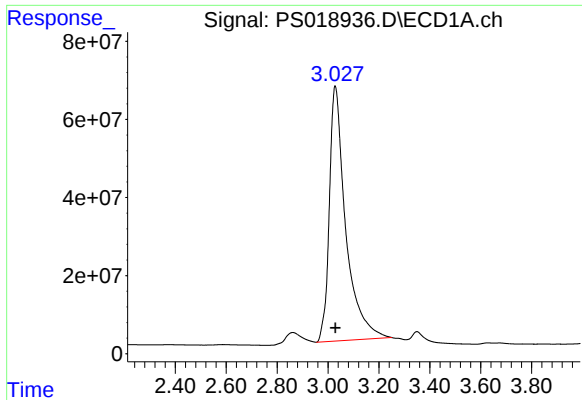

#1 Dalapon


R.T.: 3.028 min
Delta R.T.: -0.001 min
Response: 2919568189
Conc: 638.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

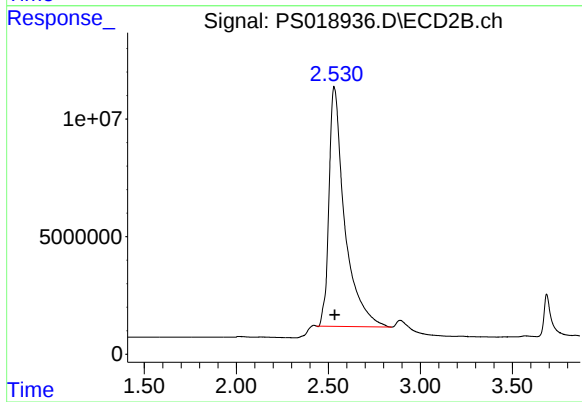


#1 Dalapon

R.T.: 2.530 min
Delta R.T.: -0.004 min
Response: 605539885
Conc: 652.86 ng/ml

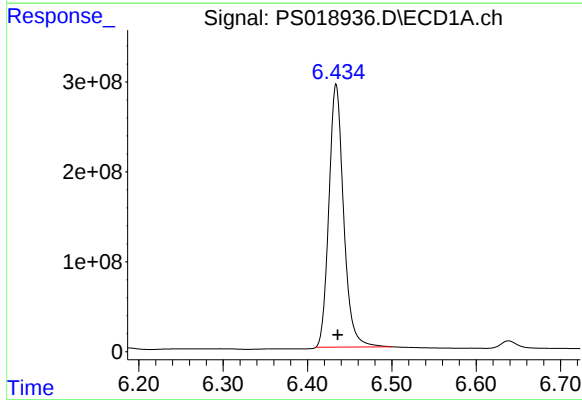


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.434 min
Delta R.T.: -0.002 min
Response: 3547646783
Conc: 884.34 ng/ml

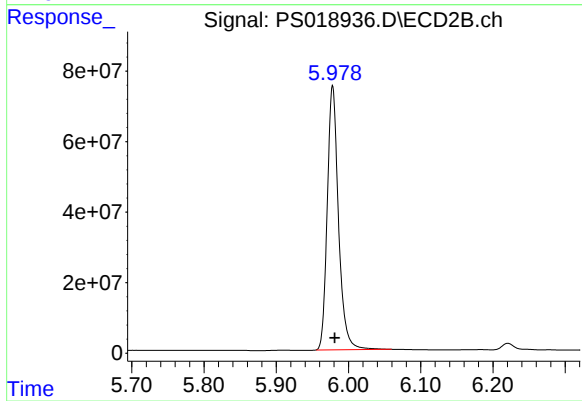

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.978 min
Delta R.T.: -0.003 min
Response: 809443431
Conc: 734.11 ng/ml

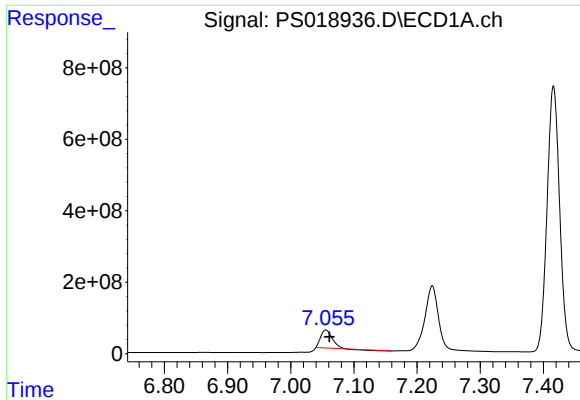

#3 4-Nitrophenol


R.T.: 7.056 min
Delta R.T.: -0.006 min
Response: 609181384
Conc: 533.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

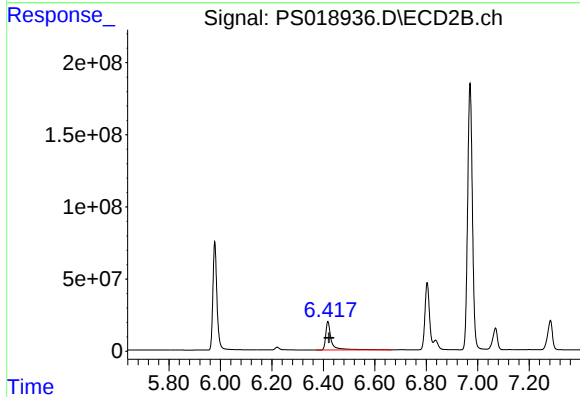


#3 4-Nitrophenol

R.T.: 6.418 min
Delta R.T.: -0.004 min
Response: 297382340
Conc: 700.10 ng/ml

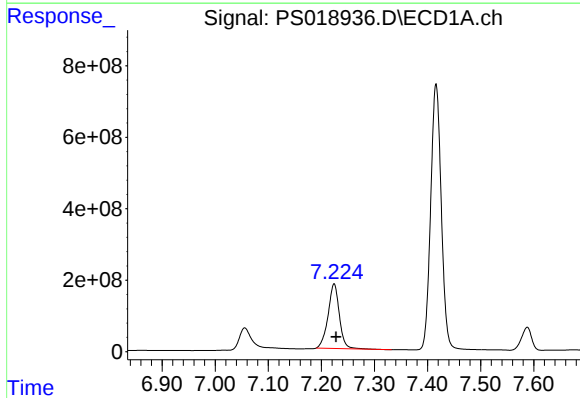


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.003 min
Response: 2688247446
Conc: 920.80 ng/ml

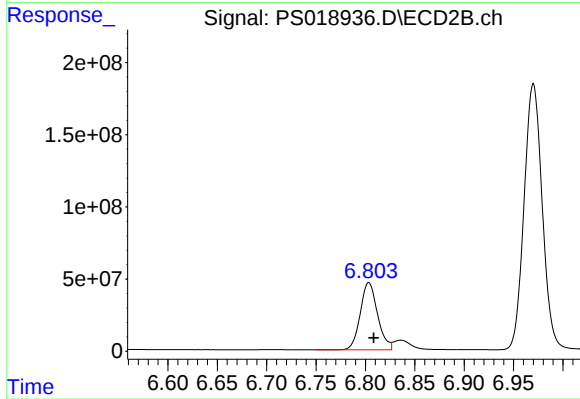

#4 2,4-DCAA


R.T.: 6.803 min
Delta R.T.: -0.005 min
Response: 567627984
Conc: 795.06 ng/ml

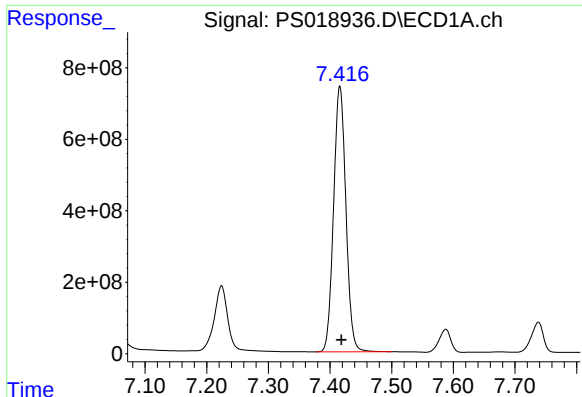

#5 DICAMBA


R.T.: 7.416 min
Delta R.T.: -0.003 min
Response: 10309221943
Conc: 819.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

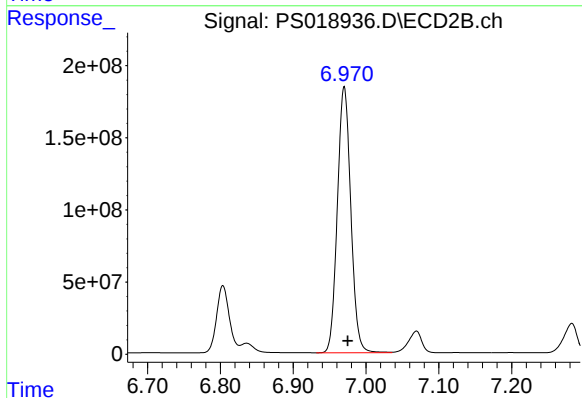


#5 DICAMBA

R.T.: 6.970 min
Delta R.T.: -0.005 min
Response: 2368425076
Conc: 743.99 ng/ml

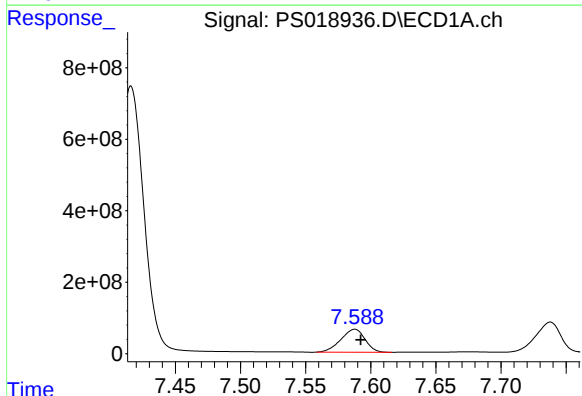


#6 MCP

R.T.: 7.588 min
Delta R.T.: -0.004 min
Response: 830420902
Conc: 81.39 ug/ml

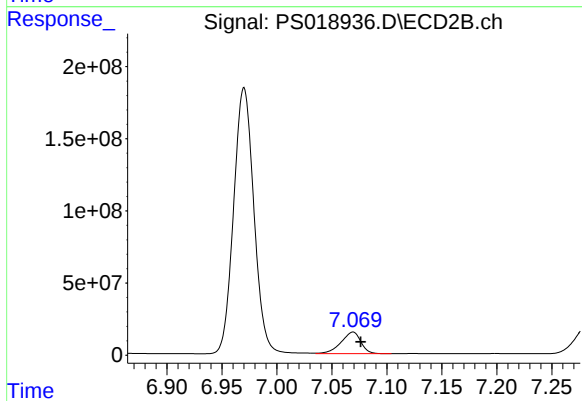

#6 MCP


R.T.: 7.069 min
Delta R.T.: -0.007 min
Response: 189753052
Conc: 74.17 ug/ml

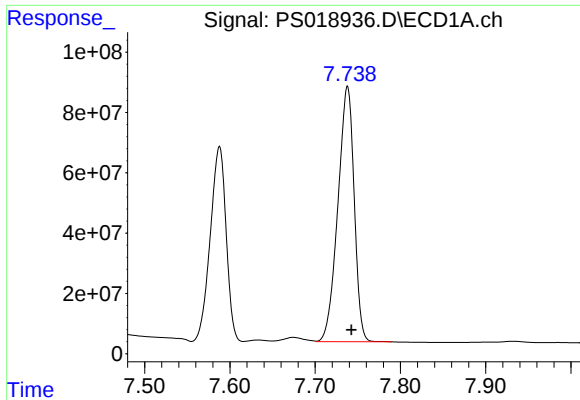

#7 MCPA


R.T.: 7.738 min
Delta R.T.: -0.004 min
Response: 1124310143
Conc: 78.99 ug/ml

Instrument :
ECD_S
ClientSampleId :

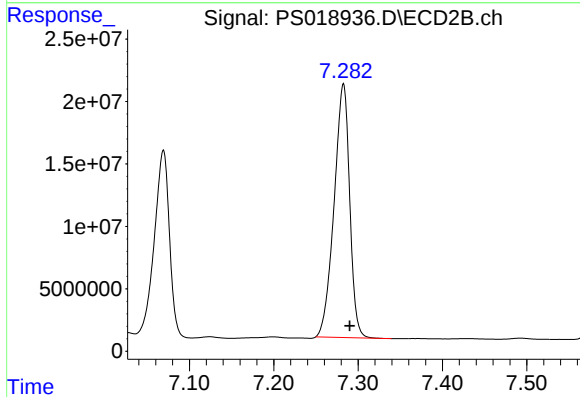


#7 MCPA

R.T.: 7.283 min
Delta R.T.: -0.008 min
Response: 260553731
Conc: 72.72 ug/ml

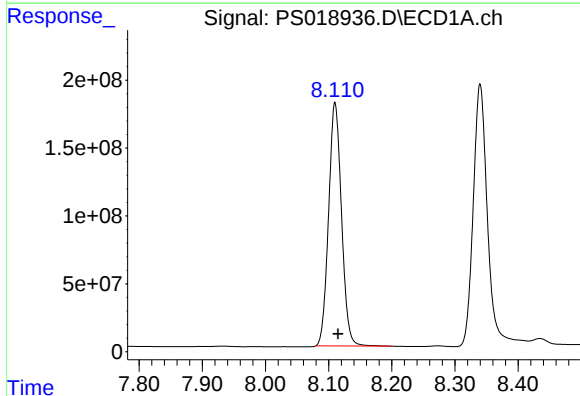


#8 DICHLORPROP

R.T.: 8.110 min
Delta R.T.: -0.005 min
Response: 2548999706
Conc: 764.66 ng/ml

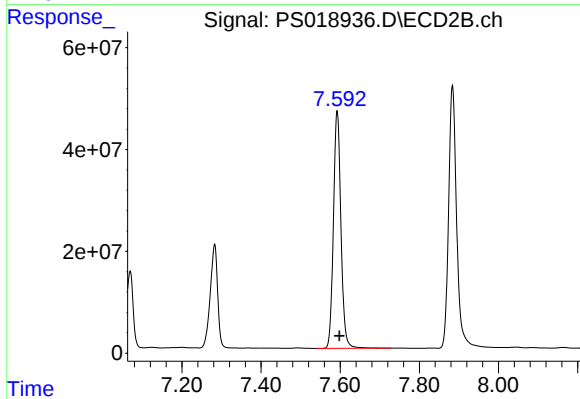

#8 DICHLORPROP


R.T.: 7.592 min
Delta R.T.: -0.006 min
Response: 613082893
Conc: 745.52 ng/ml

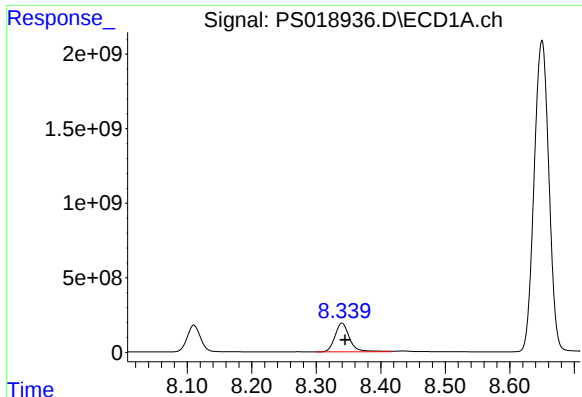

#9 2,4-D


R.T.: 8.340 min
Delta R.T.: -0.005 min
Response: 3043250643
Conc: 761.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

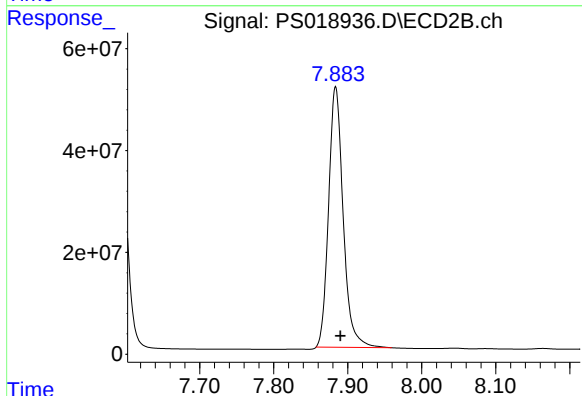


#9 2,4-D

R.T.: 7.884 min
Delta R.T.: -0.006 min
Response: 701113542
Conc: 758.59 ng/ml

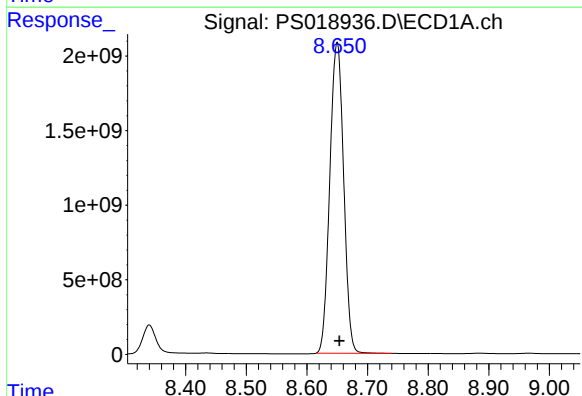


#10 Pentachlorophenol

R.T.: 8.650 min
Delta R.T.: -0.004 min
Response: 33011356816
Conc: 737.82 ng/ml

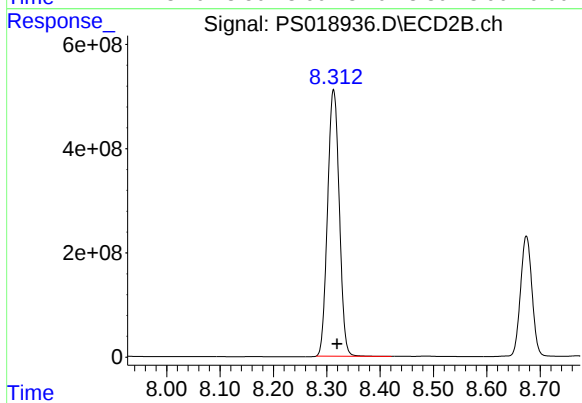

#10 Pentachlorophenol


R.T.: 8.313 min
Delta R.T.: -0.006 min
Response: 7787096603
Conc: 740.00 ng/ml

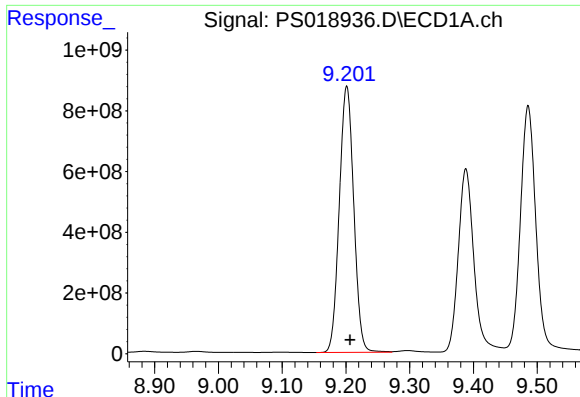

#11 2,4,5-TP (SILVEX)


R.T.: 9.201 min
Delta R.T.: -0.005 min
Response: 13818203902
Conc: 675.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

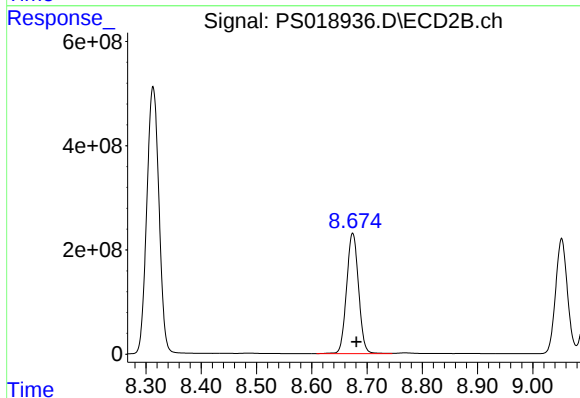


#11 2,4,5-TP (SILVEX)

R.T.: 8.674 min
Delta R.T.: -0.007 min
Response: 3470889229
Conc: 759.28 ng/ml

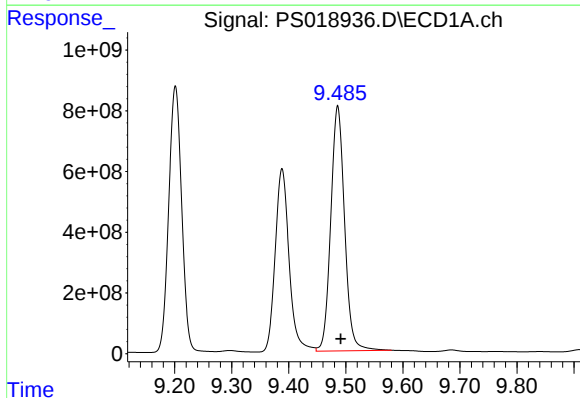


#12 2,4,5-T

R.T.: 9.486 min
Delta R.T.: -0.005 min
Response: 13582001482
Conc: 662.49 ng/ml

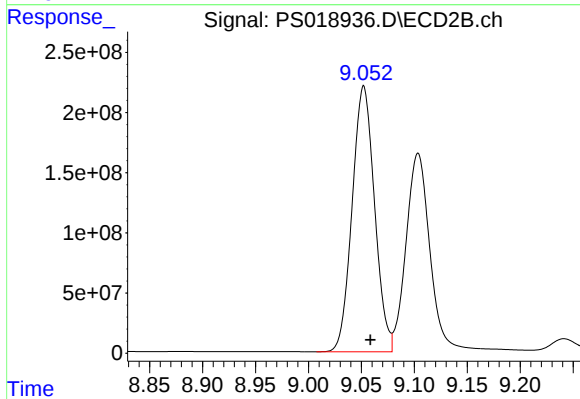

#12 2,4,5-T


R.T.: 9.052 min
Delta R.T.: -0.006 min
Response: 3251221248
Conc: 780.75 ng/ml

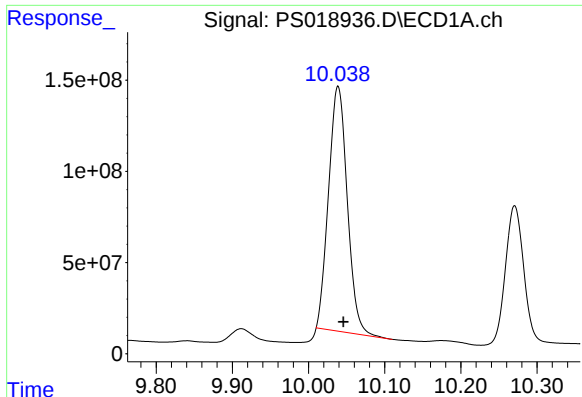

#13 2,4-DB


R.T.: 10.039 min
Delta R.T.: -0.007 min
Response: 2290540852
Conc: 674.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

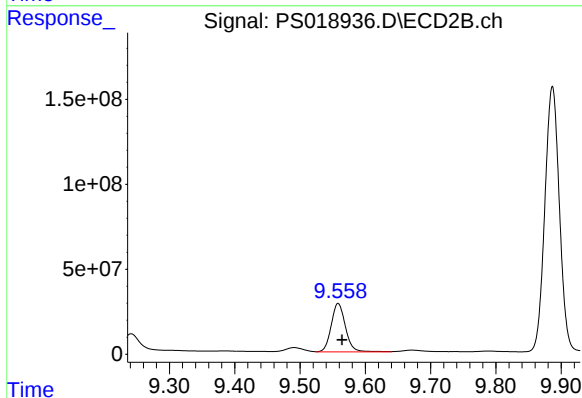


#13 2,4-DB

R.T.: 9.558 min
Delta R.T.: -0.006 min
Response: 435311831
Conc: 764.28 ng/ml

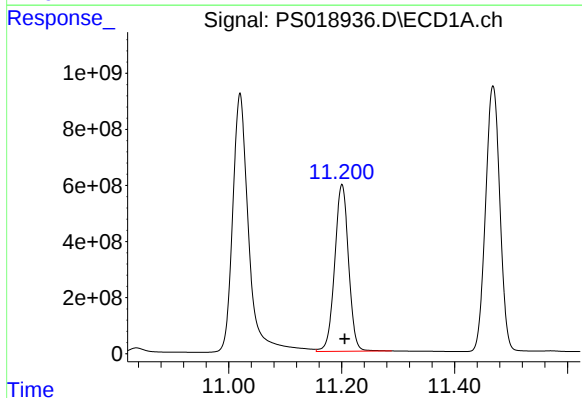


#14 DINOSEB

R.T.: 11.201 min
Delta R.T.: -0.005 min
Response: 10137897889
Conc: 620.95 ng/ml

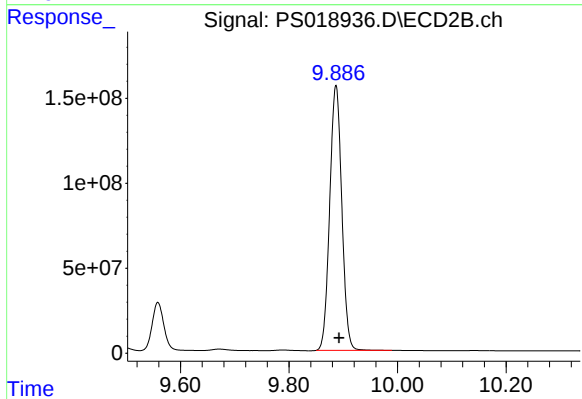

#14 DINOSEB


R.T.: 9.887 min
Delta R.T.: -0.006 min
Response: 2405023530
Conc: 745.79 ng/ml

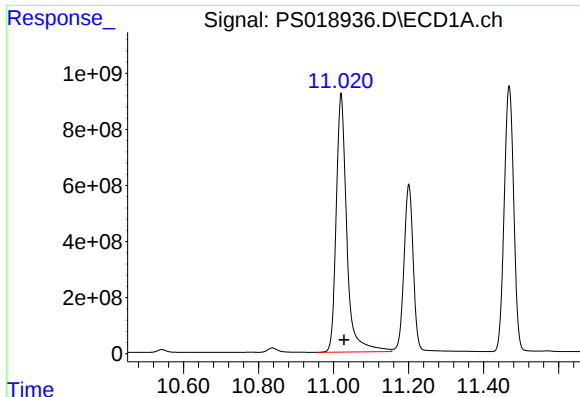

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.008 min
Response: 18087609819
Conc: 646.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

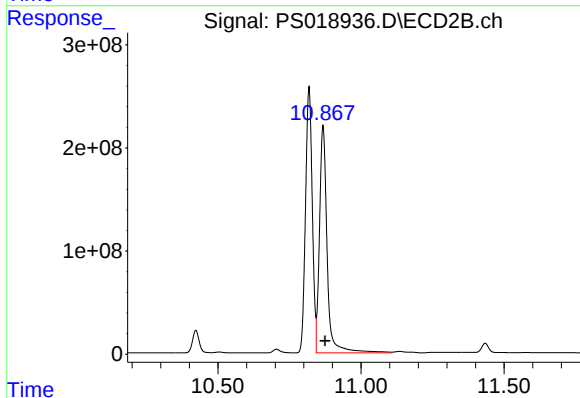


#15 Picloram

R.T.: 10.867 min
Delta R.T.: -0.008 min
Response: 4081849858
Conc: 721.91 ng/ml

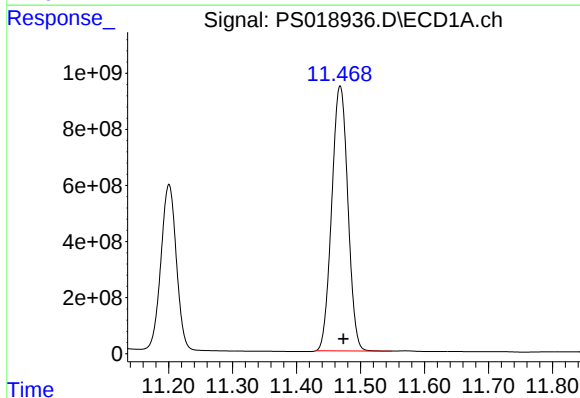

#16 DCPA

R.T.: 11.468 min
Delta R.T.: -0.005 min
Response: 16549133822
Conc: 657.50 ng/ml

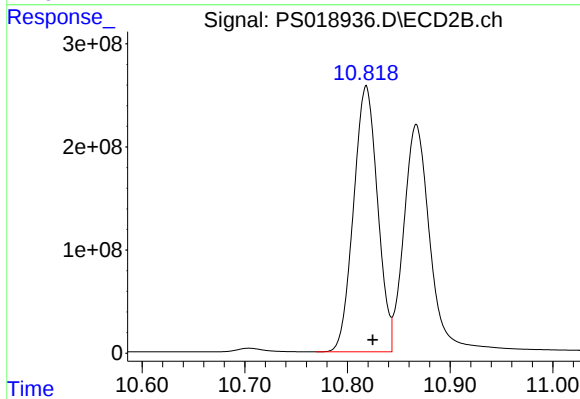

#16 DCPA

R.T.: 10.818 min
Delta R.T.: -0.006 min
Response: 4190754604
Conc: 768.86 ng/ml