

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
 Data File : PS009666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 09:31
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 05:29:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) T	MCPP	0.000	7.247	0	1924535	1.169
8) T	DICHLORPROP	0.000	7.753	0	1083237	2.152
9) T	2,4-D	0.000	7.951	0	1575106	2.629
12) T	2,4,5-T	0.000	9.248	0	2464587	<MDL
13) T	2,4-DB	0.000	9.719	0	4732355	13.347
15) T	Picloram	0.000	11.019	0	2617440	<MDL
16) T	DCPA	0.000	11.019	0	2617440	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
Data File : PS009666.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 09:31
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 05:29:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

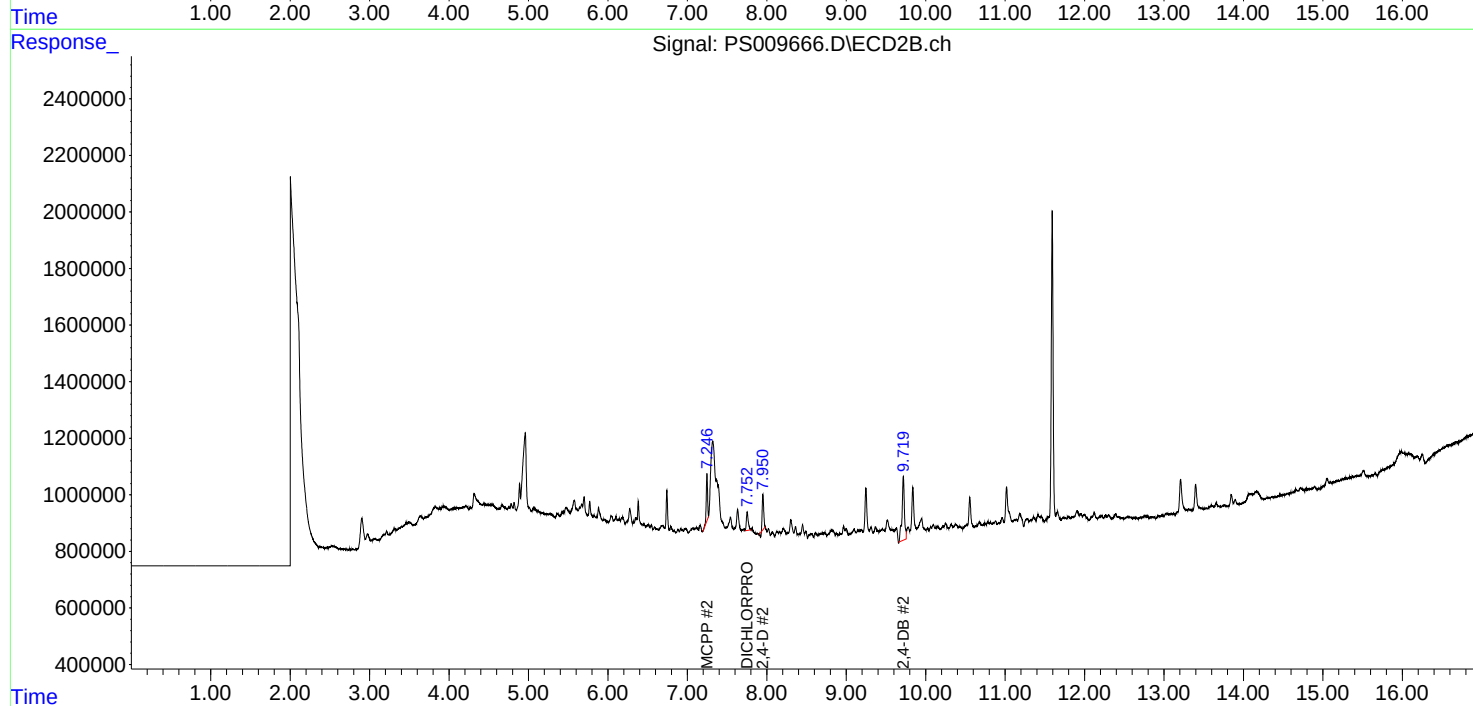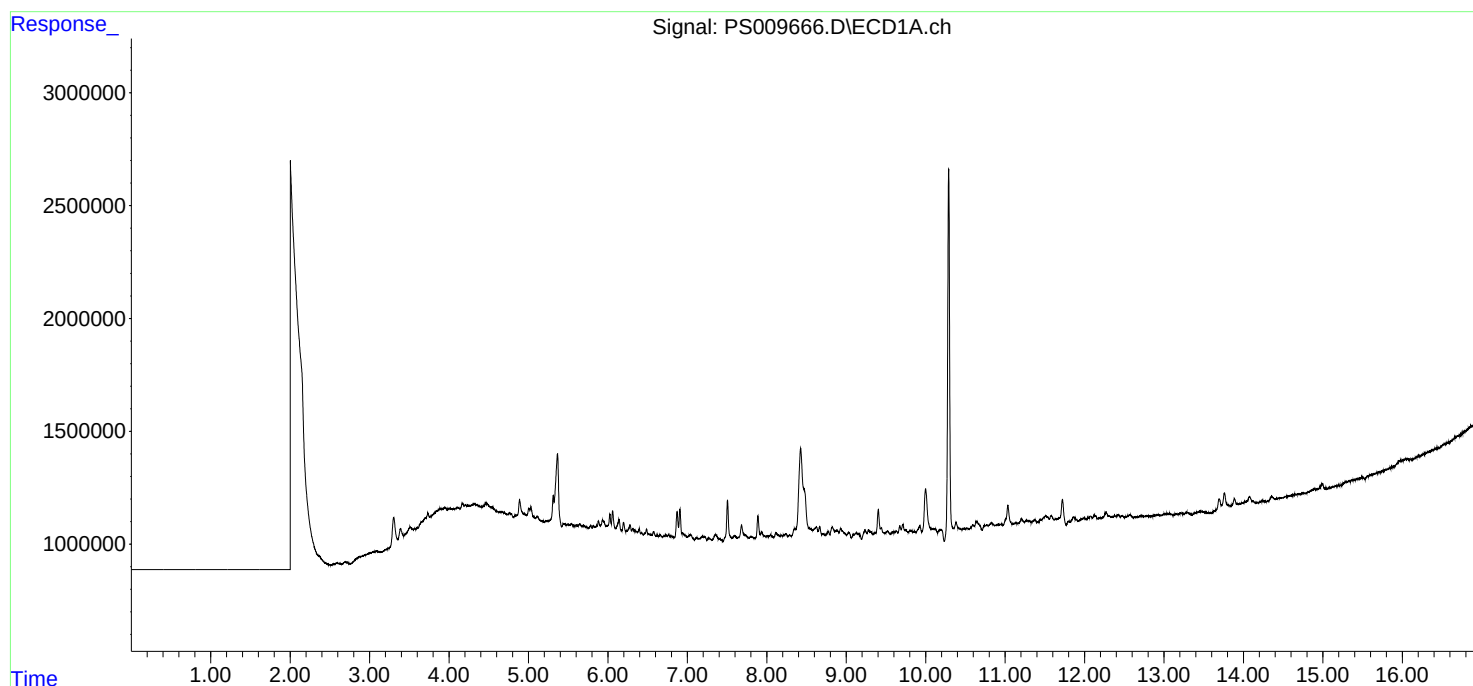


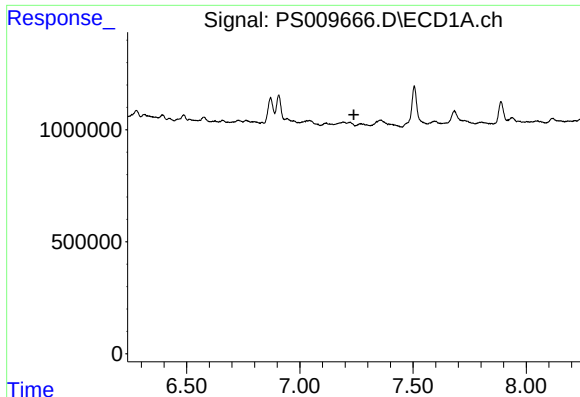

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

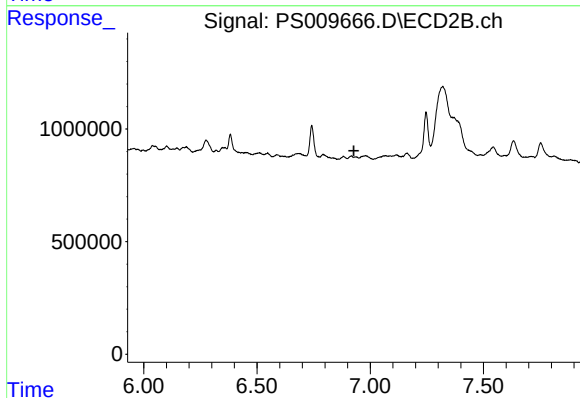


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.928 min
Response: 0
Conc: N.D.

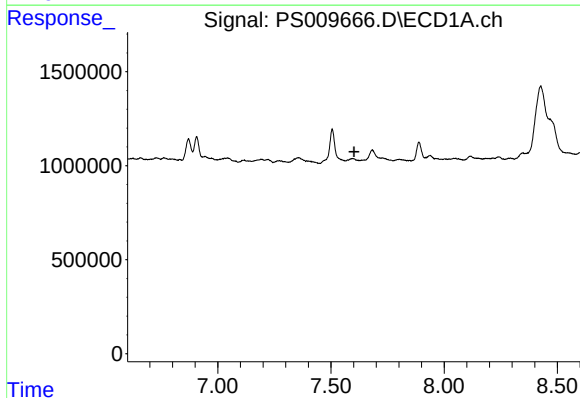


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.602 min
Response: 0
Conc: N.D.

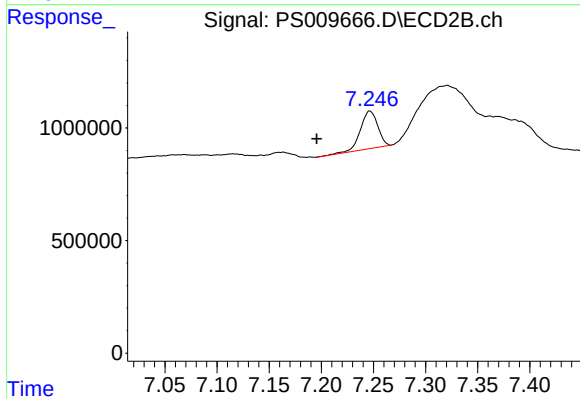

#6 MCPP


R.T.: 7.247 min
Delta R.T.: 0.051 min
Response: 1924535
Conc: 1.17 ug/ml

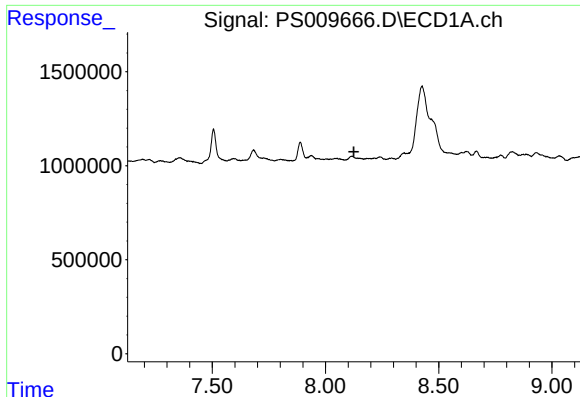

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

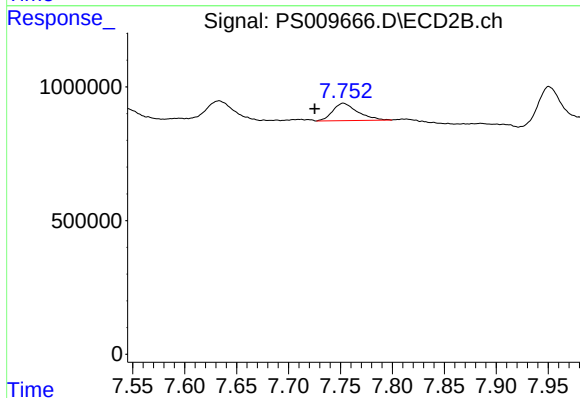


#8 DICHLORPROP

R.T.: 7.753 min
Delta R.T.: 0.028 min
Response: 1083237
Conc: 2.15 ng/ml

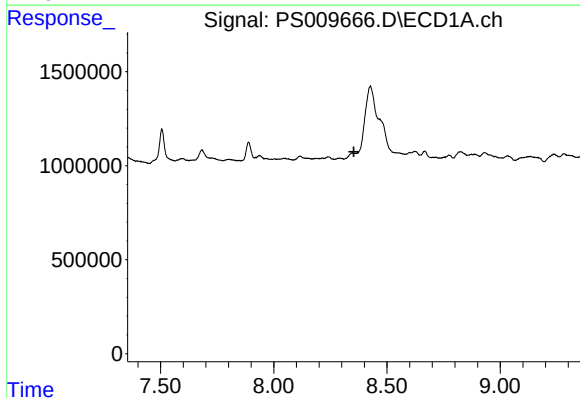


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

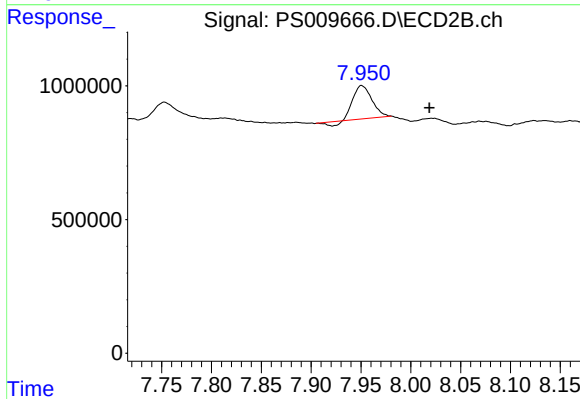

#9 2,4-D


R.T.: 7.951 min
Delta R.T.: -0.068 min
Response: 1575106
Conc: 2.63 ng/ml

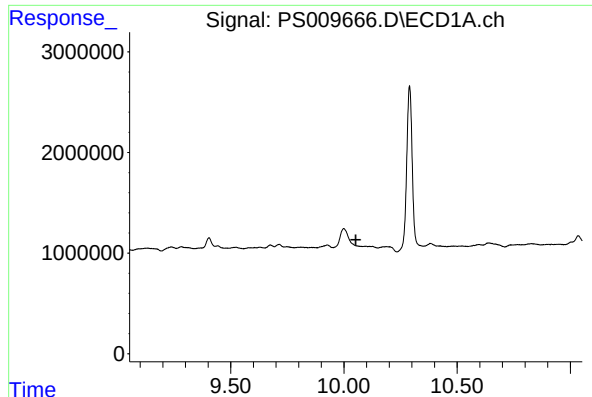

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

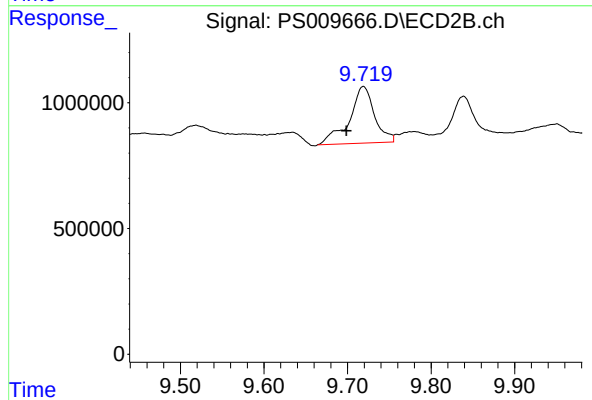

#13 2,4-DB

R.T.: 9.719 min
Delta R.T.: 0.020 min
Response: 4732355
Conc: 13.35 ng/ml