

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
 Data File : PS009674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 13:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 05:31:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.243	6.926	254.3E6	236.3E6	421.122	477.209
Target Compounds							
5) T	DICAMBA	0.000	7.129	0	5195258	N.D.	2.612
6) T	MCPD	0.000	7.129	0	5195258	N.D.	3.156
8) T	DICHLORPROP	0.000	7.750	0	1562799	N.D.	3.105
12) T	2,4,5-T	0.000	9.246	0	4776663	N.D.	1.830
15) T	Picloram	0.000	11.017	0	12582745	N.D.	3.699
16) T	DCPA	0.000	10.958	0	4621288	N.D.	1.378



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
Data File : PS009674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 13:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 05:31:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

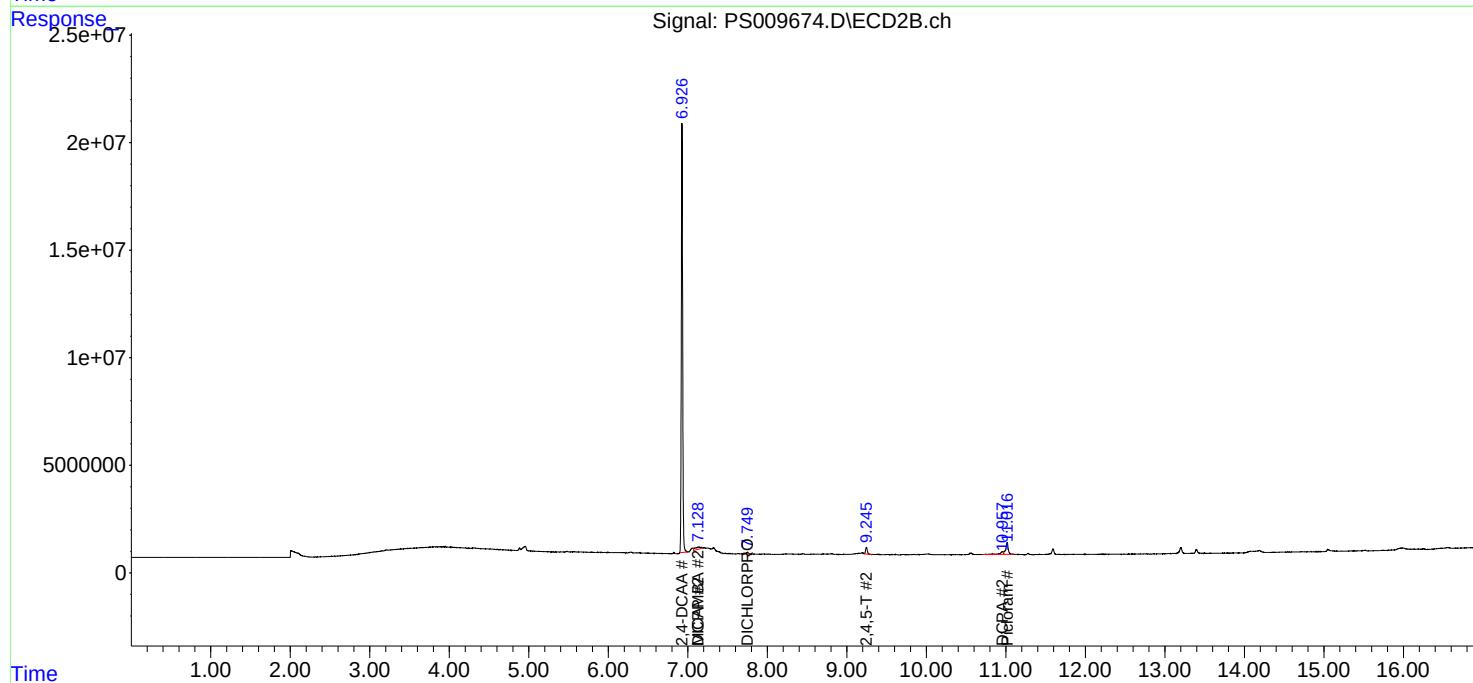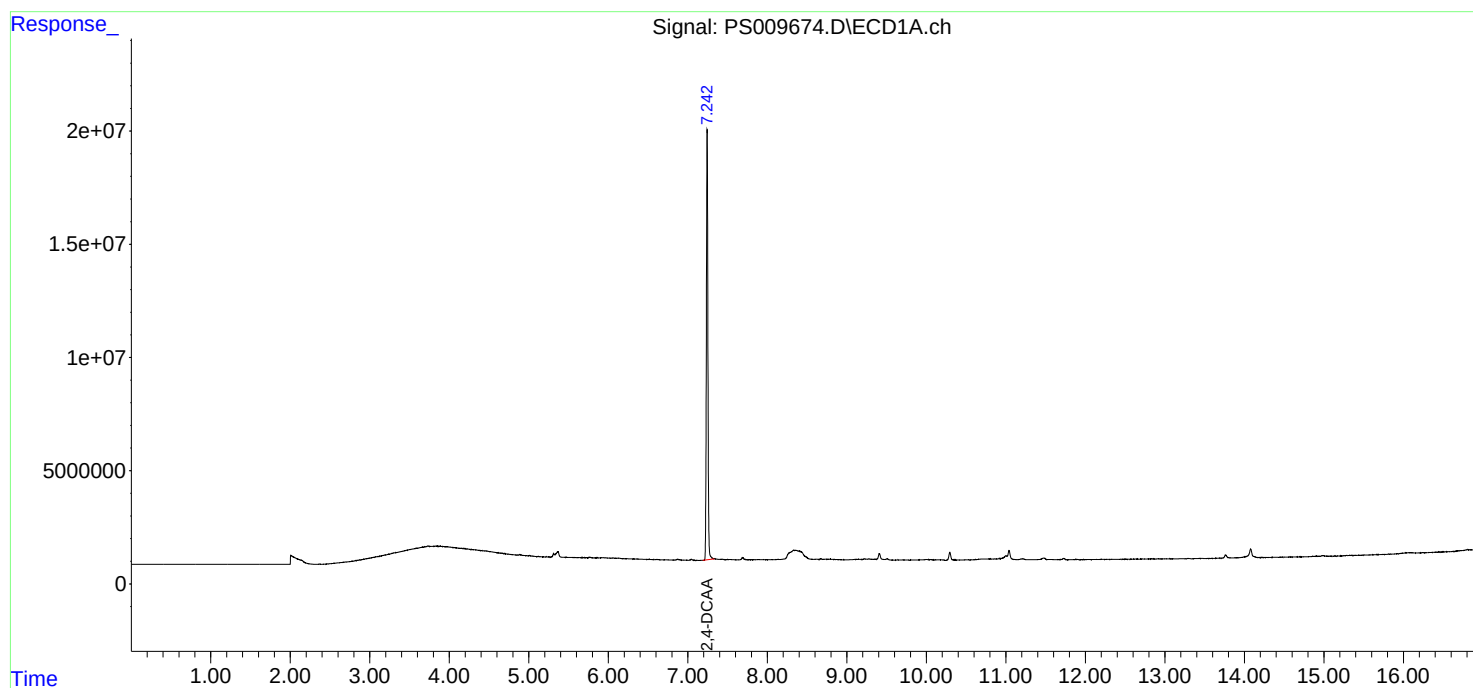


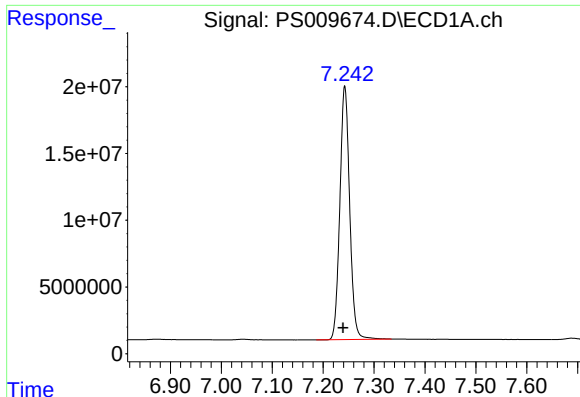

#4 2,4-DCAA


R.T.: 7.243 min
Delta R.T.: 0.004 min
Response: 254279948
Conc: 421.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

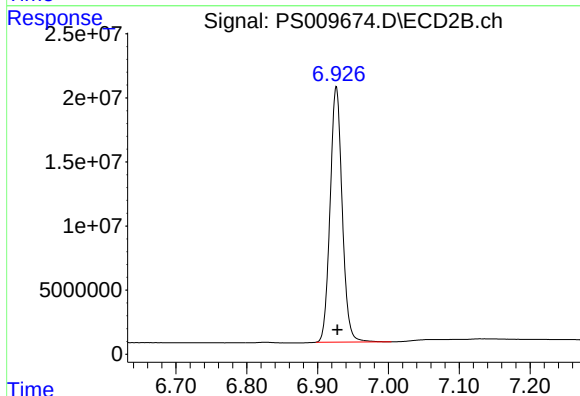


#4 2,4-DCAA

R.T.: 6.926 min
Delta R.T.: -0.002 min
Response: 236337982
Conc: 477.21 ng/ml

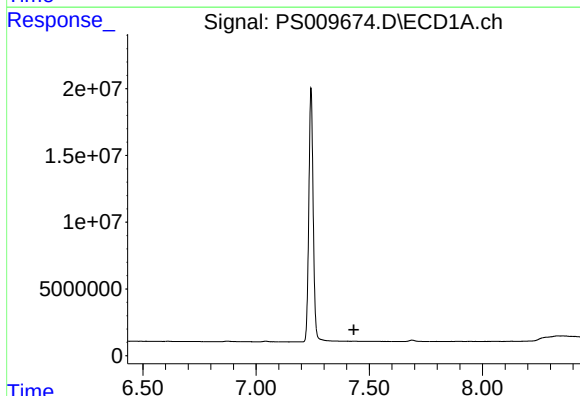


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

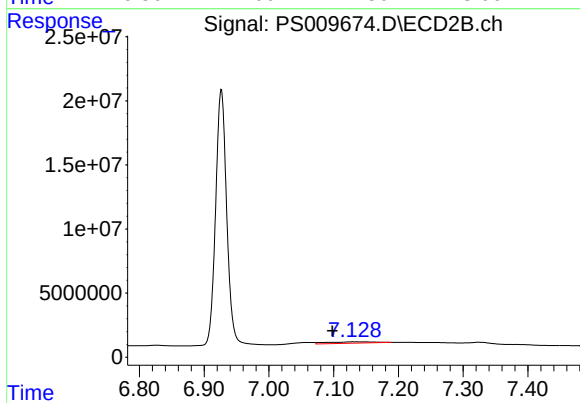

#5 DICAMBA


R.T.: 7.129 min
Delta R.T.: 0.031 min
Response: 5195258
Conc: 2.61 ng/ml

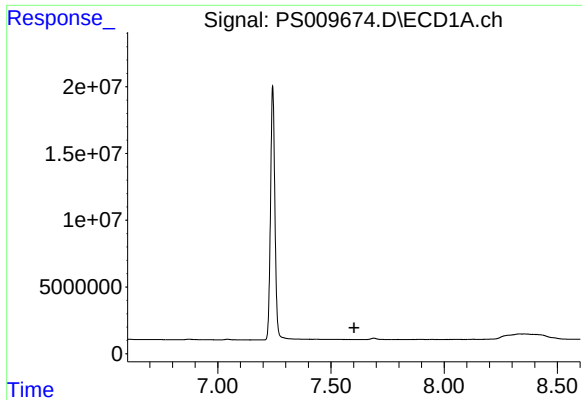

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

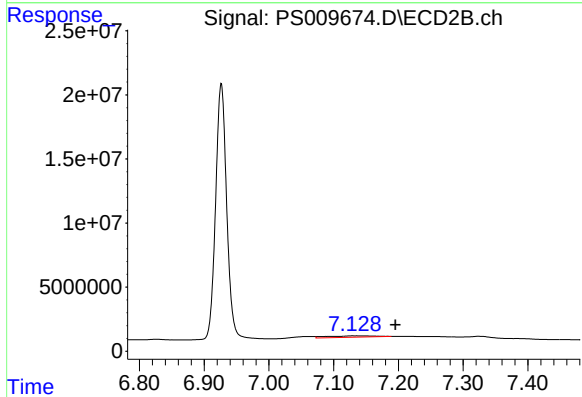


#6 MCP

R.T.: 7.129 min
Delta R.T.: -0.066 min
Response: 5195258
Conc: 3.16 ug/ml

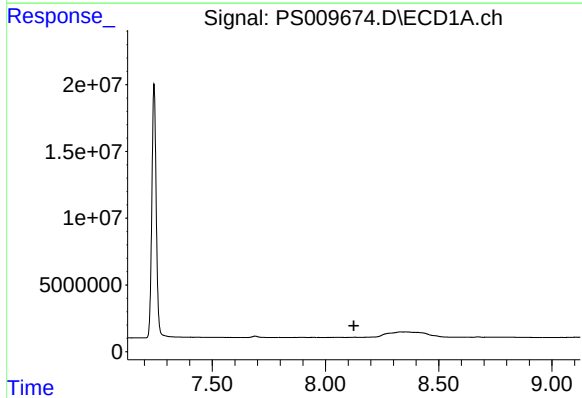


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

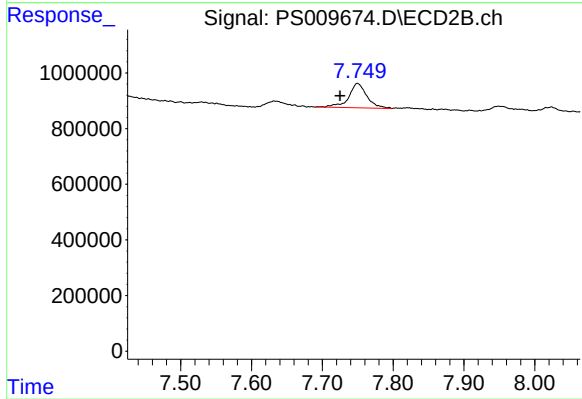

#8 DICHLORPROP


R.T.: 7.750 min
Delta R.T.: 0.025 min
Response: 1562799
Conc: 3.11 ng/ml

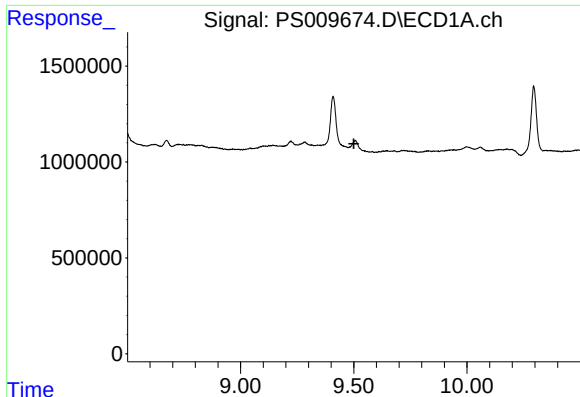

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

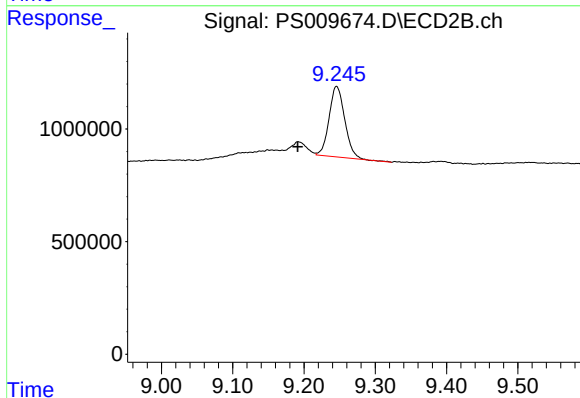


#12 2,4,5-T

R.T.: 9.246 min
Delta R.T.: 0.054 min
Response: 4776663
Conc: 1.83 ng/ml

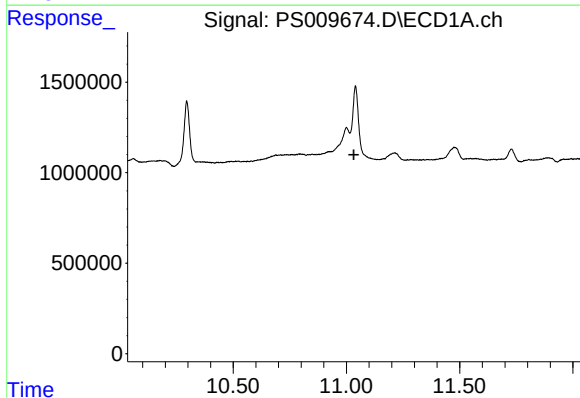


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

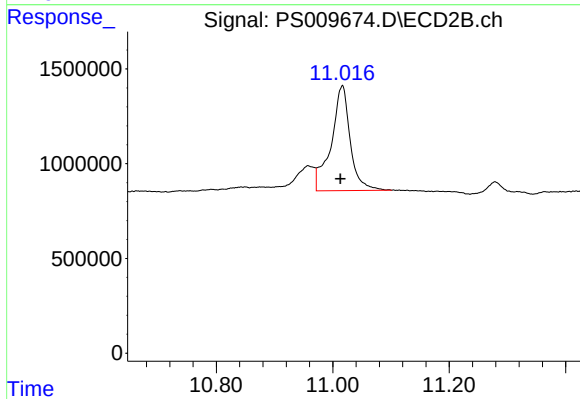

#15 Picloram


R.T.: 11.017 min
Delta R.T.: 0.004 min
Response: 12582745
Conc: 3.70 ng/ml

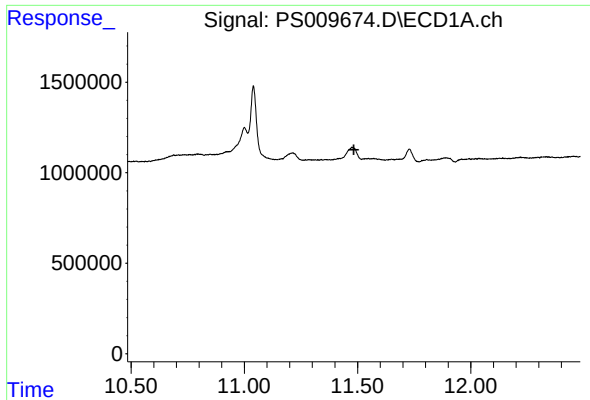

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

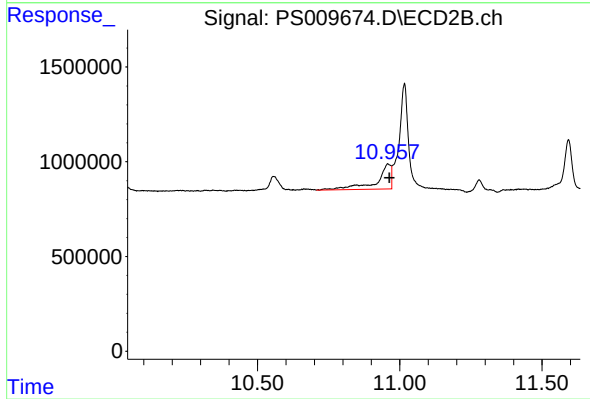

#16 DCPA

R.T.: 10.958 min
Delta R.T.: -0.006 min
Response: 4621288
Conc: 1.38 ng/ml