

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
 Data File : PS009677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 14:47
 Operator : DD\AJ
 Sample : PB127399BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127399BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 05:32:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	6.928	258.3E6	243.4E6	427.700	491.403
Target Compounds							
8) T	DICHLORPROP	0.000	7.750	0	5501286	N.D.	10.930
12) T	2,4,5-T	0.000	9.246	0	3103498	N.D.	1.189
15) T	Picloram	0.000	11.013	0	5081571	N.D.	1.494
16) T	DCPA	0.000	11.013	0	5081571	N.D.	1.516



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
Data File : PS009677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 14:47
Operator : DD\AJ
Sample : PB127399BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB127399BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 05:32:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

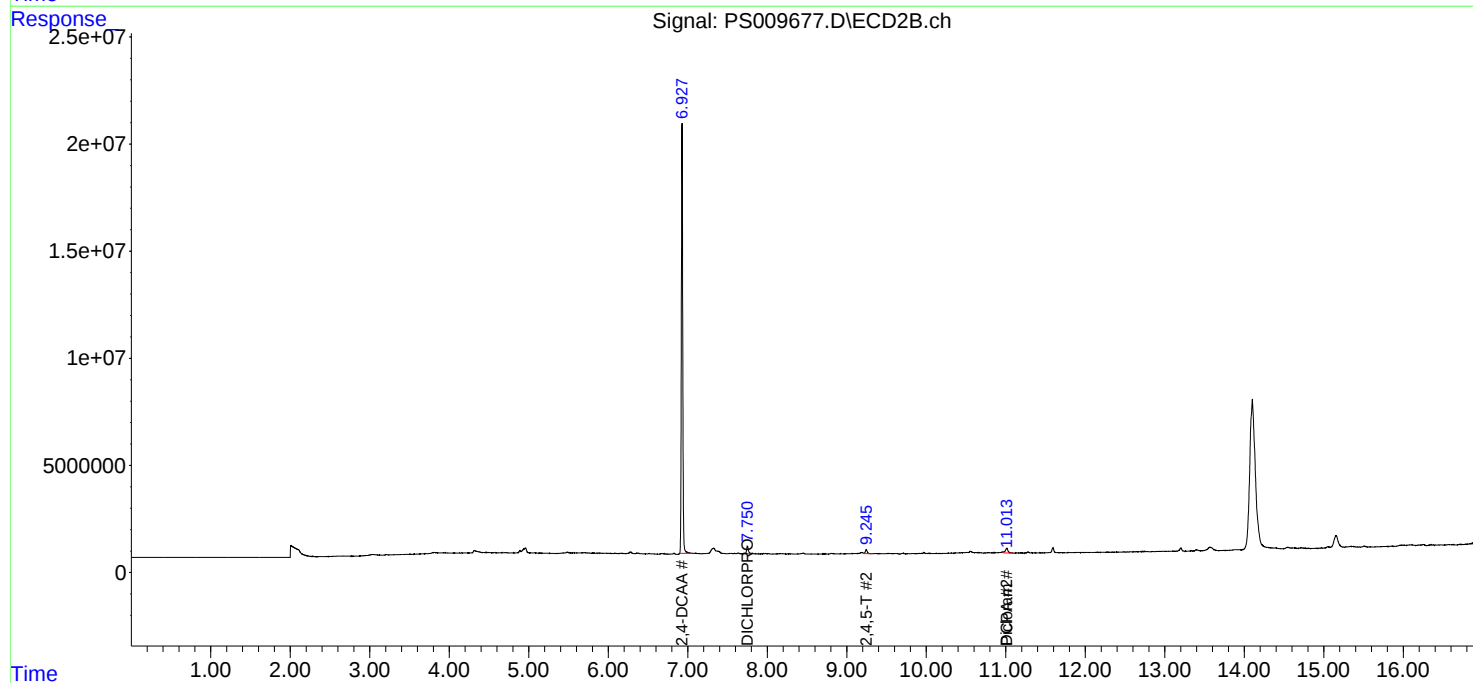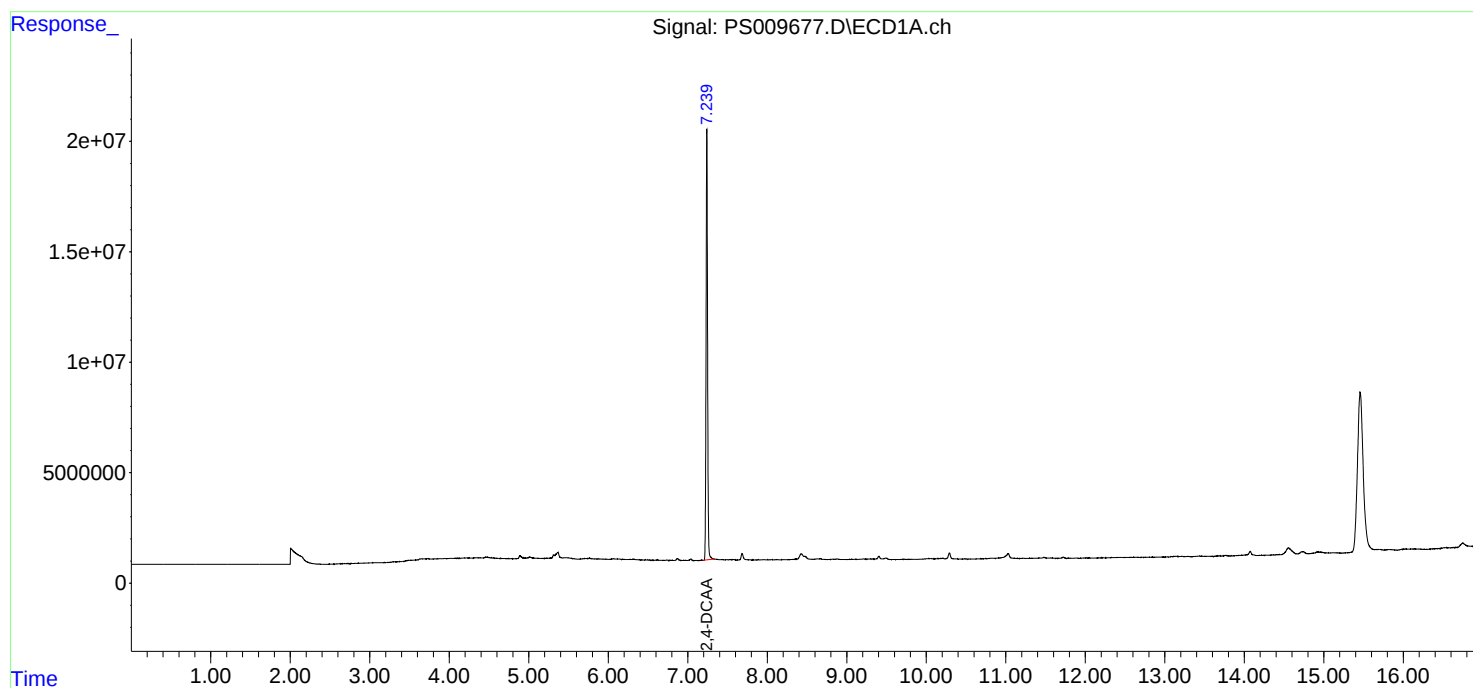


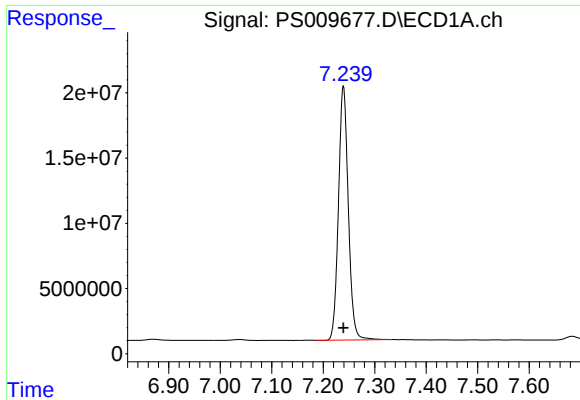

#4 2,4-DCAA


R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 258251904
Conc: 427.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127399BL

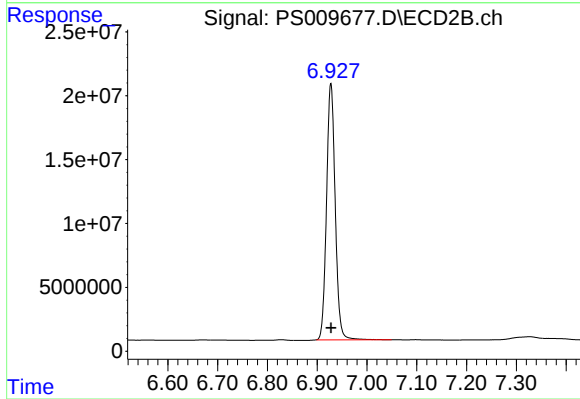


#4 2,4-DCAA

R.T.: 6.928 min
Delta R.T.: 0.000 min
Response: 243367458
Conc: 491.40 ng/ml

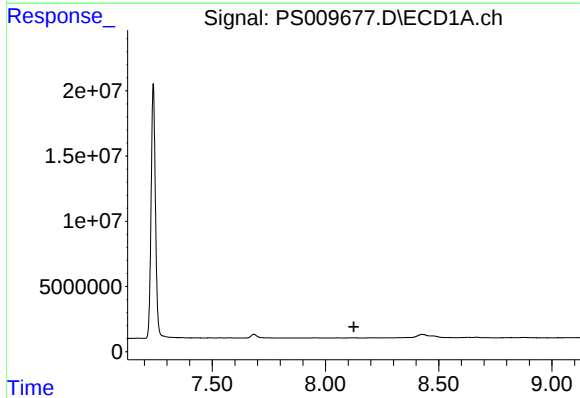


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

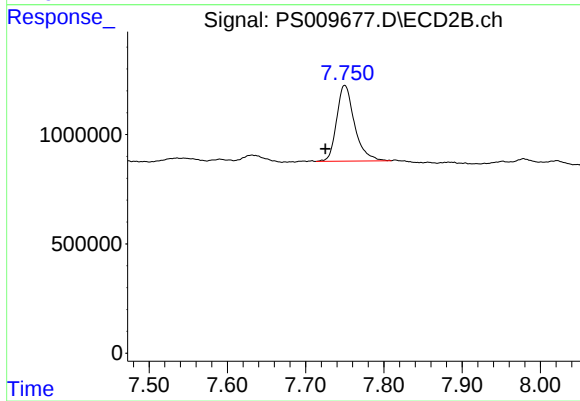

#8 DICHLORPROP


R.T.: 7.750 min
Delta R.T.: 0.025 min
Response: 5501286
Conc: 10.93 ng/ml

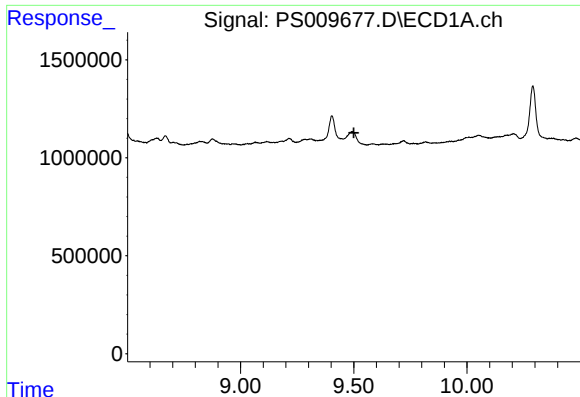

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127399BL

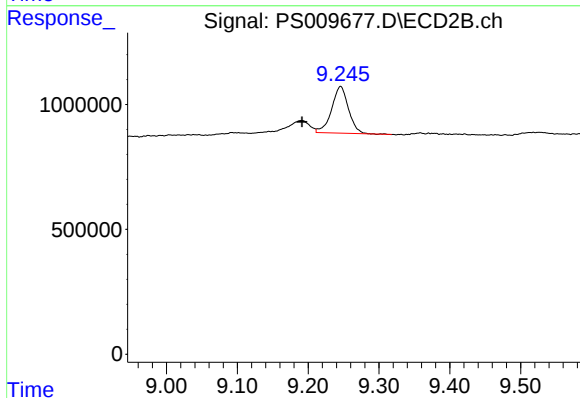


#12 2,4,5-T

R.T.: 9.246 min
Delta R.T.: 0.054 min
Response: 3103498
Conc: 1.19 ng/ml

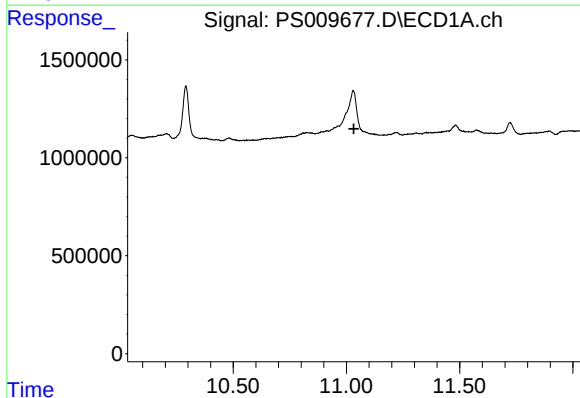


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

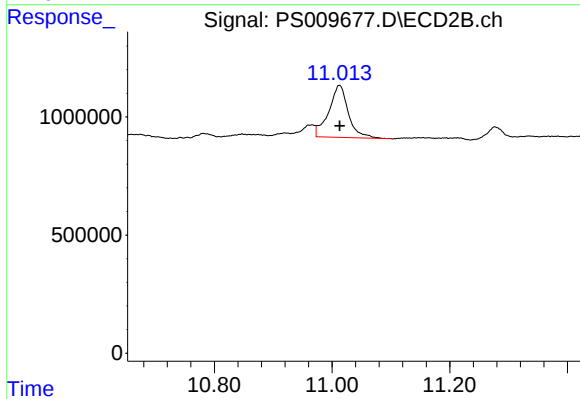

#15 Picloram


R.T.: 11.013 min
Delta R.T.: 0.000 min
Response: 5081571
Conc: 1.49 ng/ml

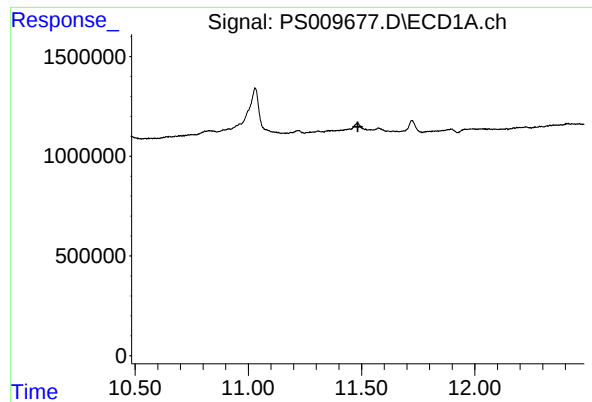

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127399BL

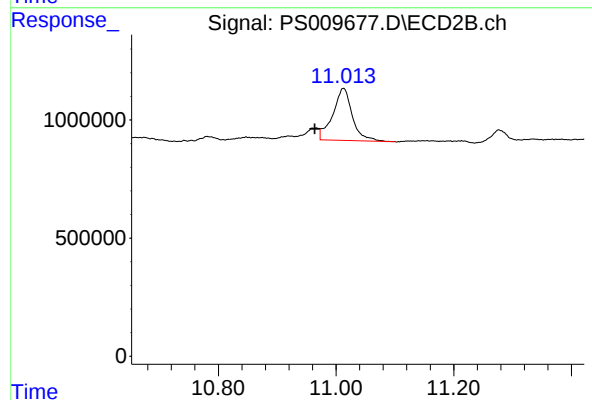

#16 DCPA

R.T.: 11.013 min
Delta R.T.: 0.049 min
Response: 5081571
Conc: 1.52 ng/ml