

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
 Data File : PS009679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 15:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 05:33:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.928	263.6E6	249.4E6	436.485	503.642
Target Compounds							
8) T	DICHLORPROP	0.000	7.752	0	1859465	N.D.	3.694
12) T	2,4,5-T	0.000	9.193	0	1192814	N.D.	<MDL
15) T	Picloram	0.000	11.017	0	6481445	N.D.	1.906
16) T	DCPA	0.000	10.965	0	1114806	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
Data File : PS009679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 15:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 05:33:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

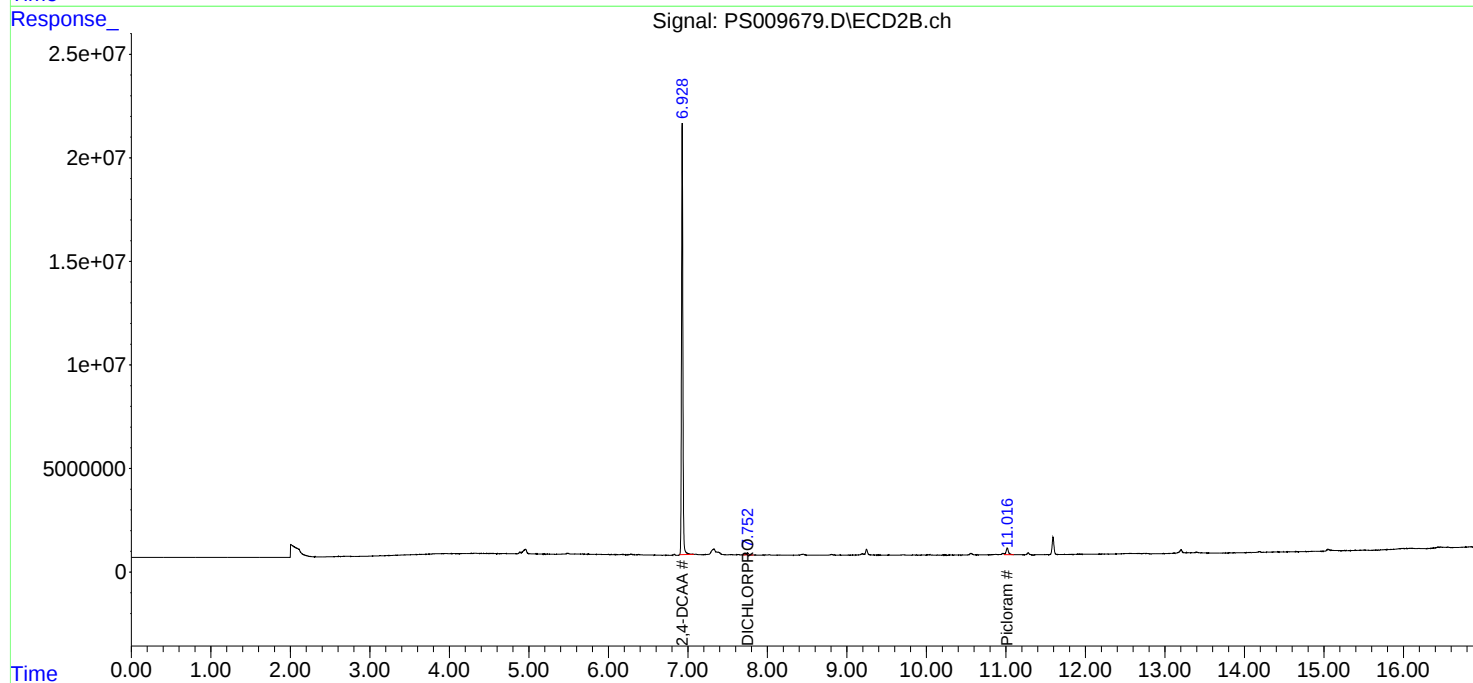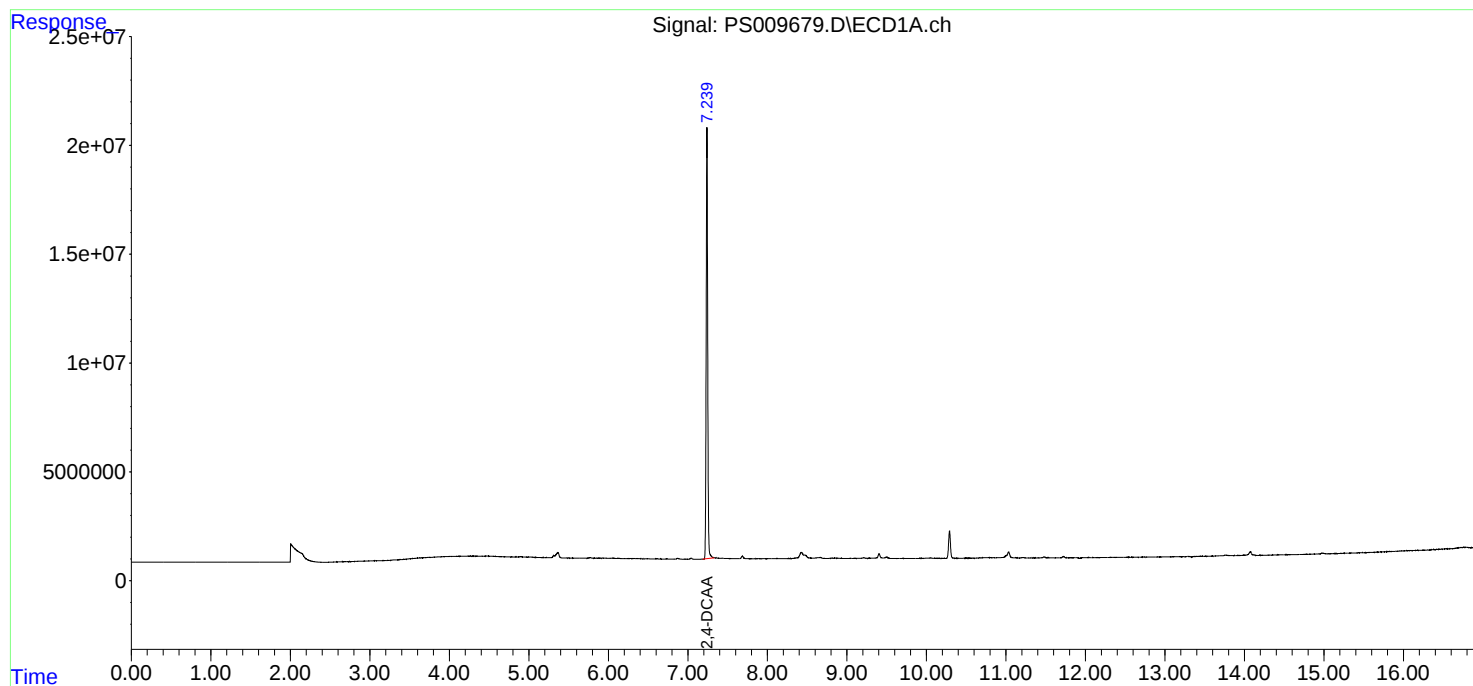


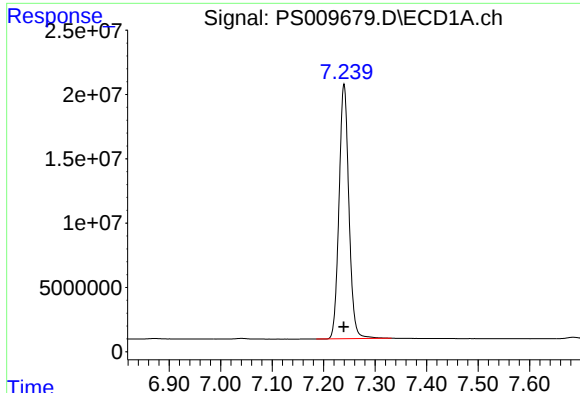

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 263556598
Conc: 436.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

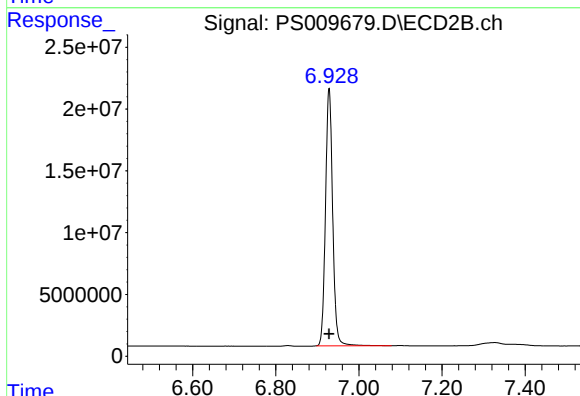


#4 2,4-DCAA

R.T.: 6.928 min
Delta R.T.: 0.000 min
Response: 249428693
Conc: 503.64 ng/ml

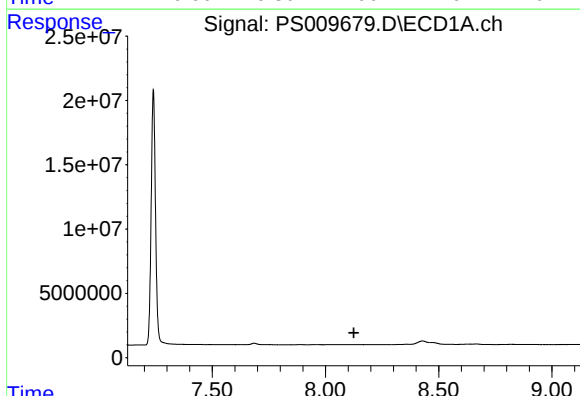


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

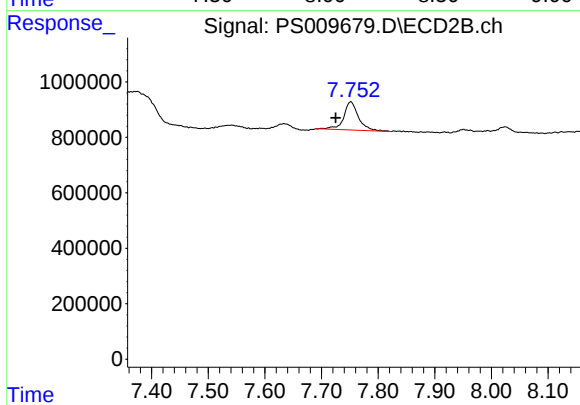

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.026 min
Response: 1859465
Conc: 3.69 ng/ml

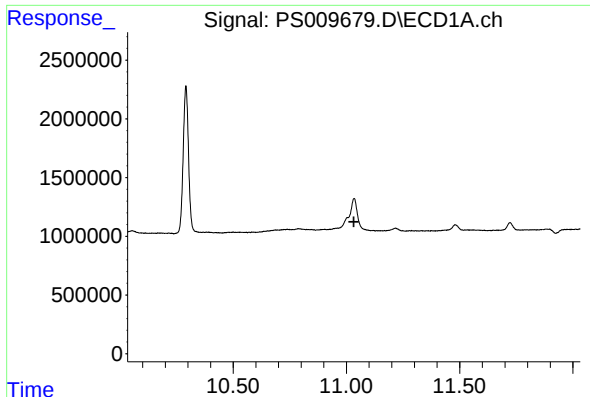

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

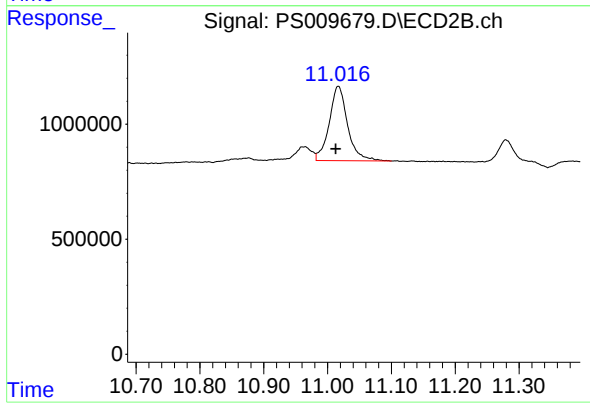

#15 Picloram

R.T.: 11.017 min
Delta R.T.: 0.004 min
Response: 6481445
Conc: 1.91 ng/ml