

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
 Data File : PS009681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 16:19
 Operator : DD\AJ
 Sample : PB128069BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB128069BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 05:33:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 09 05:27:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	6.928	280.8E6	268.8E6	465.026	542.701
Target Compounds							
8) T	DICHLORPROP	0.000	7.751	0	4830877	N.D.	9.598
12) T	2,4,5-T	0.000	9.192	0	1376957	N.D.	<MDL
14) T	DINOSEB	0.000	9.973	0	797374	N.D.	<MDL
15) T	Picloram	0.000	11.016	0	7652010	N.D.	2.250
16) T	DCPA	0.000	10.963	0	1188127	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040820\
Data File : PS009681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 16:19
Operator : DD\AJ
Sample : PB128069BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB128069BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 05:33:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040820.M
Quant Title : 8080.M
QLast Update : Thu Apr 09 05:27:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

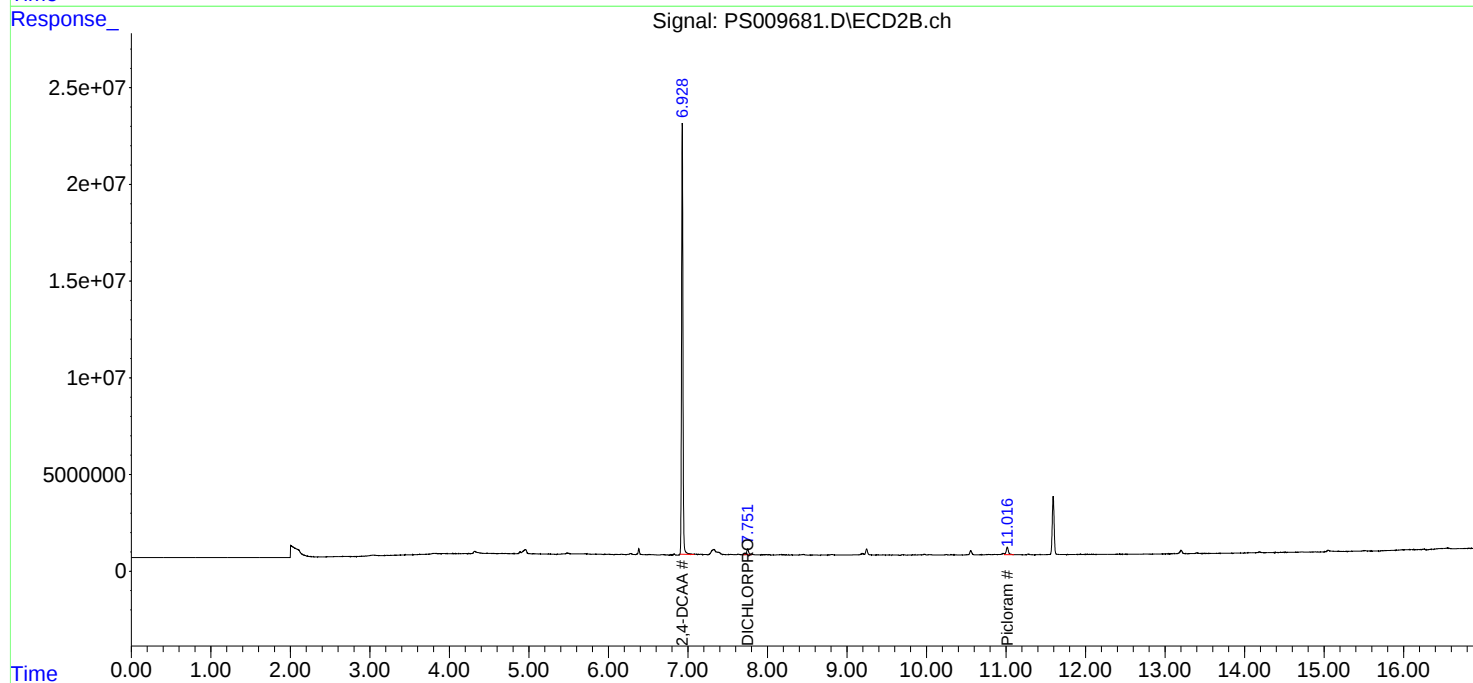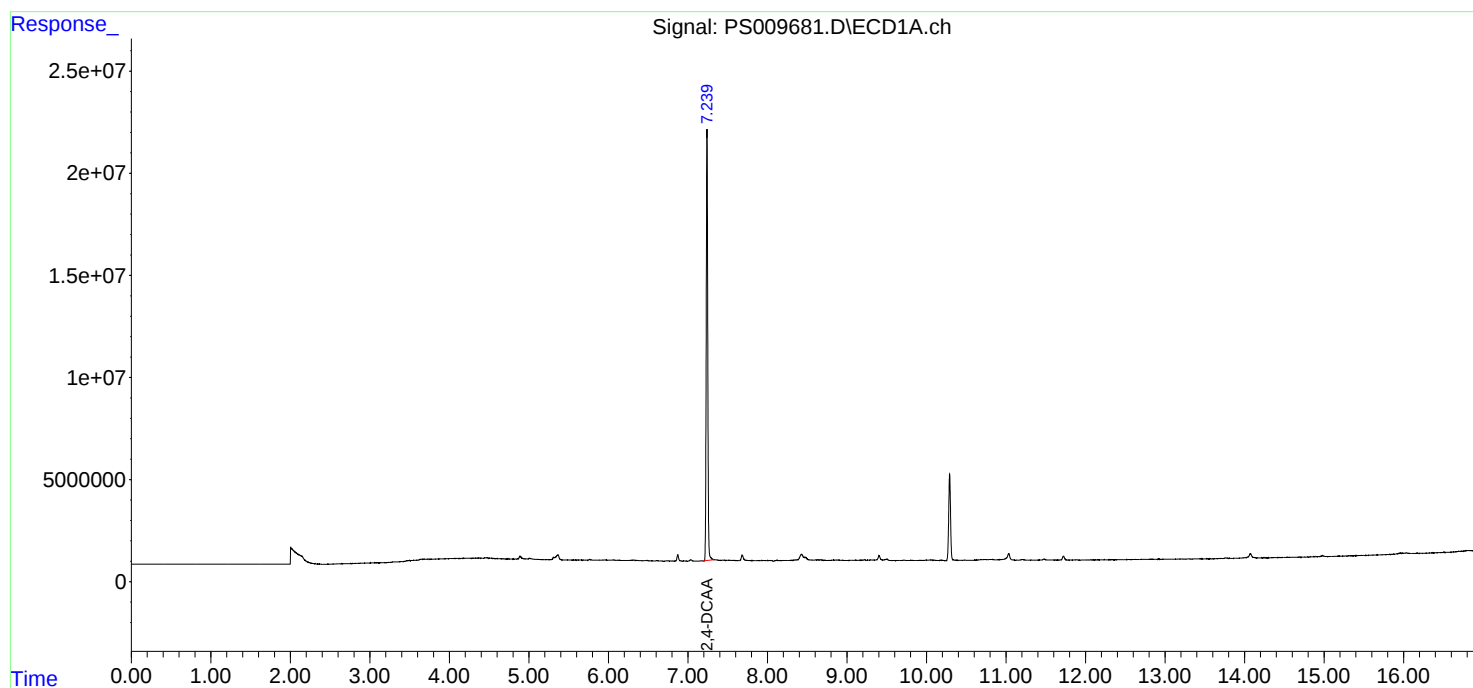


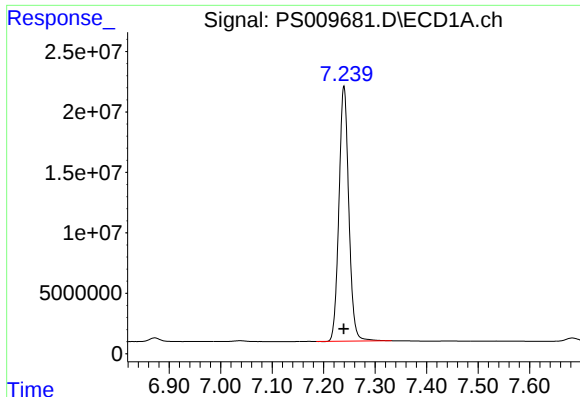

#4 2,4-DCAA


R.T.: 7.239 min
Delta R.T.: 0.000 min
Response: 280789950
Conc: 465.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB128069BL

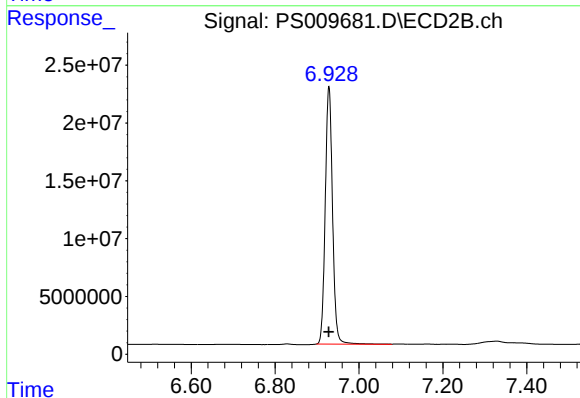


#4 2,4-DCAA

R.T.: 6.928 min
Delta R.T.: 0.000 min
Response: 268772862
Conc: 542.70 ng/ml

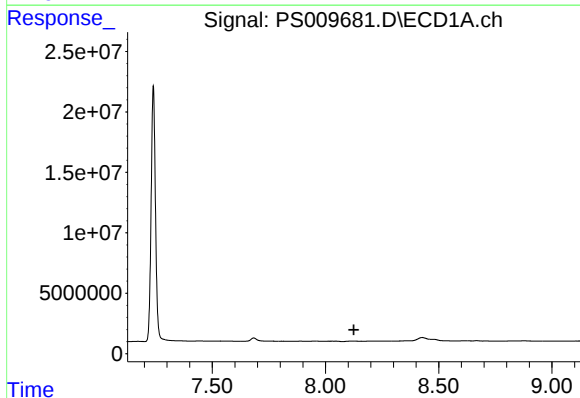


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

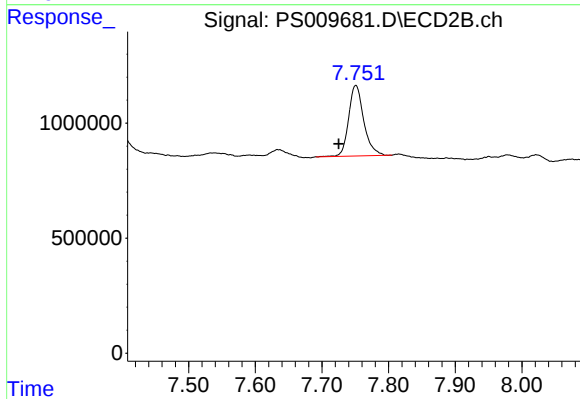

#8 DICHLORPROP

R.T.: 7.751 min
Delta R.T.: 0.026 min
Response: 4830877
Conc: 9.60 ng/ml

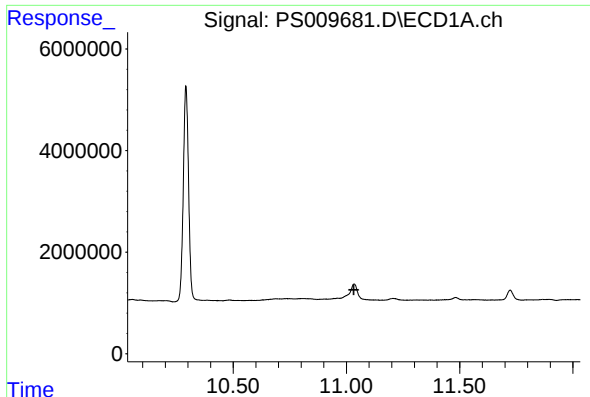

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB128069BL

#15 Picloram

R.T.: 11.016 min
Delta R.T.: 0.003 min
Response: 7652010
Conc: 2.25 ng/ml