

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040821\
 Data File : PS014532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2021 14:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 15:20:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.162	6.887	651.4E6	246.0E6	428.186	528.550
Target Compounds							
12) T	2,4,5-T	9.349f	0.000	6859573	0	<MDL	N.D. #
15) T	Picloram	10.965f	10.996f	39404084	16482760	3.522	4.396



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040821\
Data File : PS014532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2021 14:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 15:20:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

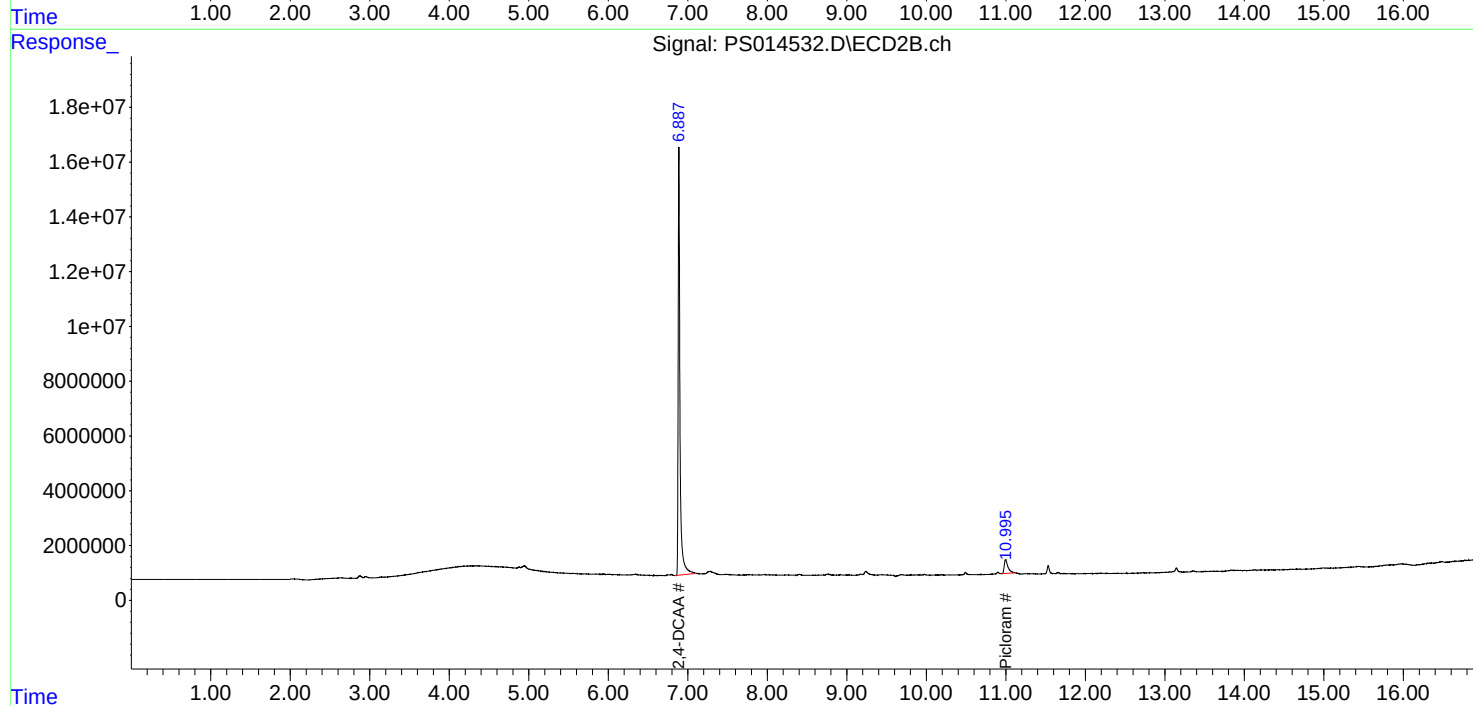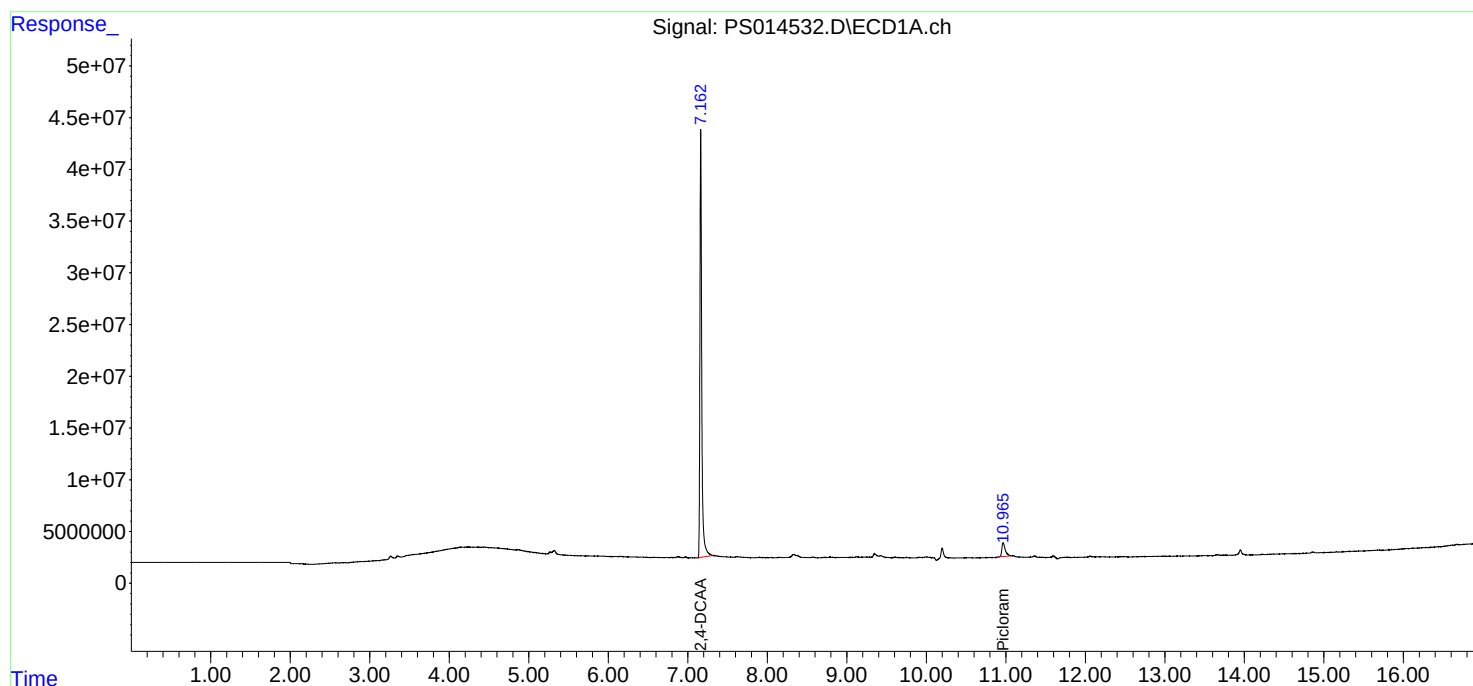


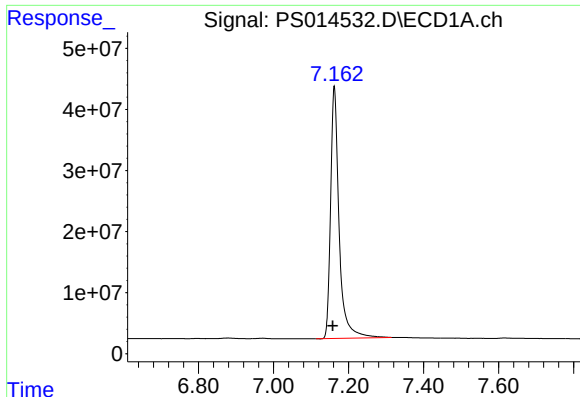

#4 2,4-DCAA


R.T.: 7.162 min
Delta R.T.: 0.004 min
Response: 651355150
Conc: 428.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

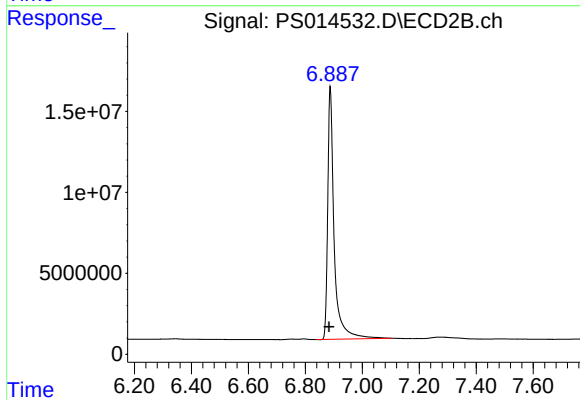


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: 0.003 min
Response: 246016056
Conc: 528.55 ng/ml

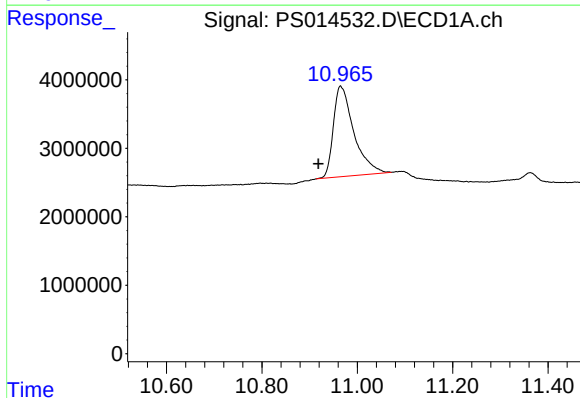

#15 Picloram

R.T.: 10.965 min
Delta R.T.: 0.046 min
Response: 39404084
Conc: 3.52 ng/ml

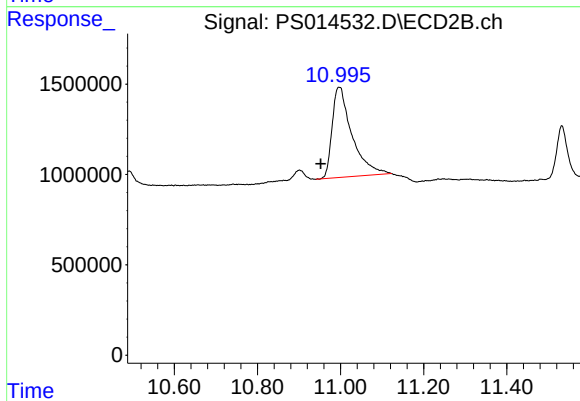

#15 Picloram

R.T.: 10.996 min
Delta R.T.: 0.043 min
Response: 16482760
Conc: 4.40 ng/ml