

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040822\
 Data File : PS018943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 10:00
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 17:52:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.804	1401.6E6	342.6E6	480.075	479.860
Target Compounds							
5) T	DICAMBA	7.418	6.970	23666766	2774344	1.882	<MDL #
8) T	DICHLORPROP	0.000	7.618	0	2797634	N.D.	3.402
10) T	Pentachlo...	8.653	8.314	12480157	2196006	<MDL	<MDL #
11) T	2,4,5-TP ...	9.211	8.678	13089413	2665934	<MDL	<MDL #
12) T	2,4,5-T	9.505	9.069	55792093	6000666	2.721	1.441 #
13) T	2,4-DB	10.087f	0.000	5284744	0	1.557	N.D. #
14) T	DINOSEB	11.202	9.890	52711808	2909349	3.229	<MDL #
15) T	Picloram	11.061	10.895	519.2E6	103.0E6	18.557	18.212
16) T	DCPA	11.471	10.820	23731953	4101175	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040822\
Data File : PS018943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 10:00
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 17:52:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

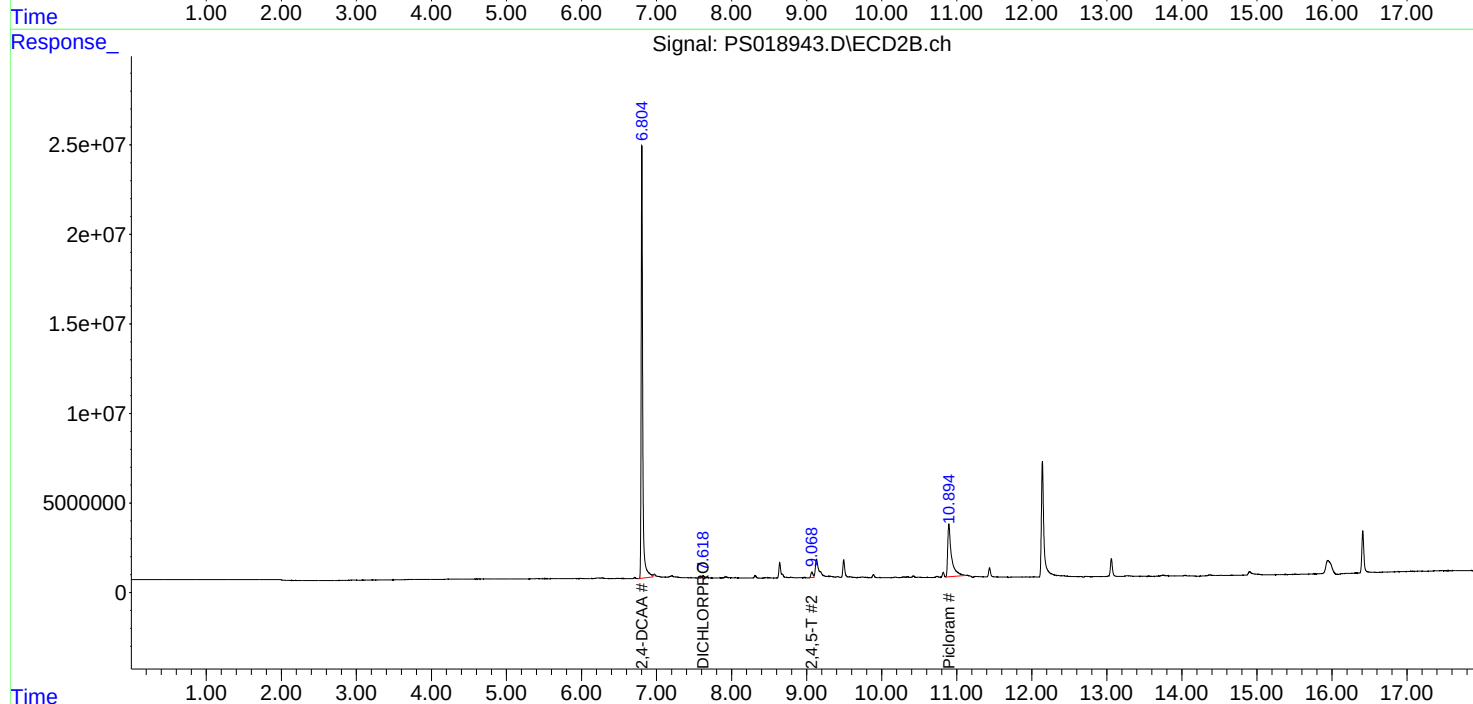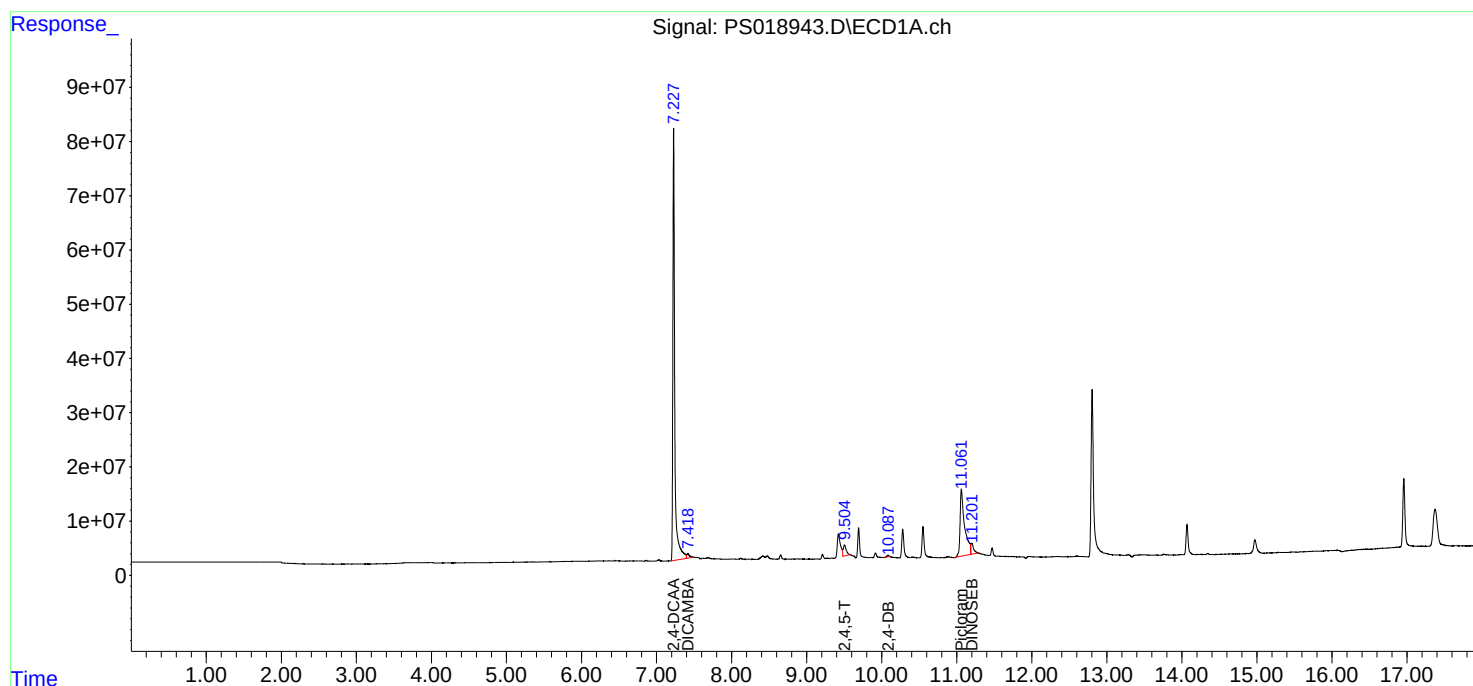


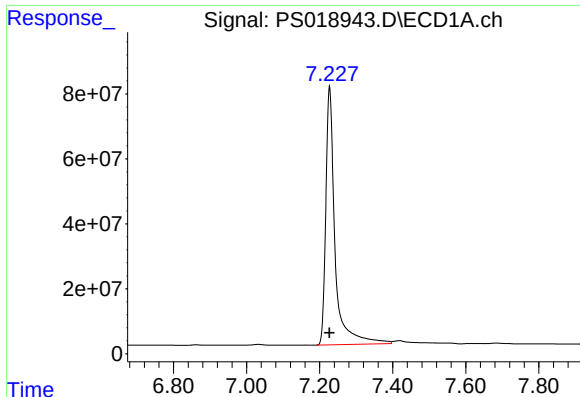

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 1401559156
Conc: 480.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

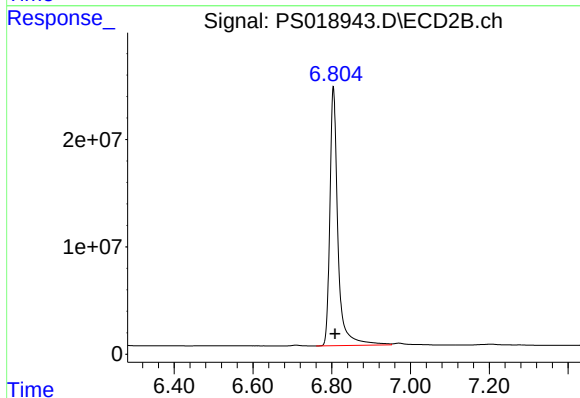


#4 2,4-DCAA

R.T.: 6.804 min
Delta R.T.: -0.004 min
Response: 342592665
Conc: 479.86 ng/ml

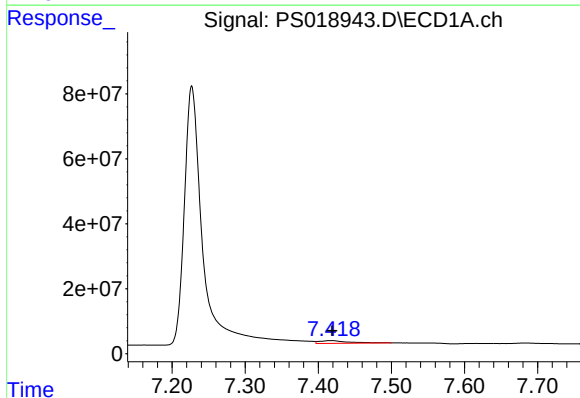


#5 DICAMBA

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 23666766
Conc: 1.88 ng/ml

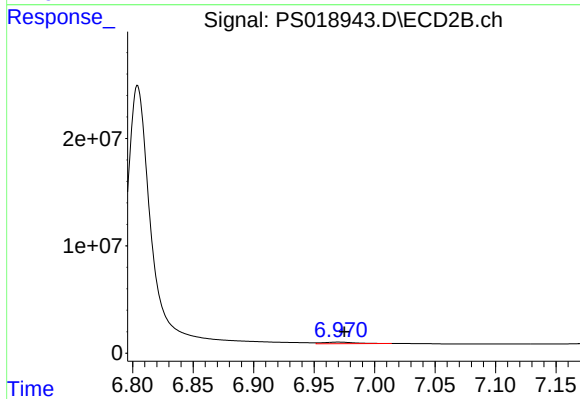

#5 DICAMBA


R.T.: 6.970 min
Delta R.T.: -0.005 min
Response: 2774344
Conc: N.D.

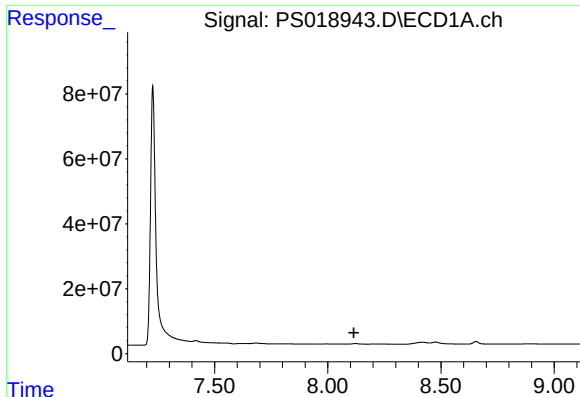

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

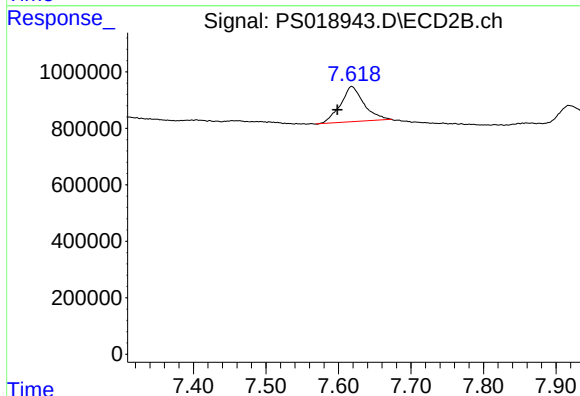


#8 DICHLORPROP

R.T.: 7.618 min
Delta R.T.: 0.020 min
Response: 2797634
Conc: 3.40 ng/ml

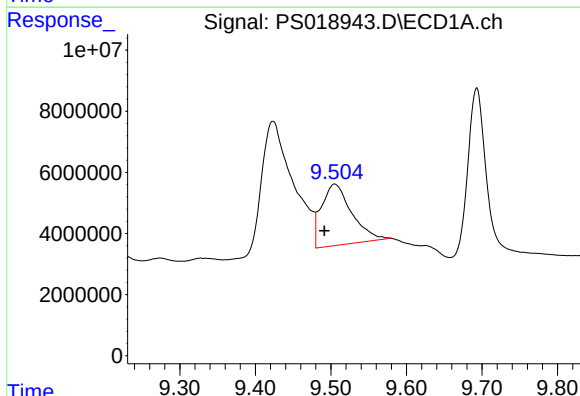


#12 2,4,5-T

R.T.: 9.505 min
Delta R.T.: 0.014 min
Response: 55792093
Conc: 2.72 ng/ml

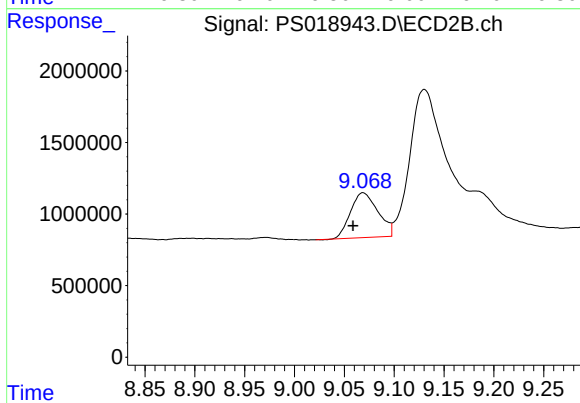

#12 2,4,5-T


R.T.: 9.069 min
Delta R.T.: 0.010 min
Response: 6000666
Conc: 1.44 ng/ml

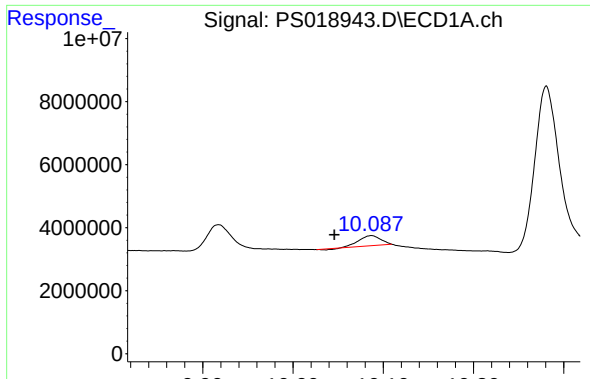

#13 2,4-DB


R.T.: 10.087 min
Delta R.T.: 0.041 min
Response: 5284744
Conc: 1.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

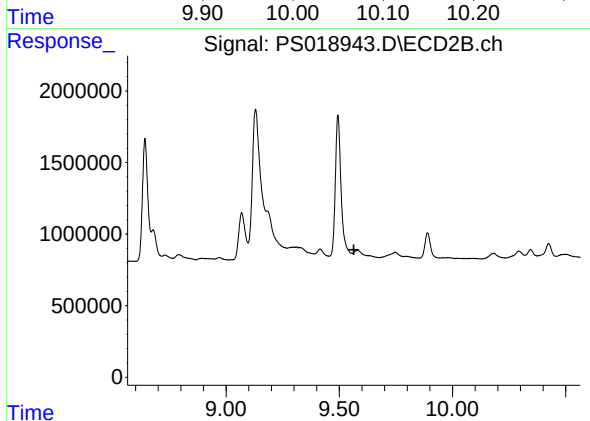


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

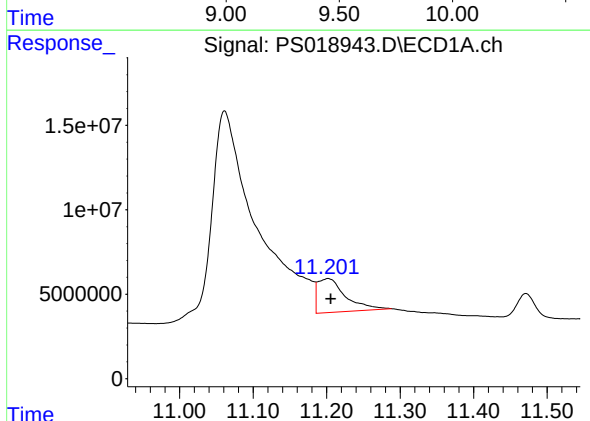


#14 DINOSEB

R.T.: 11.202 min
Delta R.T.: -0.004 min
Response: 52711808
Conc: 3.23 ng/ml

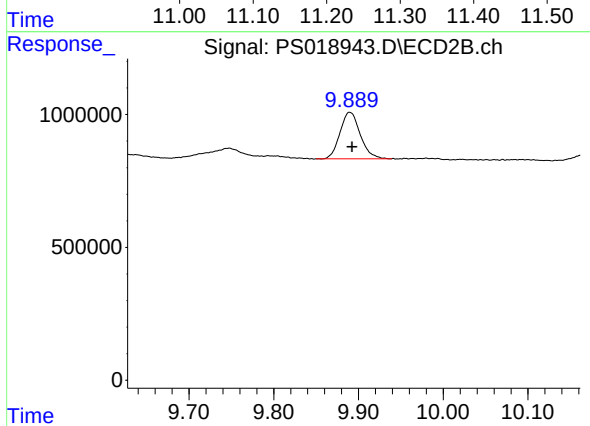

#14 DINOSEB


R.T.: 9.890 min
Delta R.T.: -0.003 min
Response: 2909349
Conc: N.D.

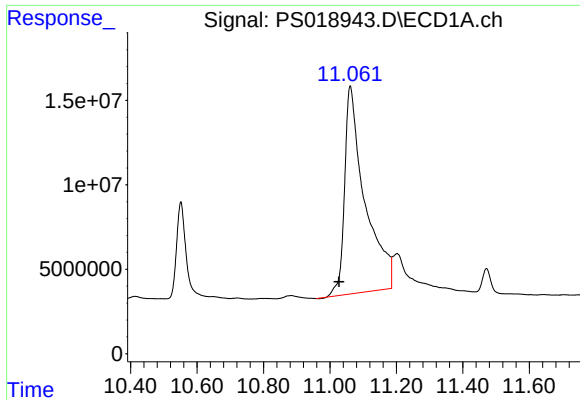

#15 Picloram

R.T.: 11.061 min
Delta R.T.: 0.033 min
Response: 519181350
Conc: 18.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

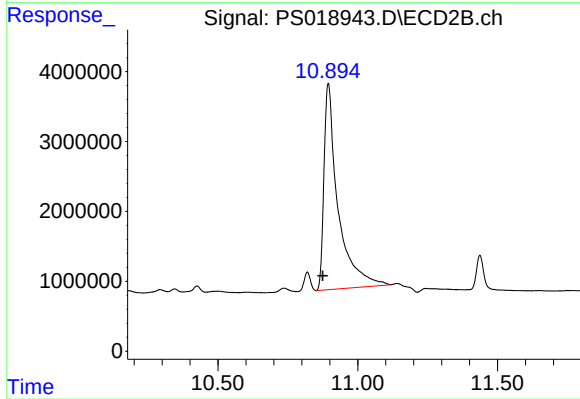

#15 Picloram

R.T.: 10.895 min
Delta R.T.: 0.020 min
Response: 102975859
Conc: 18.21 ng/ml