

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040921\
 Data File : PS014549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 20:19
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 07:44:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.884	682.7E6	256.4E6	448.767	550.785
Target Compounds							
15) T	Picloram	10.951	10.979	26377601	731640	2.358	<MDL #
16) T	DCPA	11.385	0.000	1710793	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040921\
Data File : PS014549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 20:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 07:44:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

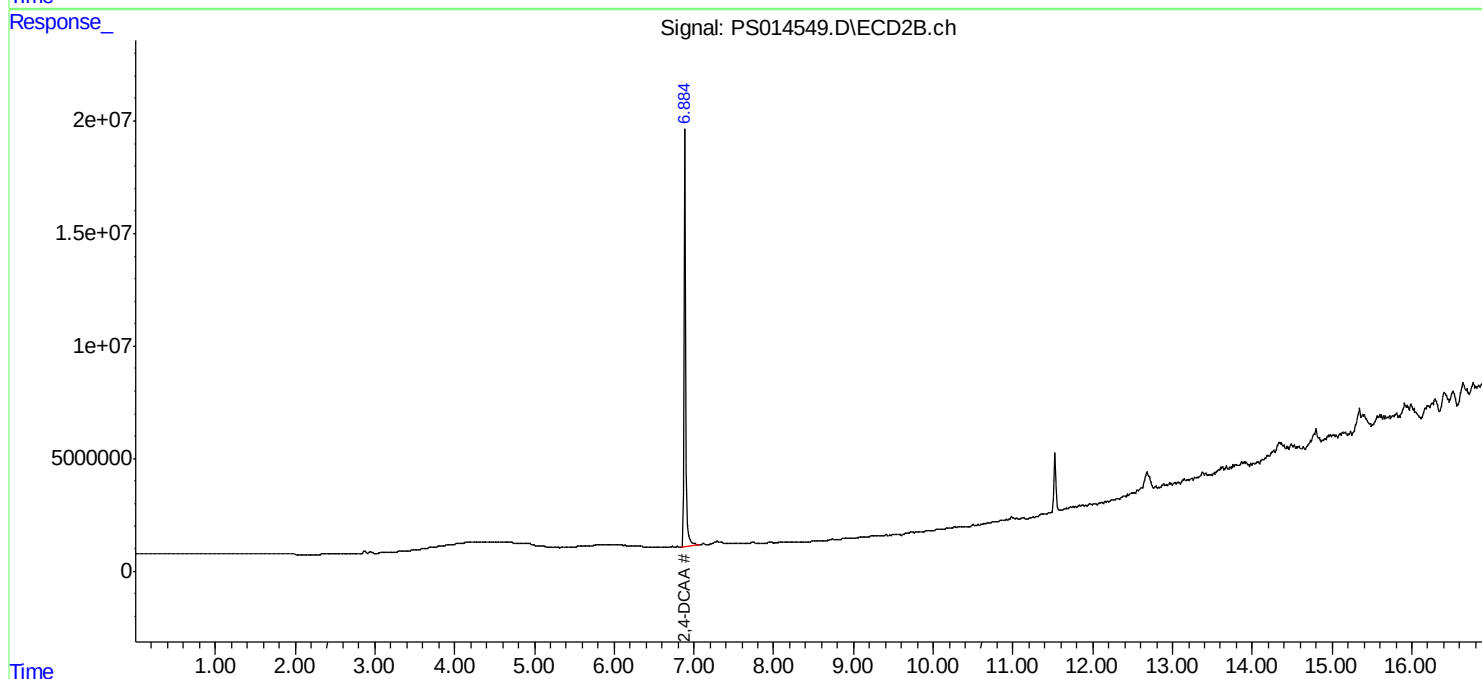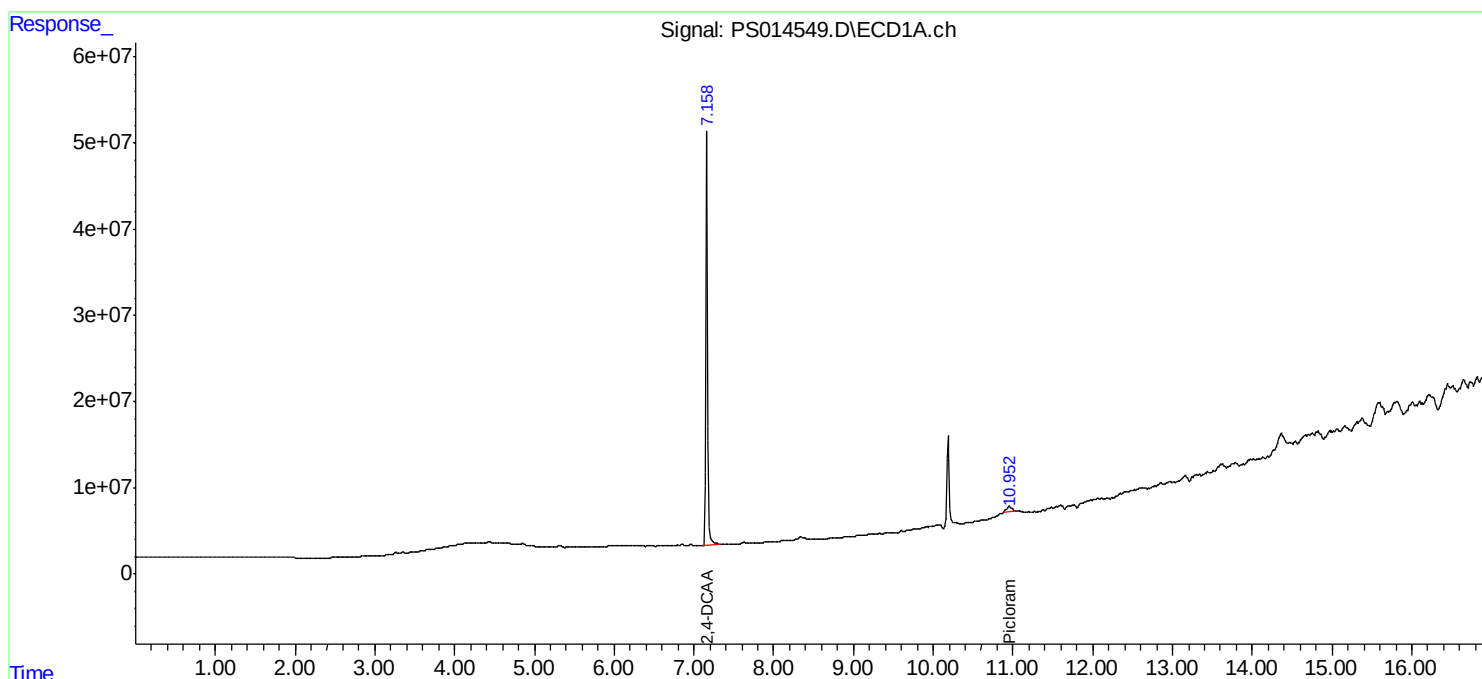


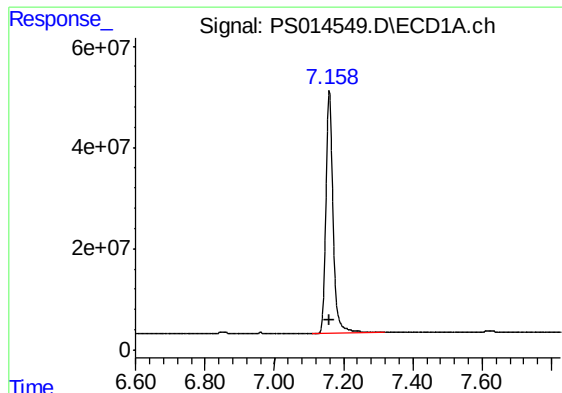

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 682662625
Conc: 448.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

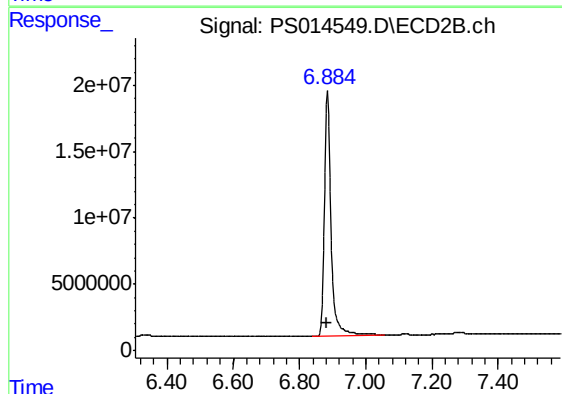


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 256365601
Conc: 550.79 ng/ml

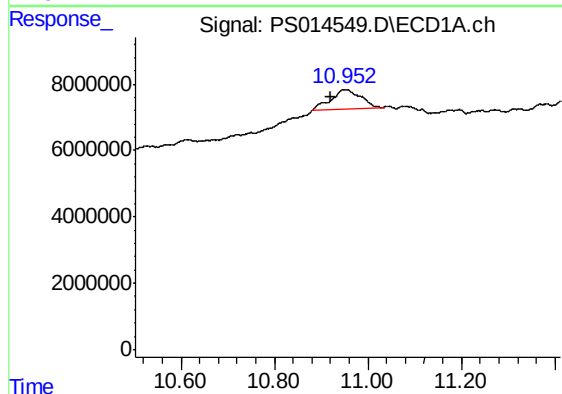

#15 Picloram

R.T.: 10.951 min
Delta R.T.: 0.032 min
Response: 26377601
Conc: 2.36 ng/ml

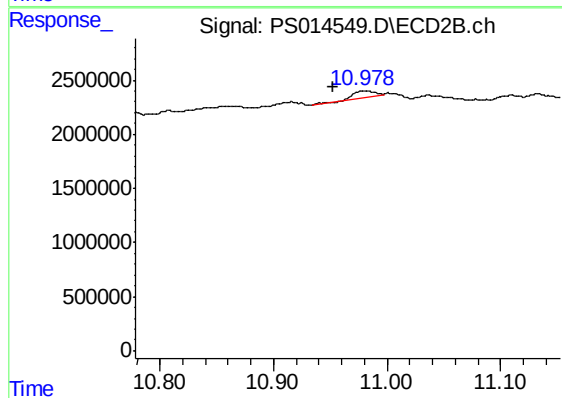

#15 Picloram

R.T.: 10.979 min
Delta R.T.: 0.026 min
Response: 731640
Conc: N.D.