

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040821\
 Data File : PS014550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 20:42
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 07:44:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.883	1195.9E6	374.9E6	786.169	805.433
Target Compounds							
1) T	Dalapon	3.005	2.601	1257.9E6	451.6E6	697.579	693.857
2) T	3,5-DICHL...	6.384	6.046	1494.8E6	547.9E6	721.423	747.107
3) T	4-Nitroph...	6.991	6.498	579.8E6	213.3E6	713.544	755.661
5) T	DICAMBA	7.346	7.049	4341.7E6	1531.6E6	746.209	757.250
6) T	MCPD	7.513	7.146	332.0E6	126.0E6	76.239	74.841
7) T	MCPA	7.662	7.361	463.6E6	180.3E6	74.496	74.223
8) T	DICHLORPROP	8.032	7.675	1032.0E6	378.0E6	737.492	748.702
9) T	2,4-D	8.260	7.970	1185.1E6	430.1E6	745.323	773.483
10) T	Pentachlo...	8.567	8.394	15511.0E6	5066.0E6	738.029	753.580
11) T	2,4,5-TP ...	9.111	8.755	6112.6E6	2079.5E6	746.677	761.243
12) T	2,4,5-T	9.395	9.135	6209.6E6	2043.7E6	754.872	781.365
13) T	2,4-DB	9.942	9.640	1155.0E6	255.8E6	759.013	737.462
14) T	DINSEB	11.096	9.971	4603.7E6	1446.3E6	714.460	751.058
15) T	Picloram	10.918	10.953	8610.4E6	2954.6E6	769.594	787.919
16) T	DCPA	11.360	10.896	9215.3E6	3121.3E6	747.873	768.657



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040921\
Data File : PS014550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 20:42
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 07:44:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

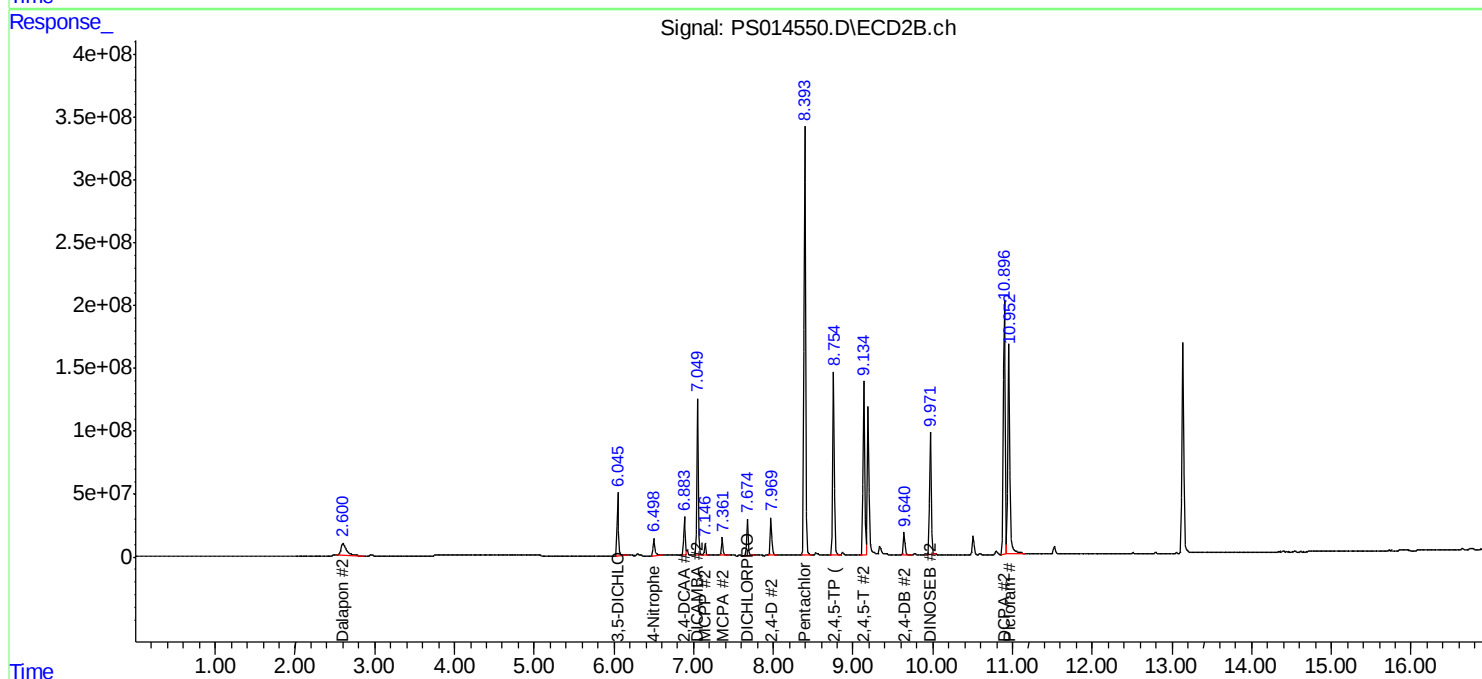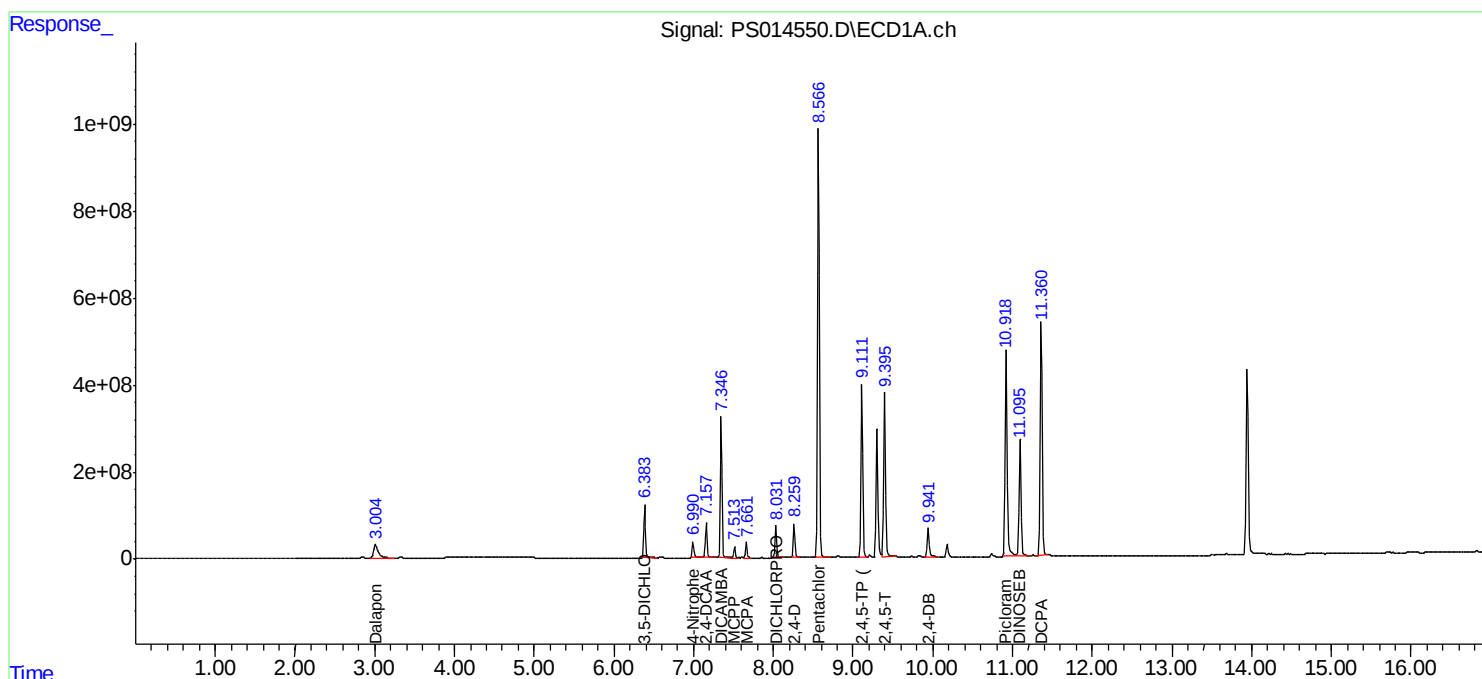


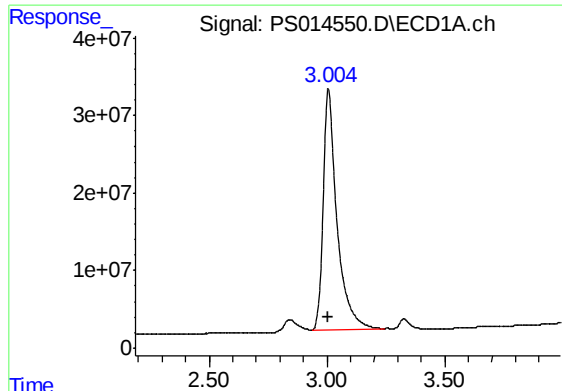

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.001 min
Response: 1257855271
Conc: 697.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

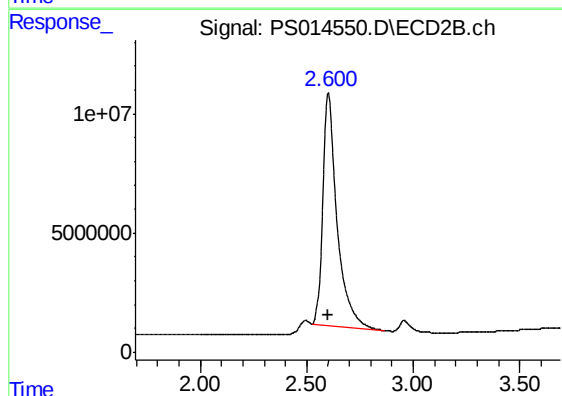


#1 Dalapon

R.T.: 2.601 min
Delta R.T.: -0.002 min
Response: 451579600
Conc: 693.86 ng/ml

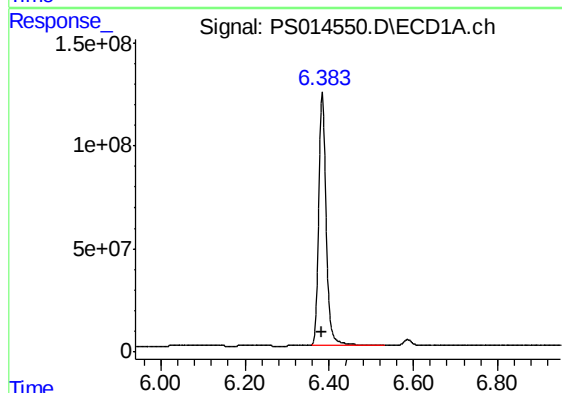


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 1494791295
Conc: 721.42 ng/ml

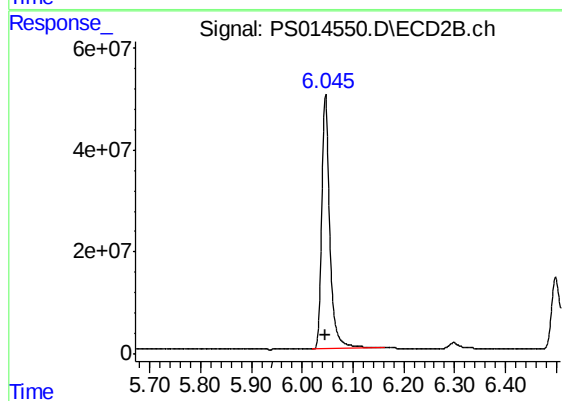

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 547850876
Conc: 747.11 ng/ml

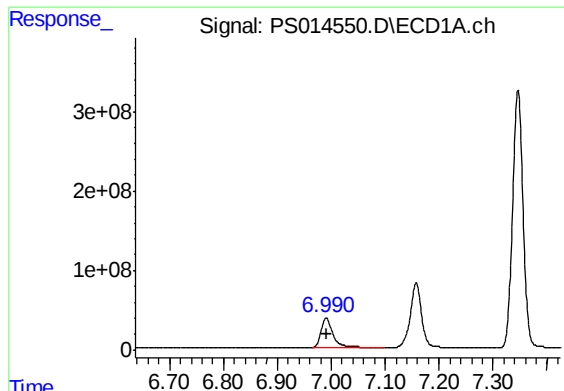

#3 4-Nitrophenol


R.T.: 6.991 min
Delta R.T.: 0.000 min
Response: 579842253
Conc: 713.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

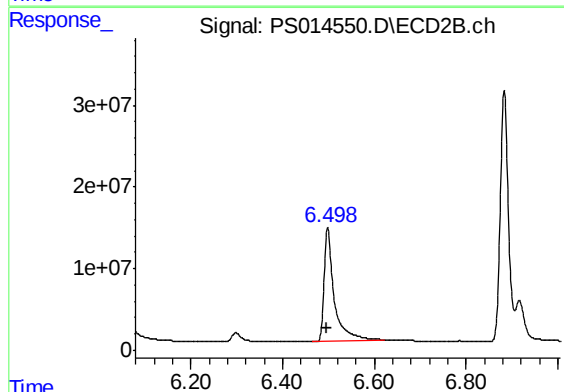


#3 4-Nitrophenol

R.T.: 6.498 min
Delta R.T.: 0.001 min
Response: 213348058
Conc: 755.66 ng/ml

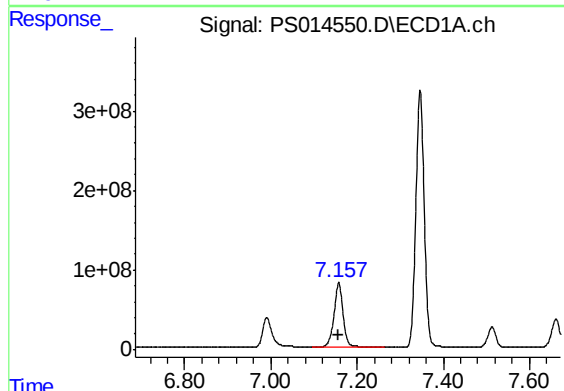


#4 2,4-DCAA

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 1195917148
Conc: 786.17 ng/ml

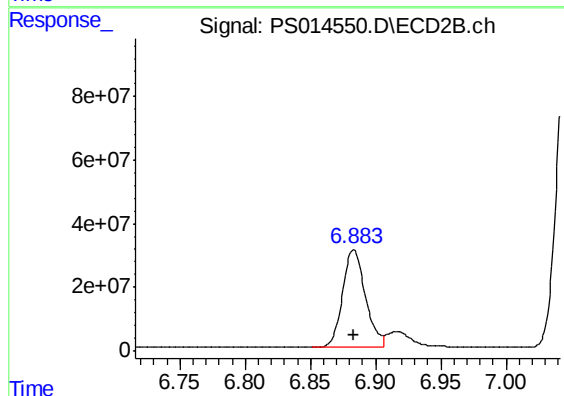

#4 2,4-DCAA


R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 374892544
Conc: 805.43 ng/ml

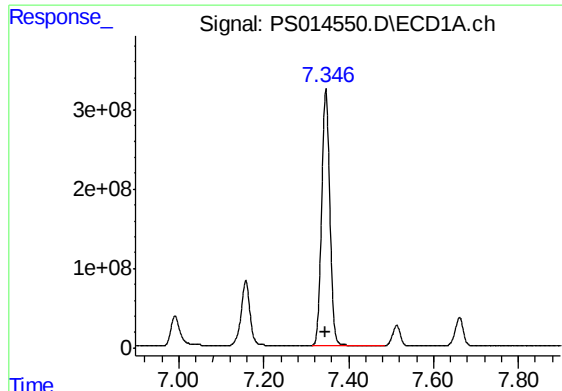

#5 DICAMBA


R.T.: 7.346 min
Delta R.T.: 0.000 min
Response: 4341711539
Conc: 746.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

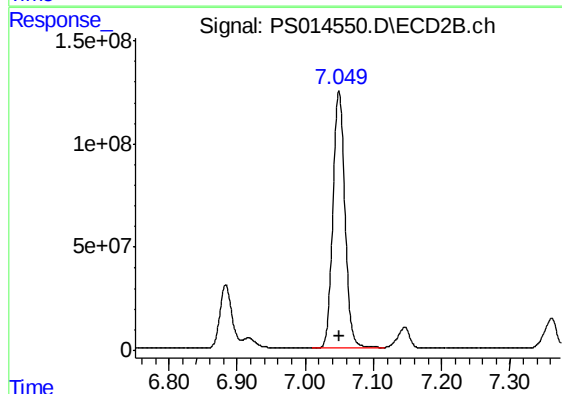


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 1531558212
Conc: 757.25 ng/ml

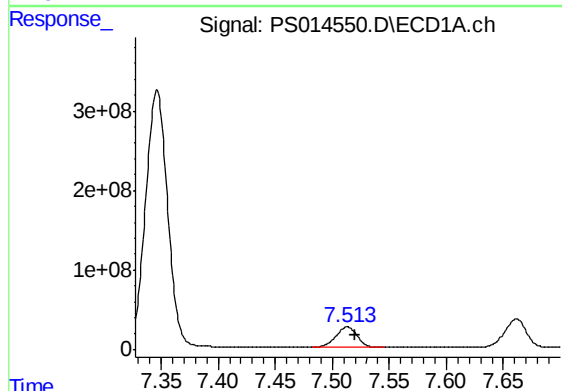


#6 MCPP

R.T.: 7.513 min
Delta R.T.: -0.006 min
Response: 331959519
Conc: 76.24 ug/ml

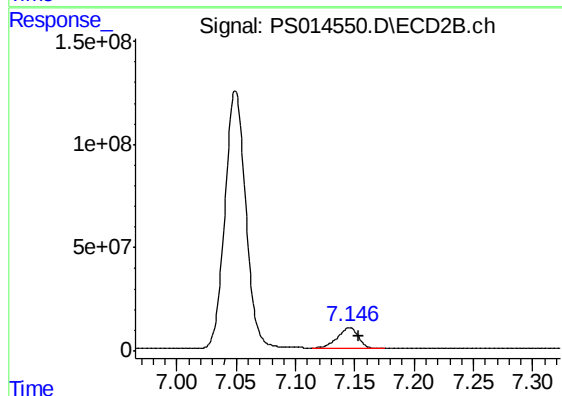

#6 MCPP


R.T.: 7.146 min
Delta R.T.: -0.007 min
Response: 126036125
Conc: 74.84 ug/ml

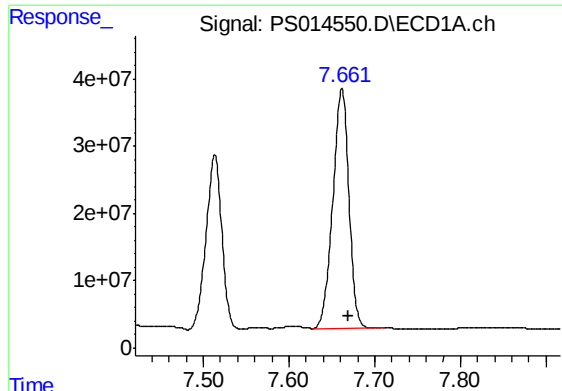

#7 MCPA


R.T.: 7.662 min
Delta R.T.: -0.008 min
Response: 463582742
Conc: 74.50 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

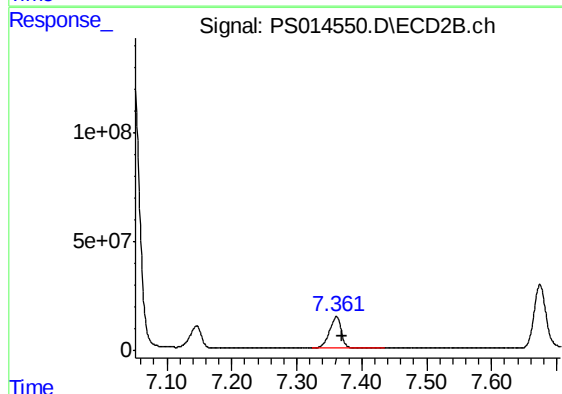


#7 MCPA

R.T.: 7.361 min
Delta R.T.: -0.009 min
Response: 180252406
Conc: 74.22 ug/ml

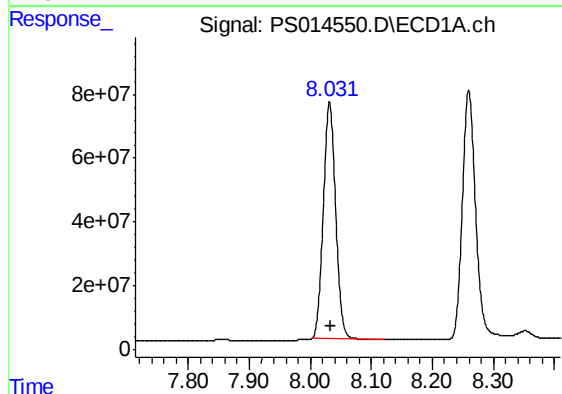


#8 DICHLORPROP

R.T.: 8.032 min
Delta R.T.: -0.001 min
Response: 1031996010
Conc: 737.49 ng/ml

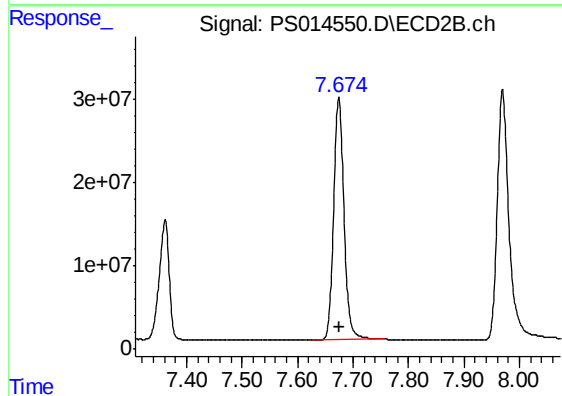

#8 DICHLORPROP


R.T.: 7.675 min
Delta R.T.: 0.000 min
Response: 377960382
Conc: 748.70 ng/ml

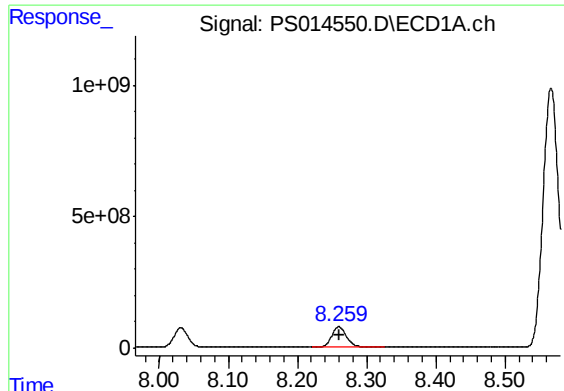

#9 2,4-D


R.T.: 8.260 min
Delta R.T.: 0.000 min
Response: 1185053689
Conc: 745.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

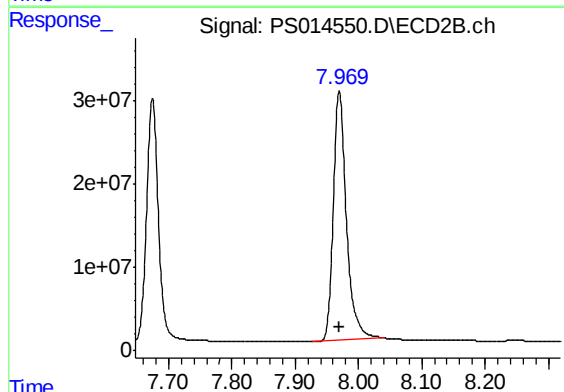


#9 2,4-D

R.T.: 7.970 min
Delta R.T.: 0.000 min
Response: 430129643
Conc: 773.48 ng/ml

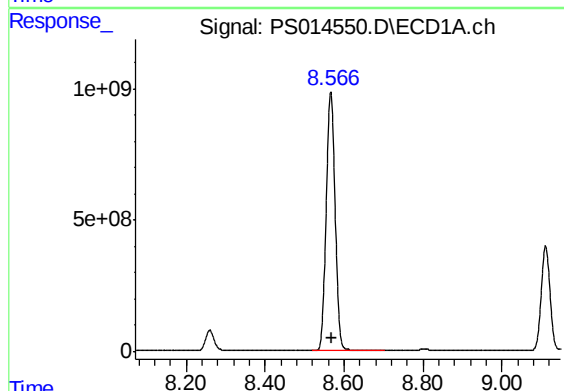


#10 Pentachlorophenol

R.T.: 8.567 min
Delta R.T.: -0.002 min
Response: 15510957193
Conc: 738.03 ng/ml

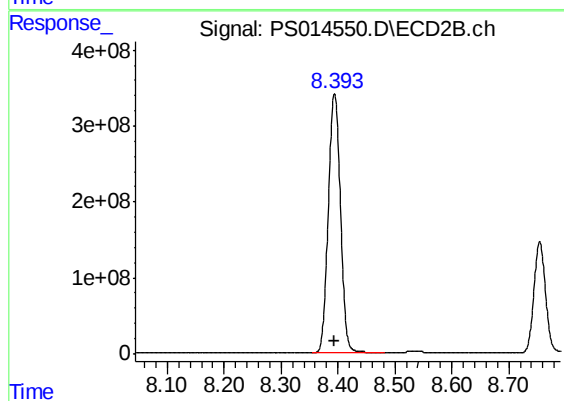

#10 Pentachlorophenol


R.T.: 8.394 min
Delta R.T.: 0.000 min
Response: 5065977044
Conc: 753.58 ng/ml

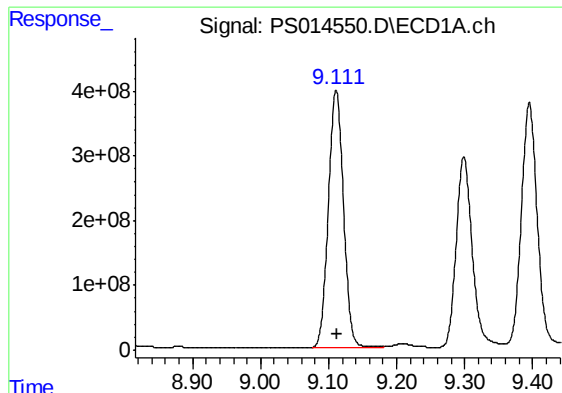

#11 2,4,5-TP (SILVEX)


R.T.: 9.111 min
Delta R.T.: -0.001 min
Response: 6112610249
Conc: 746.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

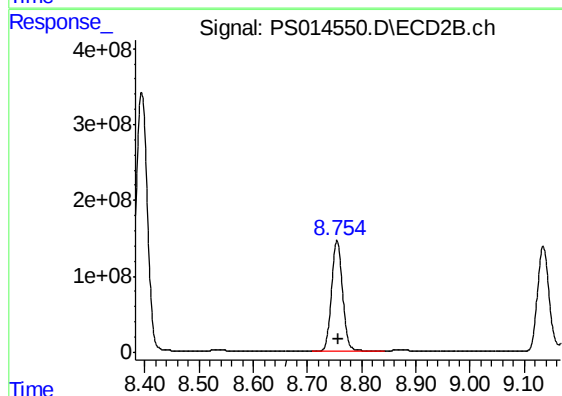


#11 2,4,5-TP (SILVEX)

R.T.: 8.755 min
Delta R.T.: -0.001 min
Response: 2079465006
Conc: 761.24 ng/ml

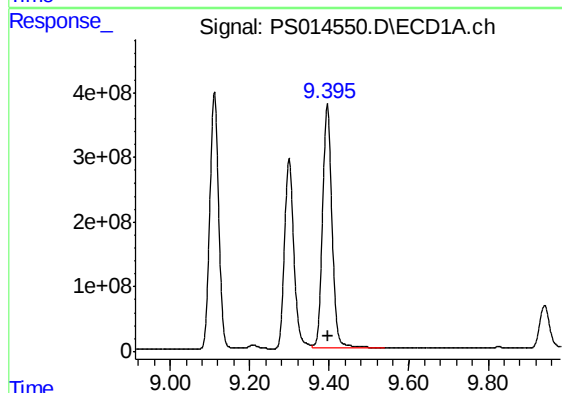


#12 2,4,5-T

R.T.: 9.395 min
Delta R.T.: 0.000 min
Response: 6209646223
Conc: 754.87 ng/ml

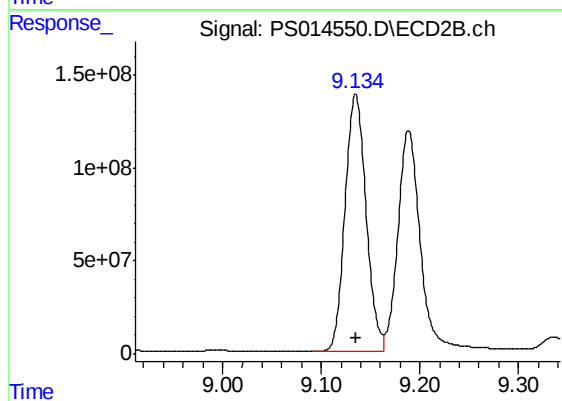

#12 2,4,5-T


R.T.: 9.135 min
Delta R.T.: 0.000 min
Response: 2043694492
Conc: 781.37 ng/ml

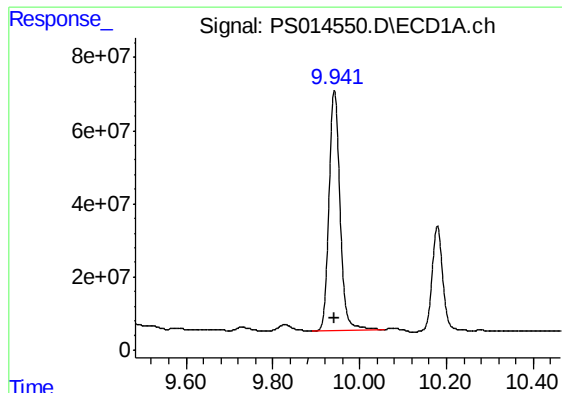

#13 2,4-DB


R.T.: 9.942 min
Delta R.T.: 0.000 min
Response: 1155031868
Conc: 759.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

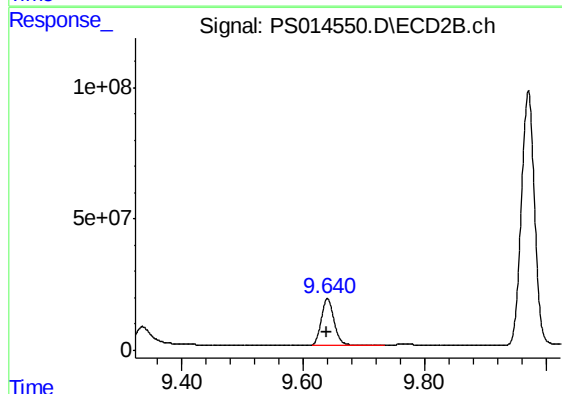


#13 2,4-DB

R.T.: 9.640 min
Delta R.T.: 0.000 min
Response: 255805000
Conc: 737.46 ng/ml

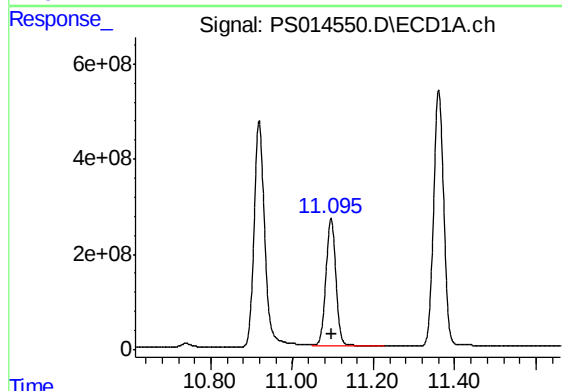


#14 DINOSEB

R.T.: 11.096 min
Delta R.T.: 0.000 min
Response: 4603730672
Conc: 714.46 ng/ml

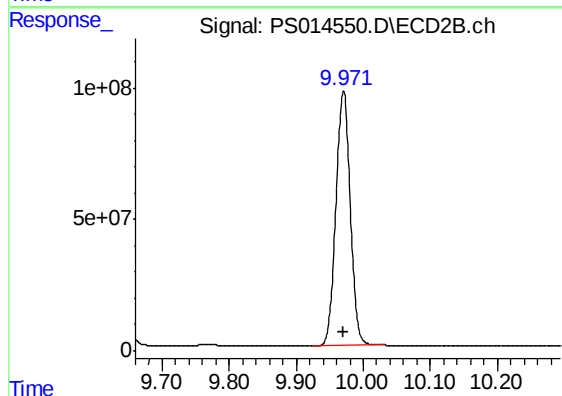

#14 DINOSEB


R.T.: 9.971 min
Delta R.T.: 0.000 min
Response: 1446294631
Conc: 751.06 ng/ml

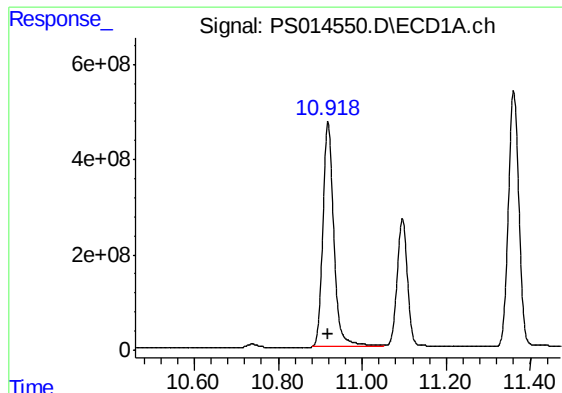

#15 Picloram


R.T.: 10.918 min
Delta R.T.: 0.000 min
Response: 8610444906
Conc: 769.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

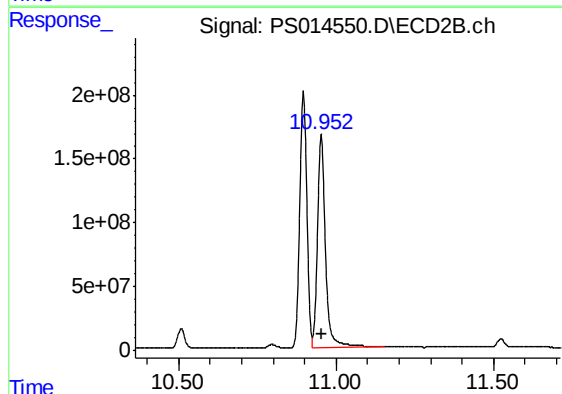


#15 Picloram

R.T.: 10.953 min
Delta R.T.: 0.000 min
Response: 2954619761
Conc: 787.92 ng/ml

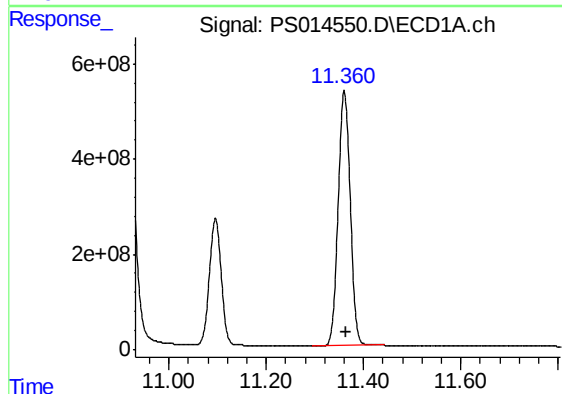

#16 DCPA

R.T.: 11.360 min
Delta R.T.: -0.003 min
Response: 9215317605
Conc: 747.87 ng/ml

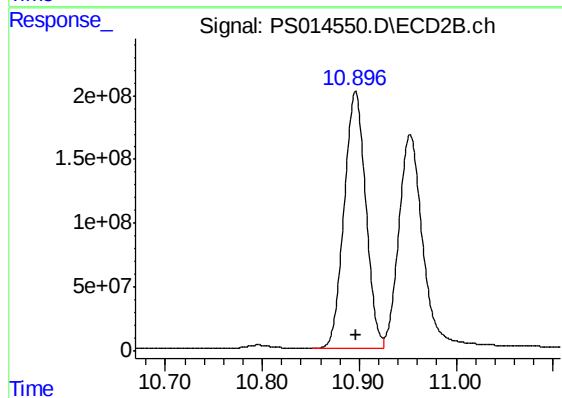

#16 DCPA

R.T.: 10.896 min
Delta R.T.: -0.001 min
Response: 3121269964
Conc: 768.66 ng/ml