

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041122\
 Data File : PS018950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 10:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:25:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.805	1628.7E6	349.8E6	557.861	489.984
Target Compounds							
11) T	2,4,5-TP ...	0.000	8.648	0	3814621	N.D.	<MDL
12) T	2,4,5-T	9.447f	0.000	74348486	0	3.627	N.D. #
13) T	2,4-DB	0.000	9.498f	0	7640383	N.D.	13.414
15) T	Picloram	11.089f	10.918f	316.9E6	62973288	11.328	11.137
16) T	DCPA	11.474	0.000	5331012	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041122\
Data File : PS018950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 10:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:25:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

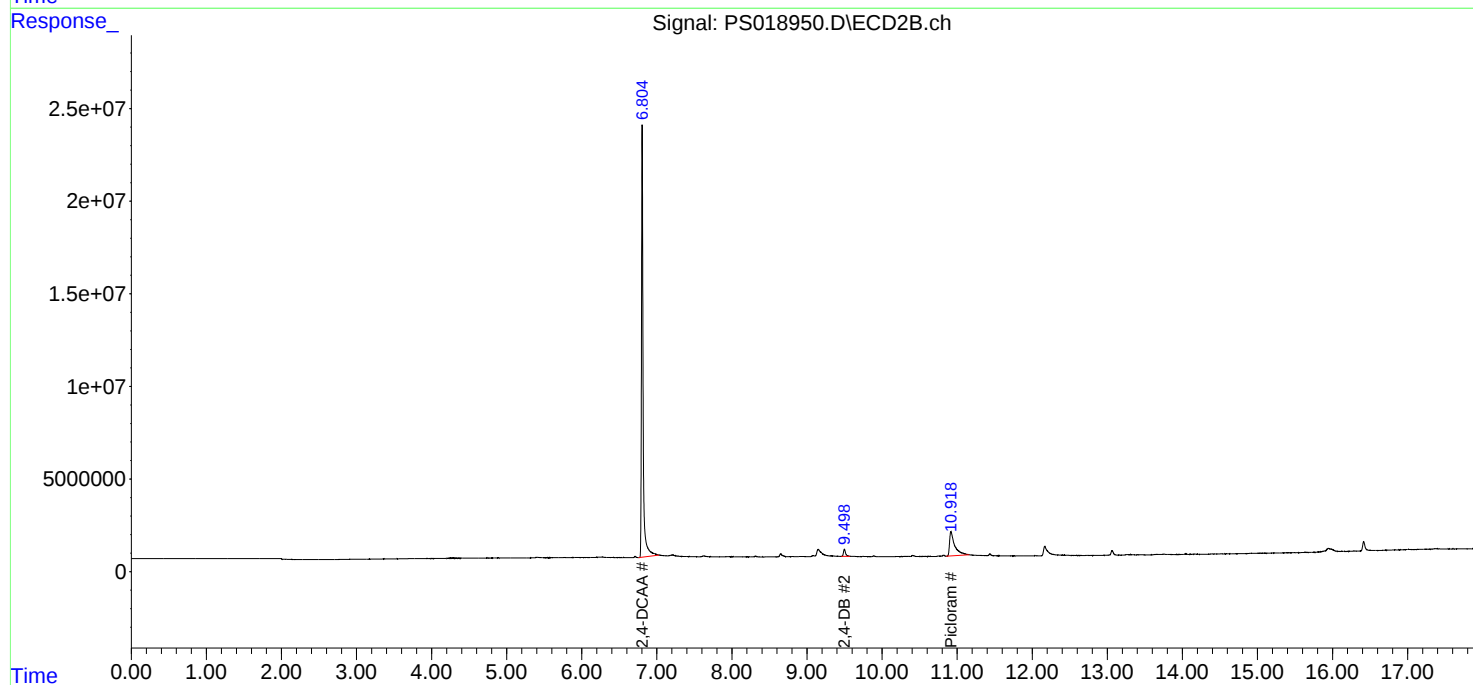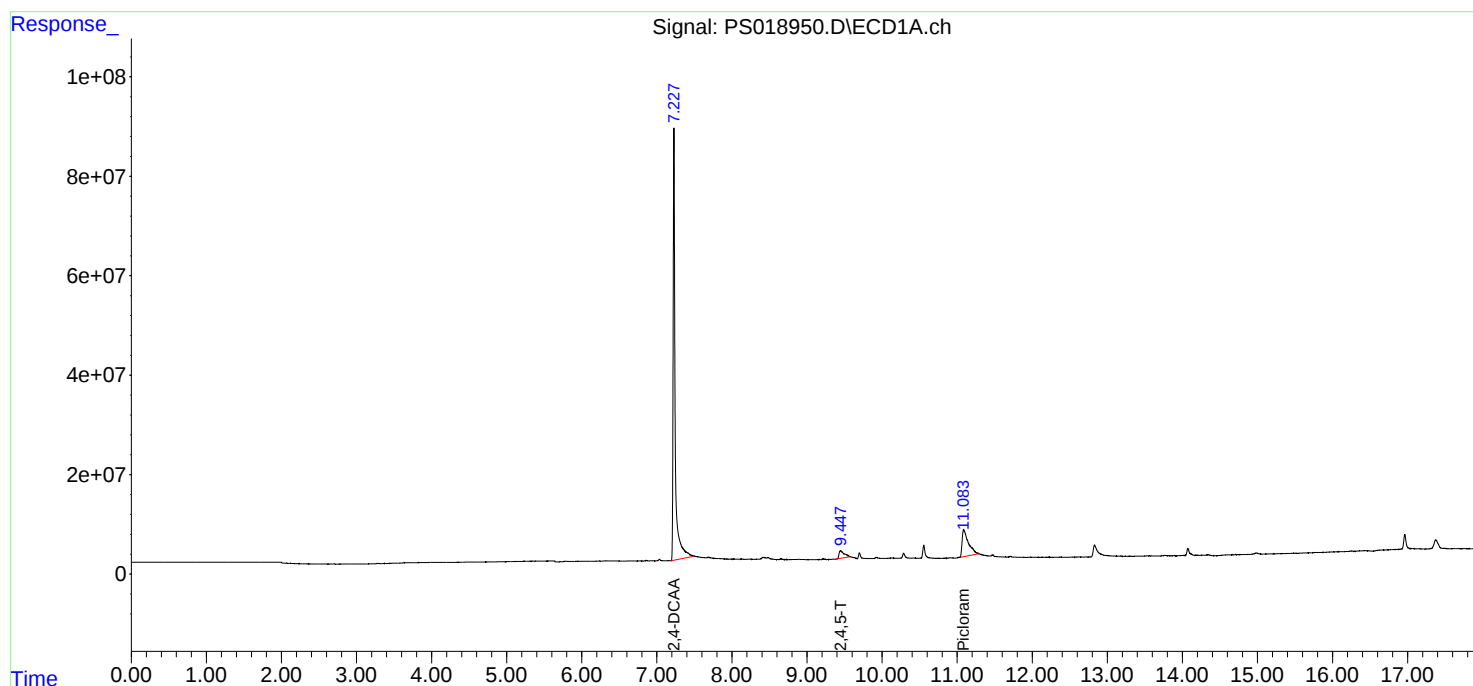


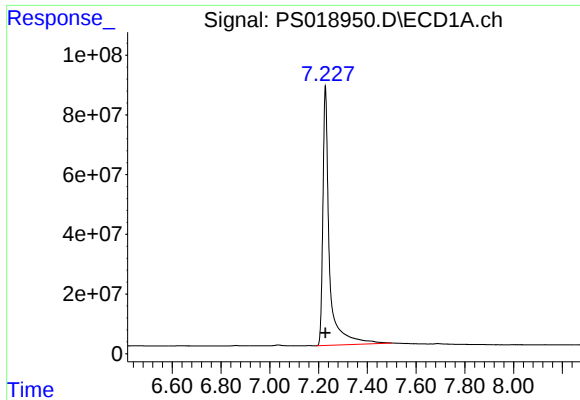

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 1628653083
Conc: 557.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

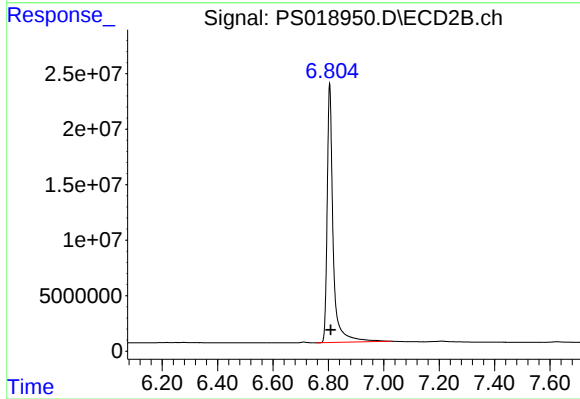


#4 2,4-DCAA

R.T.: 6.805 min
Delta R.T.: -0.004 min
Response: 349820467
Conc: 489.98 ng/ml

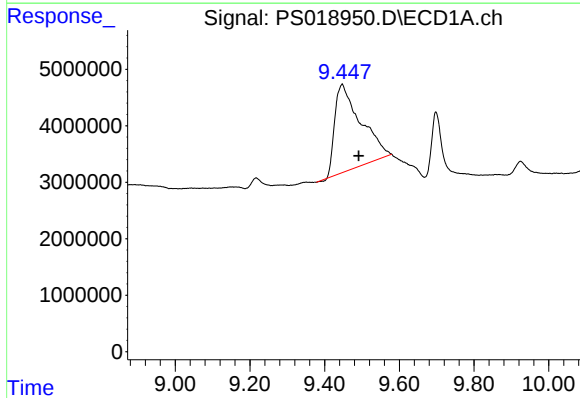


#12 2,4,5-T

R.T.: 9.447 min
Delta R.T.: -0.044 min
Response: 74348486
Conc: 3.63 ng/ml

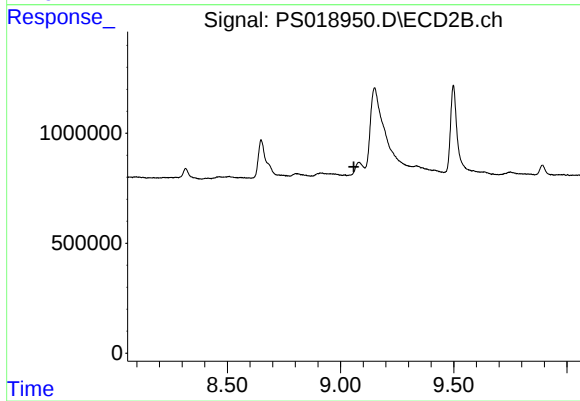

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

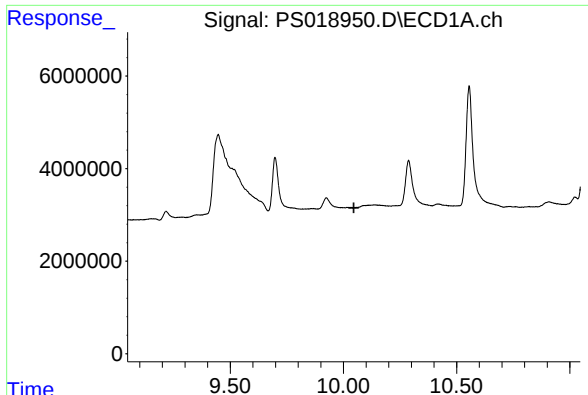

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

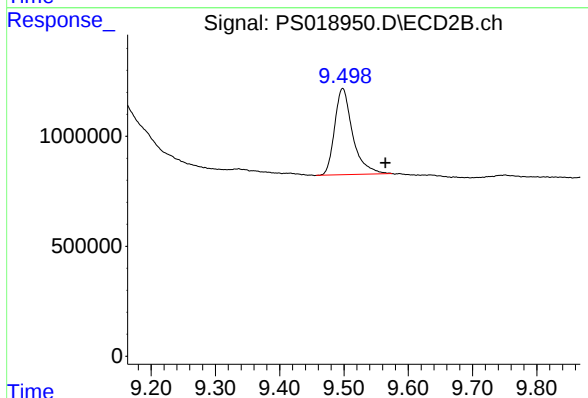


#13 2,4-DB

R.T.: 9.498 min
Delta R.T.: -0.067 min
Response: 7640383
Conc: 13.41 ng/ml

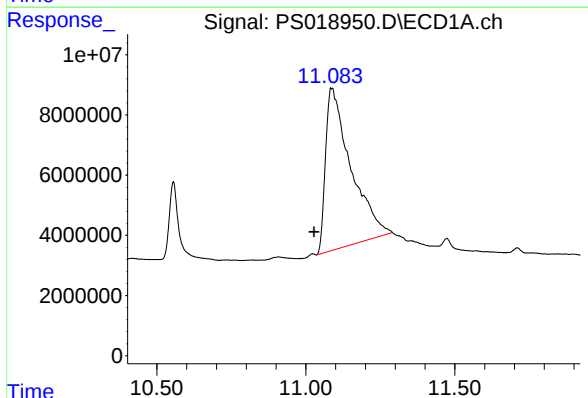

#15 Picloram

R.T.: 11.089 min
Delta R.T.: 0.061 min
Response: 316939576
Conc: 11.33 ng/ml

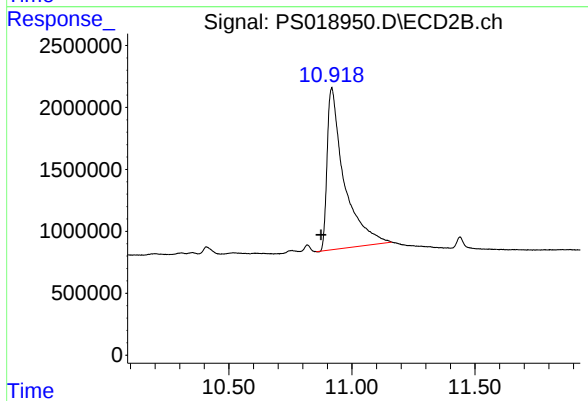

#15 Picloram

R.T.: 10.918 min
Delta R.T.: 0.043 min
Response: 62973288
Conc: 11.14 ng/ml