

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041125\
Data File : PS029813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2025 16:43
Operator : AR\AJ
Sample : Q1771-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3A

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:03:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040225.M
Quant Title : 8080.M
QLast Update : Wed Apr 02 23:52:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.954	7.495	855.5E6	258.2E6	419.610m	378.882m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041125\
Data File : PS029813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2025 16:43
Operator : AR\AJ
Sample : Q1771-09
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-3A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/14/2025
Supervised By : mohammad ahmed 04/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:03:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040225.M
Quant Title : 8080.M
QLast Update : Wed Apr 02 23:52:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

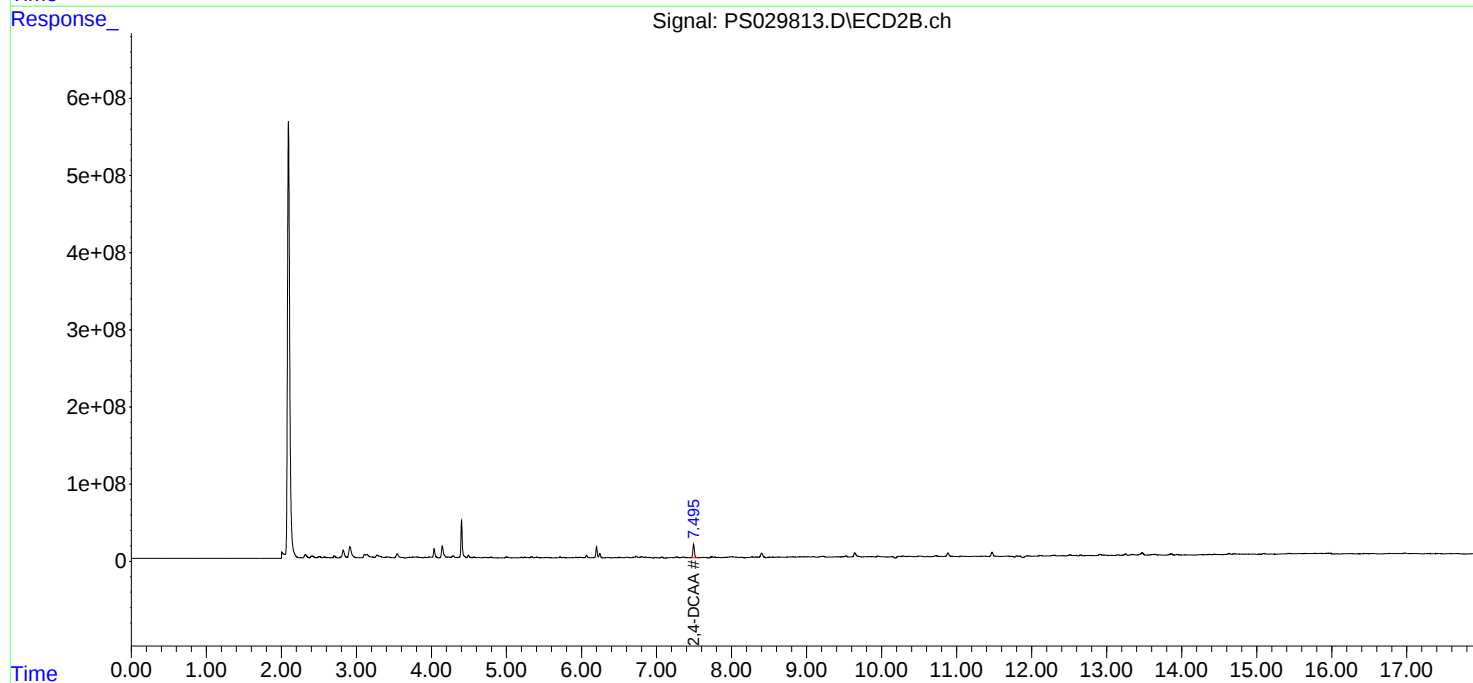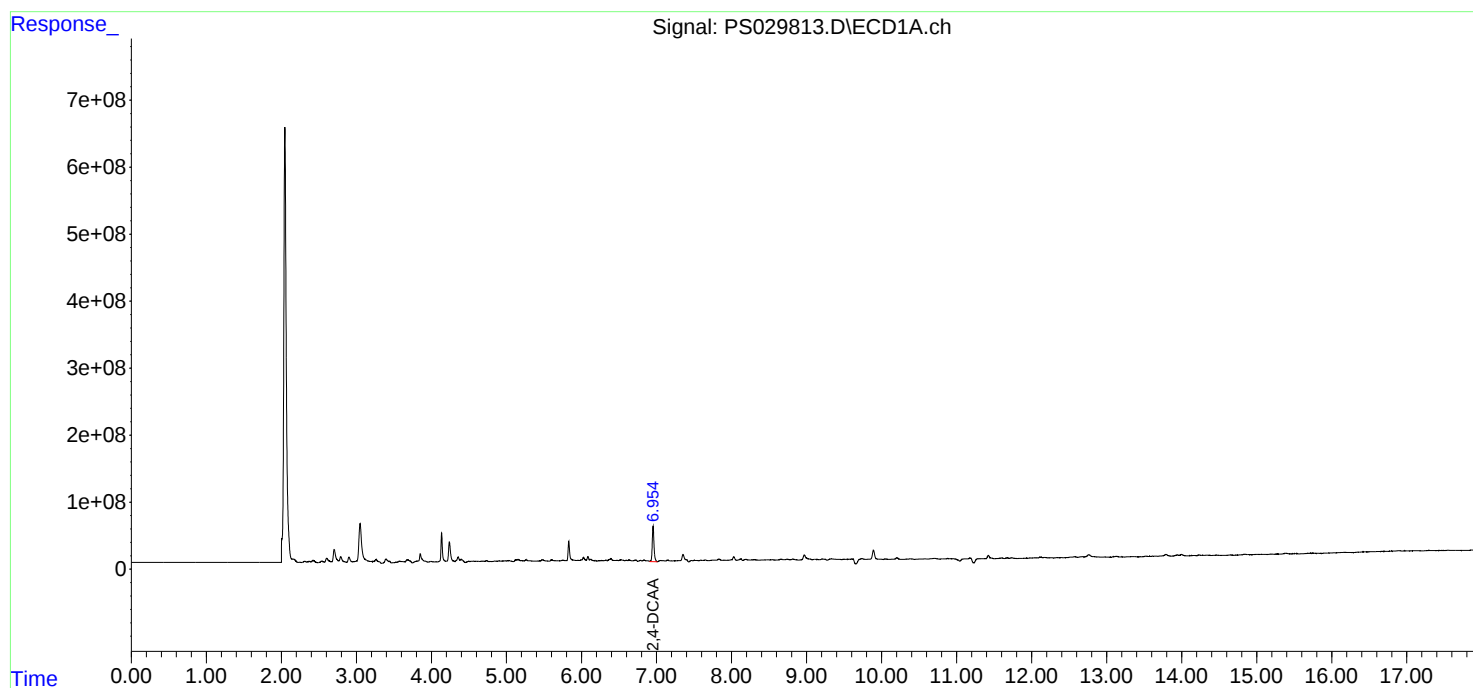

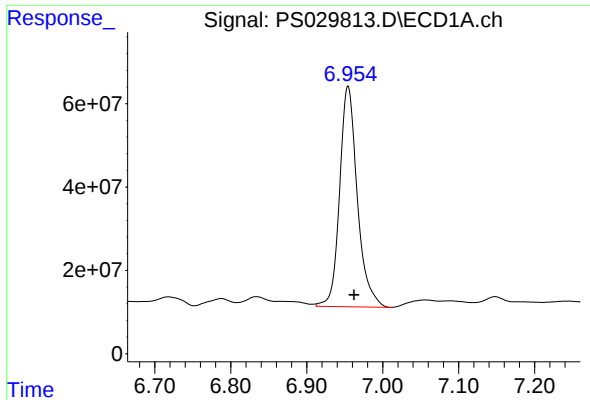


#4 2,4-DCAA

R.T.: 6.954 min
Delta R.T.: -0.009 min
Response: 855513789
Conc: 419.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3A

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/14/2025
Supervised By :mohammad ahmed 04/15/2025

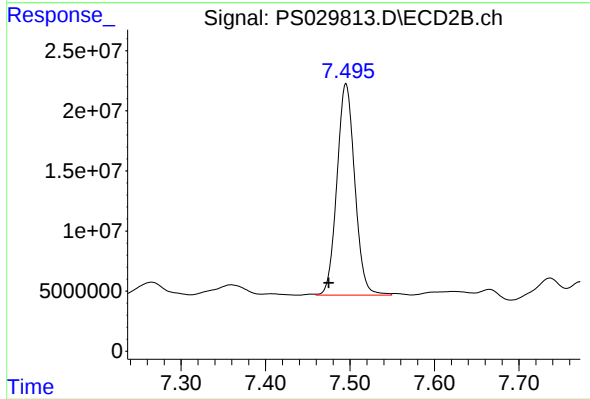

#4 2,4-DCAA

R.T.: 7.495 min
Delta R.T.: 0.020 min
Response: 258213312
Conc: 378.88 ng/ml m