

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041221\
 Data File : PS014564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 17:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 18:04:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.884	687.2E6	260.6E6	451.764	559.807
Target Compounds							
7) T	MCPA	7.629f	0.000	7355323	0	1.182	N.D. #
8) T	DICHLORPROP	0.000	7.732f	0	1343431	N.D.	2.661
13) T	2,4-DB	0.000	9.707f	0	3073104	N.D.	8.859
15) T	Picloram	10.946	0.000	3559208	0	<MDL	N.D. #
16) T	DCPA	0.000	10.852f	0	669771	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041221\
Data File : PS014564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 17:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 18:04:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

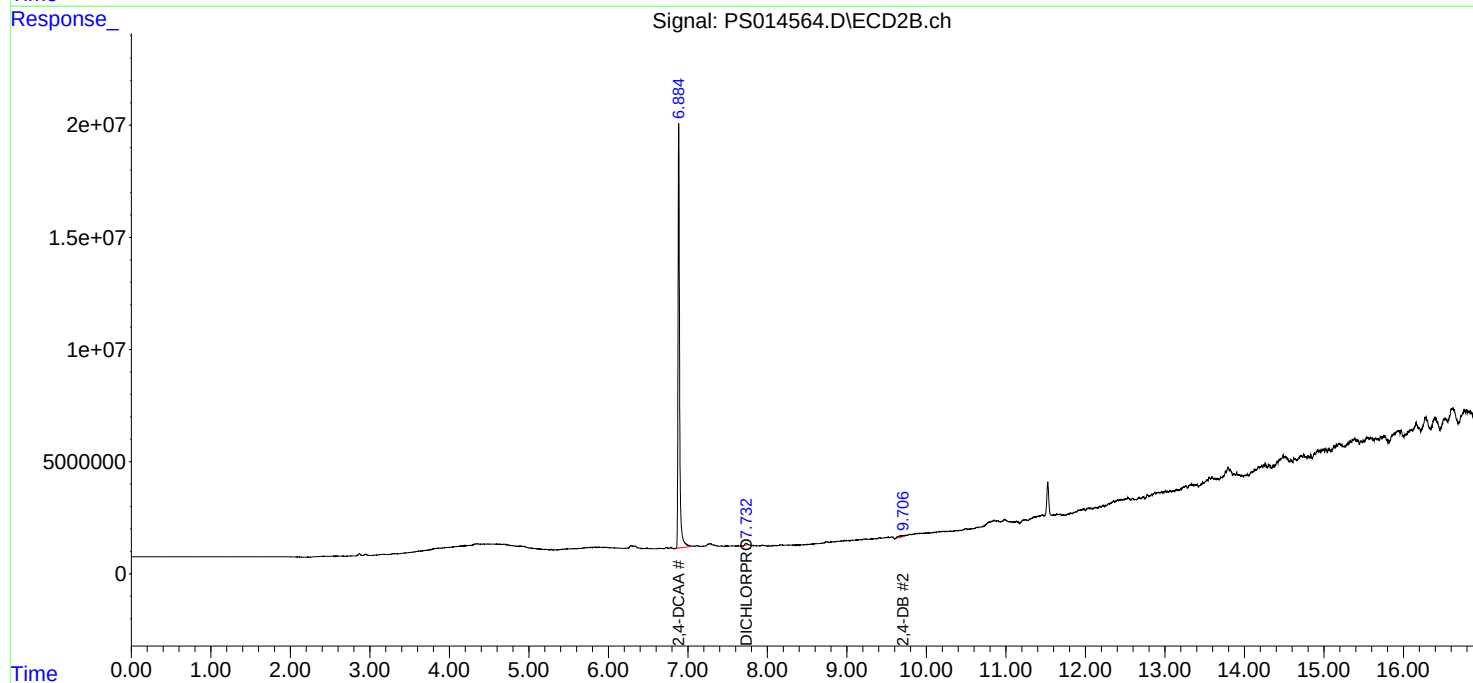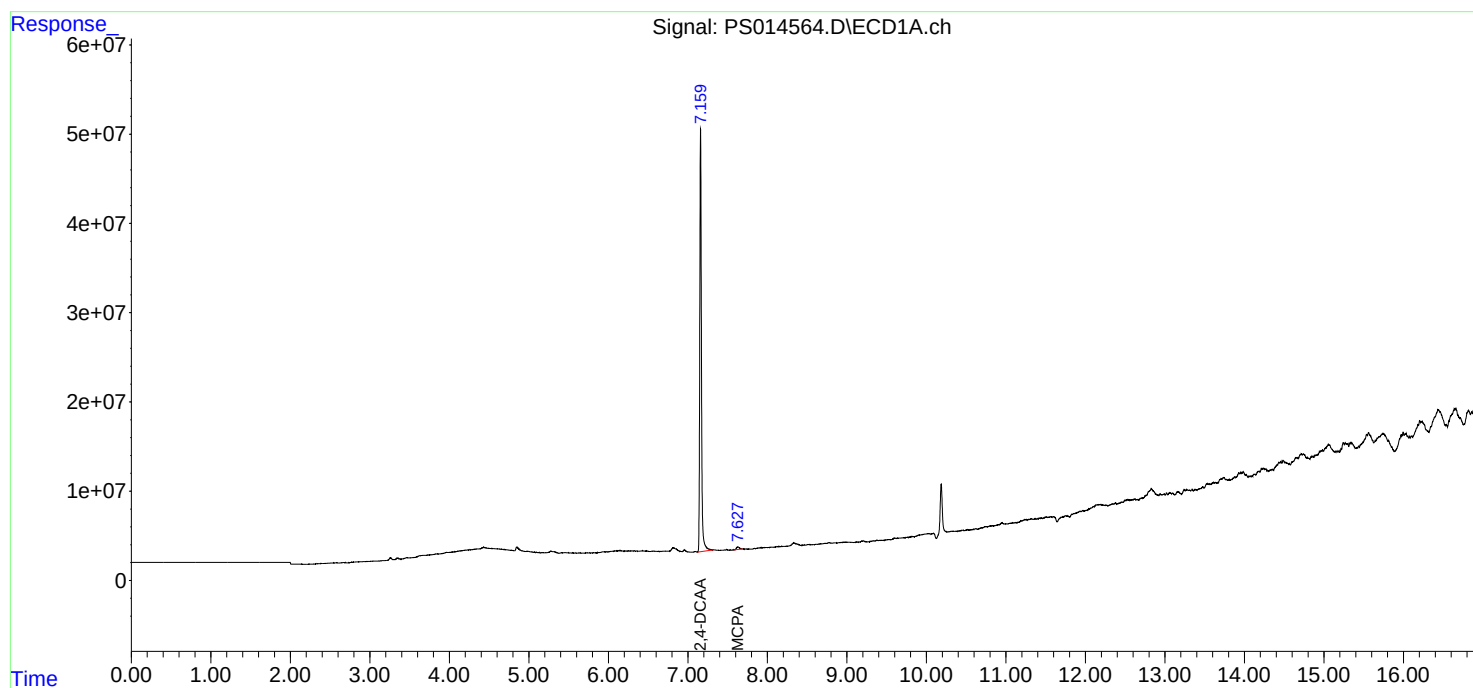


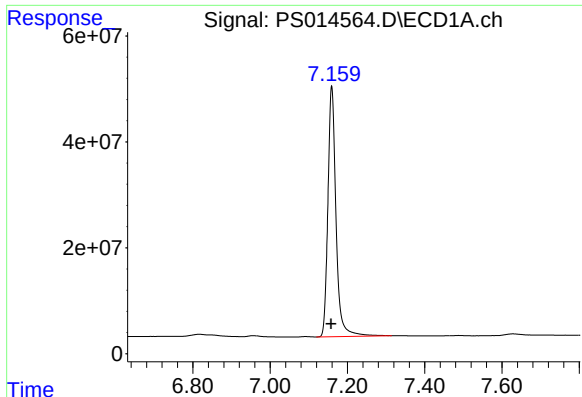

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.001 min
Response: 687222009
Conc: 451.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

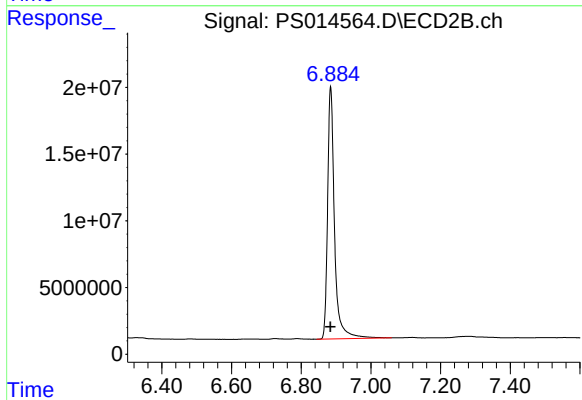


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 260564742
Conc: 559.81 ng/ml

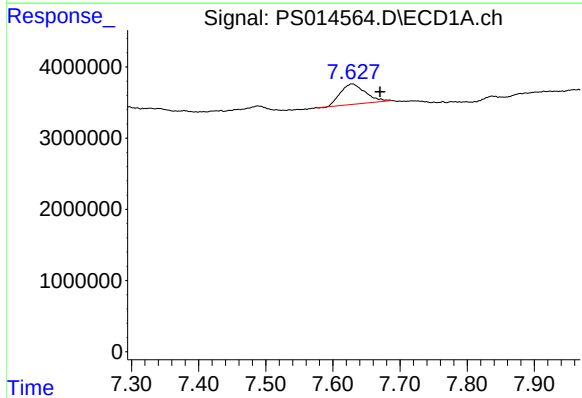


#7 MCPA

R.T.: 7.629 min
Delta R.T.: -0.042 min
Response: 7355323
Conc: 1.18 ug/ml

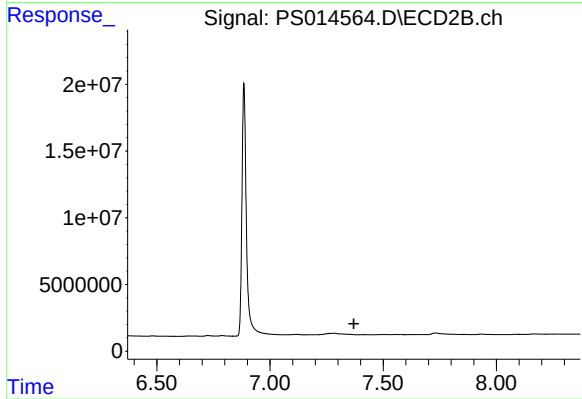

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

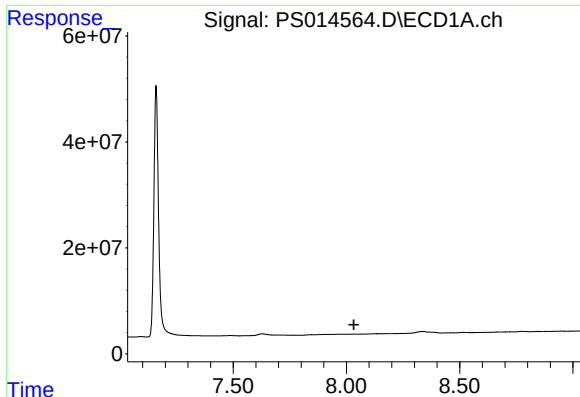

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

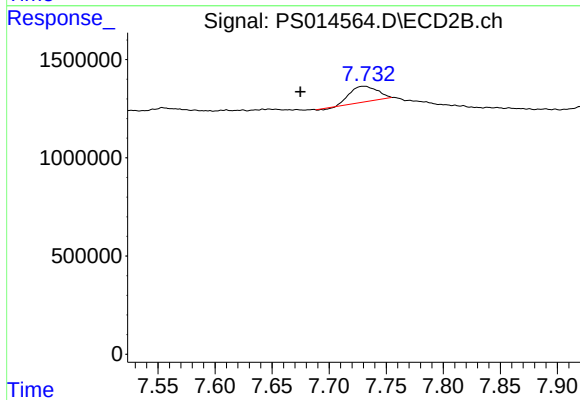


#8 DICHLORPROP

R.T.: 7.732 min
Delta R.T.: 0.057 min
Response: 1343431
Conc: 2.66 ng/ml

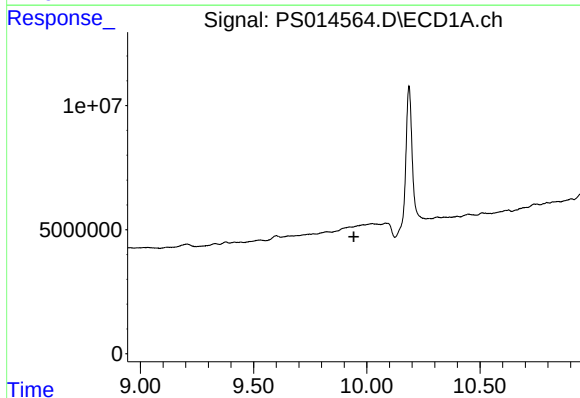

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.943 min
Response: 0
Conc: N.D.

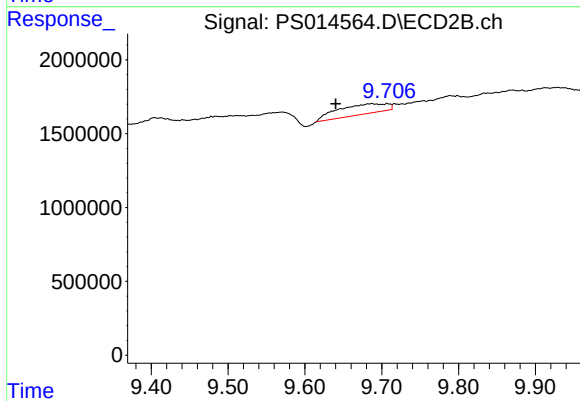

#13 2,4-DB

R.T.: 9.707 min
Delta R.T.: 0.067 min
Response: 3073104
Conc: 8.86 ng/ml