

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041222\
 Data File : PS018965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2022 09:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 15:55:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.805	1445.8E6	327.2E6	495.227	458.240
Target Compounds							
3) T	4-Nitroph...	7.029	0.000	1683103	0	1.474	N.D. #
5) T	DICAMBA	7.414	6.970	21363042	1937573	1.699	<MDL #
10) T	Pentachlo...	8.655	0.000	3957844	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.215	8.645	4151331	6610642	<MDL	1.446 #
12) T	2,4,5-T	9.512	9.078	26455135	2318892	1.290	<MDL #
13) T	2,4-DB	0.000	9.497f	0	8113845	N.D.	14.245
15) T	Picloram	11.020	10.907	1351639	61319013	<MDL	10.845 #
16) T	DCPA	11.471	0.000	6797034	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041222\
Data File : PS018965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2022 09:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:55:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

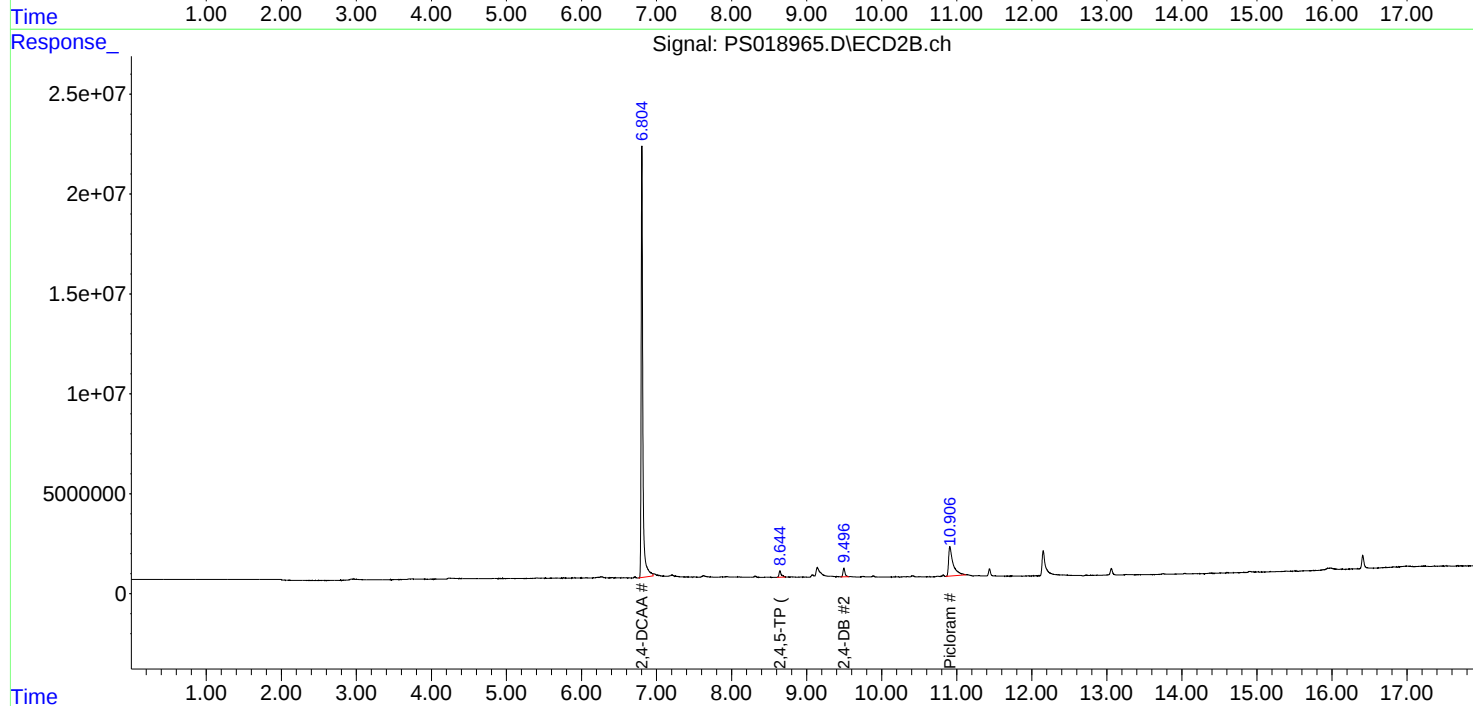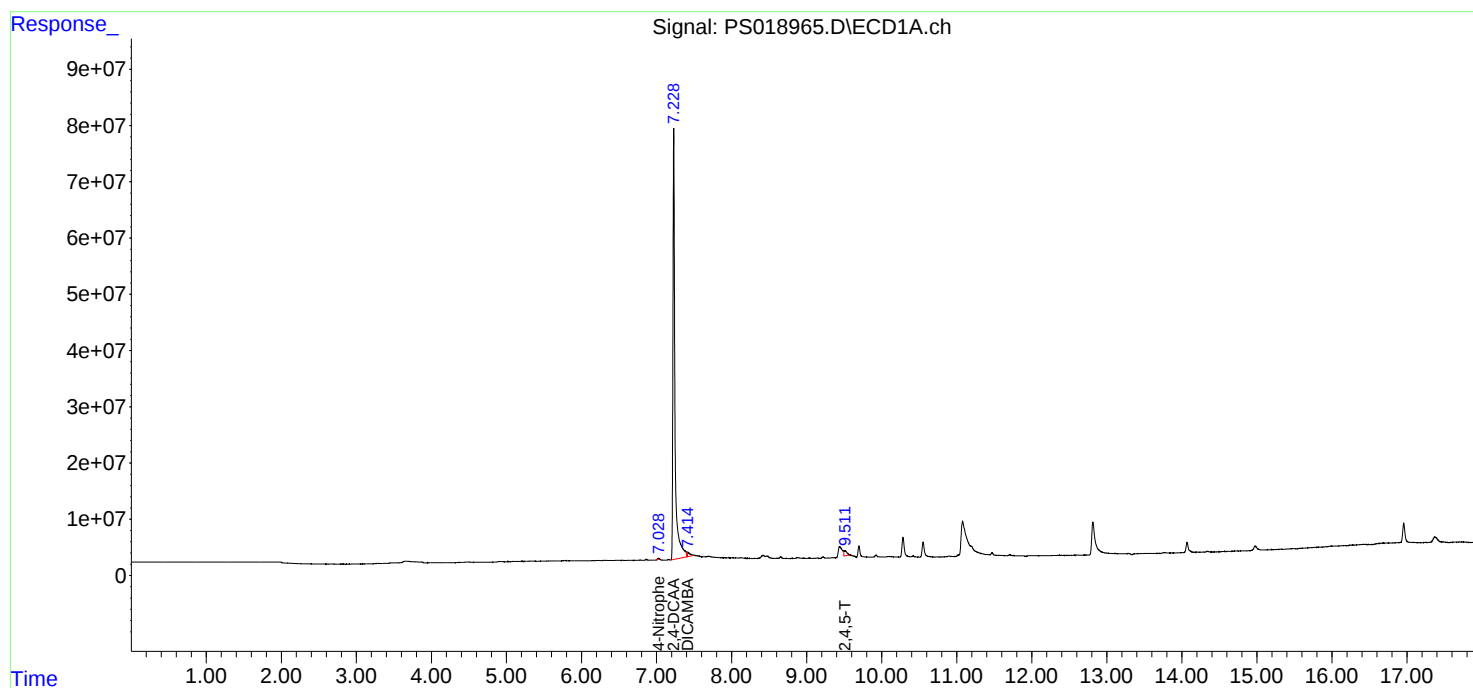


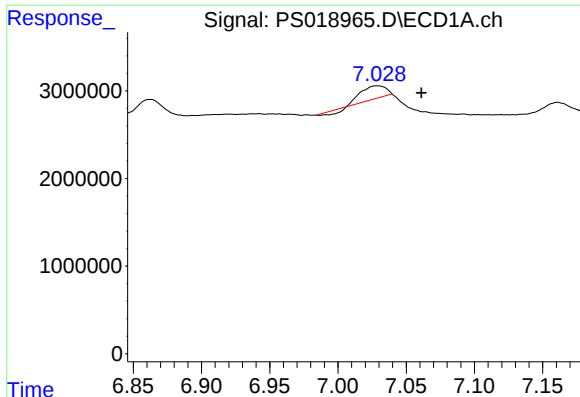

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.032 min
Response: 1683103
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

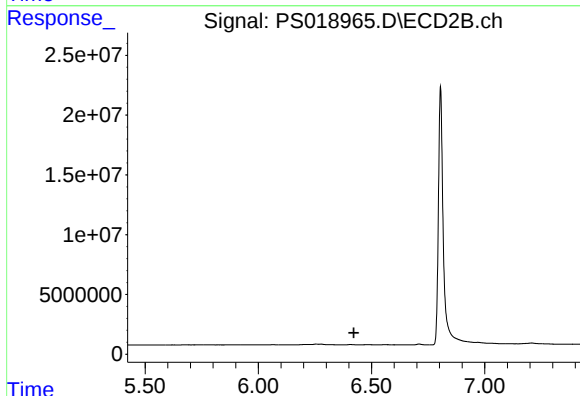


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

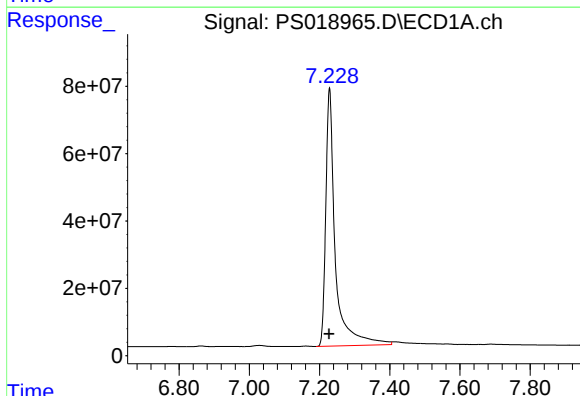


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.001 min
Response: 1445796121
Conc: 495.23 ng/ml

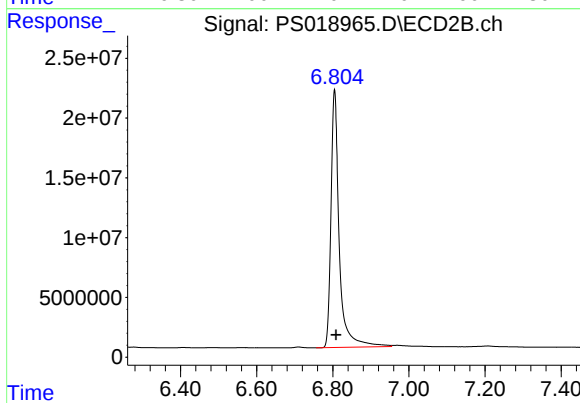

#4 2,4-DCAA


R.T.: 6.805 min
Delta R.T.: -0.004 min
Response: 327157187
Conc: 458.24 ng/ml

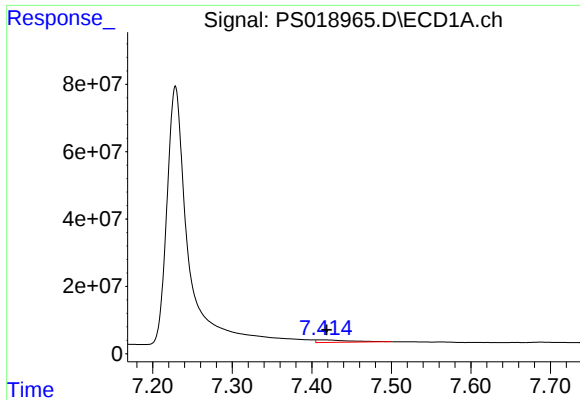

#5 DICAMBA


R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 21363042
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

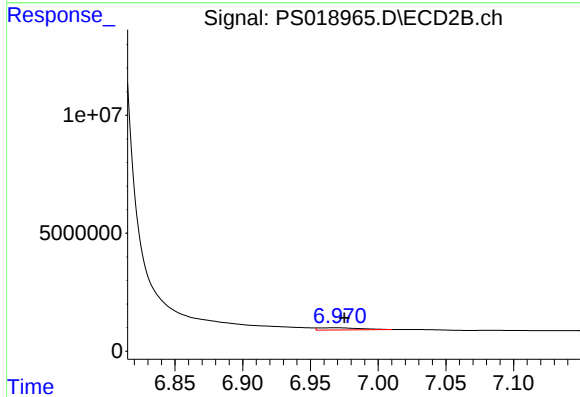


#5 DICAMBA

R.T.: 6.970 min
Delta R.T.: -0.005 min
Response: 1937573
Conc: N.D.

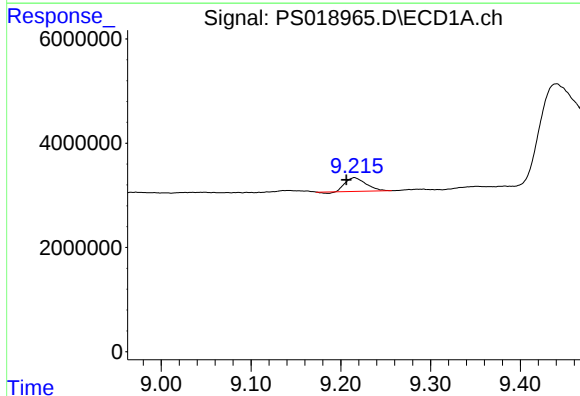


#11 2,4,5-TP (SILVEX)

R.T.: 9.215 min
Delta R.T.: 0.009 min
Response: 4151331
Conc: N.D.

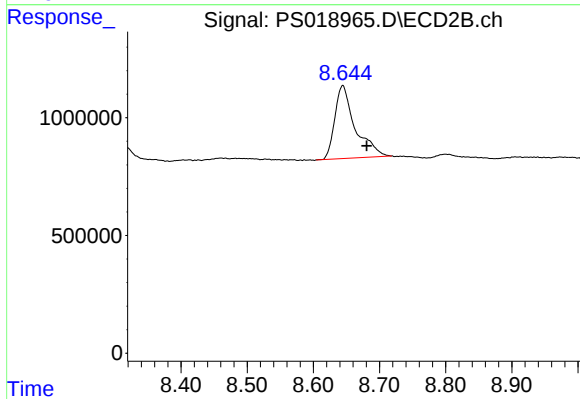

#11 2,4,5-TP (SILVEX)


R.T.: 8.645 min
Delta R.T.: -0.036 min
Response: 6610642
Conc: 1.45 ng/ml

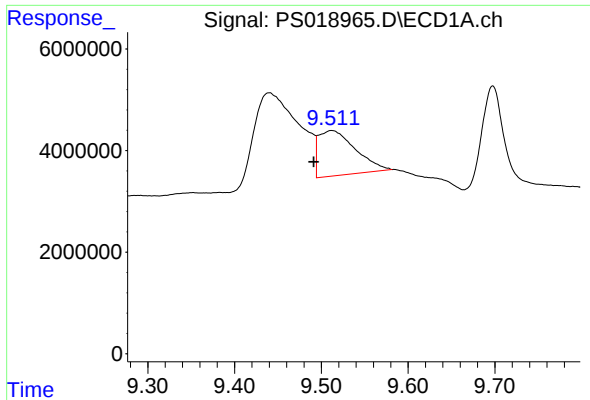

#12 2,4,5-T


R.T.: 9.512 min
Delta R.T.: 0.021 min
Response: 26455135
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

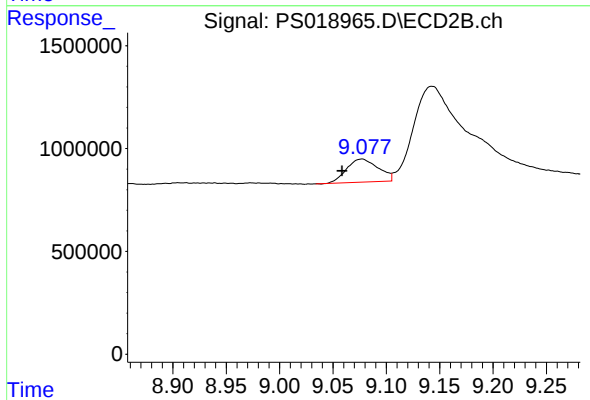


#12 2,4,5-T

R.T.: 9.078 min
Delta R.T.: 0.019 min
Response: 2318892
Conc: N.D.

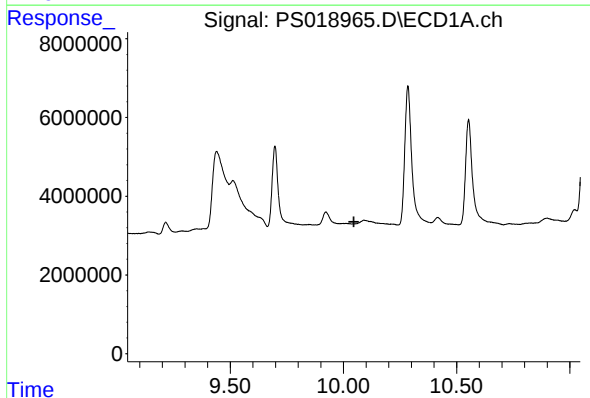


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.046 min
Response: 0
Conc: N.D.

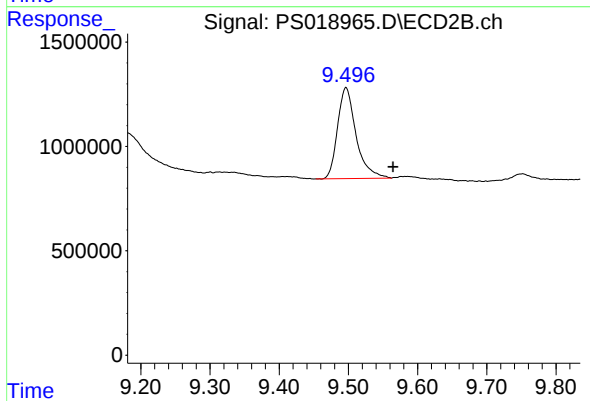

#13 2,4-DB


R.T.: 9.497 min
Delta R.T.: -0.068 min
Response: 8113845
Conc: 14.25 ng/ml

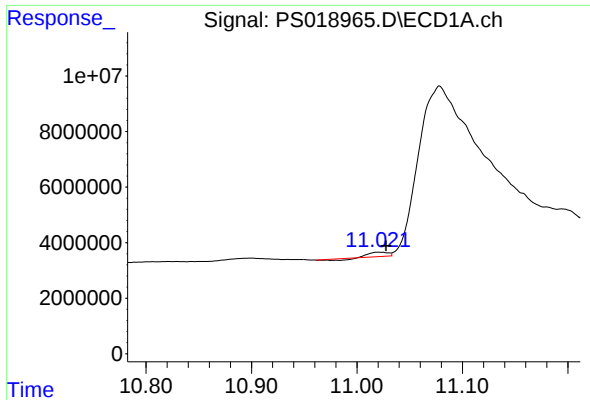

#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.007 min
Response: 1351639
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

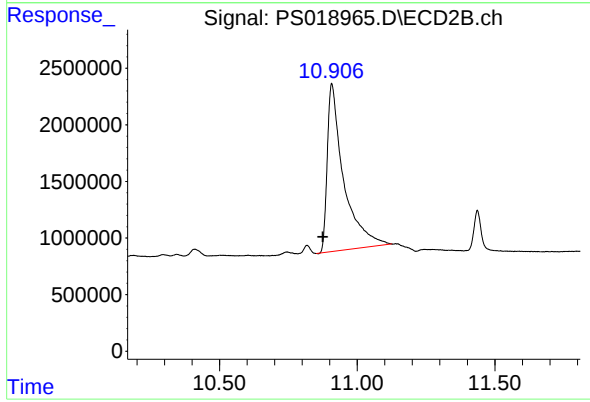

#15 Picloram

R.T.: 10.907 min
Delta R.T.: 0.032 min
Response: 61319013
Conc: 10.84 ng/ml