

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041224\
 Data File : PS026440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2024 22:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:14:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041124.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 11 14:35:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.091	7.552	1630.1E6	496.3E6	561.734	636.445
Target Compounds							
1) T	Dalapon	0.000	2.633f	0	1658039	N.D.	1.029
3) T	4-Nitroph...	6.880	7.066f	20687617	1047866	15.555	2.678 #
6) T	MCP	0.000	7.813f	0	3065496	N.D.	1.195
8) T	DICHLORPROP	7.975	8.472f	175844	15834976	<MDL	17.729 #
9) T	2,4-D	8.205	0.000	35782549	0	11.530	N.D. #
10) T	Pentachlo...	0.000	9.265	0	617718	N.D.	<MDL
11) T	2,4,5-TP ...	9.049	9.653	380477	903254	<MDL	<MDL #
12) T	2,4,5-T	9.379f	0.000	1744994	0	<MDL	N.D. #
13) T	2,4-DB	9.898	10.625	143508	865787	<MDL	1.967 #
14) T	DINOSEB	11.089	10.981	290112	641006	<MDL	<MDL #
15) T	Picloram	10.891	12.038	20168605	960448	1.221	<MDL #
16) T	DCPA	11.394	12.025	645761	1453427	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS0411224\
Data File : PS026440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 22:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:14:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041124.M
Quant Title : 8080.M
QLast Update : Thu Apr 11 14:35:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

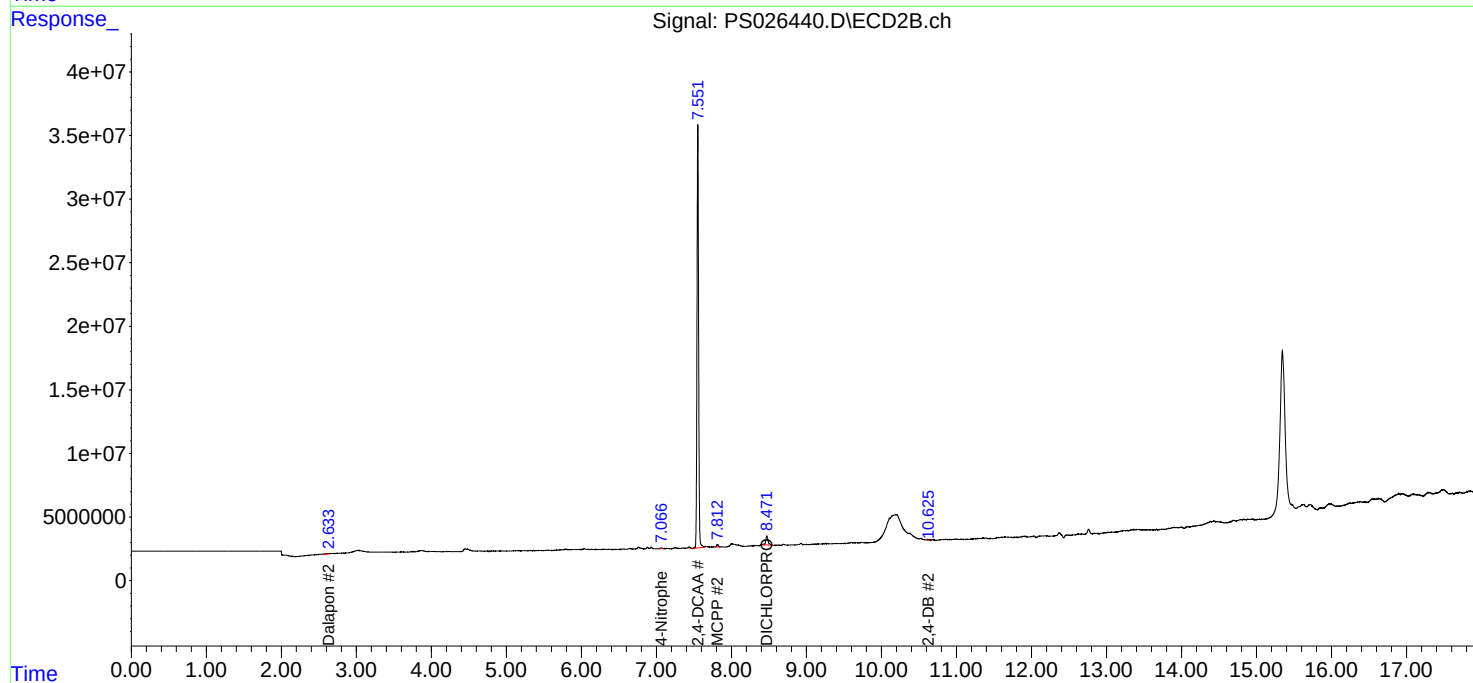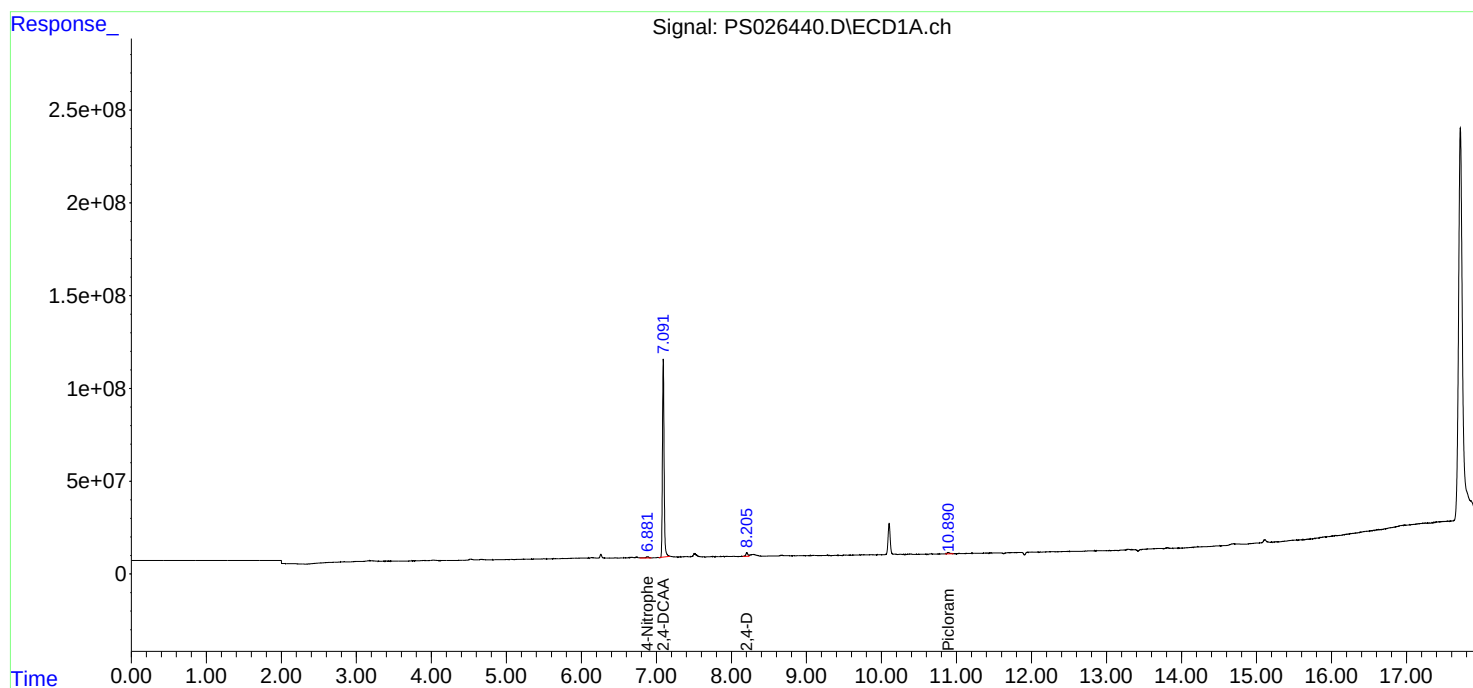


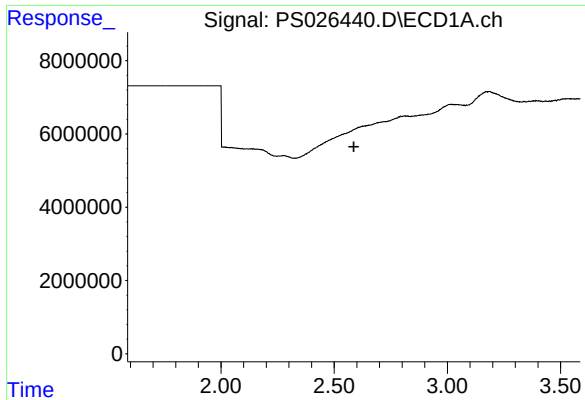

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

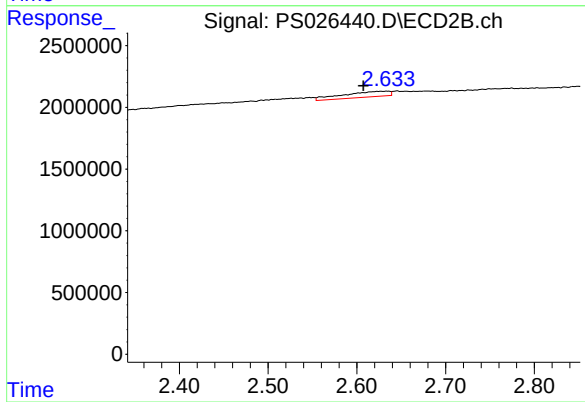


#1 Dalapon

R.T.: 2.633 min
Delta R.T.: 0.026 min
Response: 1658039
Conc: 1.03 ng/ml

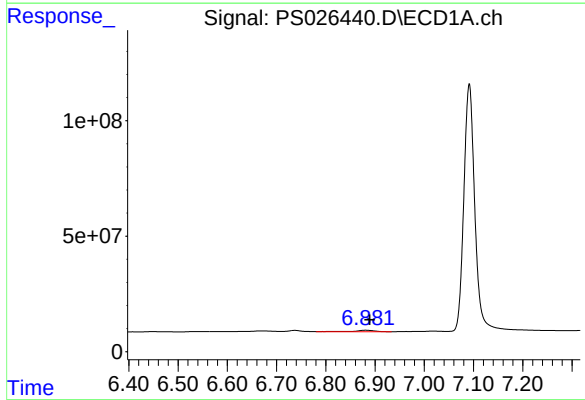


#3 4-Nitrophenol

R.T.: 6.880 min
Delta R.T.: -0.009 min
Response: 20687617
Conc: 15.55 ng/ml

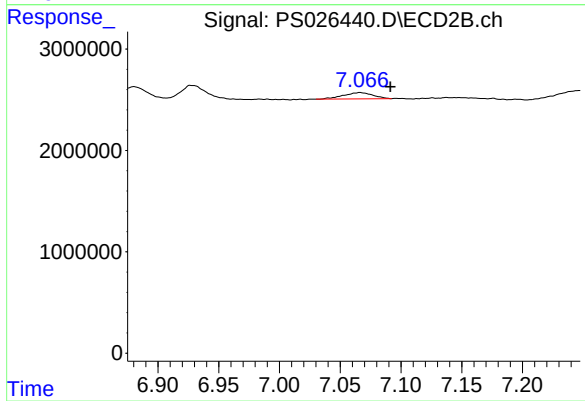

#3 4-Nitrophenol


R.T.: 7.066 min
Delta R.T.: -0.025 min
Response: 1047866
Conc: 2.68 ng/ml

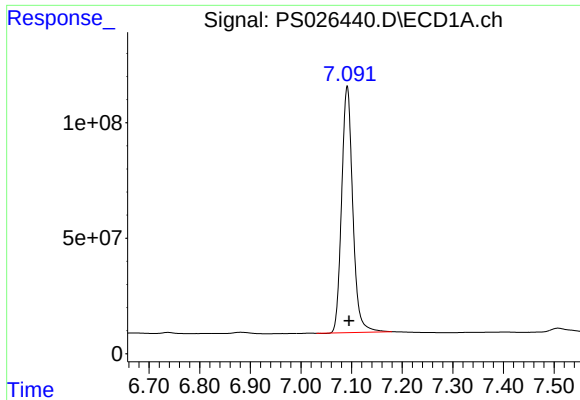

#4 2,4-DCAA


R.T.: 7.091 min
Delta R.T.: -0.003 min
Response: 1630069550
Conc: 561.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

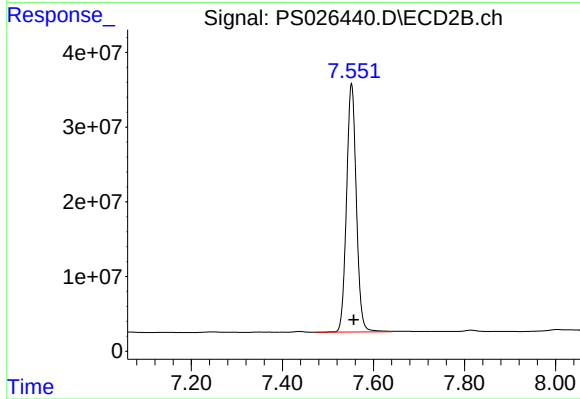


#4 2,4-DCAA

R.T.: 7.552 min
Delta R.T.: -0.005 min
Response: 496337158
Conc: 636.44 ng/ml

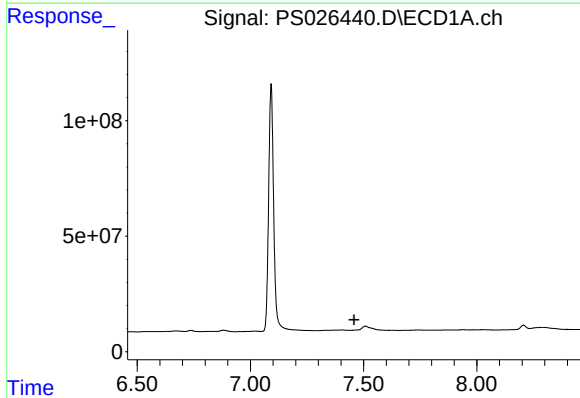


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.457 min
Response: 0
Conc: N.D.

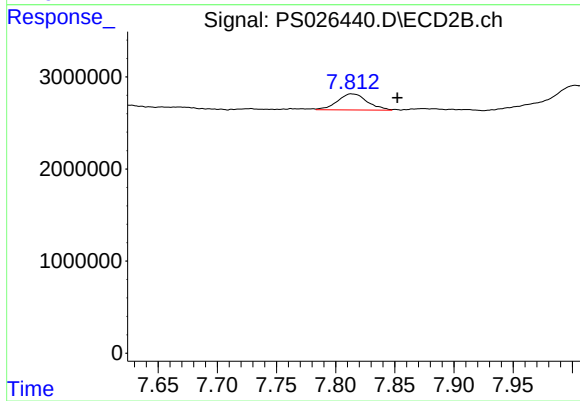

#6 MCP


R.T.: 7.813 min
Delta R.T.: -0.039 min
Response: 3065496
Conc: 1.19 ug/ml

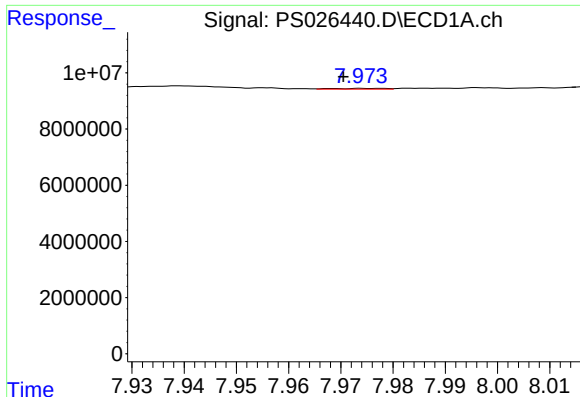

#8 DICHLORPROP


R.T.: 7.975 min
Delta R.T.: 0.004 min
Response: 175844
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

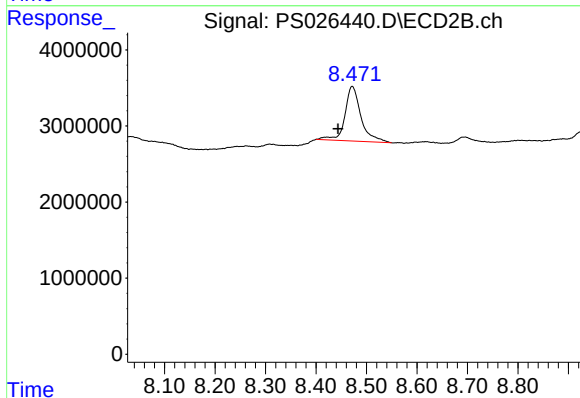


#8 DICHLORPROP

R.T.: 8.472 min
Delta R.T.: 0.028 min
Response: 15834976
Conc: 17.73 ng/ml

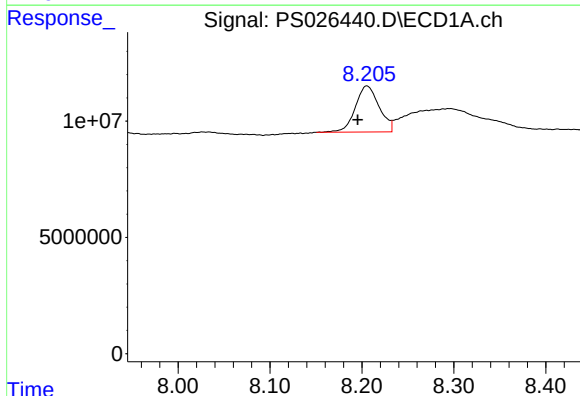


#9 2,4-D

R.T.: 8.205 min
Delta R.T.: 0.010 min
Response: 35782549
Conc: 11.53 ng/ml

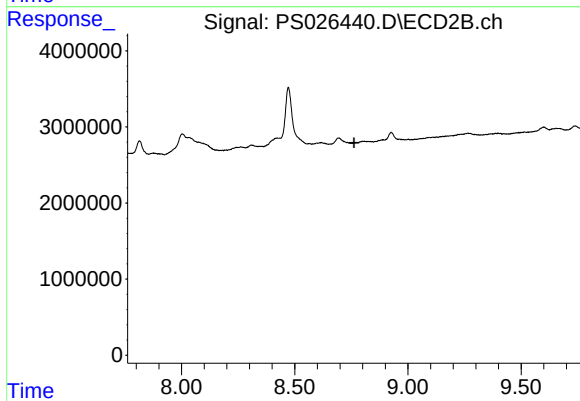

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.762 min
Response: 0
Conc: N.D.

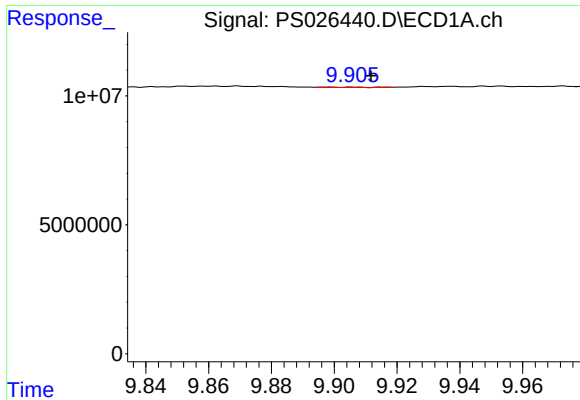

#13 2,4-DB


R.T.: 9.898 min
Delta R.T.: -0.013 min
Response: 143508
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

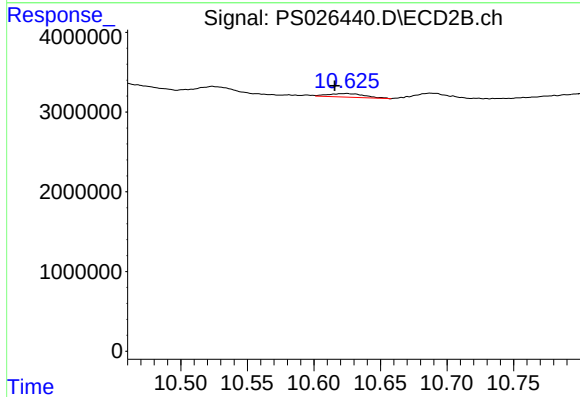


#13 2,4-DB

R.T.: 10.625 min
Delta R.T.: 0.009 min
Response: 865787
Conc: 1.97 ng/ml

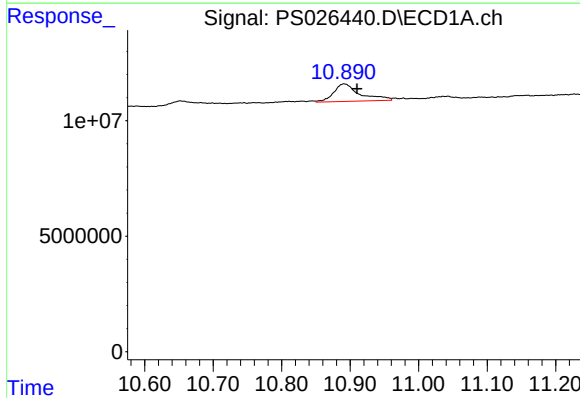

#15 Picloram

R.T.: 10.891 min
Delta R.T.: -0.019 min
Response: 20168605
Conc: 1.22 ng/ml

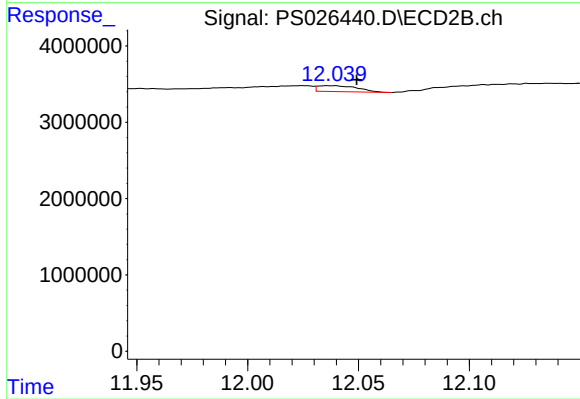

#15 Picloram

R.T.: 12.038 min
Delta R.T.: -0.011 min
Response: 960448
Conc: N.D.