

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041320\
 Data File : PS009706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2020 14:57
 Operator : DD\AJ
 Sample : L2180-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NEWPORT-TP-7FT

Manual Integrations
 APPROVED

Sohil
 4/14/2020 3:00:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 15:25:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.239	6.928	123.3E6	99346497	222.910	180.894m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041320\
Data File : PS009706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2020 14:57
Operator : DD\AJ
Sample : L2180-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
NEWPORT-TP-7FT


Manual Integrations
APPROVED

Sohil
4/14/2020 3:00:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 15:25:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

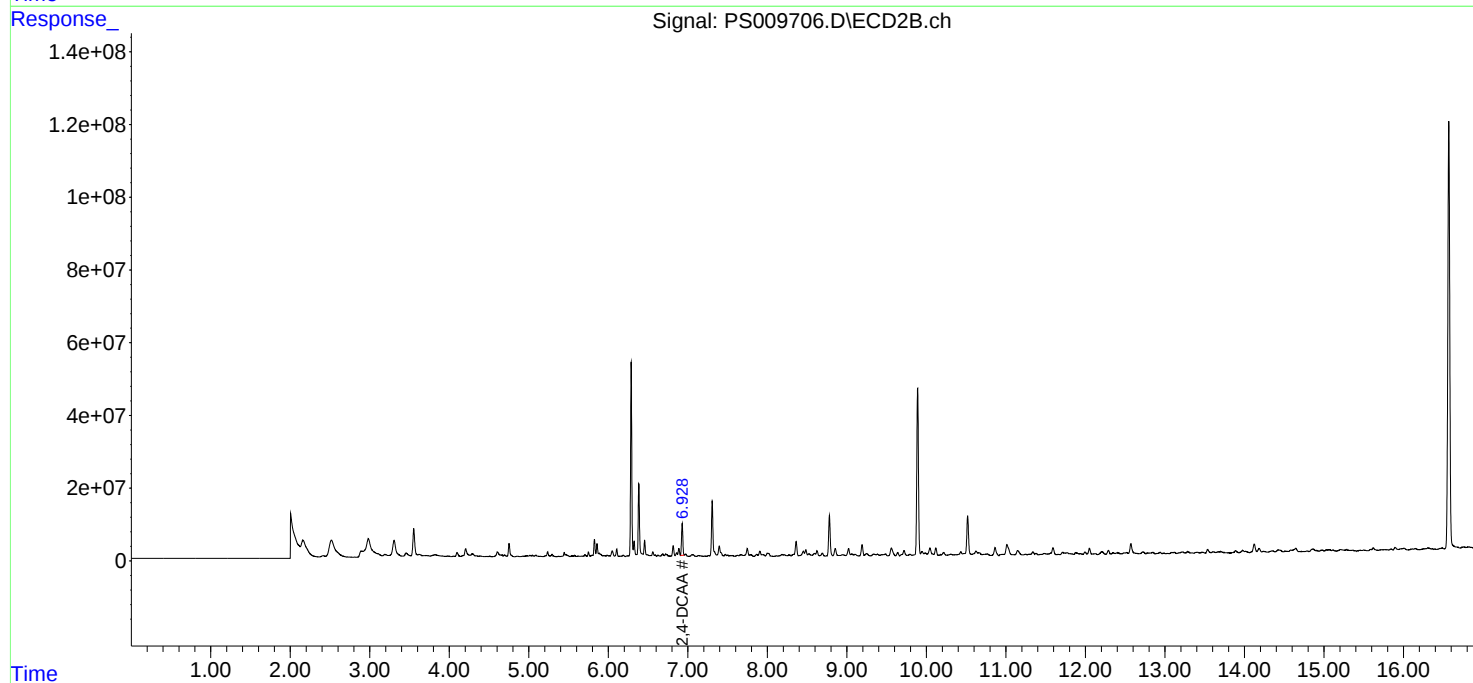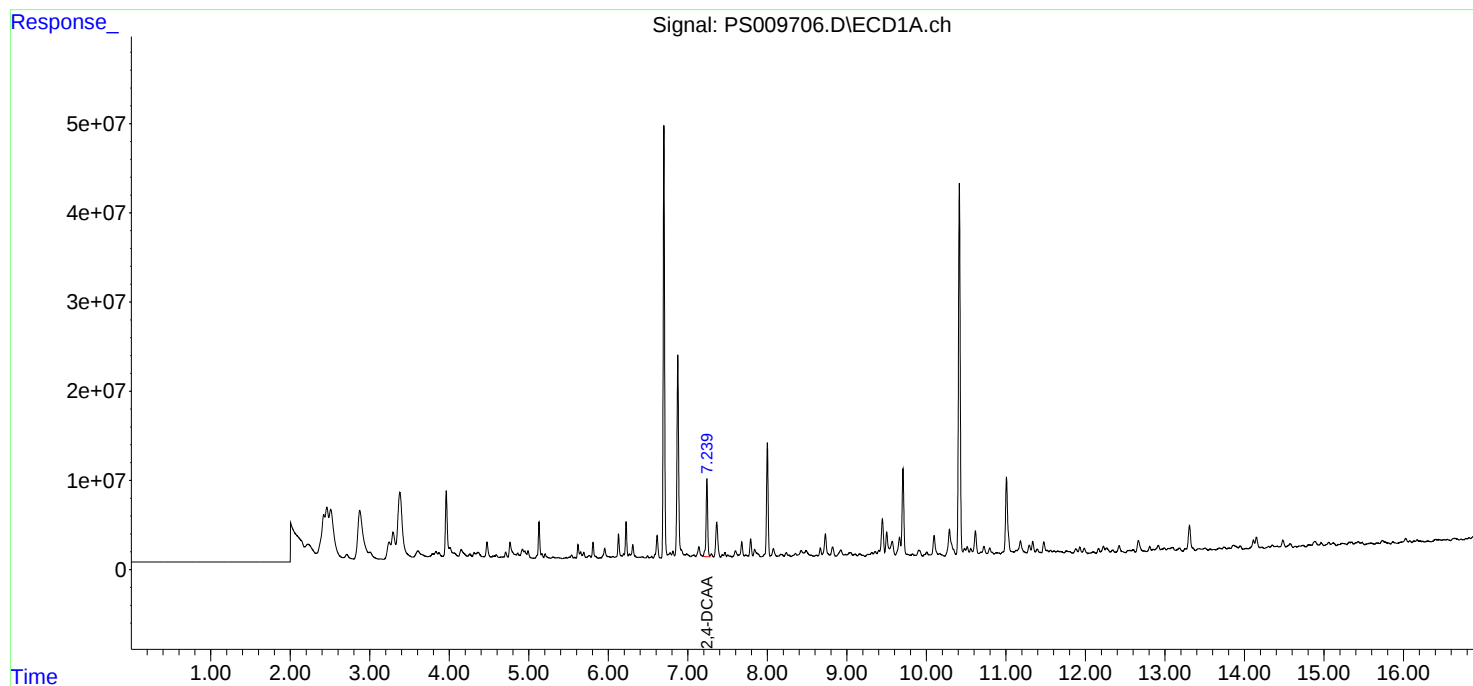

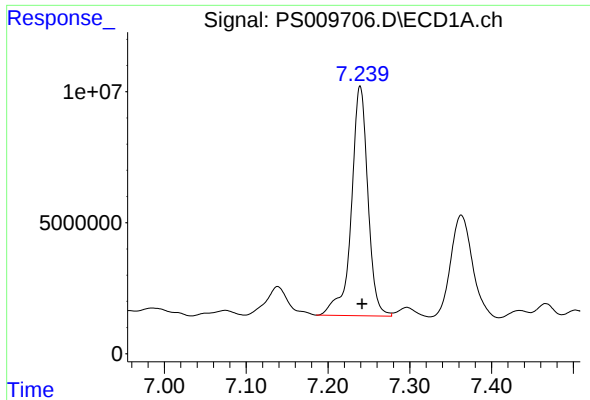


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 123306947
Conc: 222.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
NEWPORT-TP-7FT

Manual Integrations
APPROVED

Sohil
4/14/2020 3:00:37 PM

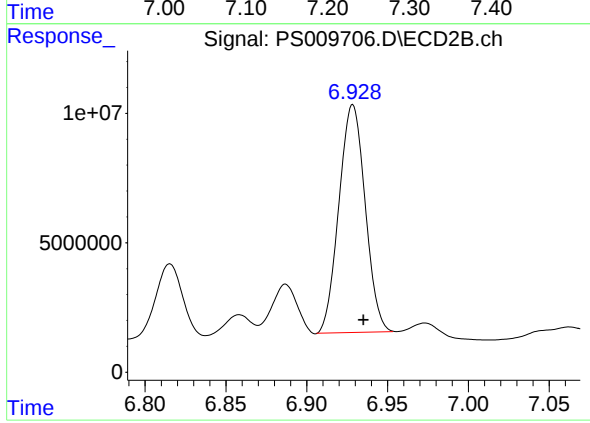

#4 2,4-DCAA

R.T.: 6.928 min
Delta R.T.: -0.007 min
Response: 99346497
Conc: 180.89 ng/ml m