

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041321\
 Data File : PS014585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 08:28
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 11:25:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
12)	T	2,4,5-T	9.414	0.000	6451321	0	<MDL	N.D.	#
13)	T	2,4-DB	9.969	0.000	6720584	0	4.416	N.D.	#
14)	T	DINOSEB	11.096	0.000	4379746	0	<MDL	N.D.	#
15)	T	Picloram	10.938	10.970	162.7E6	62812237	14.541	16.750	
16)	T	DCPA	11.362	10.900	3813768	1490555	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041321\
Data File : PS014585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 08:28
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 11:25:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

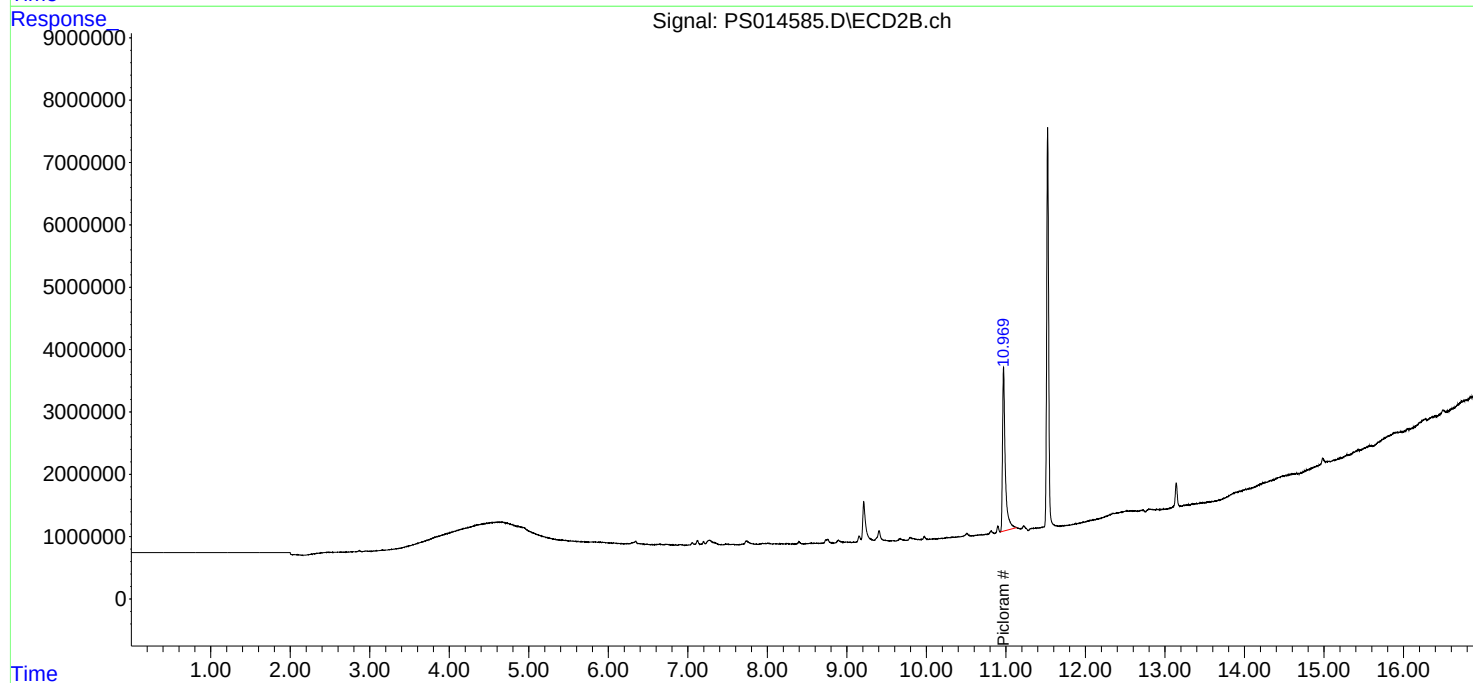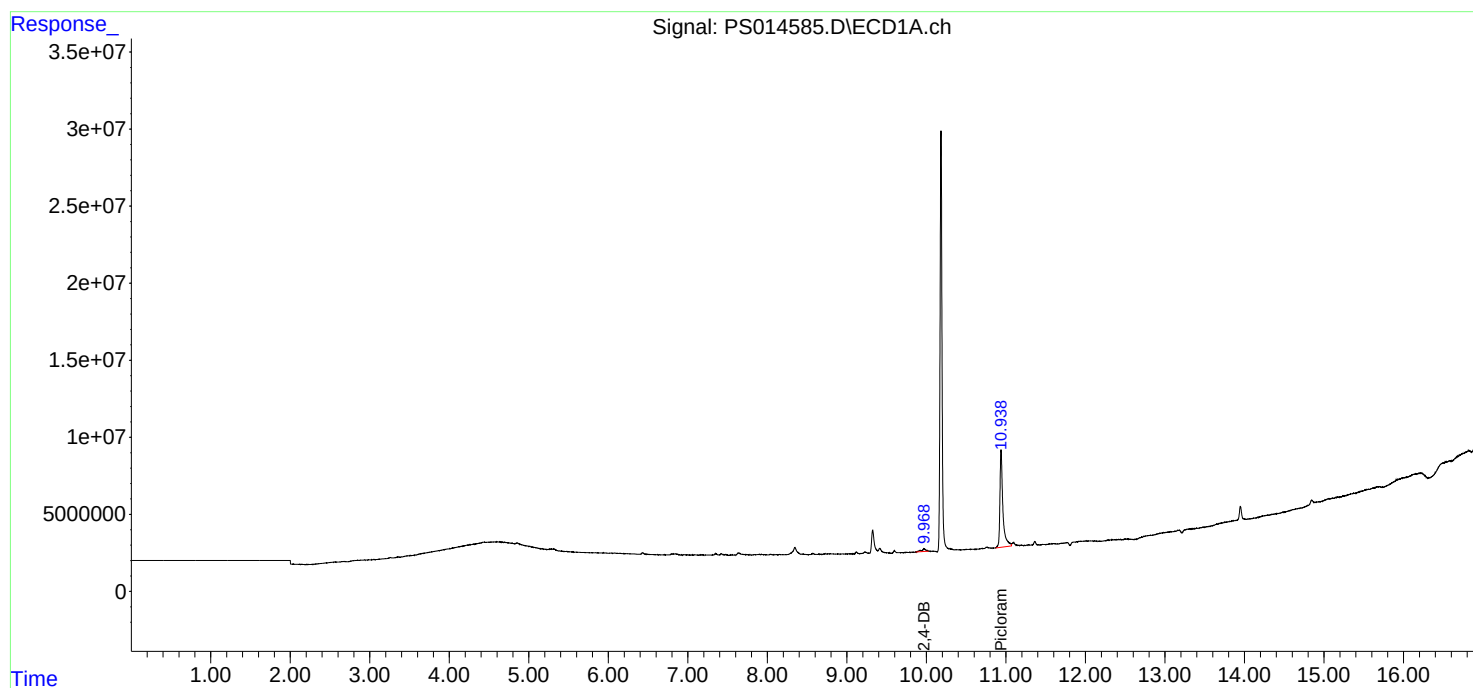


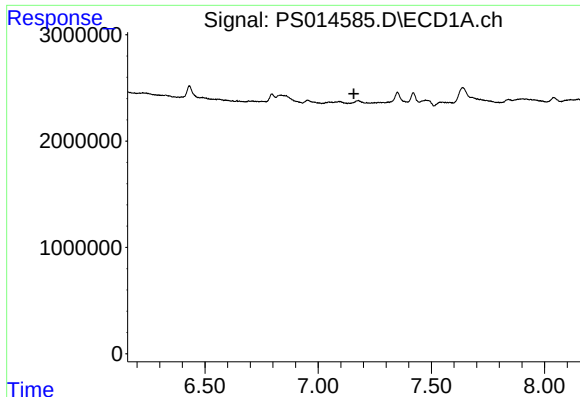

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

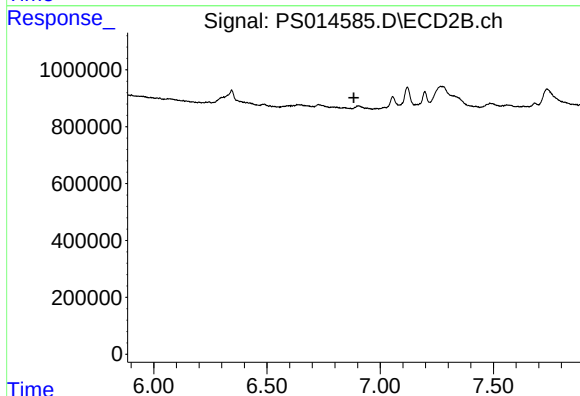


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.884 min
Response: 0
Conc: N.D.

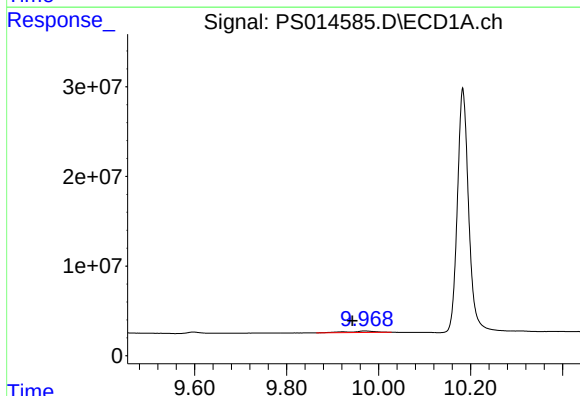


#13 2,4-DB

R.T.: 9.969 min
Delta R.T.: 0.026 min
Response: 6720584
Conc: 4.42 ng/ml

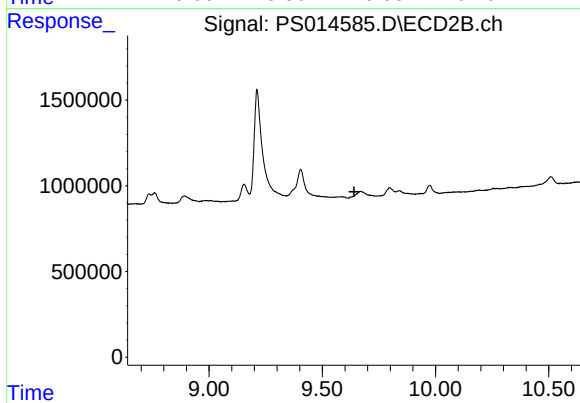

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.640 min
Response: 0
Conc: N.D.

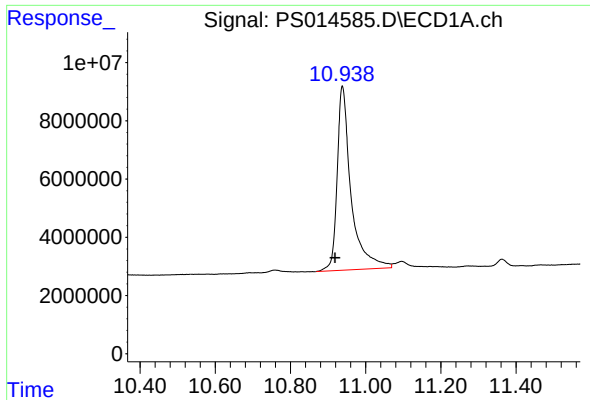

#15 Picloram

R.T.: 10.938 min
Delta R.T.: 0.019 min
Response: 162687848
Conc: 14.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

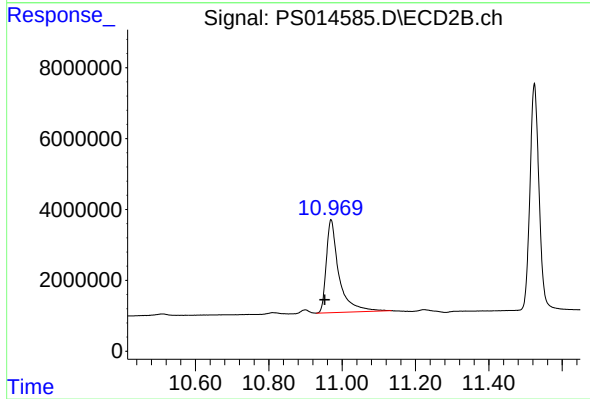

#15 Picloram

R.T.: 10.970 min
Delta R.T.: 0.017 min
Response: 62812237
Conc: 16.75 ng/ml