

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041321\
 Data File : PS014586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 08:51
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 11:25:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.885	680.1E6	253.8E6	447.099	545.174
Target Compounds							
7) T	MCPA	7.635	0.000	8501257	0	1.366	N.D. #
8) T	DICHLORPROP	0.000	7.734f	0	1264309	N.D.	2.504
12) T	2,4,5-T	9.327f	0.000	17404830	0	2.116	N.D. #
15) T	Picloram	10.942	10.974	98911373	41009557	8.841	10.936



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041321\
Data File : PS014586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 08:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 11:25:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

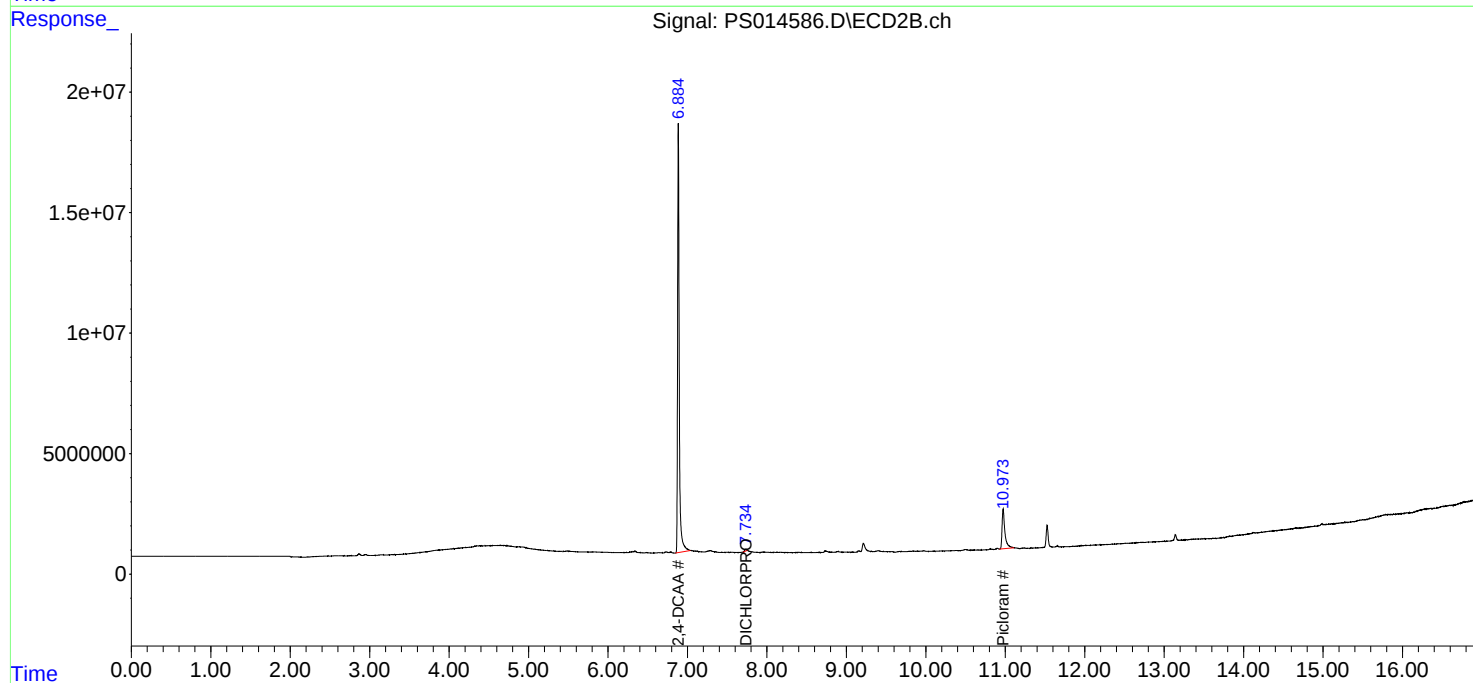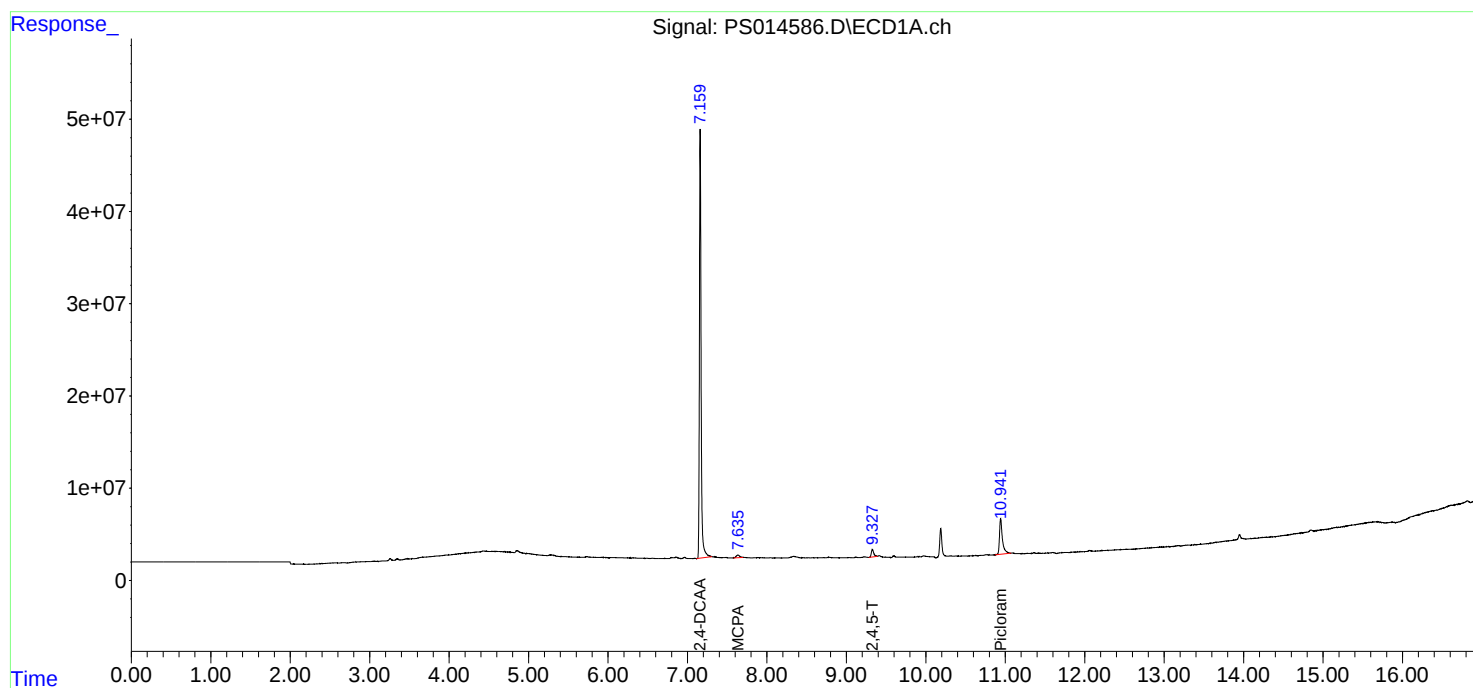


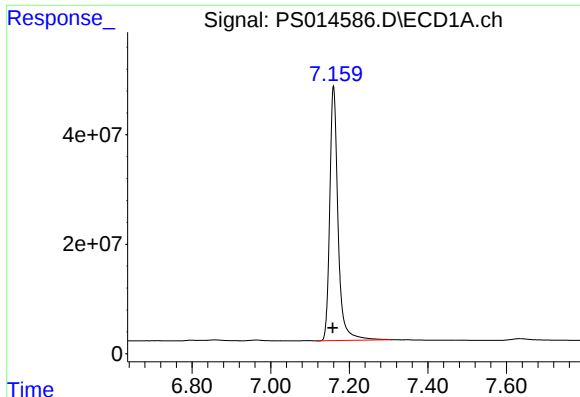

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: 0.002 min
Response: 680124779
Conc: 447.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

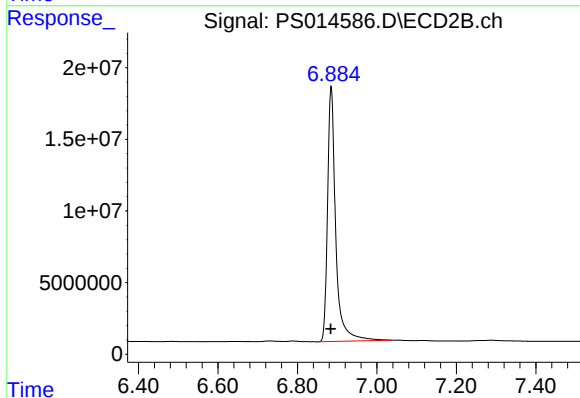


#4 2,4-DCAA

R.T.: 6.885 min
Delta R.T.: 0.001 min
Response: 253753655
Conc: 545.17 ng/ml

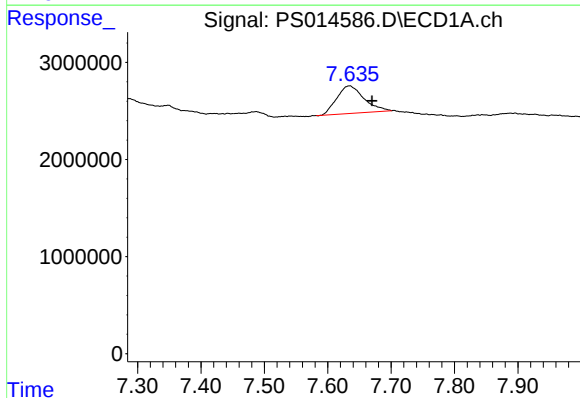


#7 MCPA

R.T.: 7.635 min
Delta R.T.: -0.035 min
Response: 8501257
Conc: 1.37 ug/ml

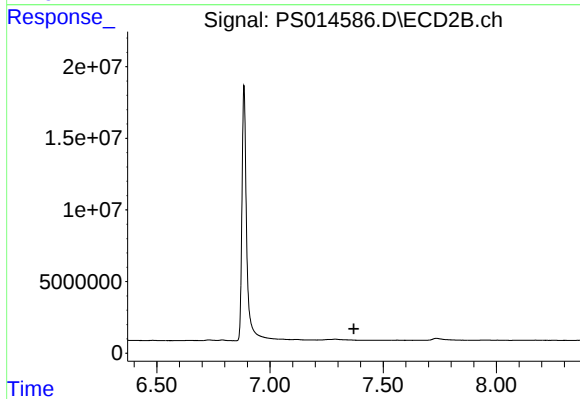

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

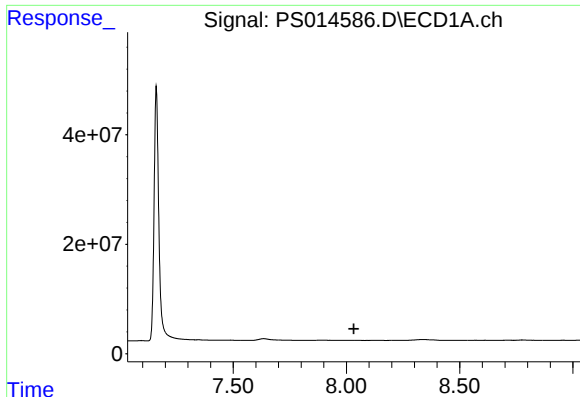

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

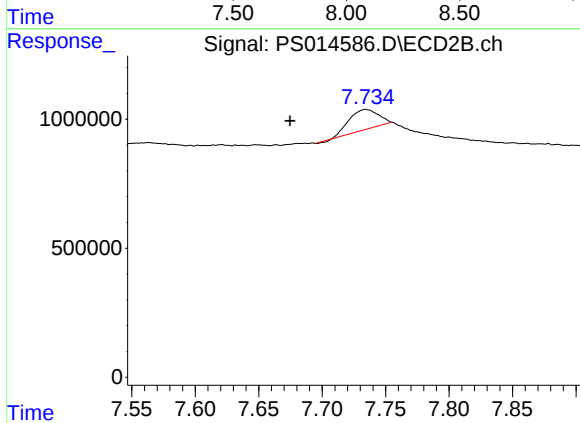


#8 DICHLORPROP

R.T.: 7.734 min
Delta R.T.: 0.059 min
Response: 1264309
Conc: 2.50 ng/ml

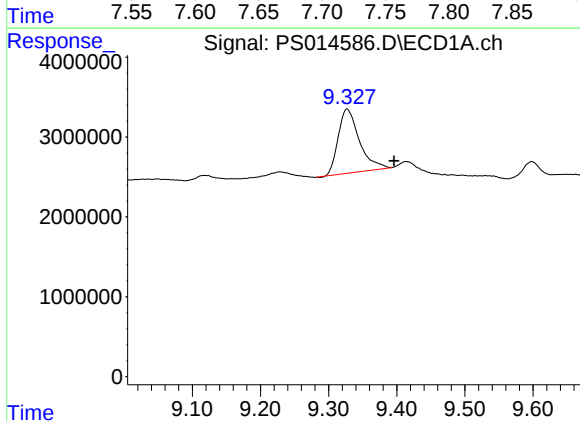


#12 2,4,5-T

R.T.: 9.327 min
Delta R.T.: -0.069 min
Response: 17404830
Conc: 2.12 ng/ml

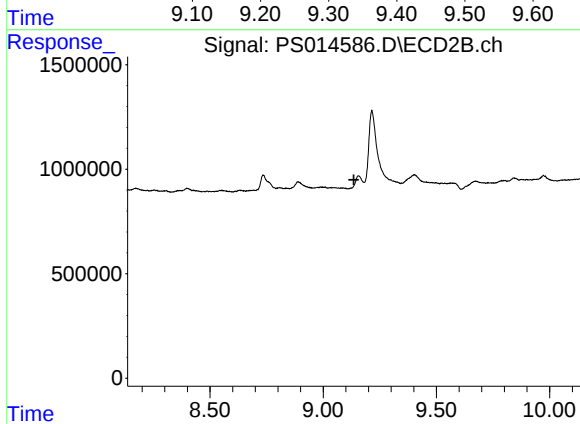

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.135 min
Response: 0
Conc: N.D.

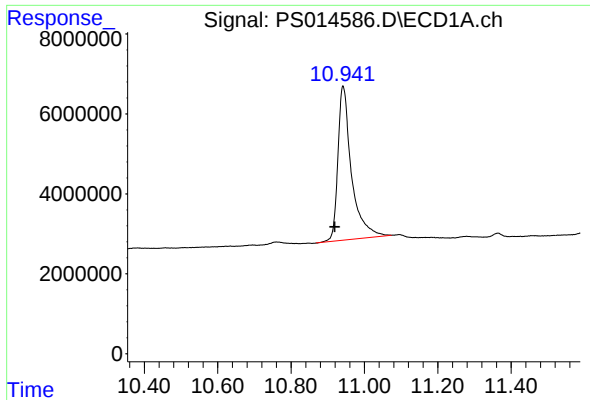

#15 Picloram

R.T.: 10.942 min
Delta R.T.: 0.023 min
Response: 98911373
Conc: 8.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

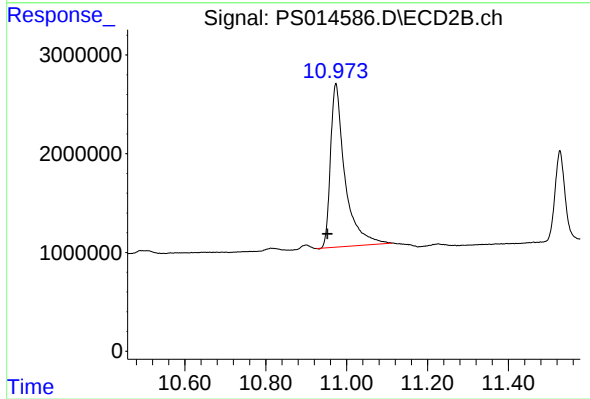

#15 Picloram

R.T.: 10.974 min
Delta R.T.: 0.021 min
Response: 41009557
Conc: 10.94 ng/ml