

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041321\
 Data File : PS014622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 23:26
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 06:40:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.884	690.1E6	256.8E6	453.673	551.811
Target Compounds							
7) T	MCPA	7.615f	0.000	7010549	0	1.127	N.D. #
8) T	DICHLORPROP	0.000	7.724f	0	1717280	N.D.	3.402
15) T	Picloram	10.942	0.000	29468668	0	2.634	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041321\
Data File : PS014622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 23:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 06:40:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

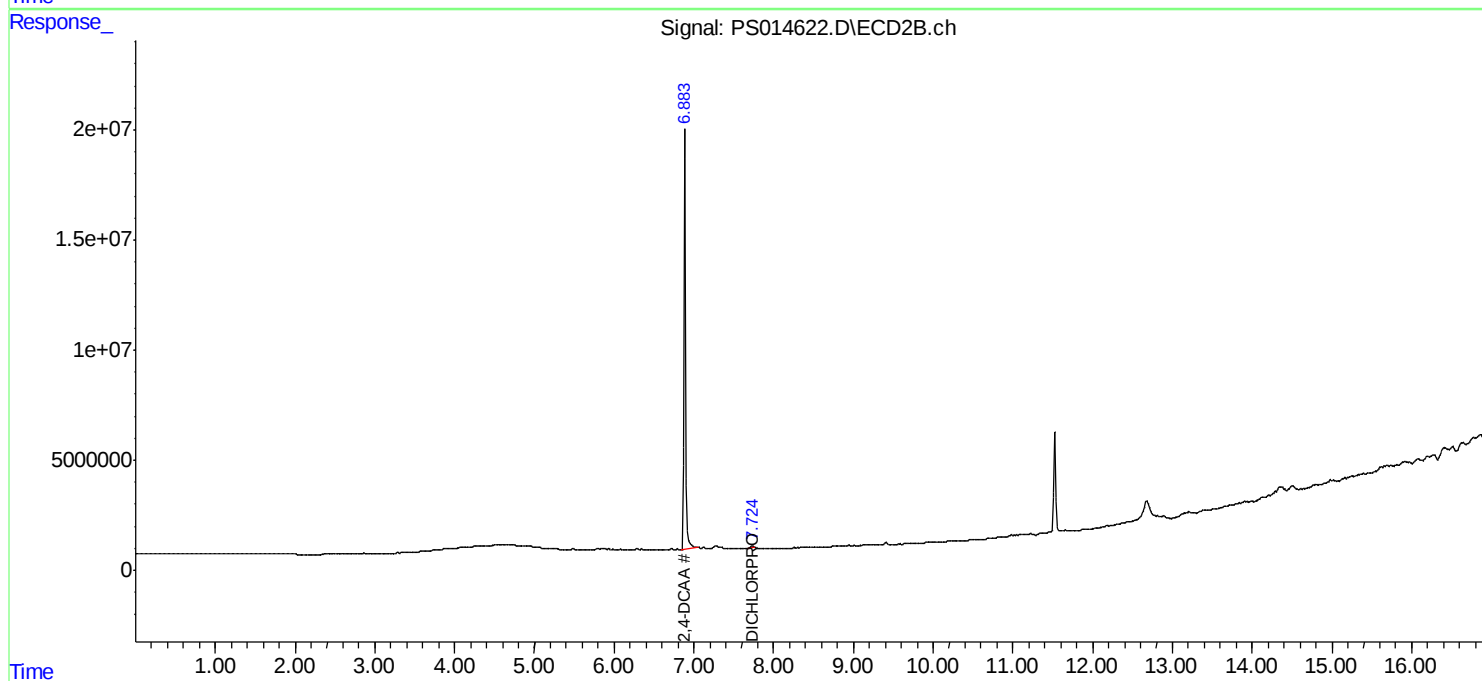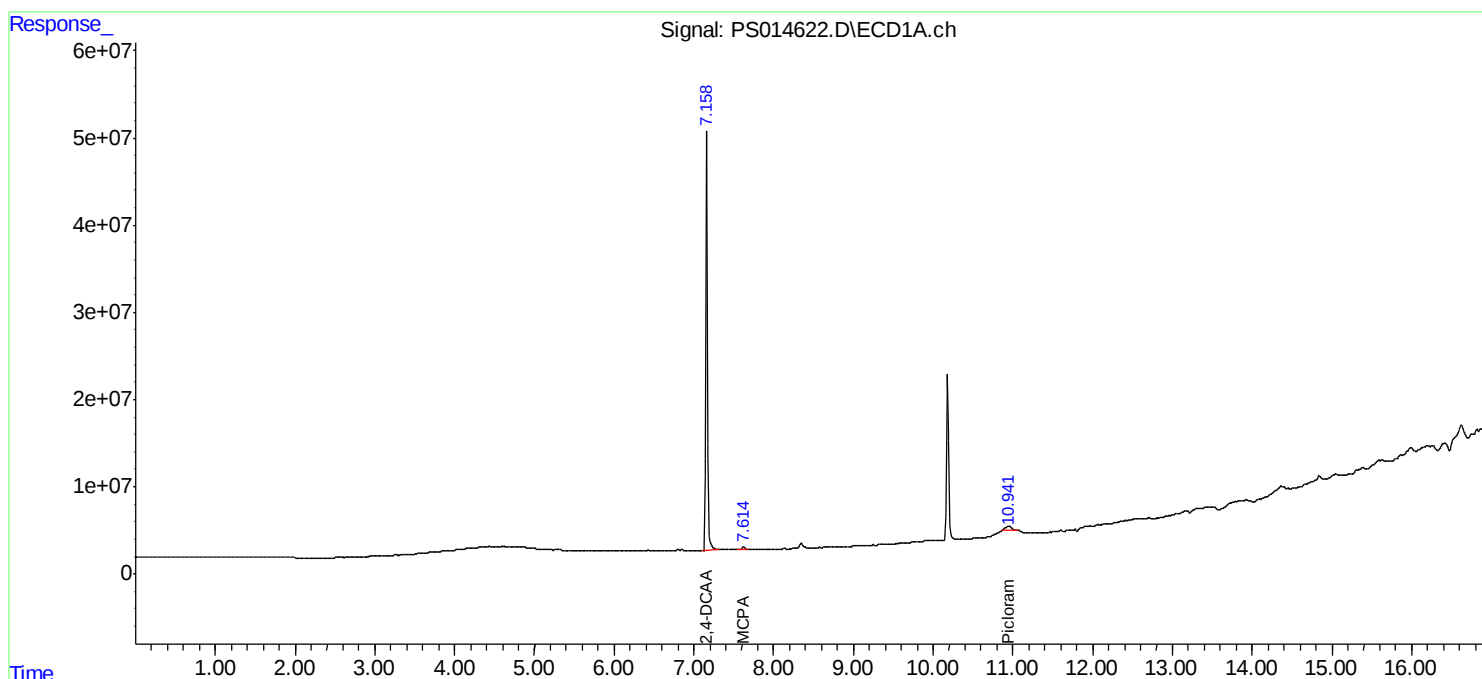


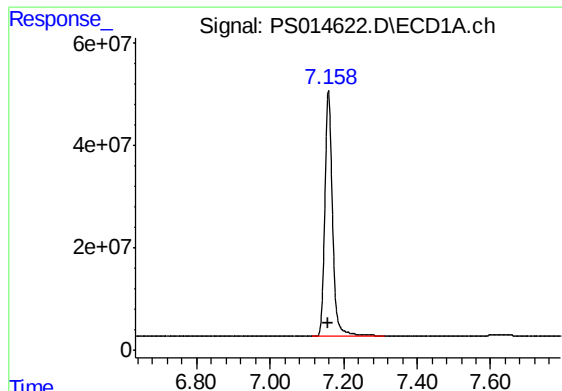

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 690125062
Conc: 453.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

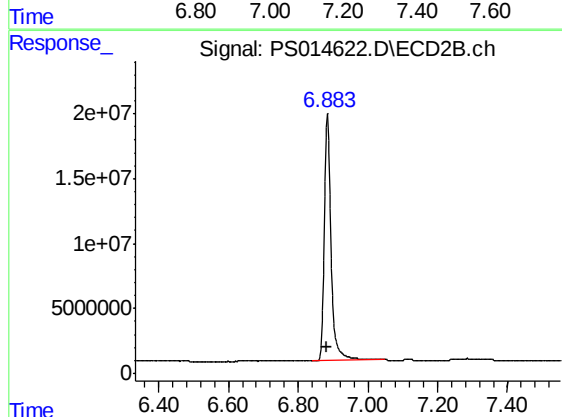


#4 2,4-DCAA

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 256843022
Conc: 551.81 ng/ml

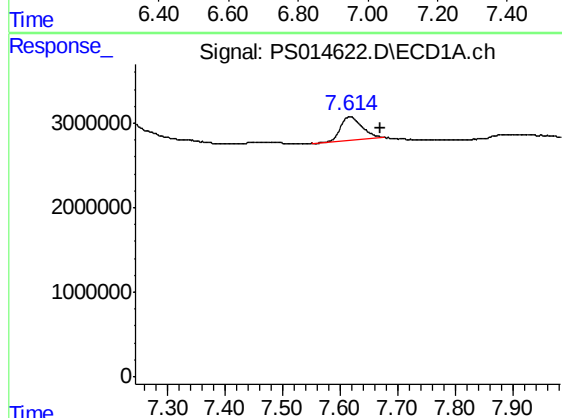


#7 MCPA

R.T.: 7.615 min
Delta R.T.: -0.055 min
Response: 7010549
Conc: 1.13 ug/ml

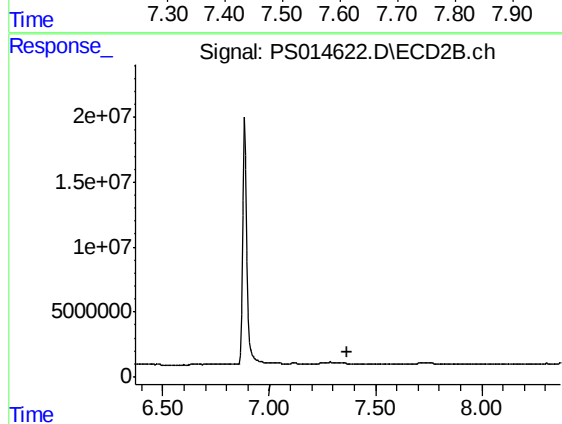

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

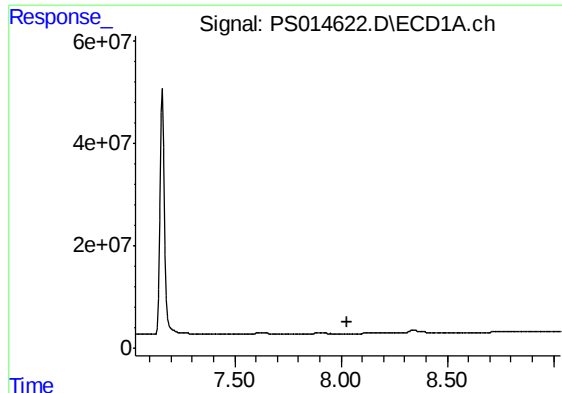

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

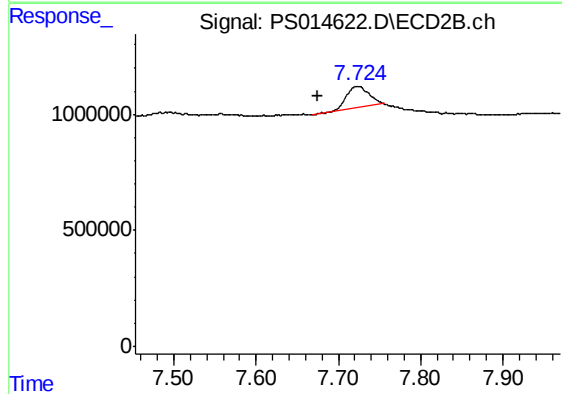


#8 DICHLORPROP

R.T.: 7.724 min
Delta R.T.: 0.050 min
Response: 1717280
Conc: 3.40 ng/ml

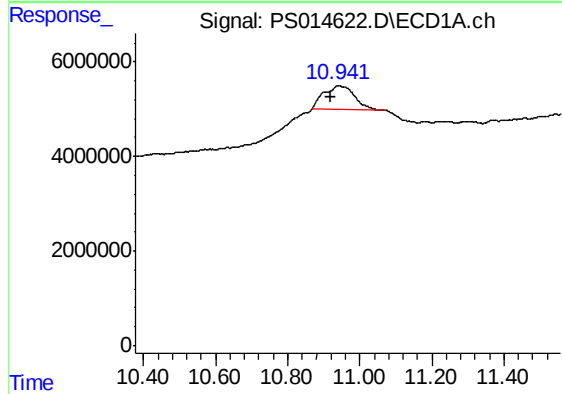

#15 Picloram

R.T.: 10.942 min
Delta R.T.: 0.023 min
Response: 29468668
Conc: 2.63 ng/ml

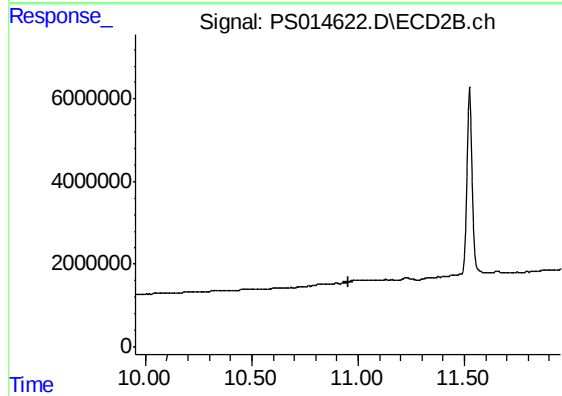

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.952 min
Response: 0
Conc: N.D.