

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041420\
 Data File : PS009736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 14:36
 Operator : DD\AJ
 Sample : L2215-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 18:05:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	6.928	206.1E6	156.0E6	372.621	284.079
Target Compounds							
2) T	3,5-DICHL...	0.000	6.105	0	31109081	N.D.	38.250
5) T	DICAMBA	0.000	7.105	0	2814383	N.D.	1.226
6) T	MCP	7.639	0.000	16166536	0	6.570	N.D. #
7) T	MCPA	7.790	7.394	22511062	25156224	7.391	9.322 #
8) T	DICHLORPROP	8.073	7.746	11348633	38499815	22.004	69.391 #
9) T	2,4-D	8.426	8.001	24902004	6478655	47.232	9.856 #
10) T	Pentachlo...	8.653	8.521	27908250	8186569	3.969	1.079 #
11) T	2,4,5-TP ...	9.248	8.853	18366327	65460248	6.700	21.958 #
12) T	2,4,5-T	9.449	9.245	58435951	4450128	22.971	1.507 #
13) T	2,4-DB	10.094	9.716	-570268	8686087	N.D.	22.881
14) T	DINOSEB	11.182	10.035	29944276	30692316	14.649	13.973
15) T	Picloram	11.006	11.027	152.5E6	24120567	50.264	5.923 #
16) T	DCPA	11.432	10.940	2998754	18805337	<MDL	4.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041420\
Data File : PS009736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 14:36
Operator : DD\AJ
Sample : L2215-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 18:05:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

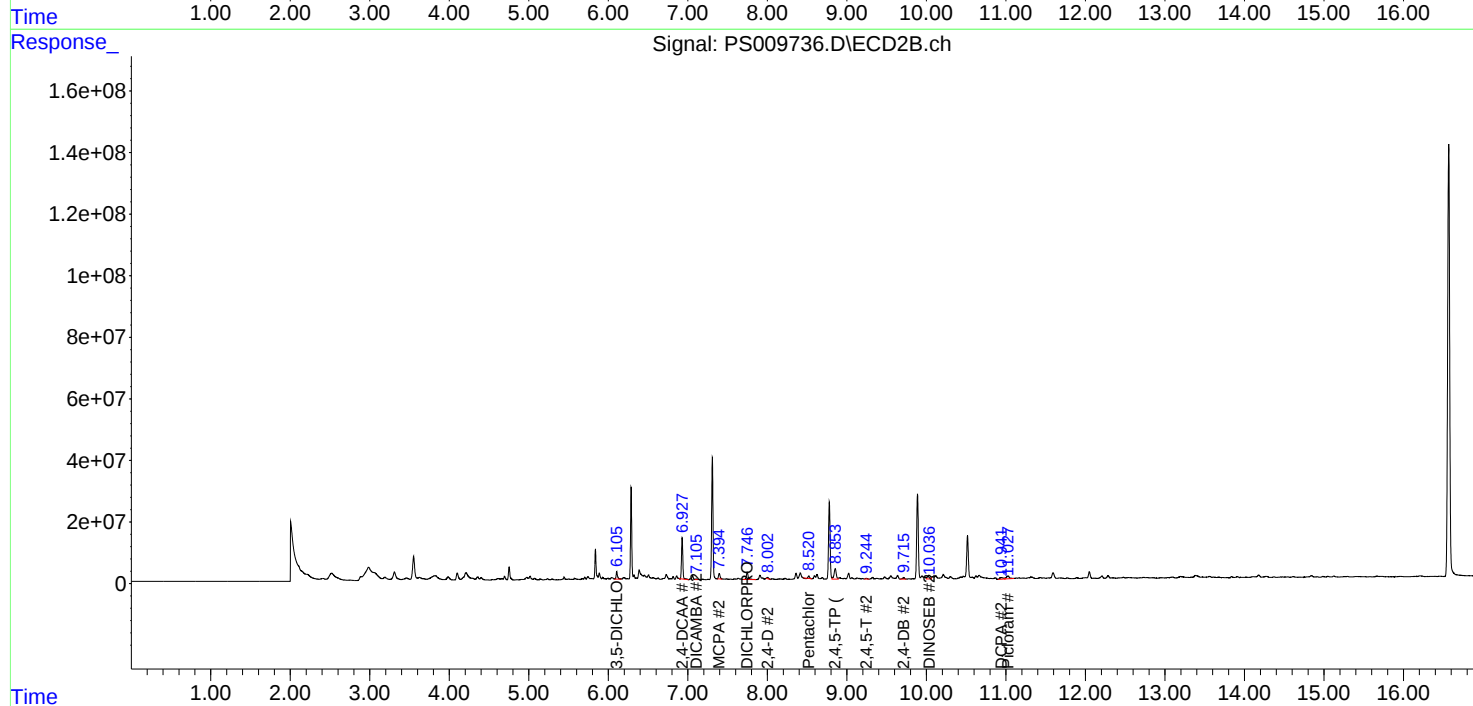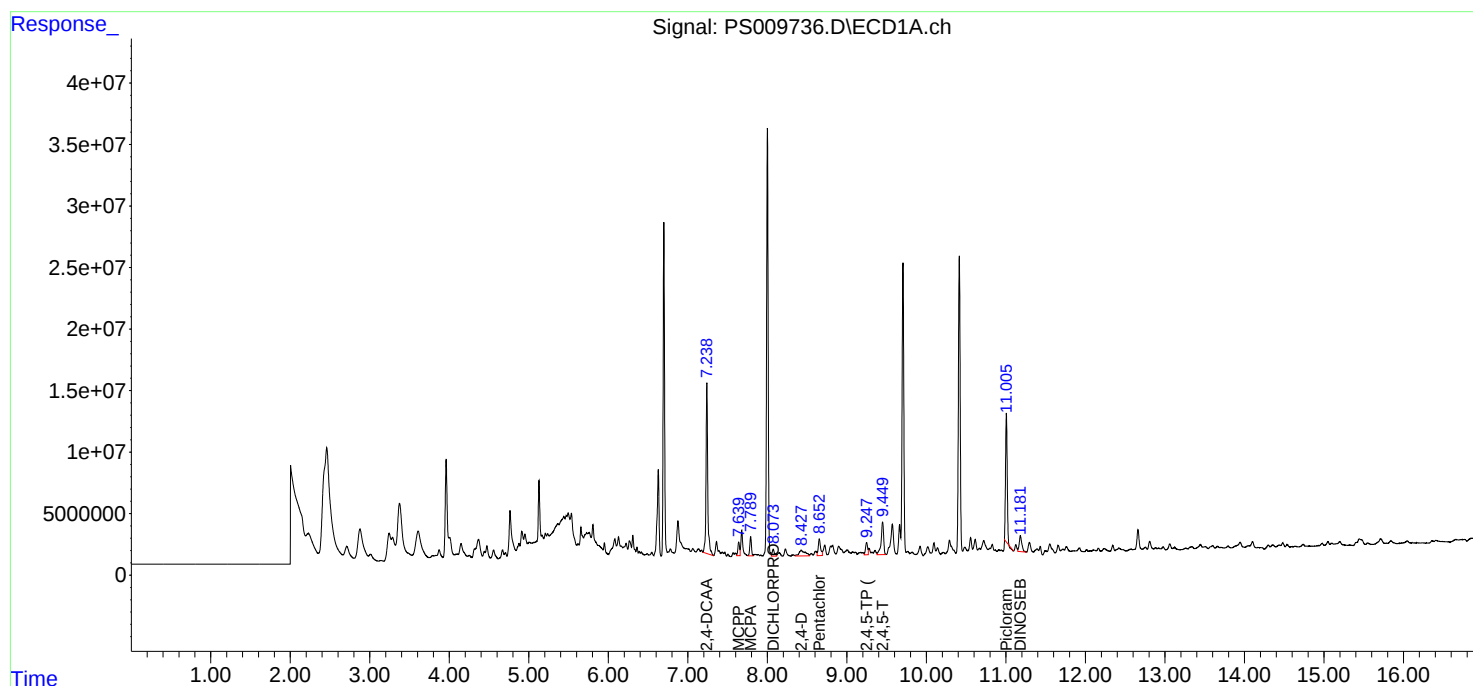


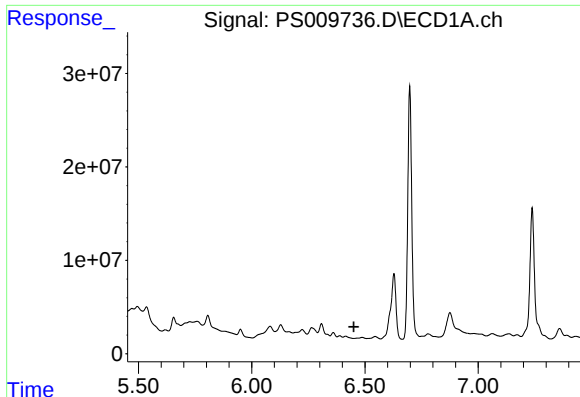

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

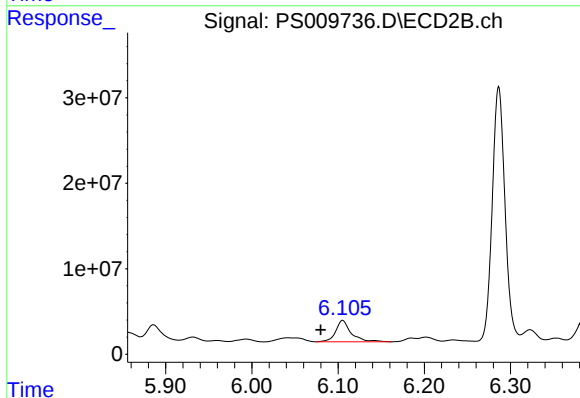


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.105 min
Delta R.T.: 0.026 min
Response: 31109081
Conc: 38.25 ng/ml

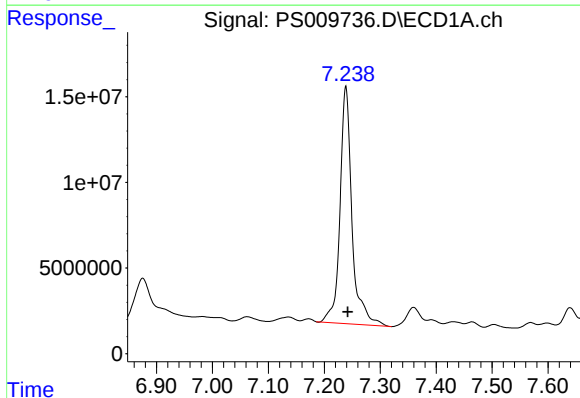


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 206122870
Conc: 372.62 ng/ml

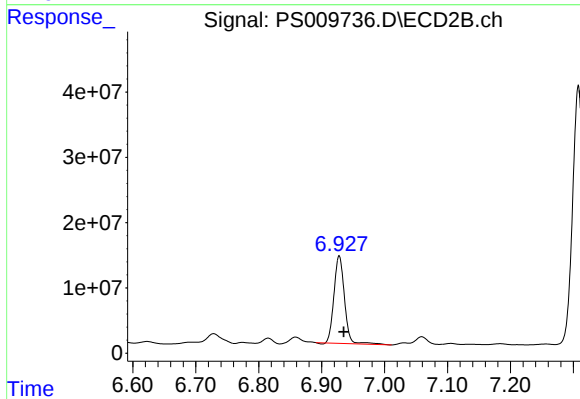

#4 2,4-DCAA


R.T.: 6.928 min
Delta R.T.: -0.007 min
Response: 156015691
Conc: 284.08 ng/ml

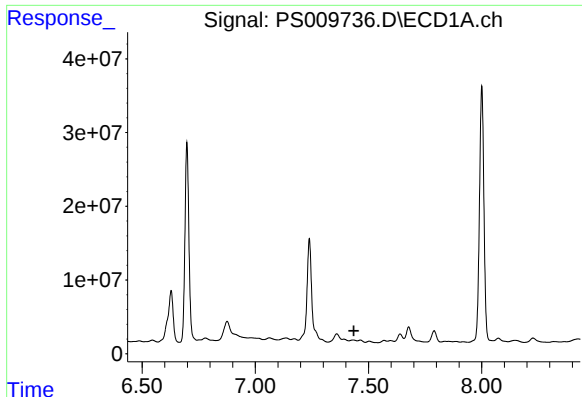

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

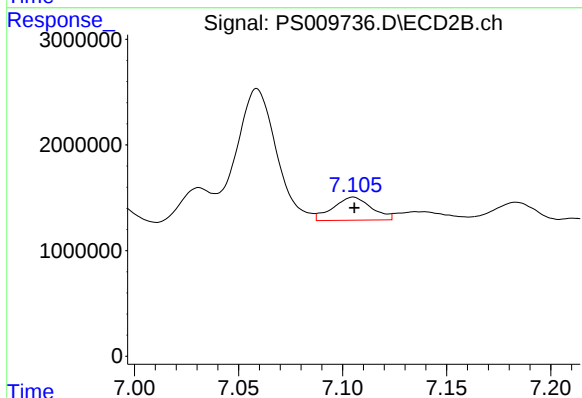


#5 DICAMBA

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 2814383
Conc: 1.23 ng/ml

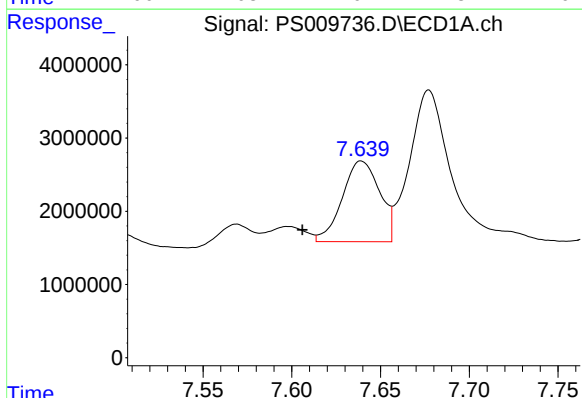


#6 MCP

R.T.: 7.639 min
Delta R.T.: 0.033 min
Response: 16166536
Conc: 6.57 ug/ml

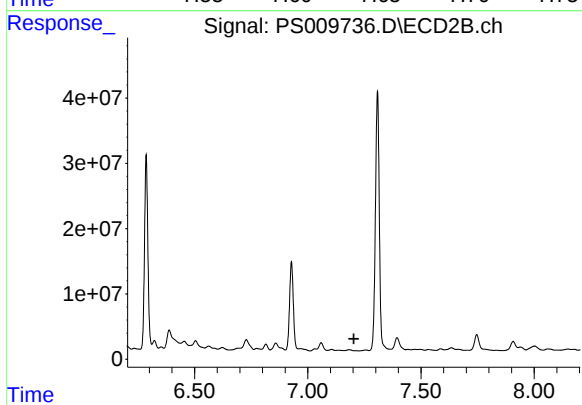

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

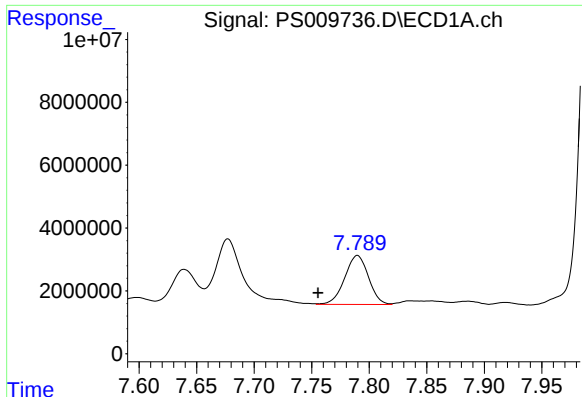

#7 MCPA


R.T.: 7.790 min
Delta R.T.: 0.034 min
Response: 22511062
Conc: 7.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

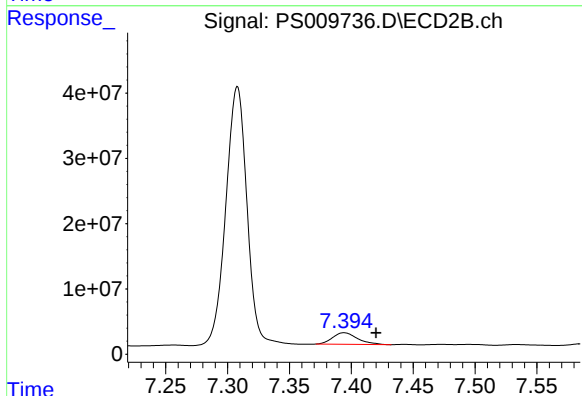


#7 MCPA

R.T.: 7.394 min
Delta R.T.: -0.026 min
Response: 25156224
Conc: 9.32 ug/ml

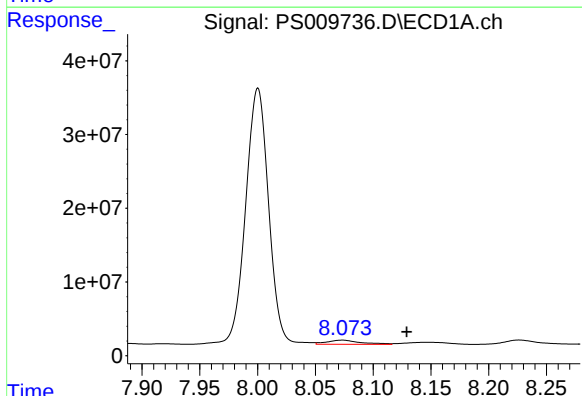


#8 DICHLORPROP

R.T.: 8.073 min
Delta R.T.: -0.056 min
Response: 11348633
Conc: 22.00 ng/ml

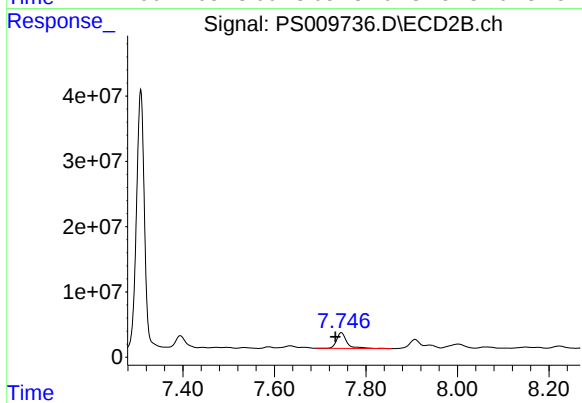

#8 DICHLORPROP


R.T.: 7.746 min
Delta R.T.: 0.013 min
Response: 38499815
Conc: 69.39 ng/ml

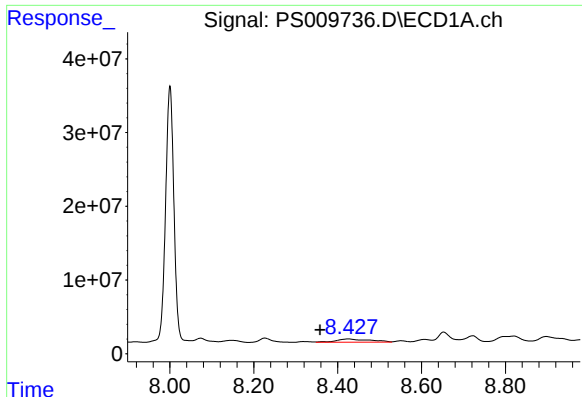

#9 2,4-D


R.T.: 8.426 min
Delta R.T.: 0.068 min
Response: 24902004
Conc: 47.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

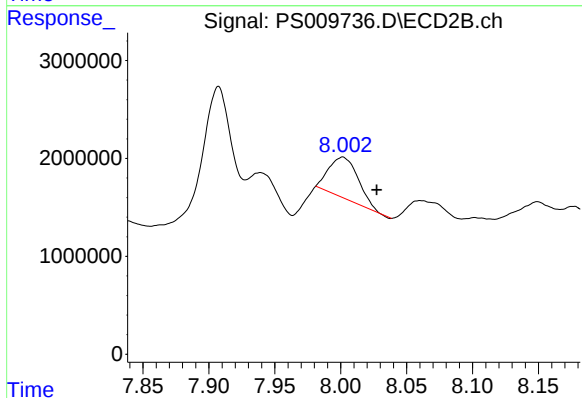


#9 2,4-D

R.T.: 8.001 min
Delta R.T.: -0.026 min
Response: 6478655
Conc: 9.86 ng/ml

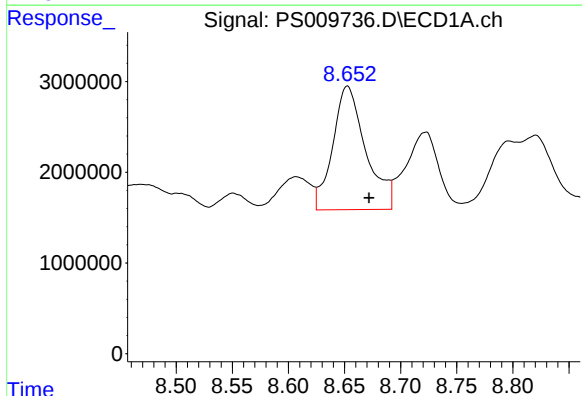


#10 Pentachlorophenol

R.T.: 8.653 min
Delta R.T.: -0.019 min
Response: 27908250
Conc: 3.97 ng/ml

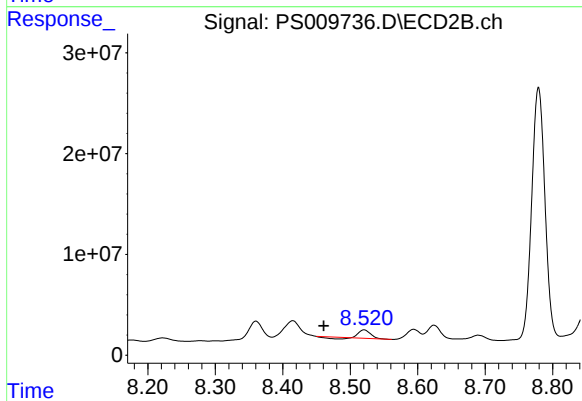

#10 Pentachlorophenol


R.T.: 8.521 min
Delta R.T.: 0.060 min
Response: 8186569
Conc: 1.08 ng/ml

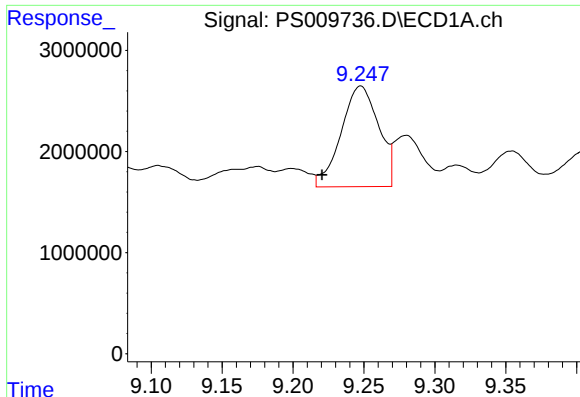

#11 2,4,5-TP (SILVEX)


R.T.: 9.248 min
Delta R.T.: 0.027 min
Response: 18366327
Conc: 6.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

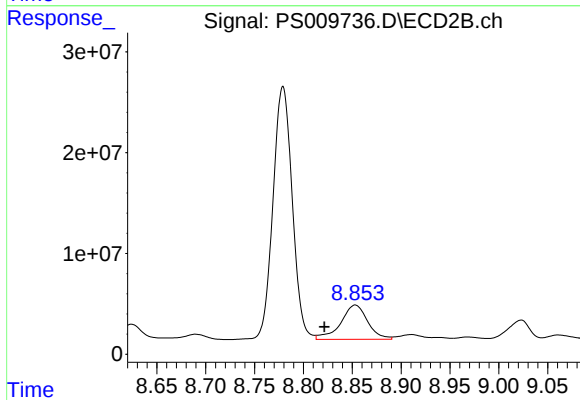


#11 2,4,5-TP (SILVEX)

R.T.: 8.853 min
Delta R.T.: 0.032 min
Response: 65460248
Conc: 21.96 ng/ml

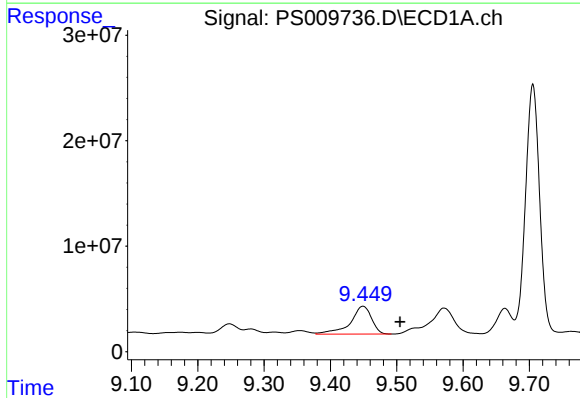


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: -0.056 min
Response: 58435951
Conc: 22.97 ng/ml

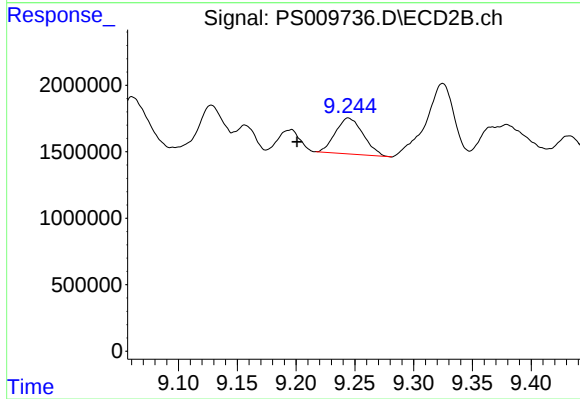

#12 2,4,5-T


R.T.: 9.245 min
Delta R.T.: 0.044 min
Response: 4450128
Conc: 1.51 ng/ml

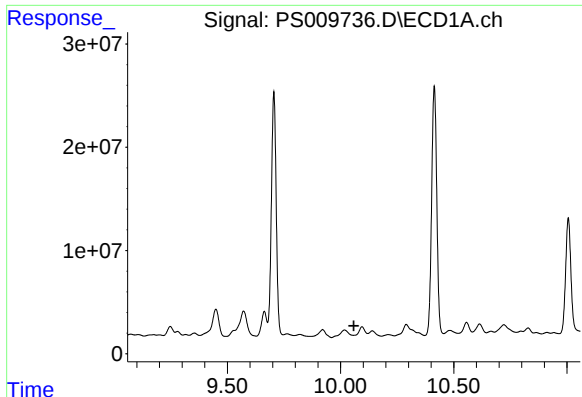

#13 2,4-DB


R.T.: 10.094 min
Delta R.T.: 0.036 min
Response: -570268
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

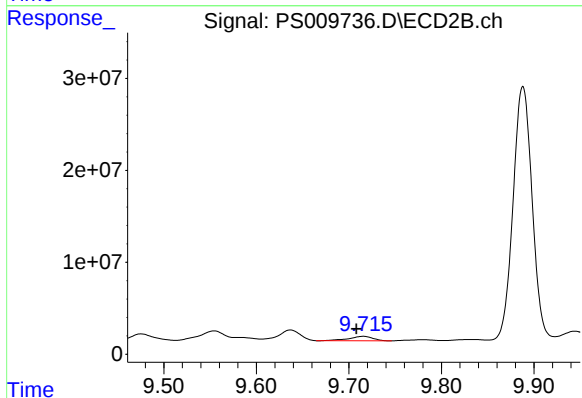


#13 2,4-DB

R.T.: 9.716 min
Delta R.T.: 0.007 min
Response: 8686087
Conc: 22.88 ng/ml

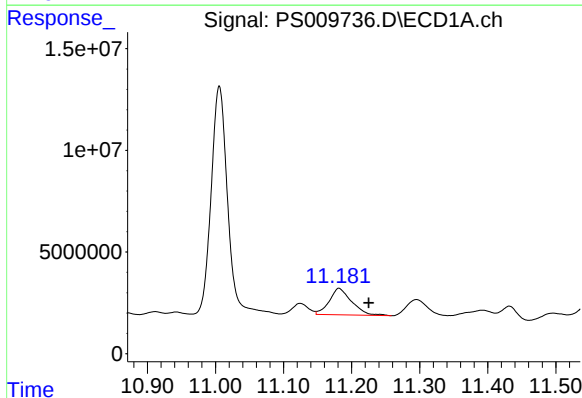


#14 DINOSEB

R.T.: 11.182 min
Delta R.T.: -0.043 min
Response: 29944276
Conc: 14.65 ng/ml

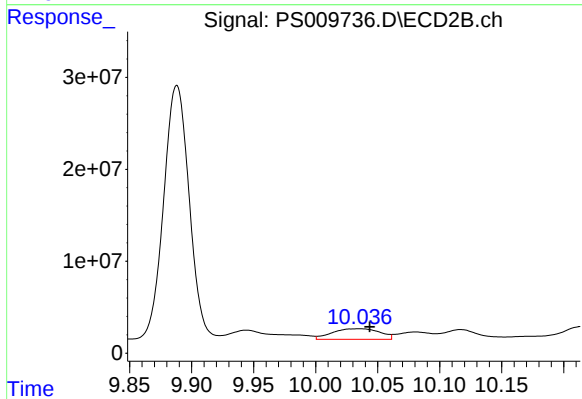

#14 DINOSEB


R.T.: 10.035 min
Delta R.T.: -0.008 min
Response: 30692316
Conc: 13.97 ng/ml

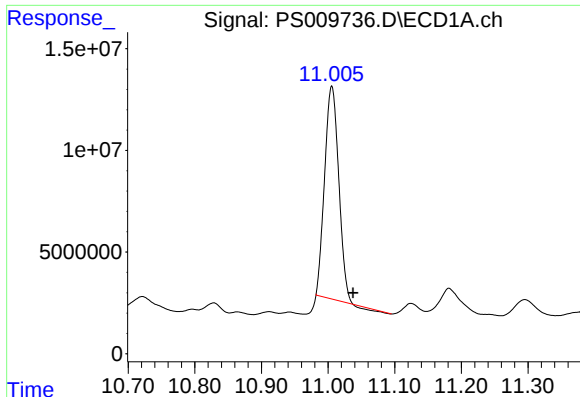

#15 Picloram


R.T.: 11.006 min
Delta R.T.: -0.032 min
Response: 152547127
Conc: 50.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

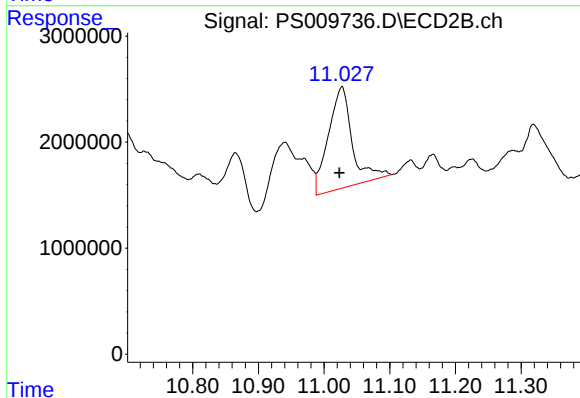


#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.004 min
Response: 24120567
Conc: 5.92 ng/ml

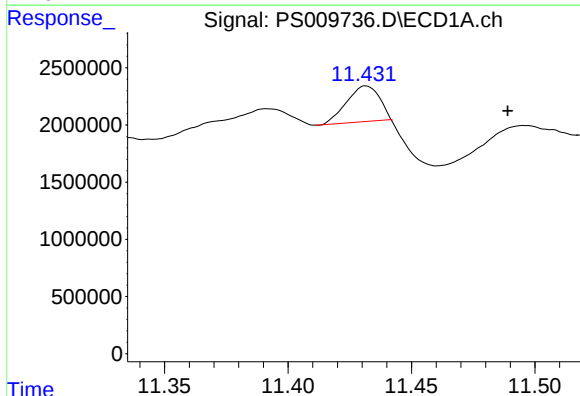

#16 DCPA

R.T.: 11.432 min
Delta R.T.: -0.057 min
Response: 2998754
Conc: N.D.

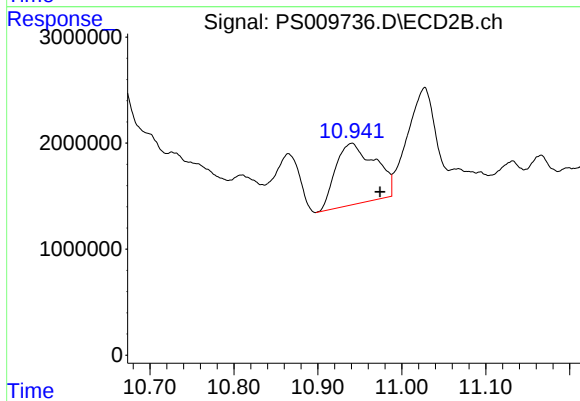

#16 DCPA

R.T.: 10.940 min
Delta R.T.: -0.034 min
Response: 18805337
Conc: 4.86 ng/ml