

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041421\
 Data File : PS014641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 08:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 12:43:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.883	708.2E6	263.8E6	465.552	566.657
Target Compounds							
2) T	3,5-DICHL...	6.426f	0.000	5135656	0	2.479	N.D. #
5) T	DICAMBA	0.000	7.050	0	1090340	N.D.	<MDL
6) T	MCP	0.000	7.116	0	2284326	N.D.	1.356
7) T	MCPA	7.612f	0.000	8251035	0	1.326	N.D. #
8) T	DICHLORPROP	0.000	7.721f	0	1681358	N.D.	3.331
12) T	2,4,5-T	9.405	9.147	8411893	2293578	1.023	<MDL #
13) T	2,4-DB	9.959	0.000	4758191	0	3.127	N.D. #
14) T	DINOSEB	11.095	0.000	6341329	0	<MDL	N.D. #
15) T	Picloram	10.931	10.963	203.3E6	75242813	18.174	20.065
16) T	DCPA	11.360	10.896	5941178	2350228	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041421\
Data File : PS014641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 08:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 12:43:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

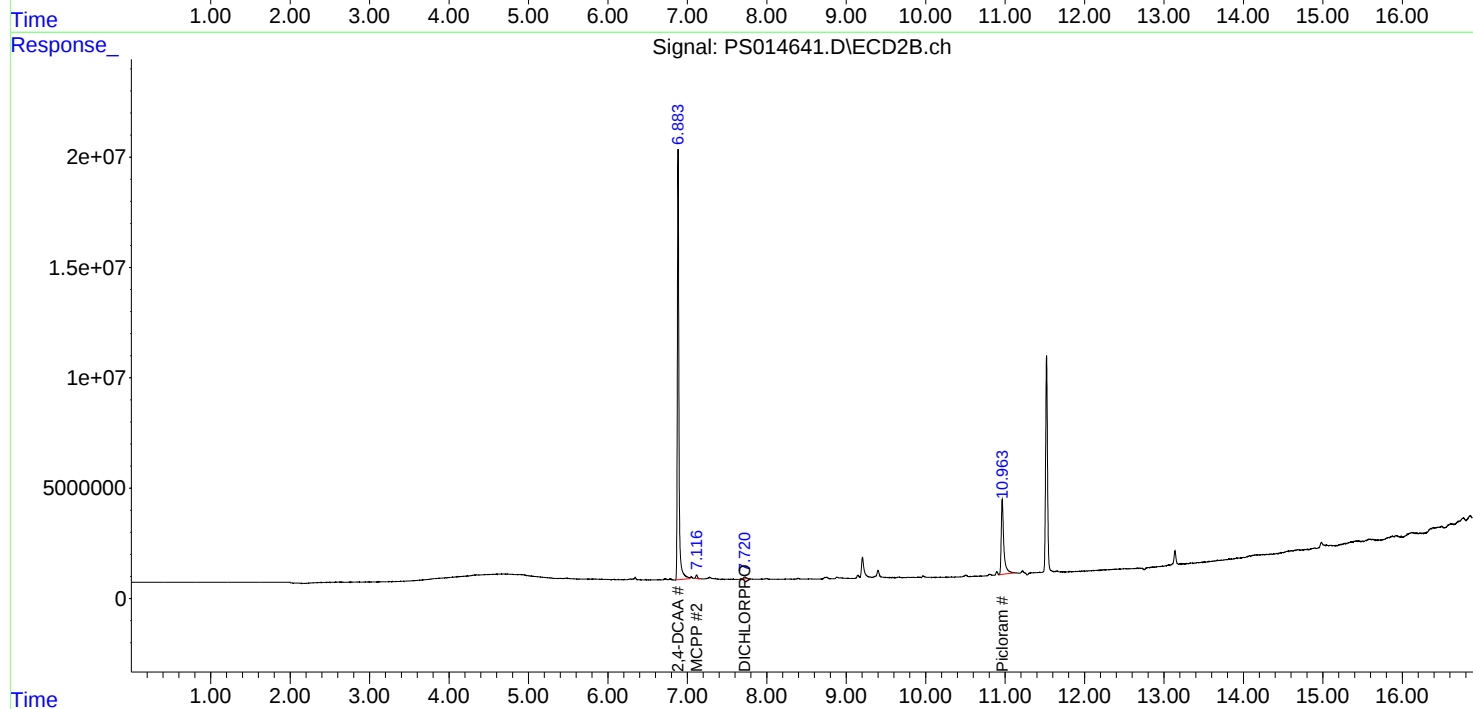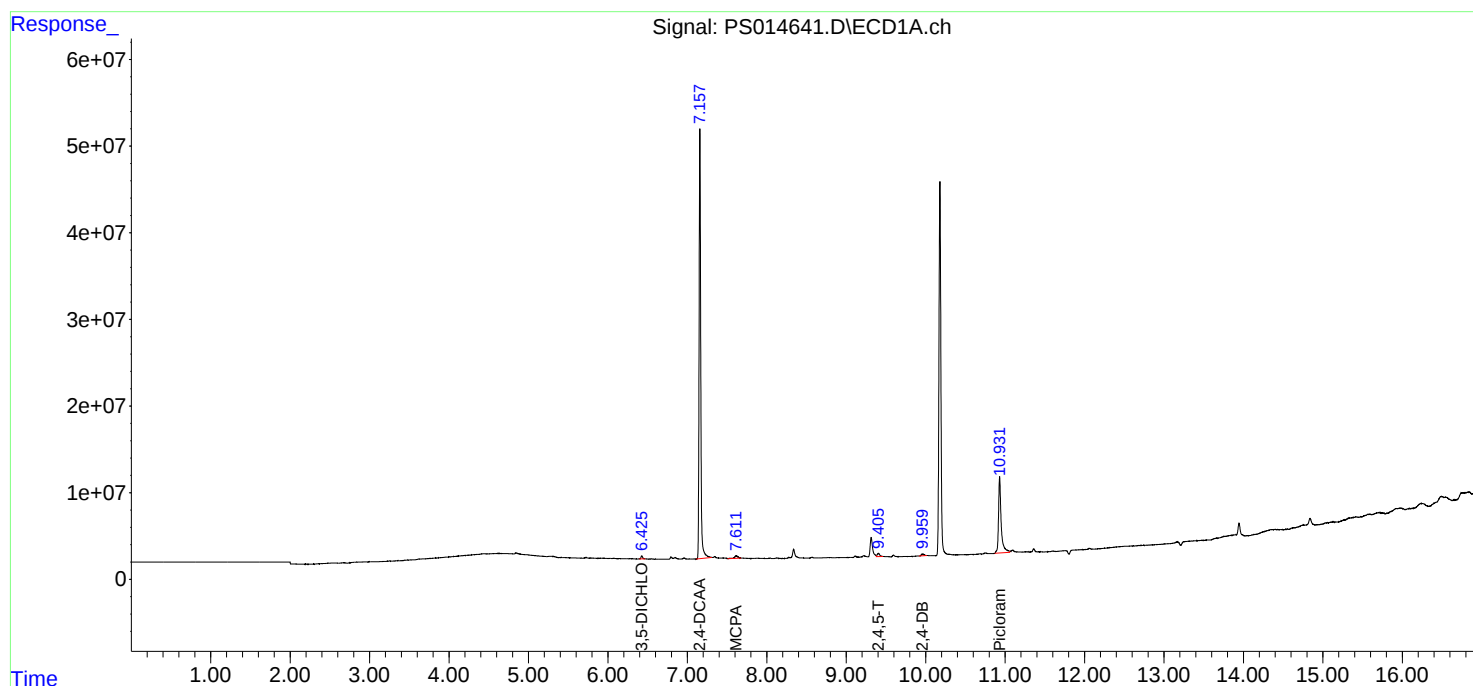


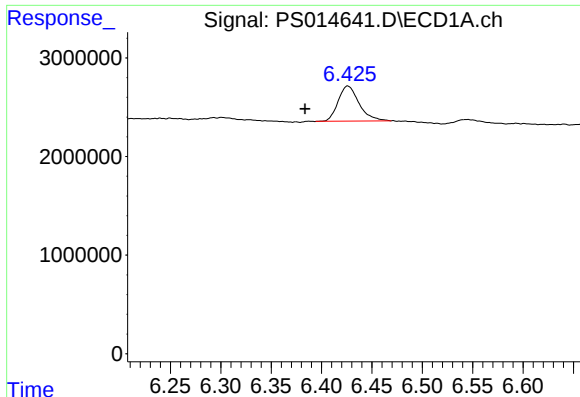

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.426 min
Delta R.T.: 0.042 min
Response: 5135656
Conc: 2.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

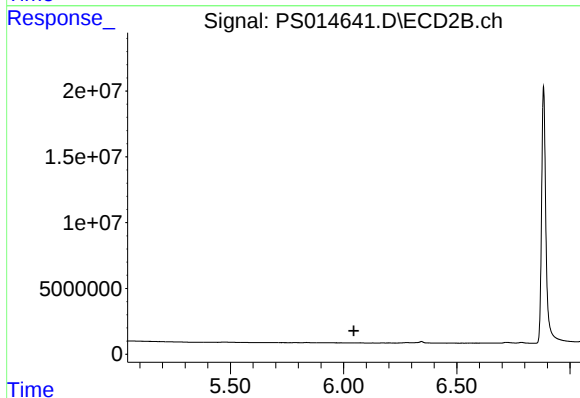


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

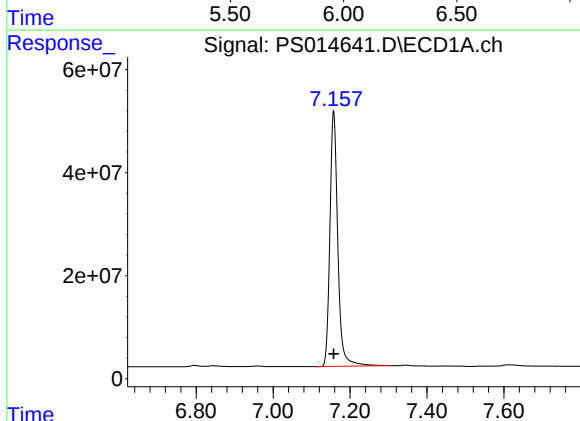


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 708195403
Conc: 465.55 ng/ml

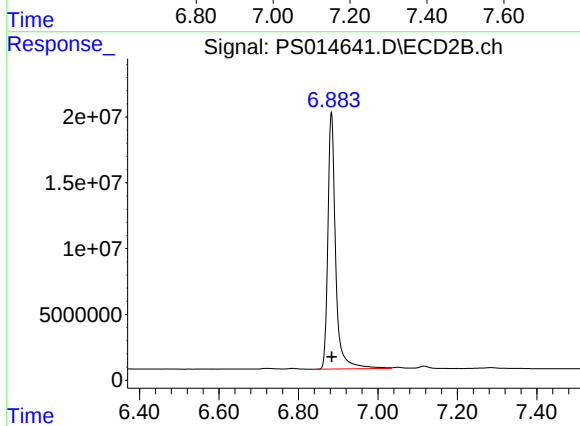

#4 2,4-DCAA


R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 263753003
Conc: 566.66 ng/ml

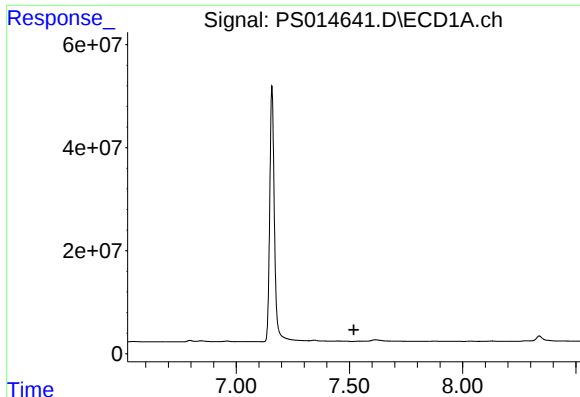

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

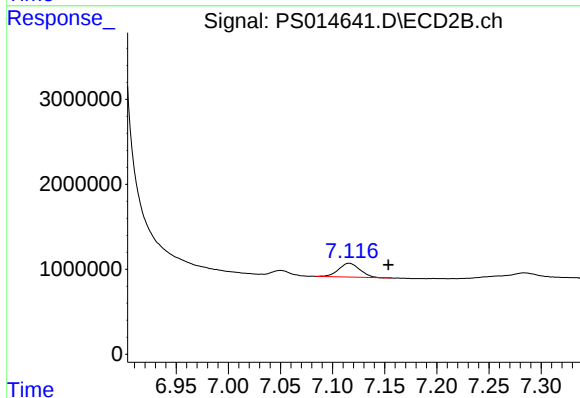


#6 MCPP

R.T.: 7.116 min
Delta R.T.: -0.037 min
Response: 2284326
Conc: 1.36 ug/ml

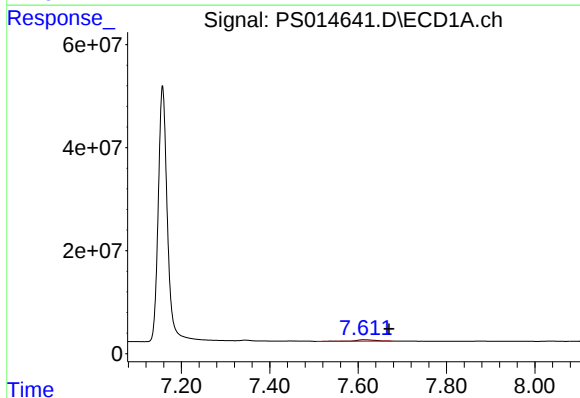


#7 MCPA

R.T.: 7.612 min
Delta R.T.: -0.058 min
Response: 8251035
Conc: 1.33 ug/ml

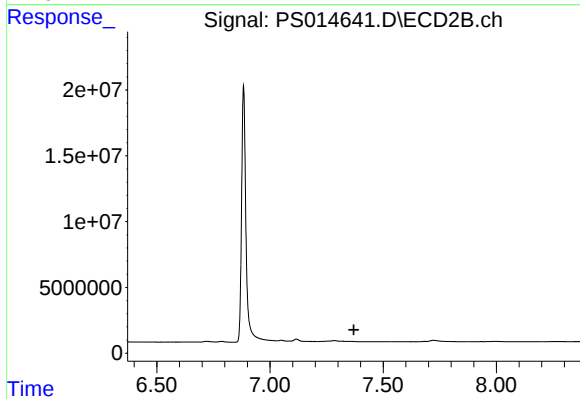

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

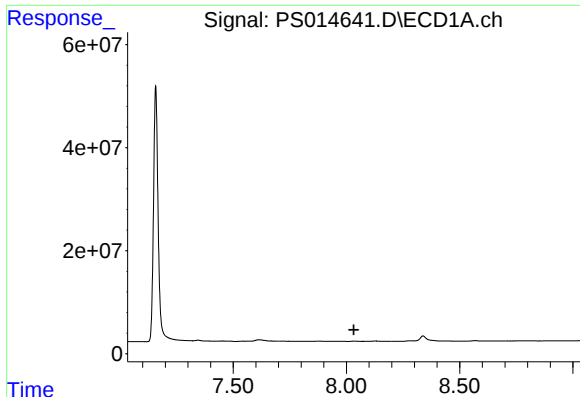

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

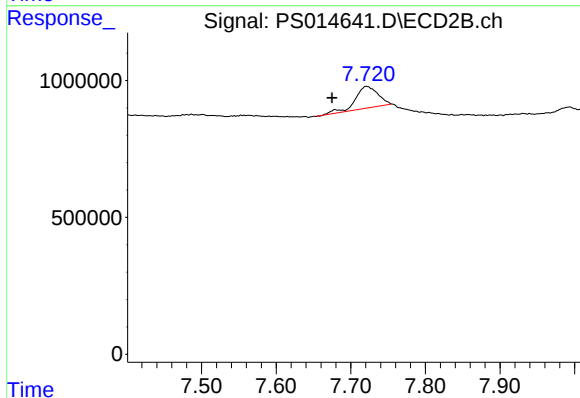


#8 DICHLORPROP

R.T.: 7.721 min
Delta R.T.: 0.046 min
Response: 1681358
Conc: 3.33 ng/ml

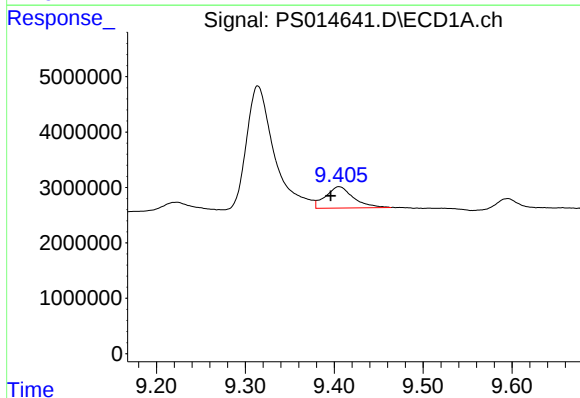


#12 2,4,5-T

R.T.: 9.405 min
Delta R.T.: 0.009 min
Response: 8411893
Conc: 1.02 ng/ml

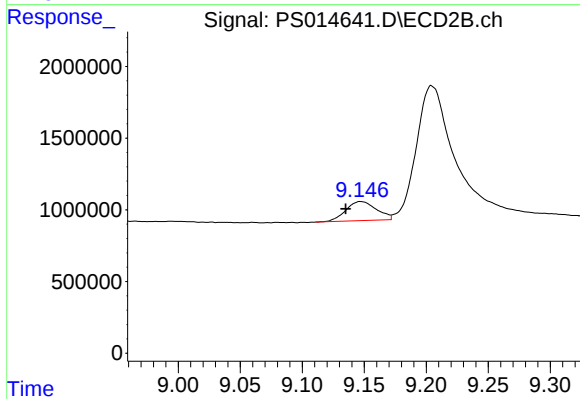

#12 2,4,5-T


R.T.: 9.147 min
Delta R.T.: 0.012 min
Response: 2293578
Conc: N.D.

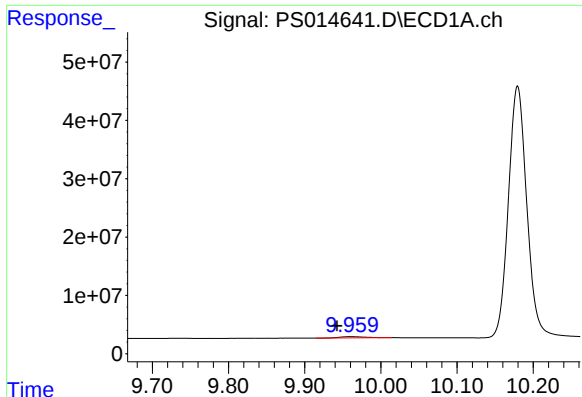

#13 2,4-DB


R.T.: 9.959 min
Delta R.T.: 0.017 min
Response: 4758191
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

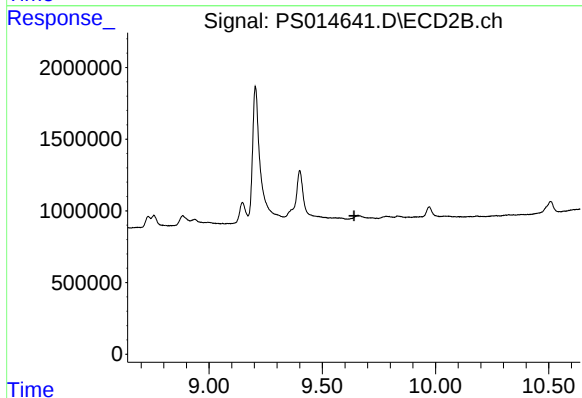


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.640 min
Response: 0
Conc: N.D.

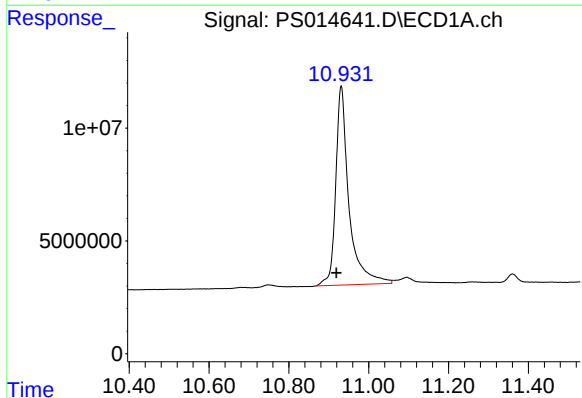

#15 Picloram

R.T.: 10.931 min
Delta R.T.: 0.012 min
Response: 203338811
Conc: 18.17 ng/ml

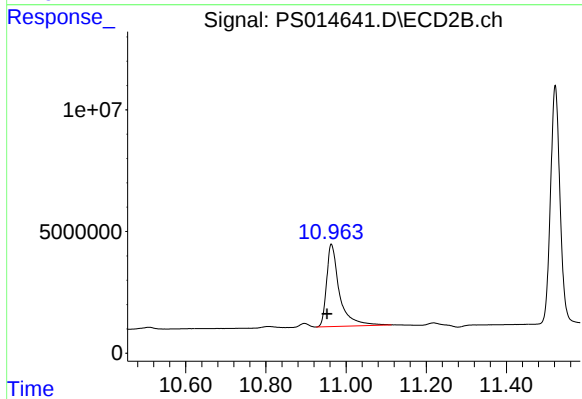

#15 Picloram

R.T.: 10.963 min
Delta R.T.: 0.011 min
Response: 75242813
Conc: 20.07 ng/ml