

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041421\
 Data File : PS014652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 13:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 14:57:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.880	711.6E6	260.0E6	467.770	558.516
Target Compounds							
2) T	3,5-DICHL...	6.423	0.000	3971847	0	1.917	N.D. #
5) T	DICAMBA	0.000	7.112f	0	1780638	N.D.	<MDL
6) T	MCP	0.000	7.112f	0	1780638	N.D.	1.057
7) T	MCPA	7.607f	0.000	7764490	0	1.248	N.D. #
8) T	DICHLORPROP	0.000	7.715	0	2002723	N.D.	3.967
15) T	Picloram	10.891	0.000	2286735	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041421\
Data File : PS014652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 13:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 14:57:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

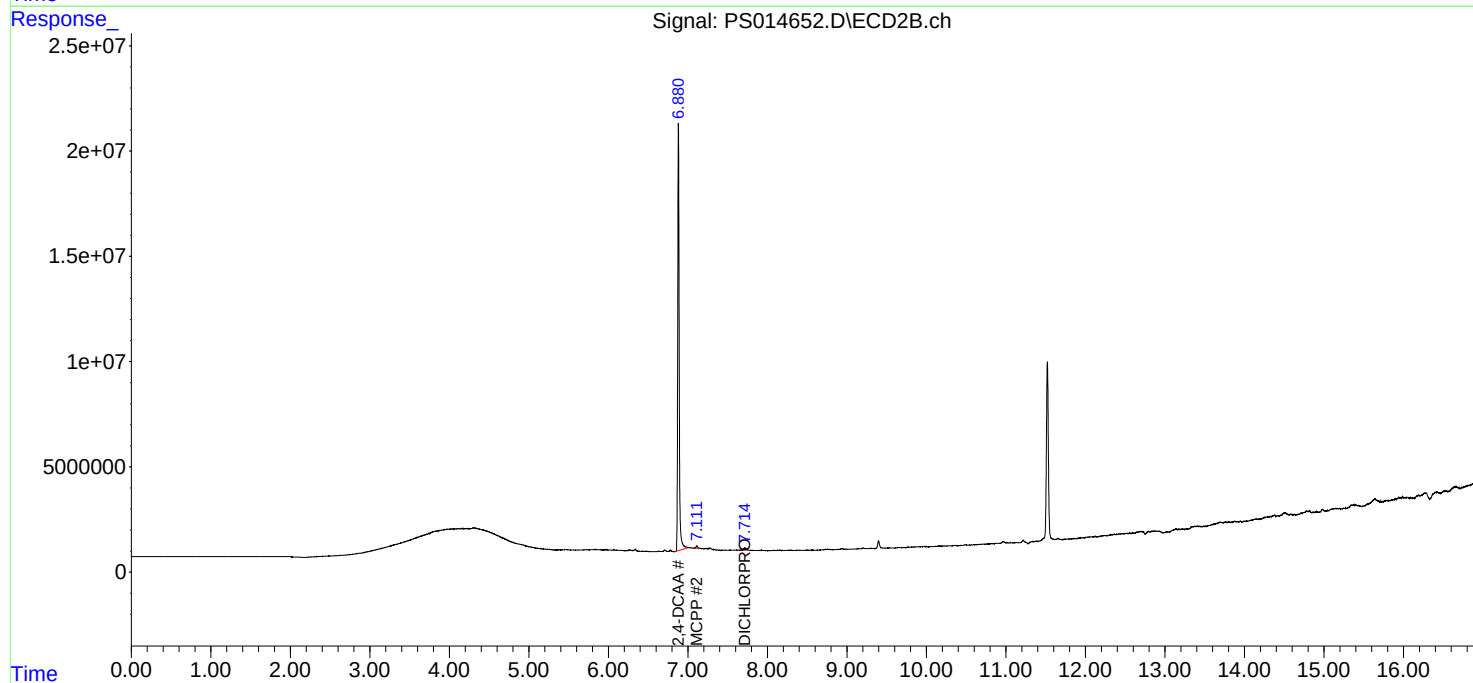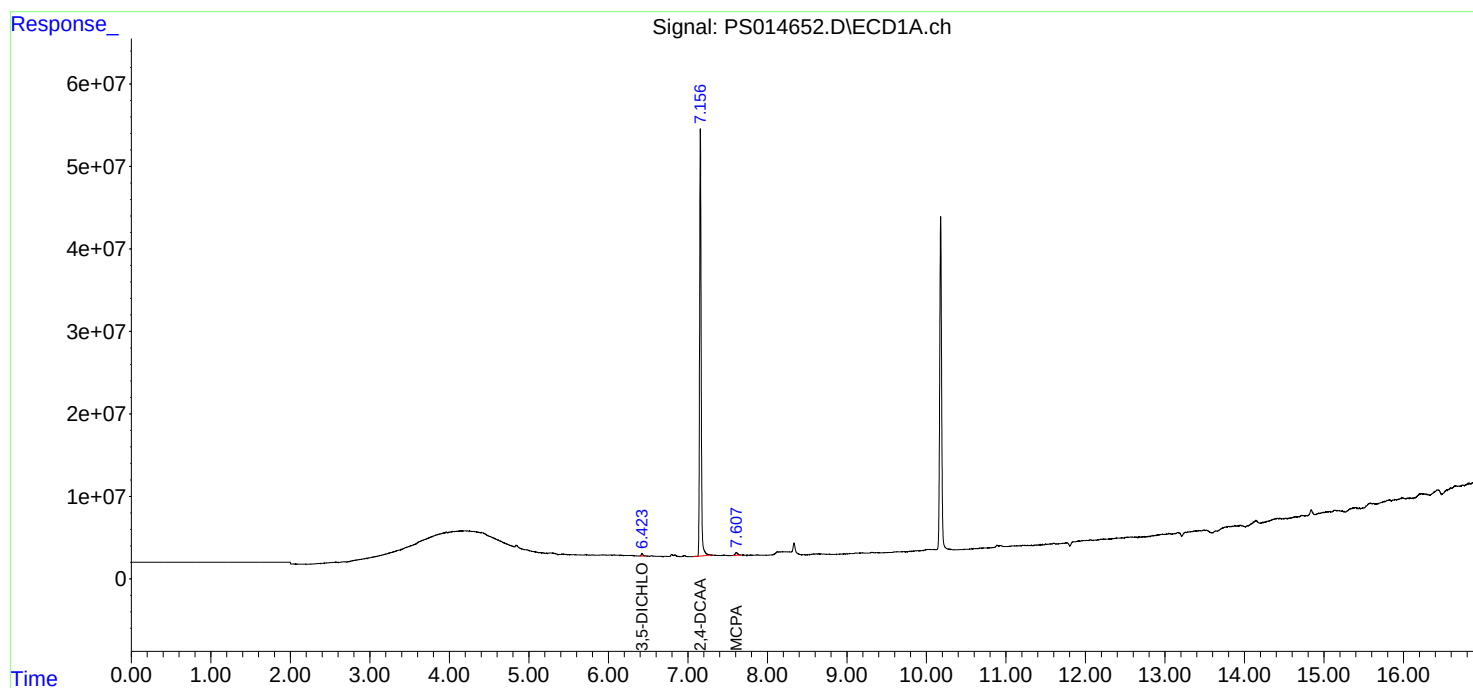


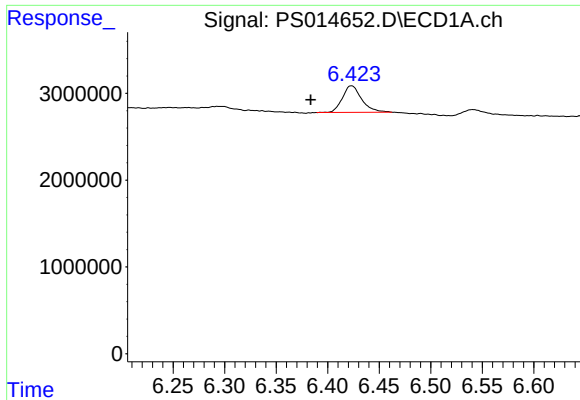

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.423 min
Delta R.T.: 0.039 min
Response: 3971847
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

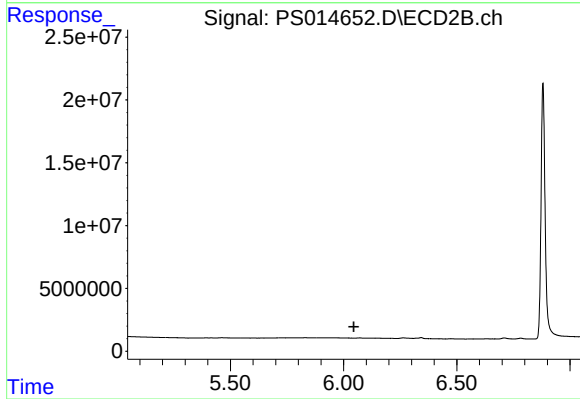


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.045 min
Response: 0
Conc: N.D.

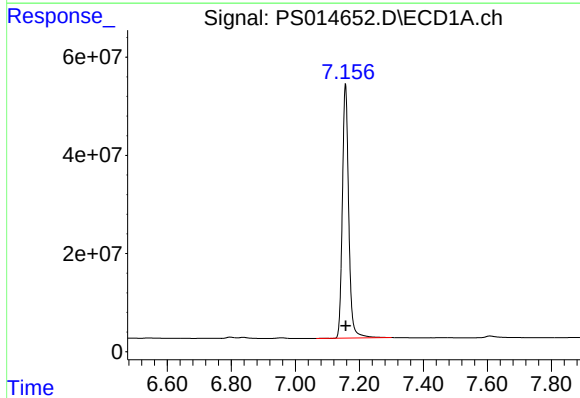


#4 2,4-DCAA

R.T.: 7.157 min
Delta R.T.: -0.001 min
Response: 711570213
Conc: 467.77 ng/ml

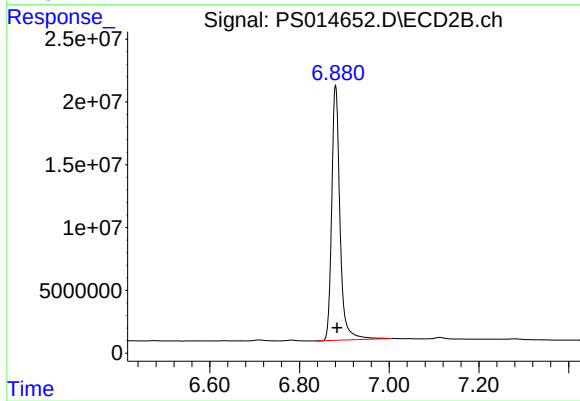

#4 2,4-DCAA


R.T.: 6.880 min
Delta R.T.: -0.003 min
Response: 259963743
Conc: 558.52 ng/ml

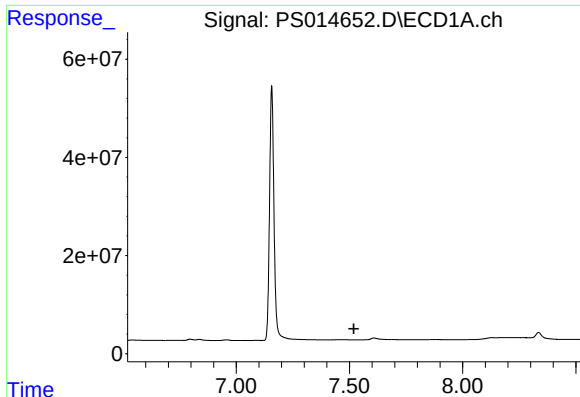

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.520 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

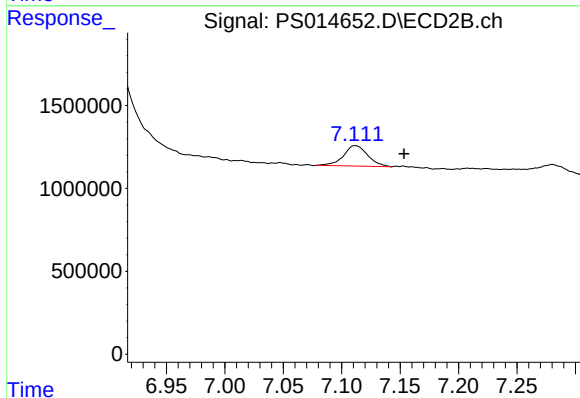


#6 MCPP

R.T.: 7.112 min
Delta R.T.: -0.042 min
Response: 1780638
Conc: 1.06 ug/ml

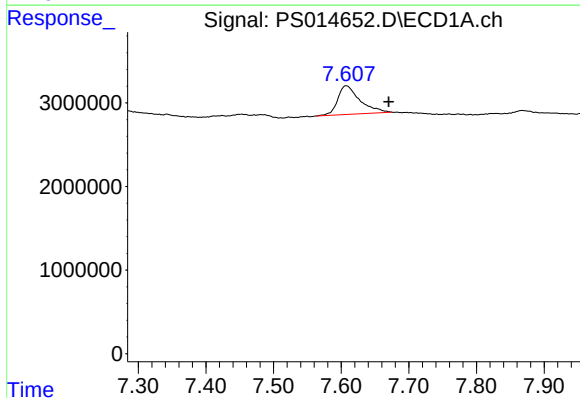


#7 MCPA

R.T.: 7.607 min
Delta R.T.: -0.063 min
Response: 7764490
Conc: 1.25 ug/ml

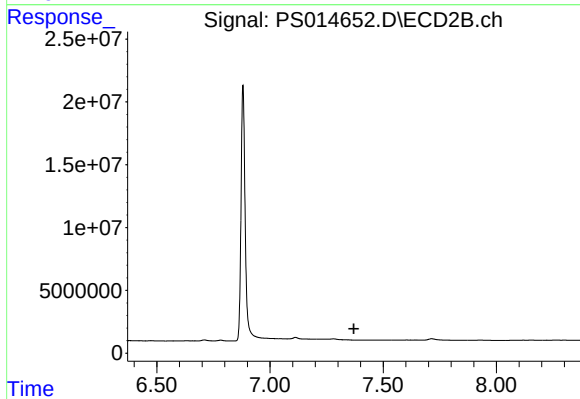

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

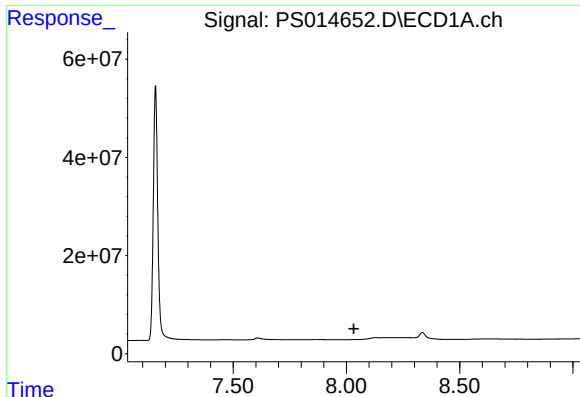

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

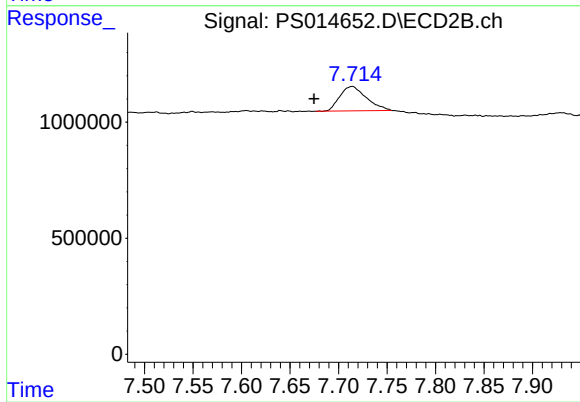

#8 DICHLORPROP

R.T.: 7.715 min
Delta R.T.: 0.040 min
Response: 2002723
Conc: 3.97 ng/ml