

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041422\
 Data File : PS018985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2022 10:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 03:22:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041422.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 15 02:14:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.803	1535.8E6	359.8E6	434.494	473.763
Target Compounds							
9) T	2,4-D	8.418f	0.000	25784040	0	6.482	N.D. #
11) T	2,4,5-TP ...	0.000	8.644	0	2971613	N.D.	<MDL
12) T	2,4,5-T	9.452f	0.000	26658357	0	1.439	N.D. #
13) T	2,4-DB	0.000	9.495f	0	3868416	N.D.	6.564
15) T	Picloram	11.015	10.918	11139170	16488327	<MDL	2.826 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041422\
Data File : PS018985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2022 10:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 03:22:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041422.M
Quant Title : 8080.M
QLast Update : Fri Apr 15 02:14:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

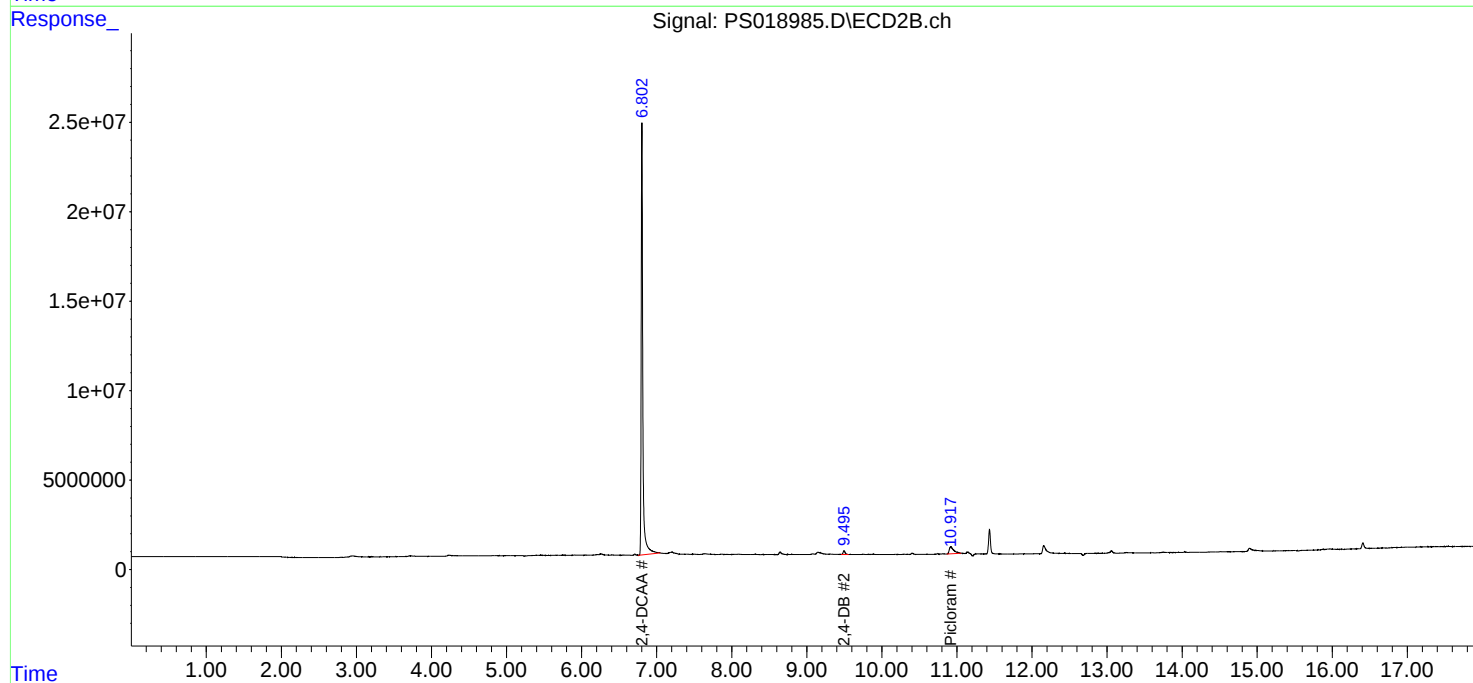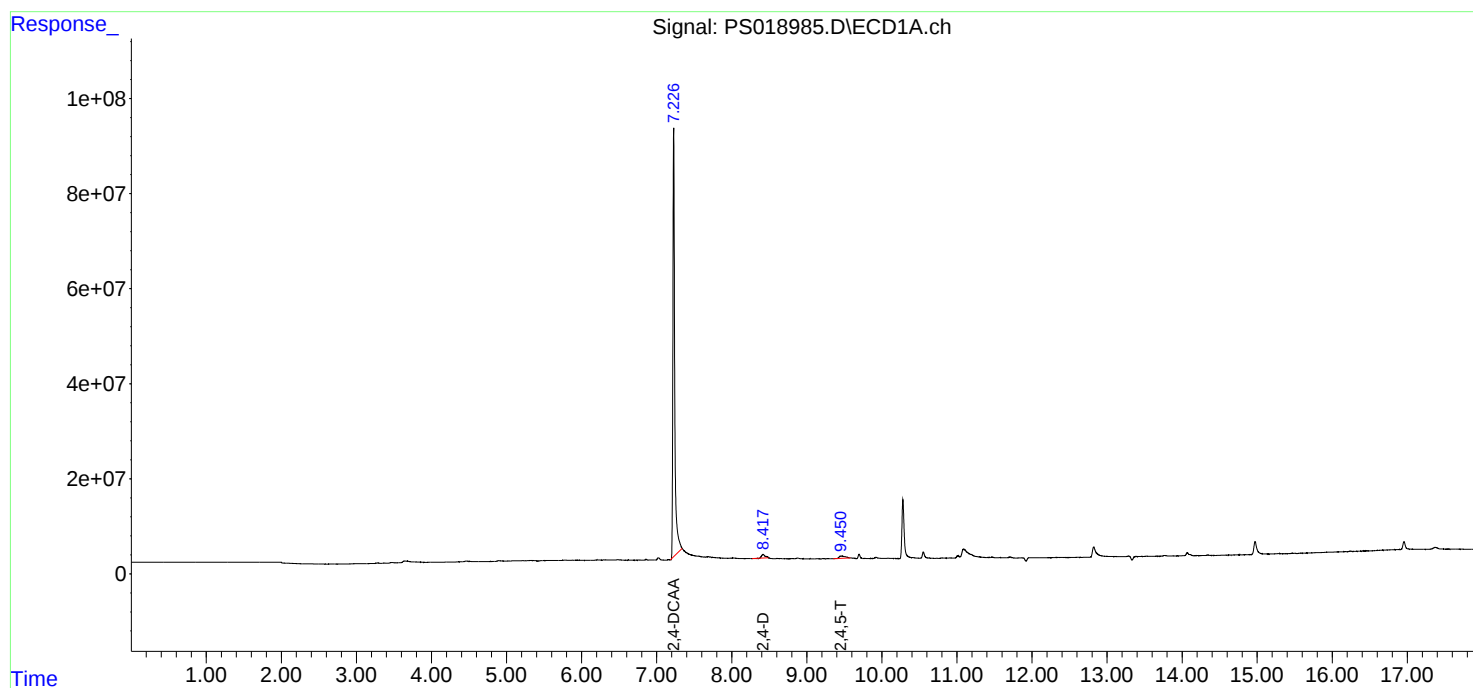


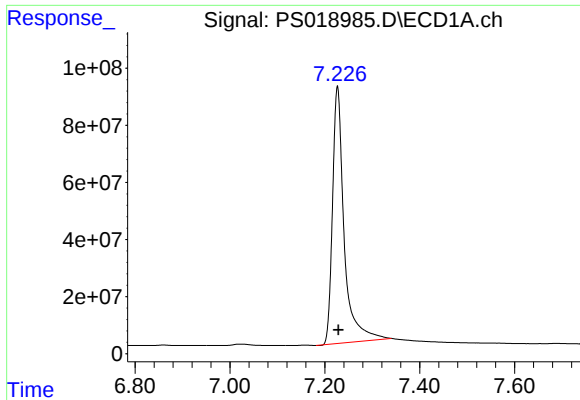

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: -0.002 min
Response: 1535790840
Conc: 434.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

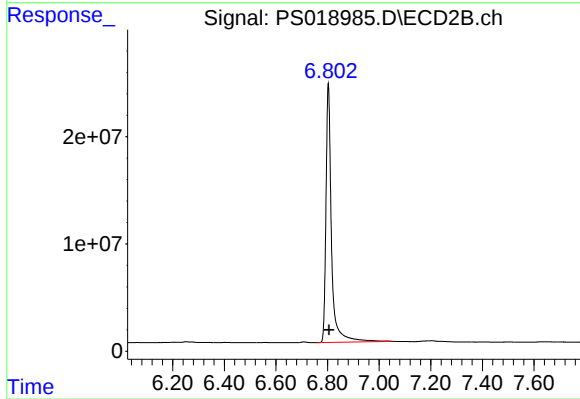


#4 2,4-DCAA

R.T.: 6.803 min
Delta R.T.: -0.003 min
Response: 359845706
Conc: 473.76 ng/ml

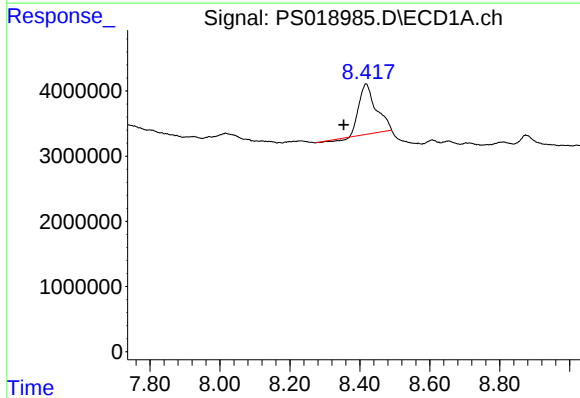


#9 2,4-D

R.T.: 8.418 min
Delta R.T.: 0.064 min
Response: 25784040
Conc: 6.48 ng/ml

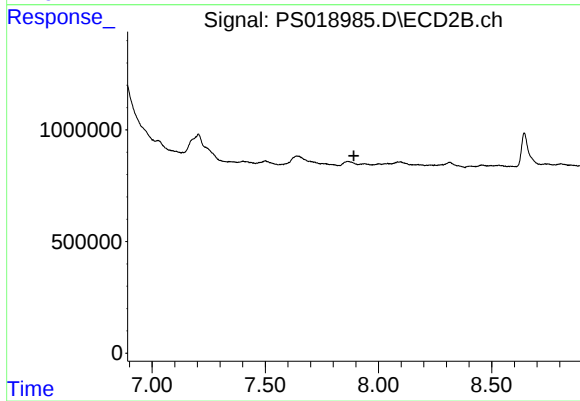

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.891 min
Response: 0
Conc: N.D.

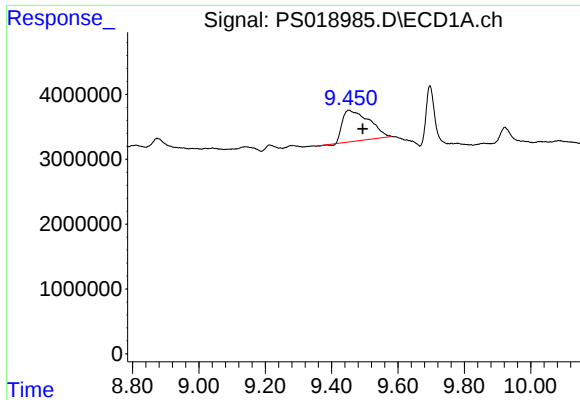

#12 2,4,5-T


R.T.: 9.452 min
Delta R.T.: -0.042 min
Response: 26658357
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

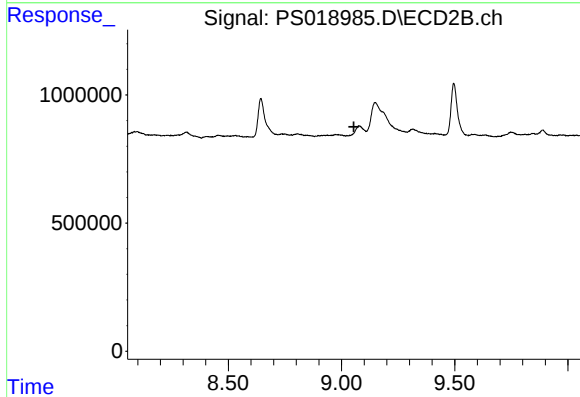


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.055 min
Response: 0
Conc: N.D.

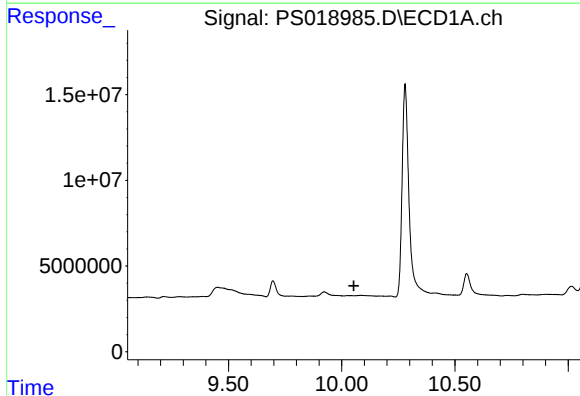


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.053 min
Response: 0
Conc: N.D.

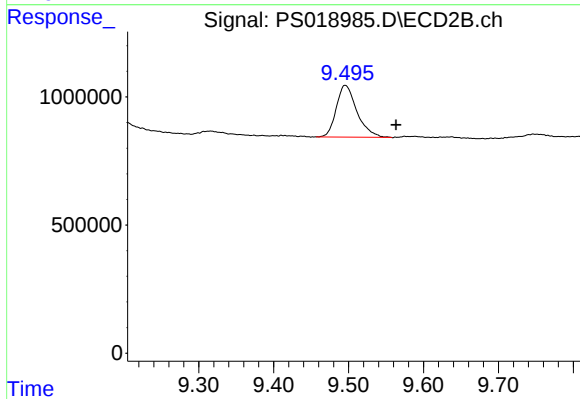

#13 2,4-DB


R.T.: 9.495 min
Delta R.T.: -0.068 min
Response: 3868416
Conc: 6.56 ng/ml

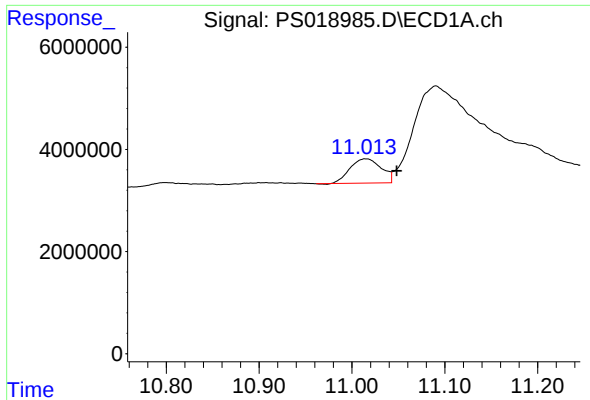

#15 Picloram

R.T.: 11.015 min
Delta R.T.: -0.033 min
Response: 11139170
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

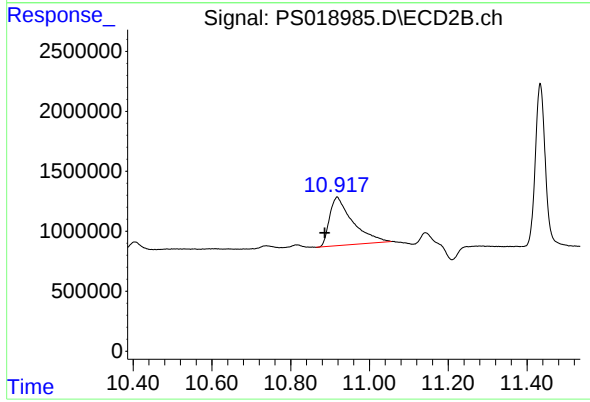

#15 Picloram

R.T.: 10.918 min
Delta R.T.: 0.031 min
Response: 16488327
Conc: 2.83 ng/ml