

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041422\
 Data File : PS019011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 04:32
 Operator : AJ\MA
 Sample : I.BLNK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 05:14:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041422.M
 Quant Title : 8080.M
 QLast Update : Fri Apr 15 02:14:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.223	6.801	1559.8E6	358.4E6	441.288	471.868
Target Compounds							
7) T	MCPA	7.676f	0.000	13729874	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.617	0	2623527	N.D.	3.040
9) T	2,4-D	8.414f	0.000	17737866	0	4.459	N.D. #
11) T	2,4,5-TP ...	9.263f	8.630f	6358065	3983805	<MDL	<MDL #
12) T	2,4,5-T	9.488	9.111f	8463257	1457982	<MDL	<MDL #
14) T	DINOSEB	11.150f	0.000	17794813	0	1.100	N.D. #
15) T	Picloram	11.035	10.876	30887886	20195120	1.293	3.461 #
16) T	DCPA	0.000	10.876f	0	20195120	N.D.	3.437



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041422\
Data File : PS019011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 04:32
Operator : AJ\MA
Sample : I.BLNK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 05:14:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041422.M
Quant Title : 8080.M
QLast Update : Fri Apr 15 02:14:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

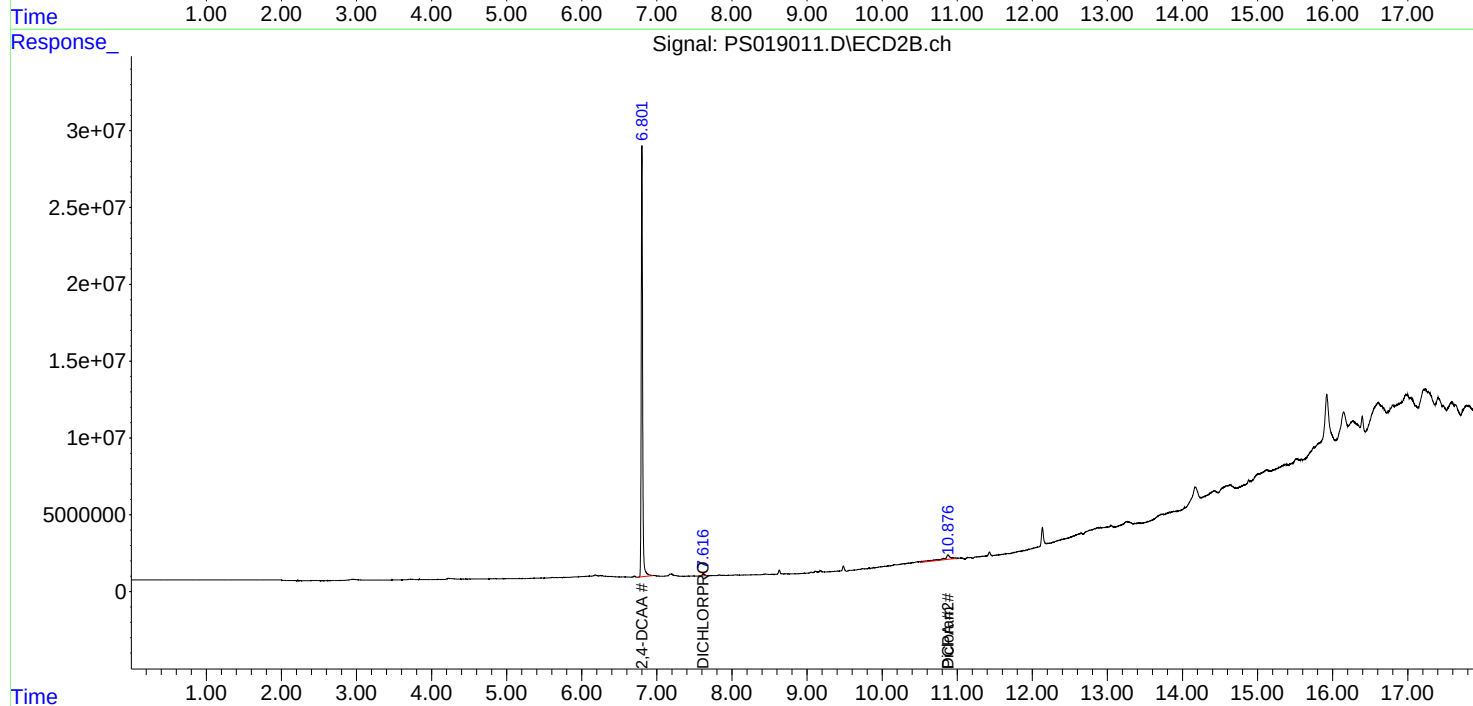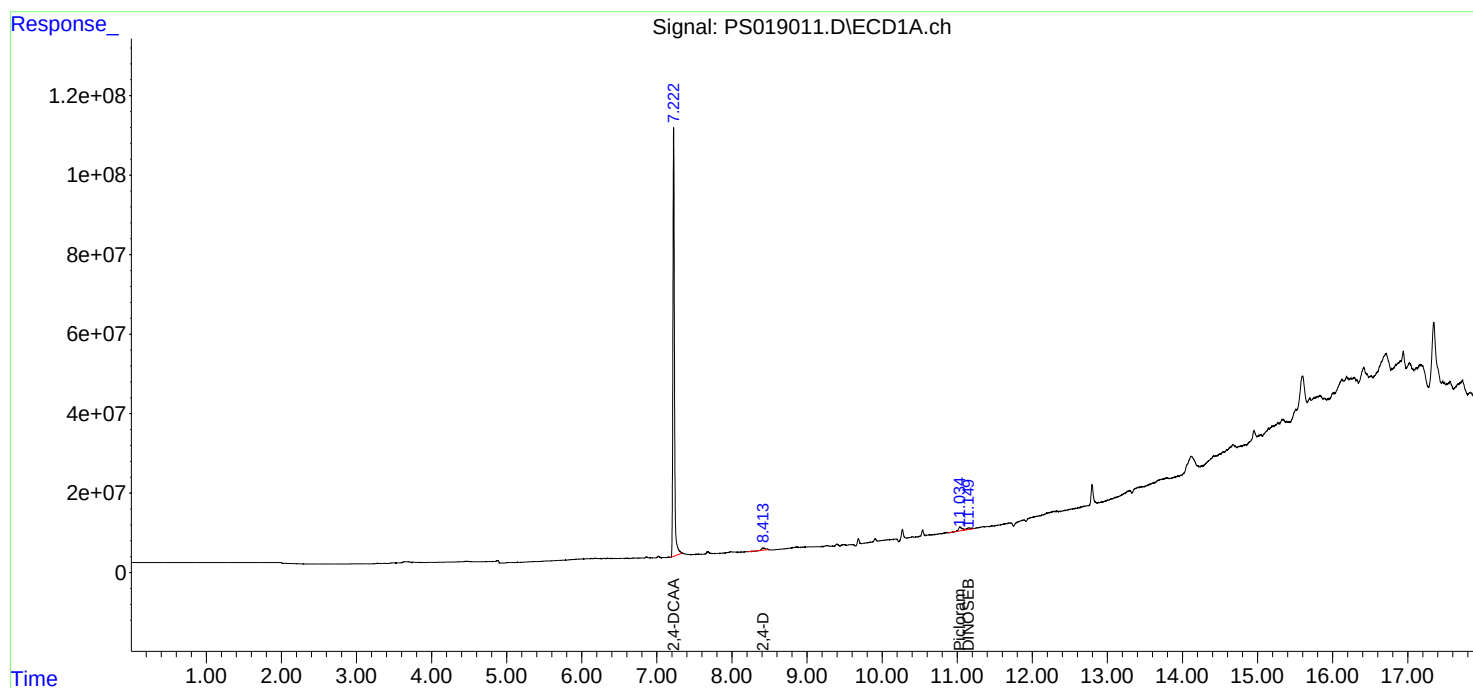


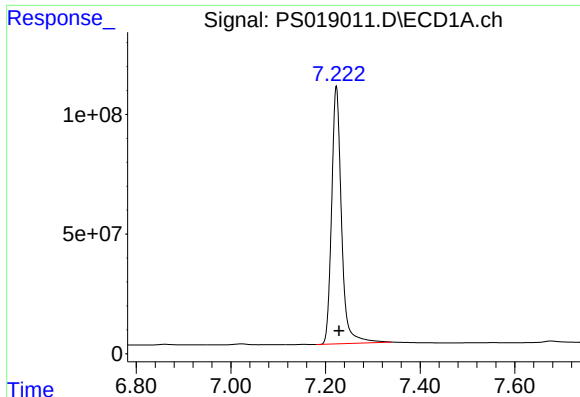

#4 2,4-DCAA


R.T.: 7.223 min
Delta R.T.: -0.006 min
Response: 1559806150
Conc: 441.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

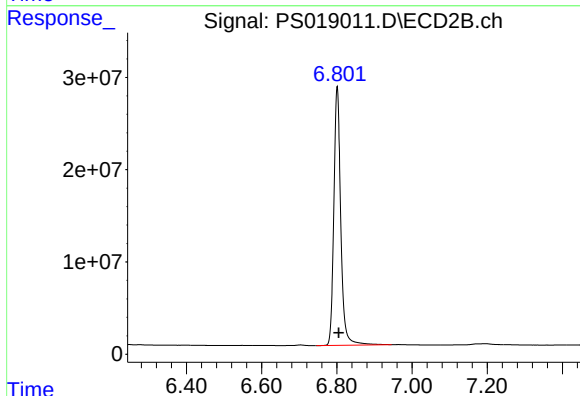


#4 2,4-DCAA

R.T.: 6.801 min
Delta R.T.: -0.004 min
Response: 358405942
Conc: 471.87 ng/ml

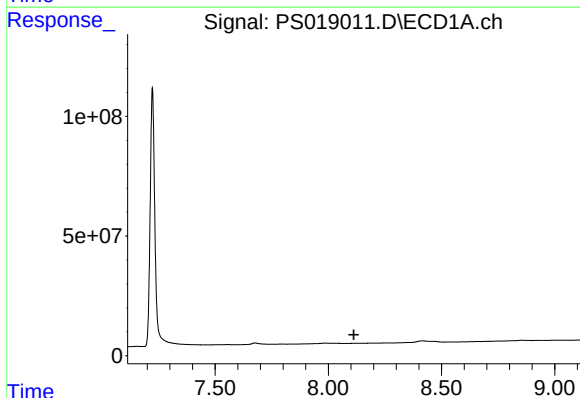


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

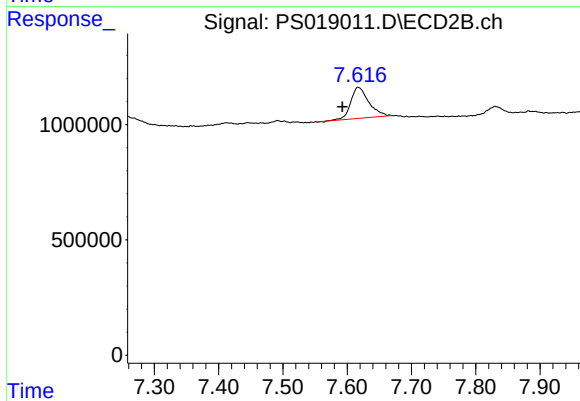

#8 DICHLORPROP


R.T.: 7.617 min
Delta R.T.: 0.024 min
Response: 2623527
Conc: 3.04 ng/ml

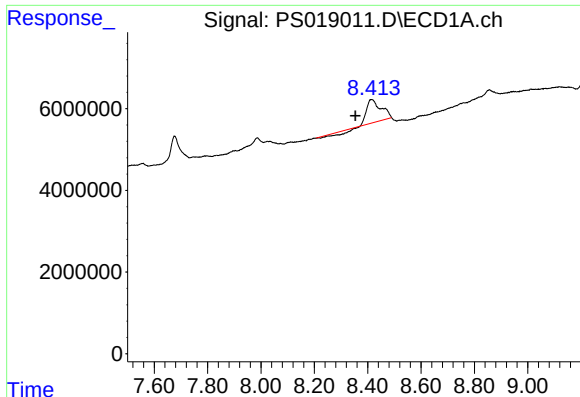

#9 2,4-D


R.T.: 8.414 min
Delta R.T.: 0.061 min
Response: 17737866
Conc: 4.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

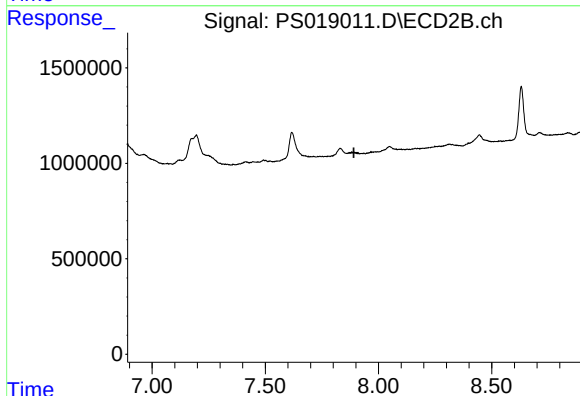


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.891 min
Response: 0
Conc: N.D.

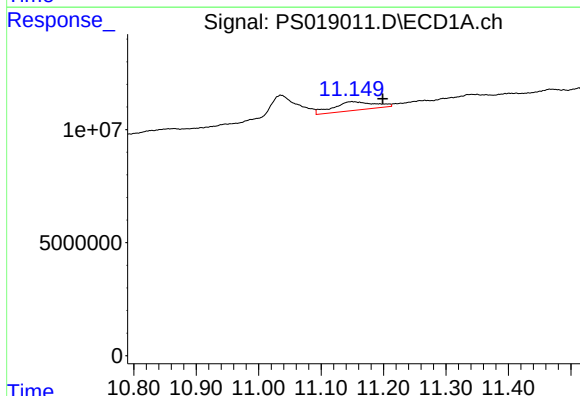


#14 DINOSEB

R.T.: 11.150 min
Delta R.T.: -0.049 min
Response: 17794813
Conc: 1.10 ng/ml

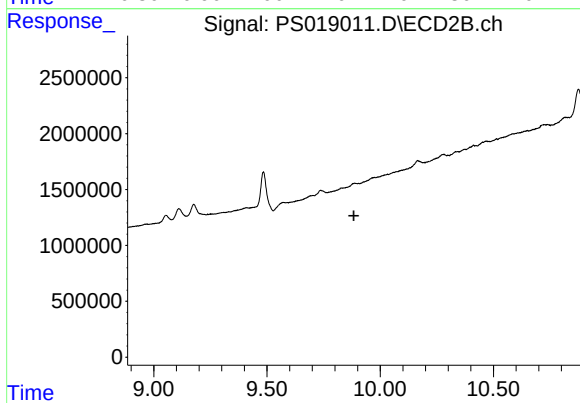

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

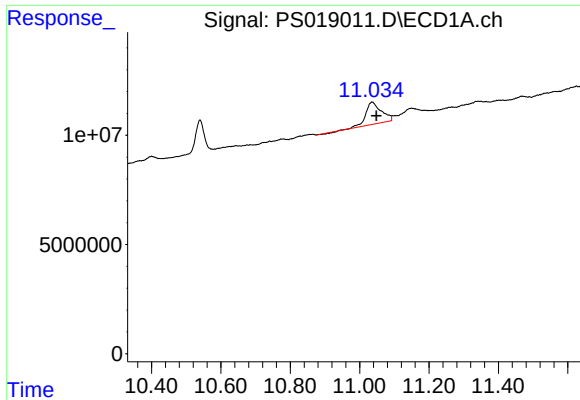

#15 Picloram


R.T.: 11.035 min
Delta R.T.: -0.013 min
Response: 30887886
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

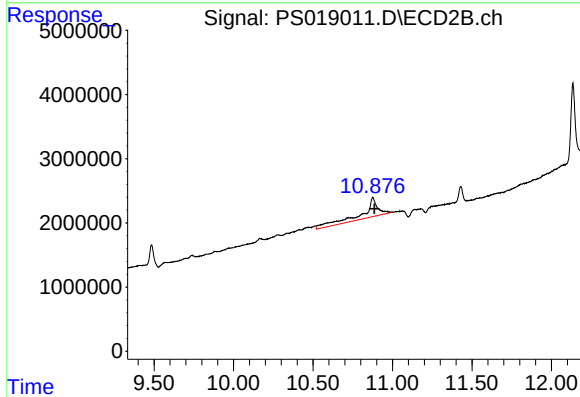


#15 Picloram

R.T.: 10.876 min
Delta R.T.: -0.011 min
Response: 20195120
Conc: 3.46 ng/ml

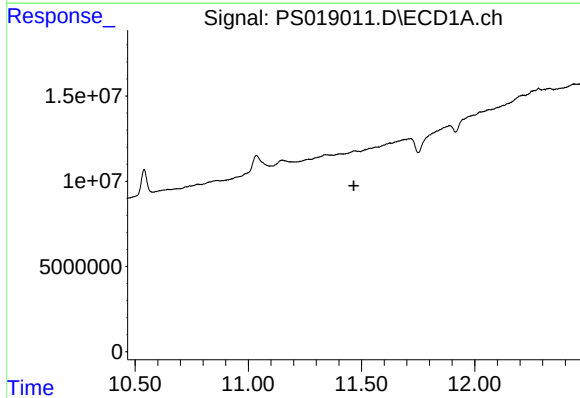

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.466 min
Response: 0
Conc: N.D.

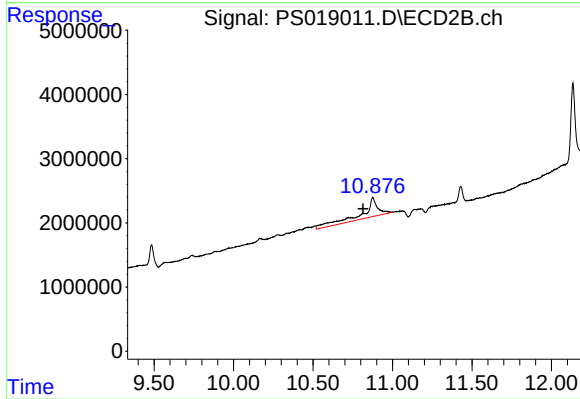

#16 DCPA

R.T.: 10.876 min
Delta R.T.: 0.061 min
Response: 20195120
Conc: 3.44 ng/ml